

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041574.D
 Acq On : 30 Aug 2023 11:28
 Operator : MA/JU
 Sample : 04134-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHJ0

Quant Time: Aug 31 02:25:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	8337	0.400	ng/ul	0.00
4) Naphthalene-d8	10.949	136	20877	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.754	164	10733	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.506	188	18777	0.400	ng/ul	0.00
17) Chrysene-d12	21.691	240	6478	0.400	ng/ul	0.00
23) Perylene-d12	24.257	264	7637	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.452	96	54442	4.425	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.522	152	7811	0.310	ng/ul	0.00
18) Fluoranthene-d10	19.524	212	11093	0.347	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.130	266	185129	25.656	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041574.D
Acq On : 30 Aug 2023 11:28
Operator : MA/JU
Sample : 04134-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHJ0


Quant Time: Aug 31 02:25:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

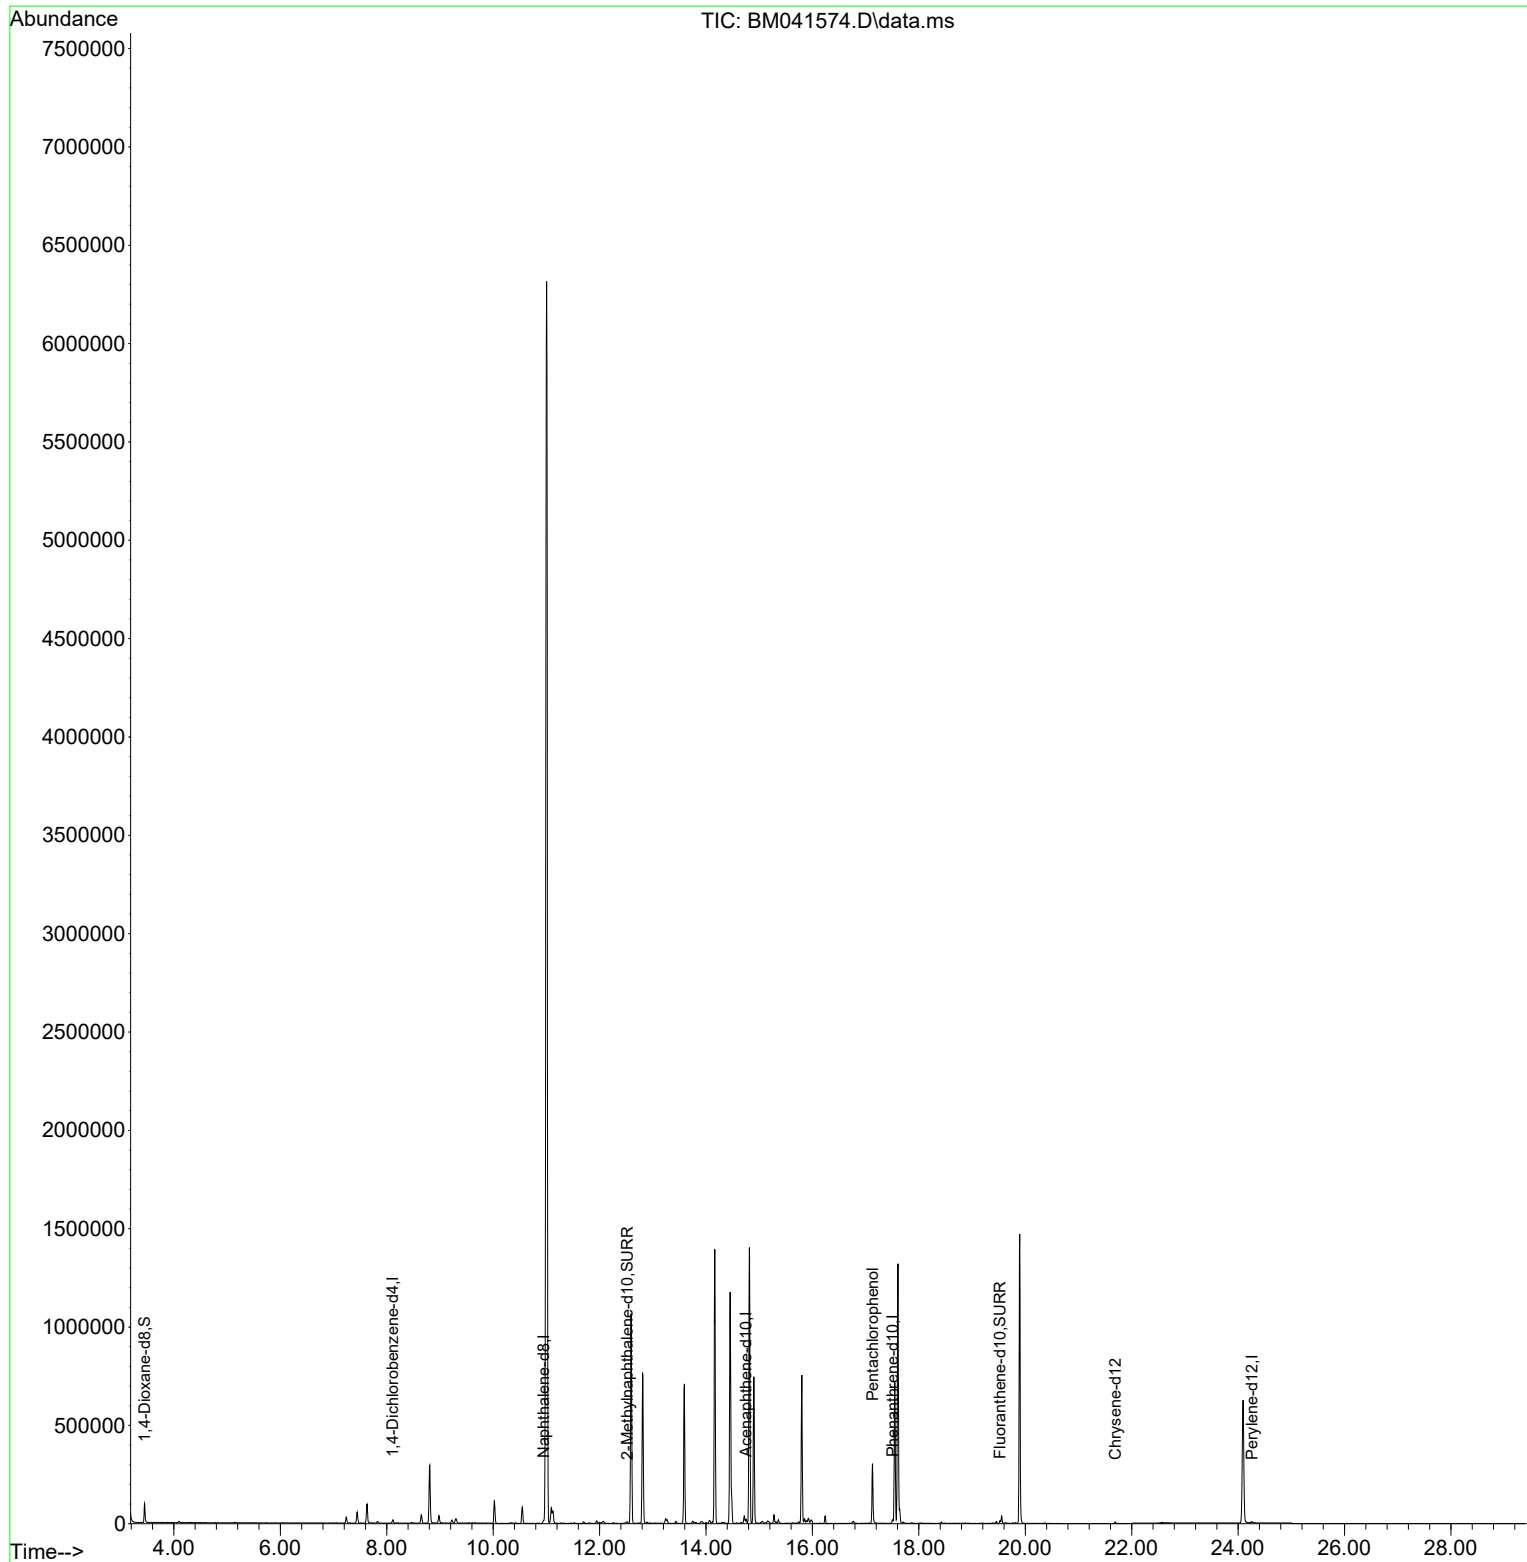

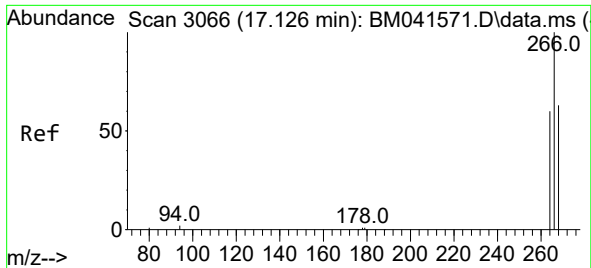

#14
Pentachlorophenol
Concen: 25.656 ng/ul
RT: 17.130 min Scan# 3067
Delta R.T. 0.004 min
Lab File: BM041574.D
Acq: 30 Aug 2023 11:28

Instrument :
BNA_M
ClientSampleId :
DCHJ0

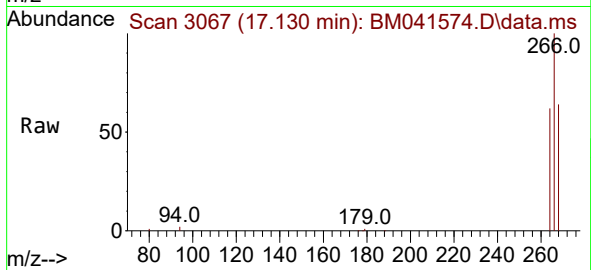

Tgt Ion:266 Resp: 185129
Ion Ratio Lower Upper
266 100
264 62.8 49.3 73.9
268 63.9 50.2 75.4

