

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041579.D
 Acq On : 30 Aug 2023 14:34
 Operator : MA/JU
 Sample : 04134-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHJ7

Quant Time: Aug 31 02:17:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	7572	0.400	ng/ul	0.00
4) Naphthalene-d8	10.946	136	19023	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.750	164	9769	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.502	188	18811	0.400	ng/ul	0.00
17) Chrysene-d12	21.692	240	6891	0.400	ng/ul	0.00
23) Perylene-d12	24.256	264	8202	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	54432	4.871	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.518	152	8018	0.349	ng/ul	0.00
18) Fluoranthene-d10	19.525	212	12660	0.372	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	17.127	266	34797	4.814	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041579.D
Acq On : 30 Aug 2023 14:34
Operator : MA/JU
Sample : 04134-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHJ7


Quant Time: Aug 31 02:17:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

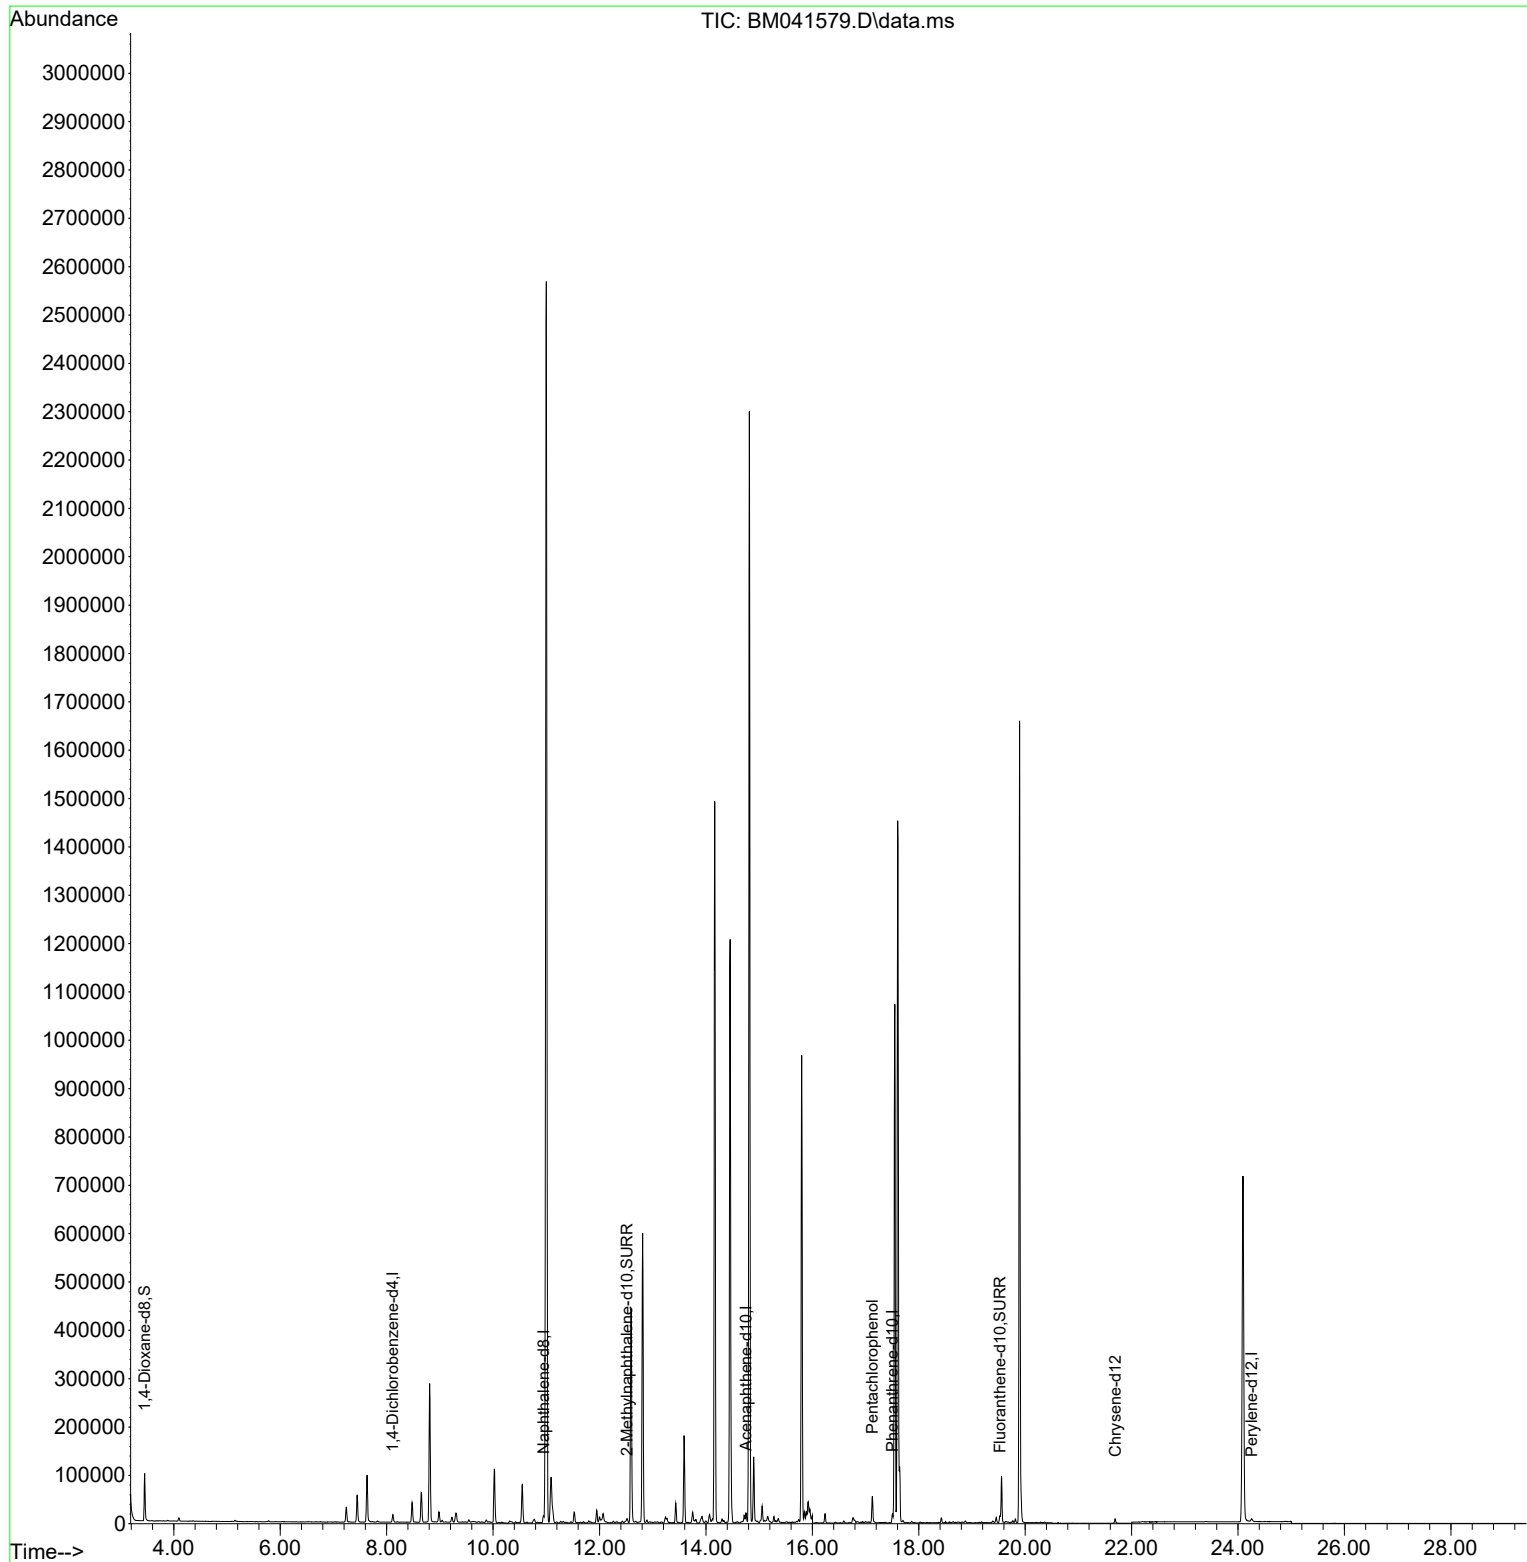

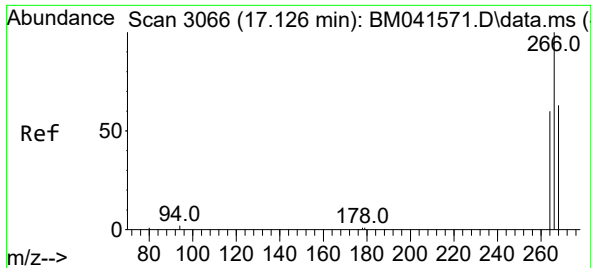

#14
 Pentachlorophenol
 Concen: 4.814 ng/ul
 RT: 17.127 min Scan# 30
 Delta R.T. 0.001 min
 Lab File: BM041579.D
 Acq: 30 Aug 2023 14:34

Instrument :
 BNA_M
 ClientSampleId :
 DCHJ7

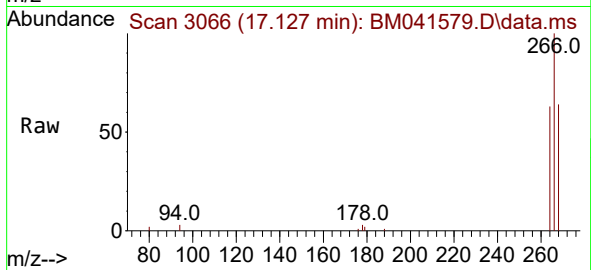

Tgt Ion:	266	Resp:	34797
Ion	Ratio	Lower	Upper
266	100		
264	62.8	49.3	73.9
268	63.9	50.2	75.4

