

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041582.D
 Acq On : 30 Aug 2023 16:27
 Operator : MA/JU
 Sample : 04134-02RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHJ0RE

Quant Time: Aug 31 02:17:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	7780	0.400	ng/ul	0.00
4) Naphthalene-d8	10.950	136	20191	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.754	164	10971	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.506	188	18920	0.400	ng/ul	0.00
17) Chrysene-d12	21.688	240	7293	0.400	ng/ul	0.00
23) Perylene-d12	24.251	264	8815	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.452	96	55157	4.804	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.522	152	8849	0.363	ng/ul	0.00
18) Fluoranthene-d10	19.524	212	13198	0.367	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.126	266	209063	28.754	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041582.D
Acq On : 30 Aug 2023 16:27
Operator : MA/JU
Sample : 04134-02RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHJ0RE


Quant Time: Aug 31 02:17:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

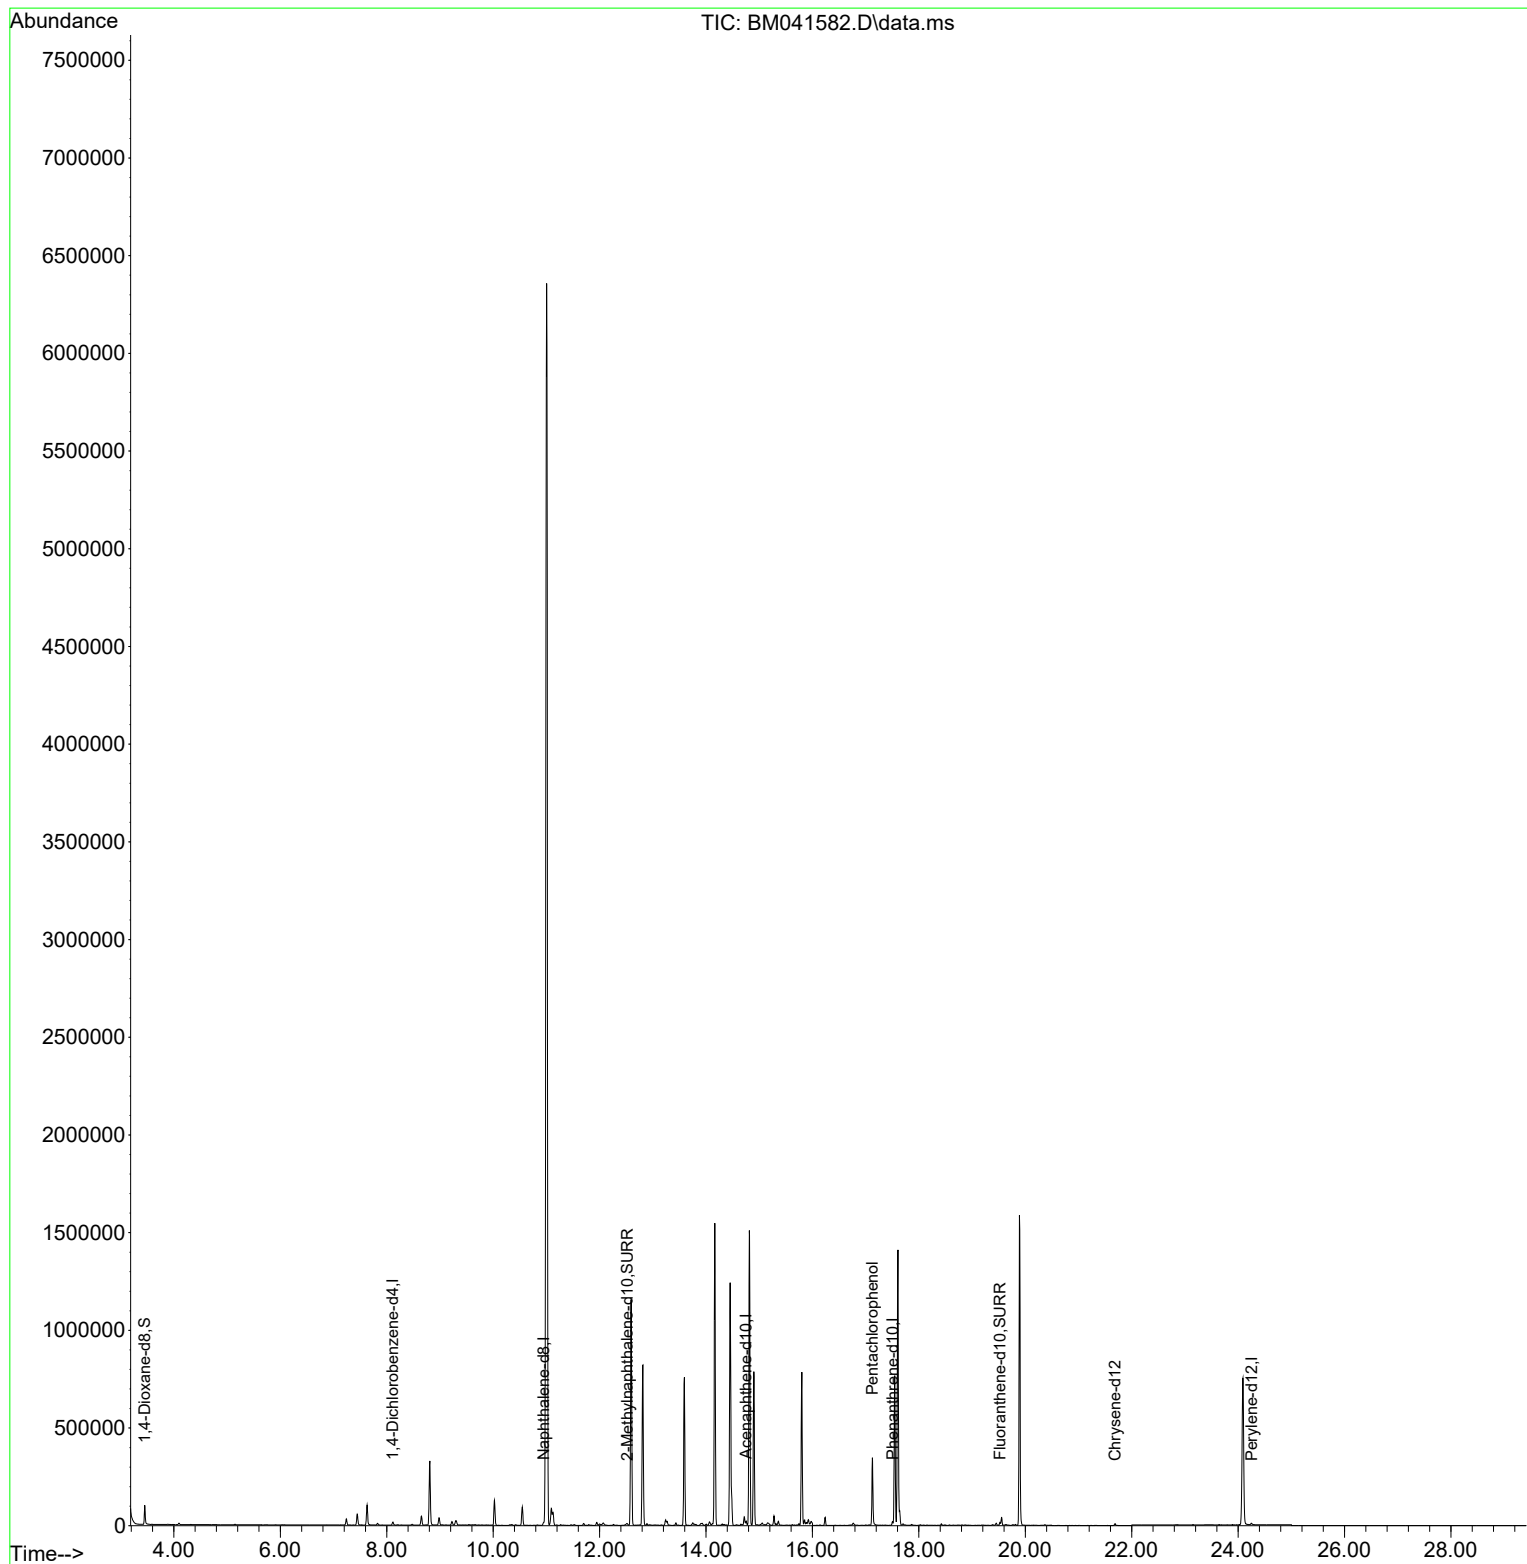

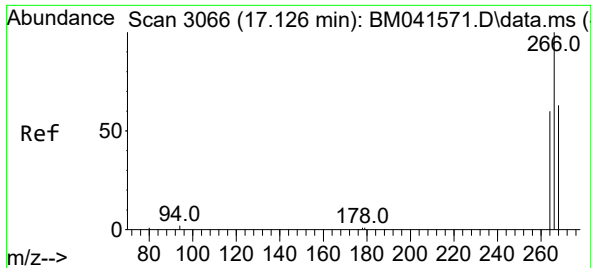

#14
 Pentachlorophenol
 Concen: 28.754 ng/ul
 RT: 17.126 min Scan# 3066
 Delta R.T. 0.000 min
 Lab File: BM041582.D
 Acq: 30 Aug 2023 16:27

Instrument :
 BNA_M
 ClientSampleId :
 DCHJ0RE

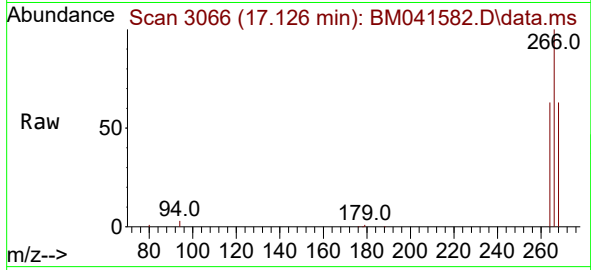

Tgt Ion:266 Resp: 209063

Ion	Ratio	Lower	Upper
266	100		
264	62.7	49.3	73.9
268	63.9	50.2	75.4

