

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041584.D
 Acq On : 30 Aug 2023 17:44
 Operator : MA/JU
 Sample : 04134-06RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHJ9RE

Quant Time: Aug 31 02:18:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	6218	0.400	ng/ul	0.00
4) Naphthalene-d8	10.949	136	15549	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.754	164	8462	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.506	188	14352	0.400	ng/ul	0.00
17) Chrysene-d12	21.688	240	5214	0.400	ng/ul	0.00
23) Perylene-d12	24.251	264	6223	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.452	96	44456	4.844	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.522	152	6958	0.371	ng/ul	0.00
18) Fluoranthene-d10	19.524	212	9863	0.384	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	17.126	266	152576	27.664	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041584.D
Acq On : 30 Aug 2023 17:44
Operator : MA/JU
Sample : 04134-06RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHJ9RE


Quant Time: Aug 31 02:18:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

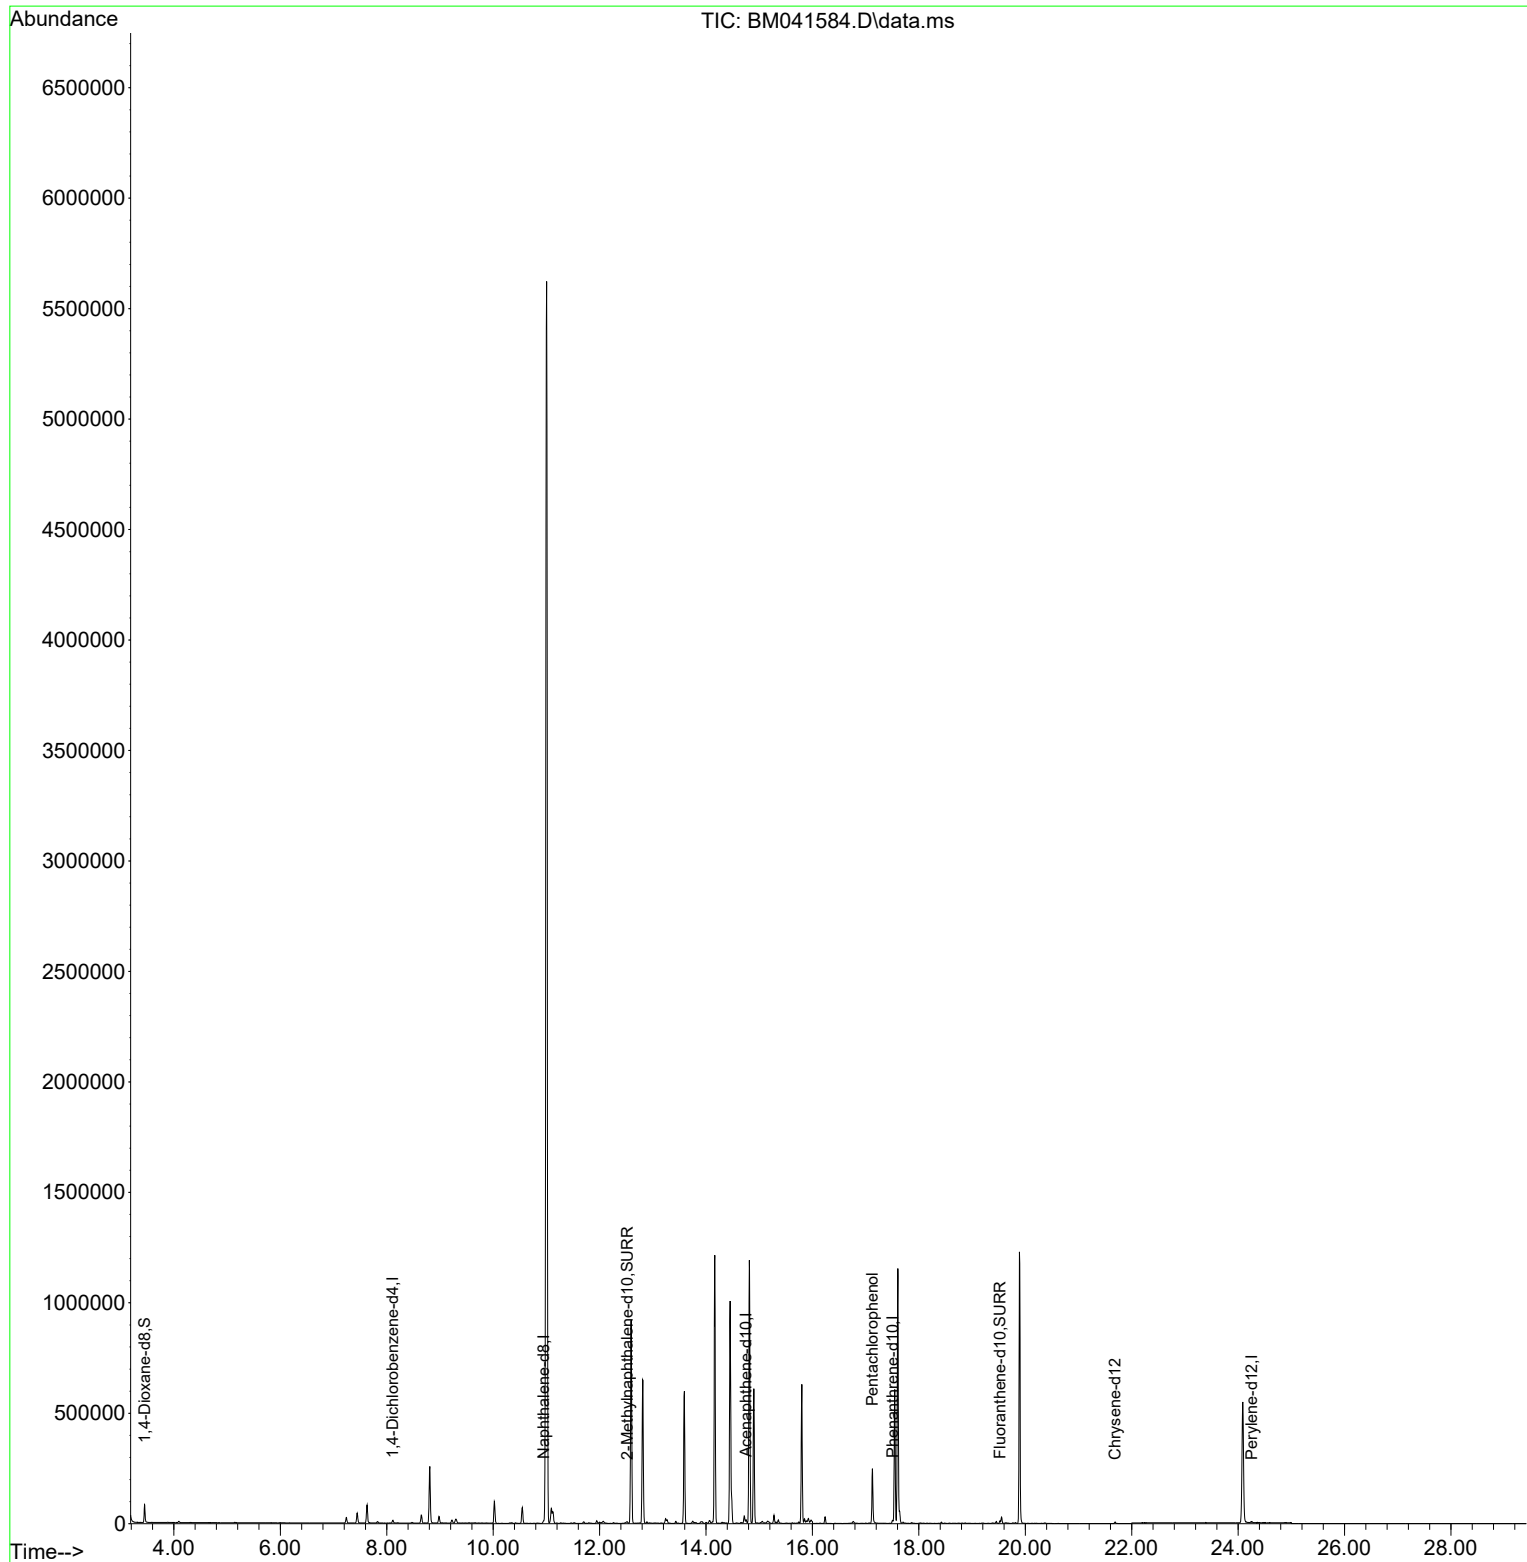

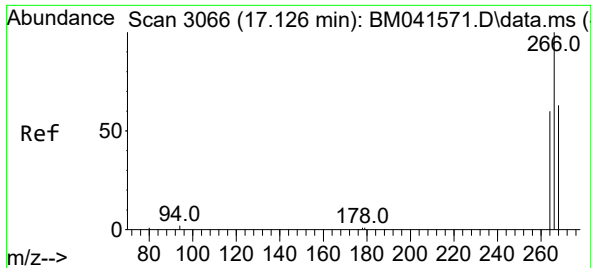

#14
 Pentachlorophenol
 Concen: 27.664 ng/ul
 RT: 17.126 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: BM041584.D
 Acq: 30 Aug 2023 17:44

Instrument :
 BNA_M
 ClientSampleId :
 DCHJ9RE

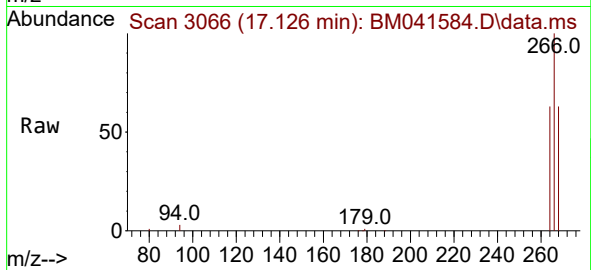

Tgt Ion:266 Resp: 152576
 Ion Ratio Lower Upper
 266 100
 264 62.7 49.3 73.9
 268 64.0 50.2 75.4

