

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041591.D
 Acq On : 30 Aug 2023 23:07
 Operator : MA/JU
 Sample : 04134-04DL 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHJ7DL

Quant Time: Aug 31 02:19:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	5846	0.400	ng/ul	0.00
4) Naphthalene-d8	10.944	136	13231	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.749	164	5918	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.502	188	10999	0.400	ng/ul	0.00
17) Chrysene-d12	21.685	240	3598	0.400	ng/ul	0.00
23) Perylene-d12	24.246	264	4209	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.452	96	11926	1.382	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	1467	0.092	ng/ul	0.00
18) Fluoranthene-d10	19.520	212	1869	0.105	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.122	266	4436	1.049	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041591.D
Acq On : 30 Aug 2023 23:07
Operator : MA/JU
Sample : 04134-04DL 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHJ7DL

Quant Time: Aug 31 02:19:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

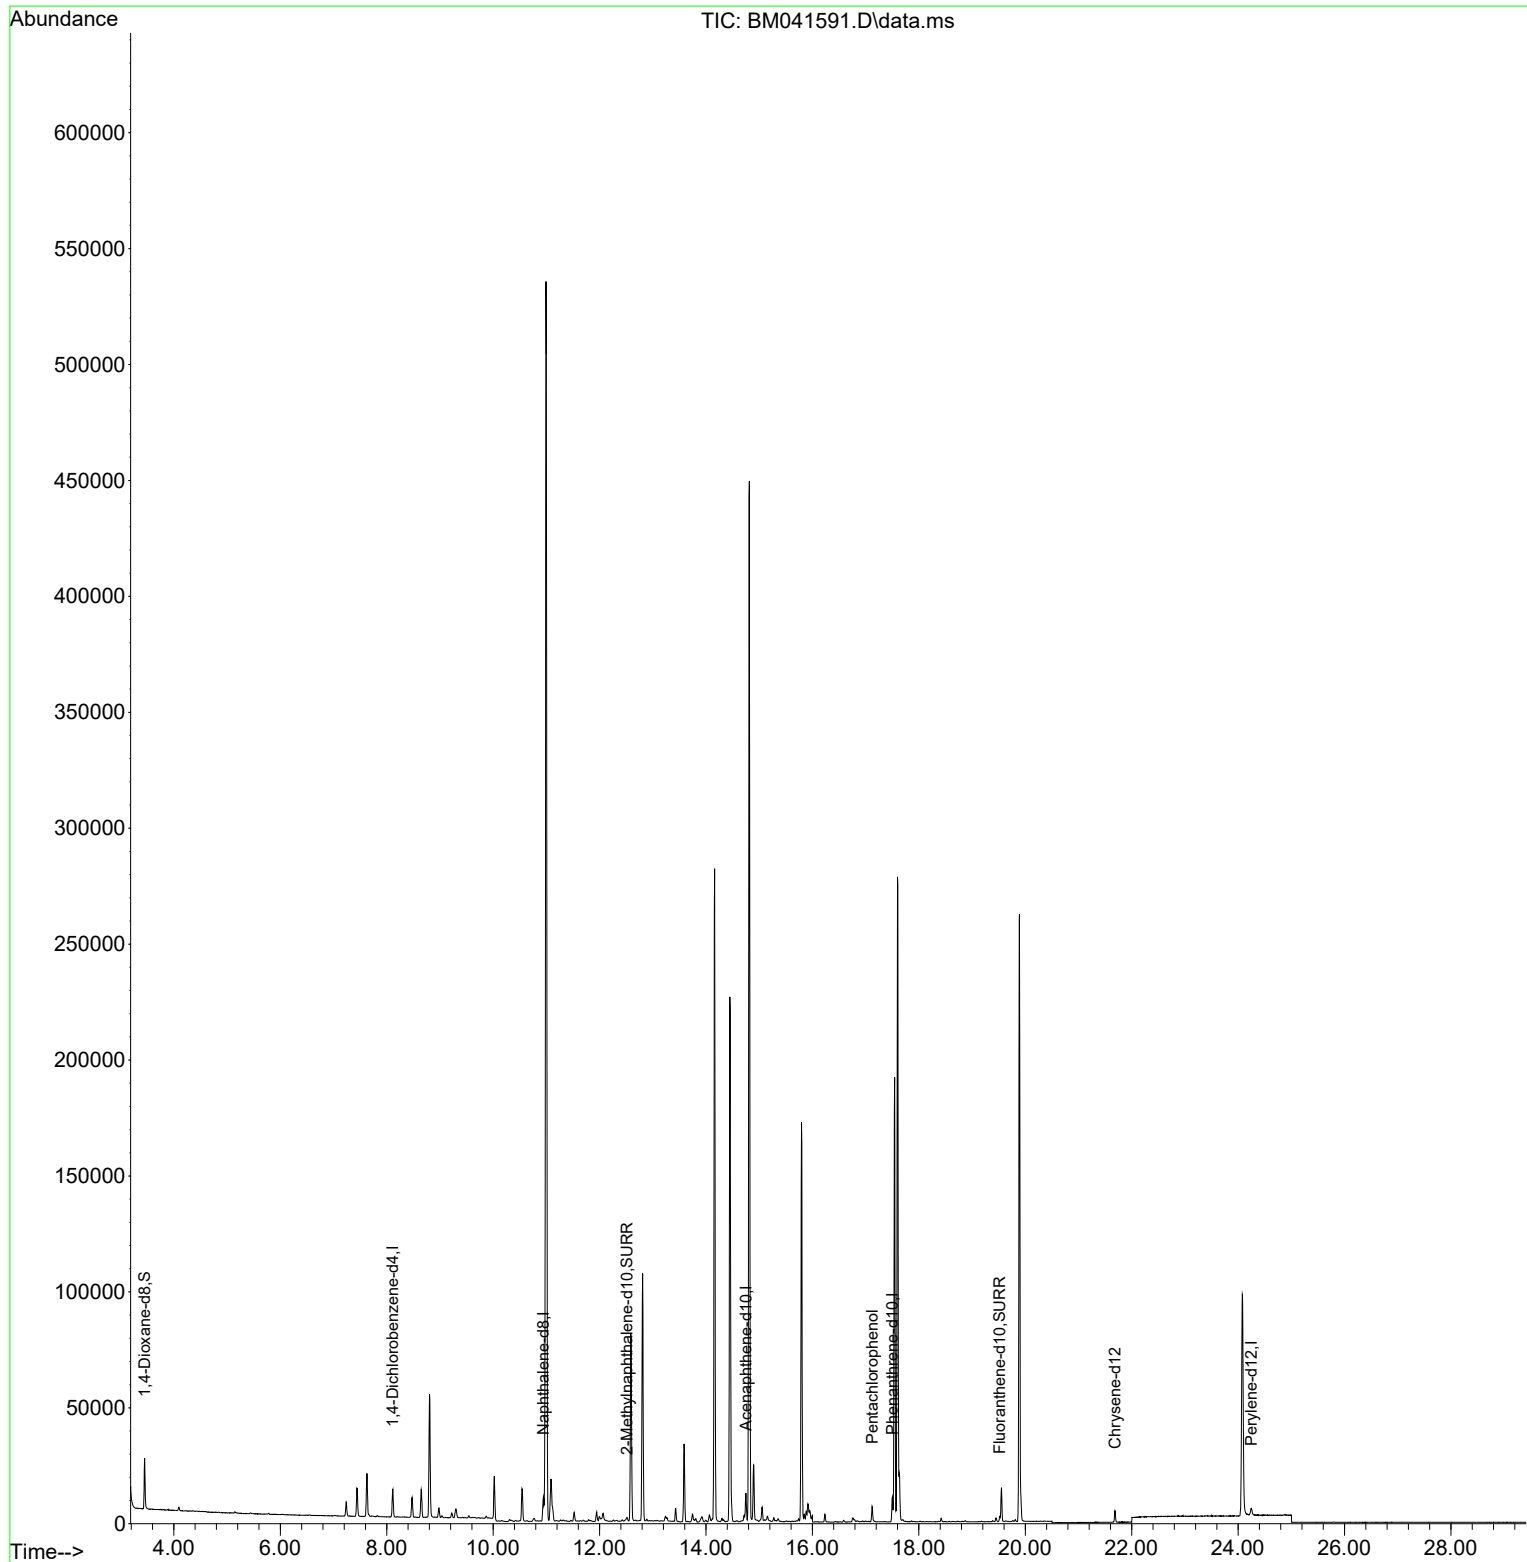

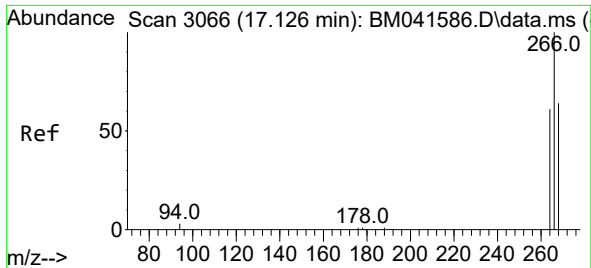

#14
 Pentachlorophenol
 Concen: 1.049 ng/ul
 RT: 17.122 min Scan# 3065
 Delta R.T. -0.004 min
 Lab File: BM041591.D
 Acq: 30 Aug 2023 23:07

Instrument :
 BNA_M
 ClientSampleId :
 DCHJ7DL

Tgt Ion:	266	Resp:	4436
Ion	Ratio	Lower	Upper
266	100		
264	62.8	49.3	73.9
268	64.3	50.2	75.4

