

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041592.D
 Acq On : 30 Aug 2023 23:44
 Operator : MA/JU
 Sample : 04159-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHI9

Quant Time: Aug 31 02:19:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.115	152	6237	0.400	ng/ul	0.00
4) Naphthalene-d8	10.946	136	15258	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.750	164	7393	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.503	188	14386	0.400	ng/ul	0.00
17) Chrysene-d12	21.686	240	5058	0.400	ng/ul	0.00
23) Perylene-d12	24.244	264	5910	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	35199	3.824	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.519	152	5355	0.291	ng/ul	0.00
18) Fluoranthene-d10	19.521	212	7942	0.318	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.123	266	758	0.137	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041592.D
Acq On : 30 Aug 2023 23:44
Operator : MA/JU
Sample : 04159-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHI9

Quant Time: Aug 31 02:19:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

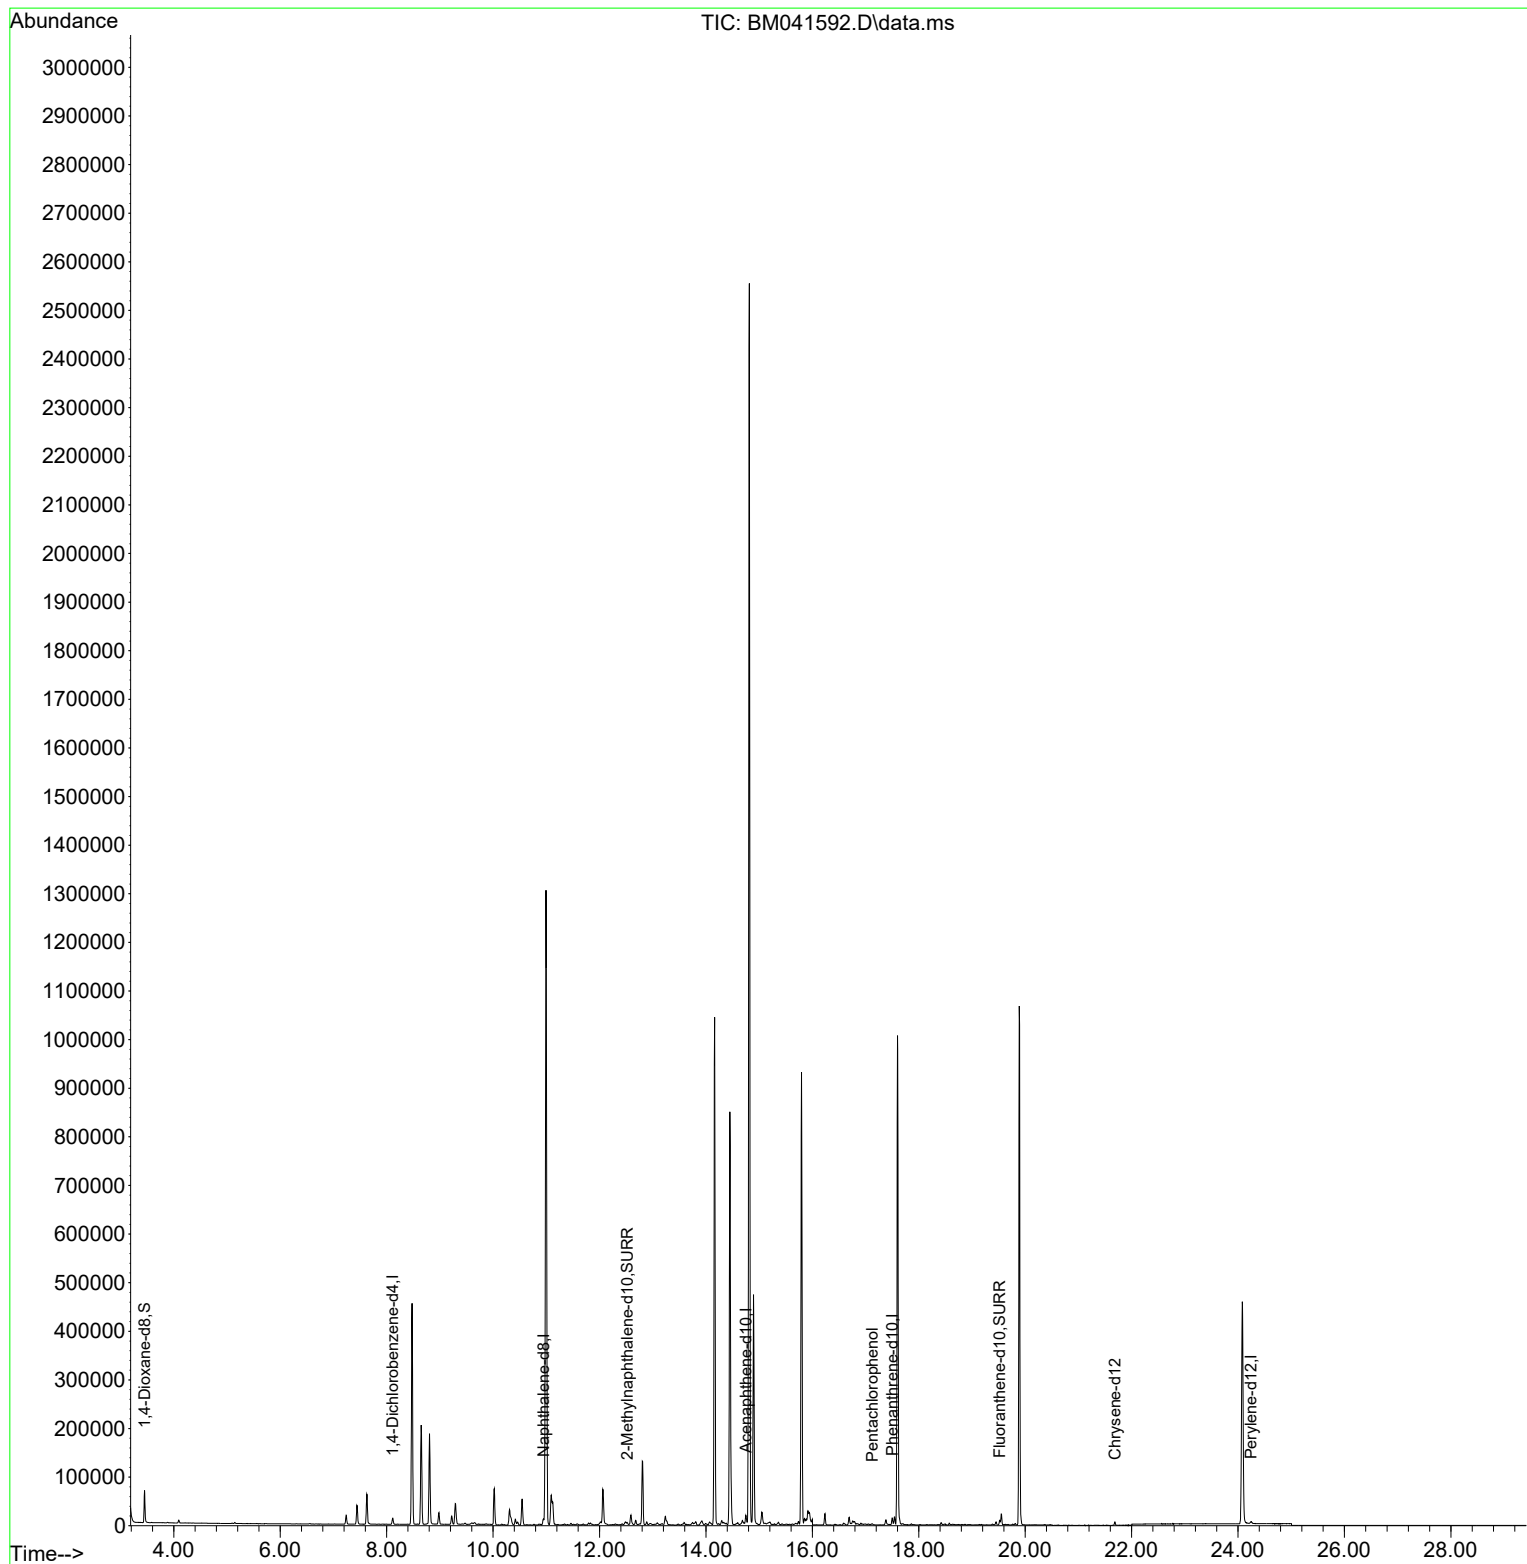

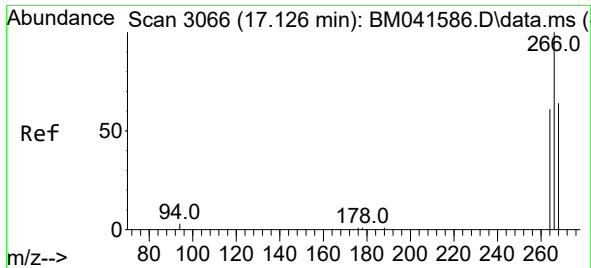

#14
 Pentachlorophenol
 Concen: 0.137 ng/ul
 RT: 17.123 min Scan# 30
 Delta R.T. -0.003 min
 Lab File: BM041592.D
 Acq: 30 Aug 2023 23:44

Instrument :
 BNA_M
 ClientSampleId :
 DCHI9

Tgt Ion:	266	Resp:	758
Ion	Ratio	Lower	Upper
266	100		
264	62.1	49.3	73.9
268	65.0	50.2	75.4

