

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041596.D
 Acq On : 31 Aug 2023 02:11
 Operator : MA/JU
 Sample : 04134-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHK1

Quant Time: Aug 31 04:05:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	8514	0.400	ng/ul	0.00
4) Naphthalene-d8	10.944	136	20094	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.749	164	8747	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.502	188	15758	0.400	ng/ul	0.00
17) Chrysene-d12	21.685	240	5833	0.400	ng/ul	0.00
23) Perylene-d12	24.243	264	7537	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	55281	4.399	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	7443	0.307	ng/ul	0.00
18) Fluoranthene-d10	19.520	212	10052	0.349	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.122	266	27496	4.541	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041596.D
Acq On : 31 Aug 2023 02:11
Operator : MA/JU
Sample : 04134-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHK1


Quant Time: Aug 31 04:05:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

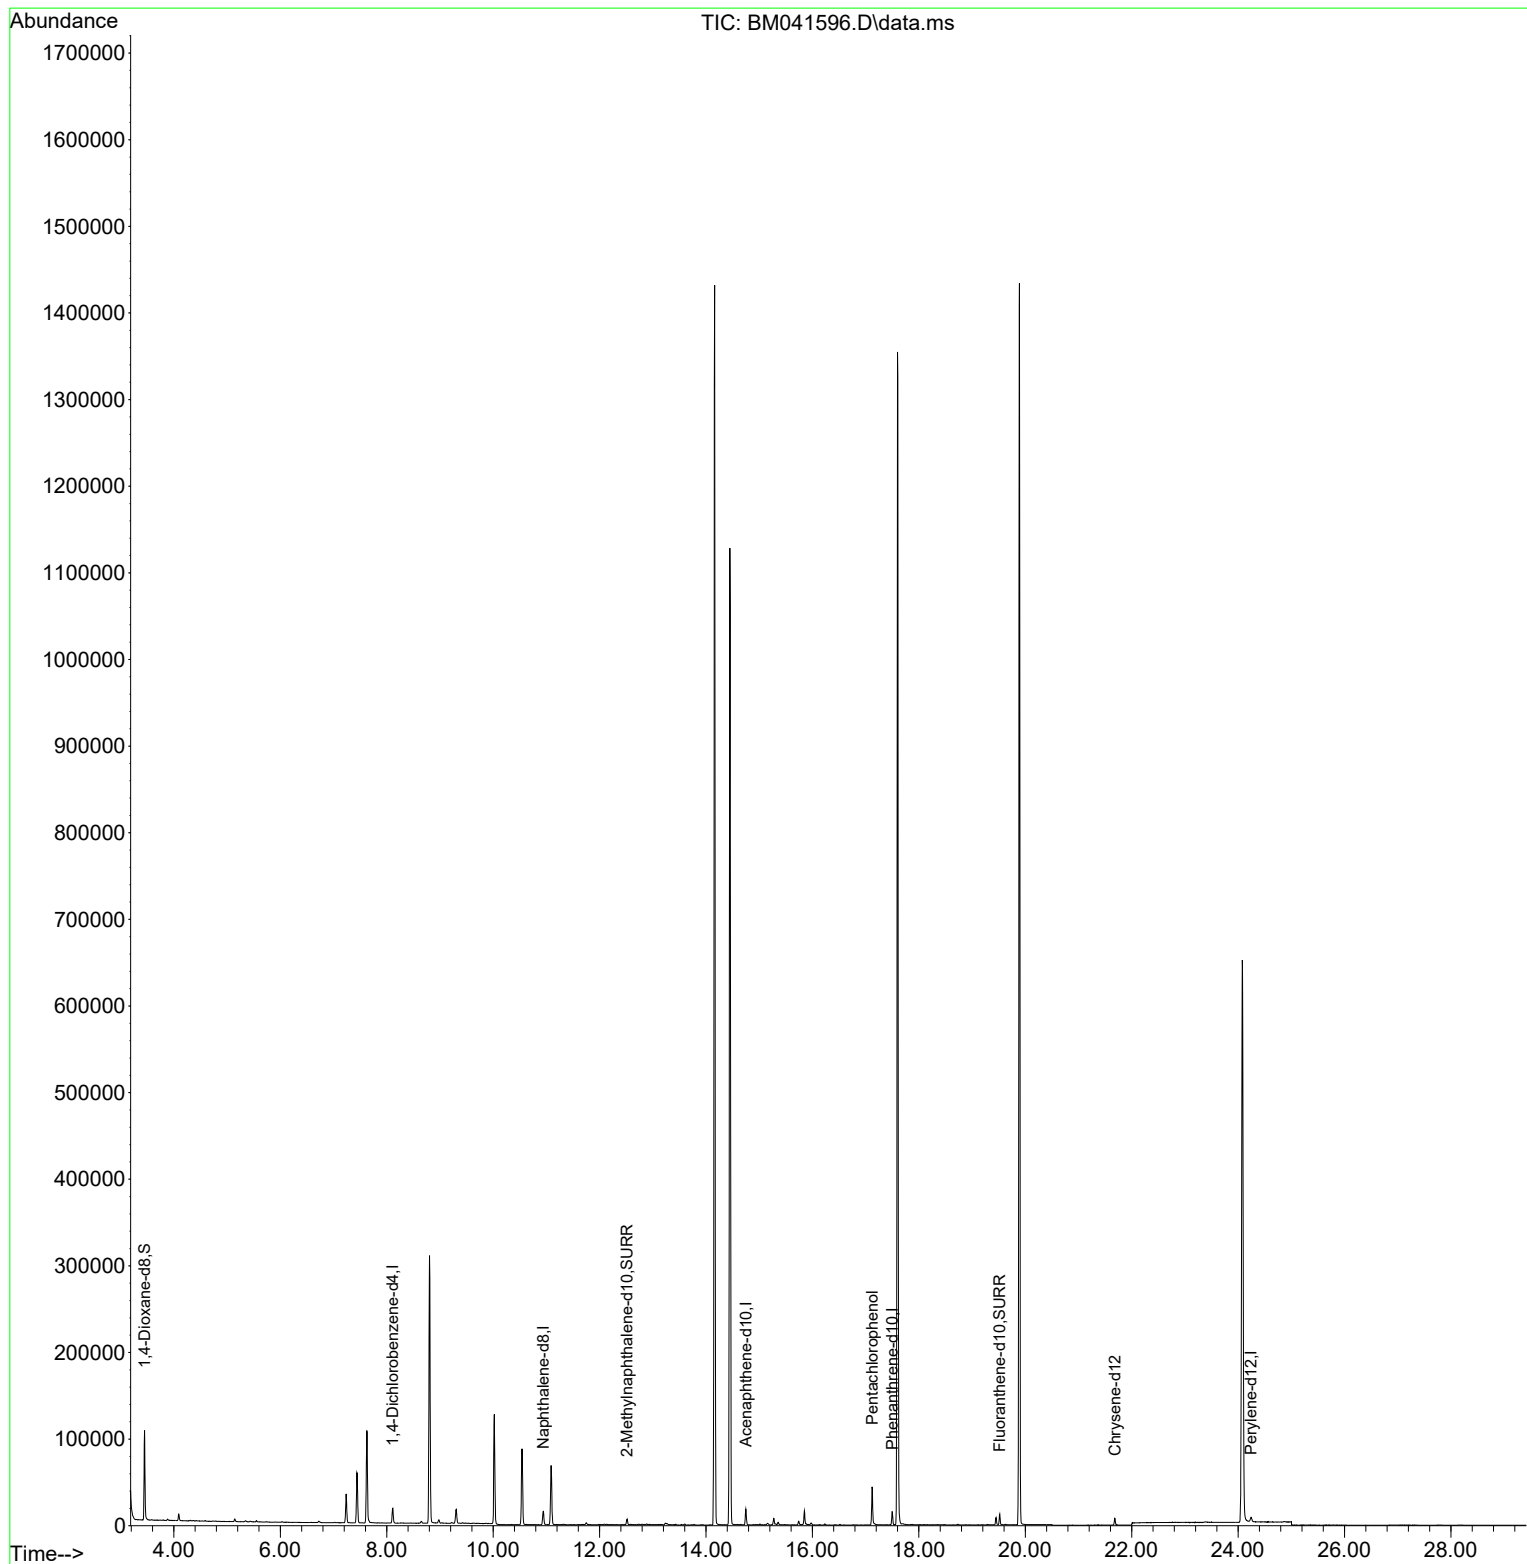

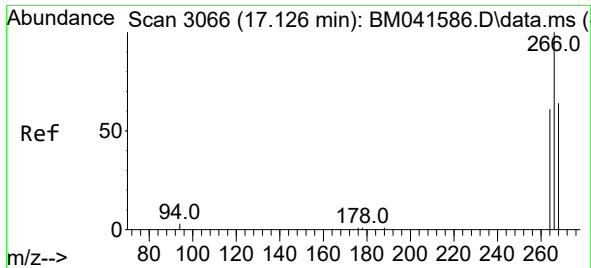

#14
Pentachlorophenol
Concen: 4.541 ng/ul
RT: 17.122 min Scan# 30
Delta R.T. -0.004 min
Lab File: BM041596.D
Acq: 31 Aug 2023 02:11

Instrument :
BNA_M
ClientSampleId :
DCHK1

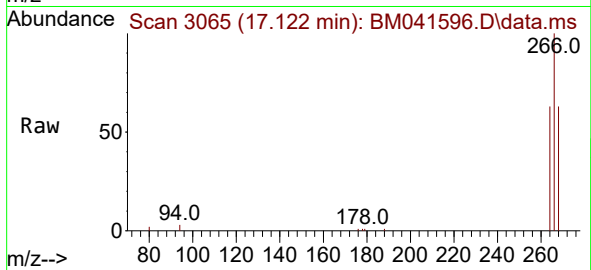

Tgt Ion:266 Resp: 27496
Ion Ratio Lower Upper
266 100
264 62.8 49.3 73.9
268 64.0 50.2 75.4

