

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041598.D
 Acq On : 31 Aug 2023 03:25
 Operator : MA/JU
 Sample : 04134-10
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHK4

Quant Time: Aug 31 04:07:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	7933	0.400	ng/ul	0.00
4) Naphthalene-d8	10.944	136	18536	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.749	164	8240	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.498	188	16133	0.400	ng/ul	0.00
17) Chrysene-d12	21.682	240	6581	0.400	ng/ul	0.00
23) Perylene-d12	24.240	264	8132	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	51094	4.364	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	6464	0.289	ng/ul	0.00
18) Fluoranthene-d10	19.520	212	10778	0.332	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	17.122	266	86256	13.913	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041598.D
Acq On : 31 Aug 2023 03:25
Operator : MA/JU
Sample : 04134-10
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHK4


Quant Time: Aug 31 04:07:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

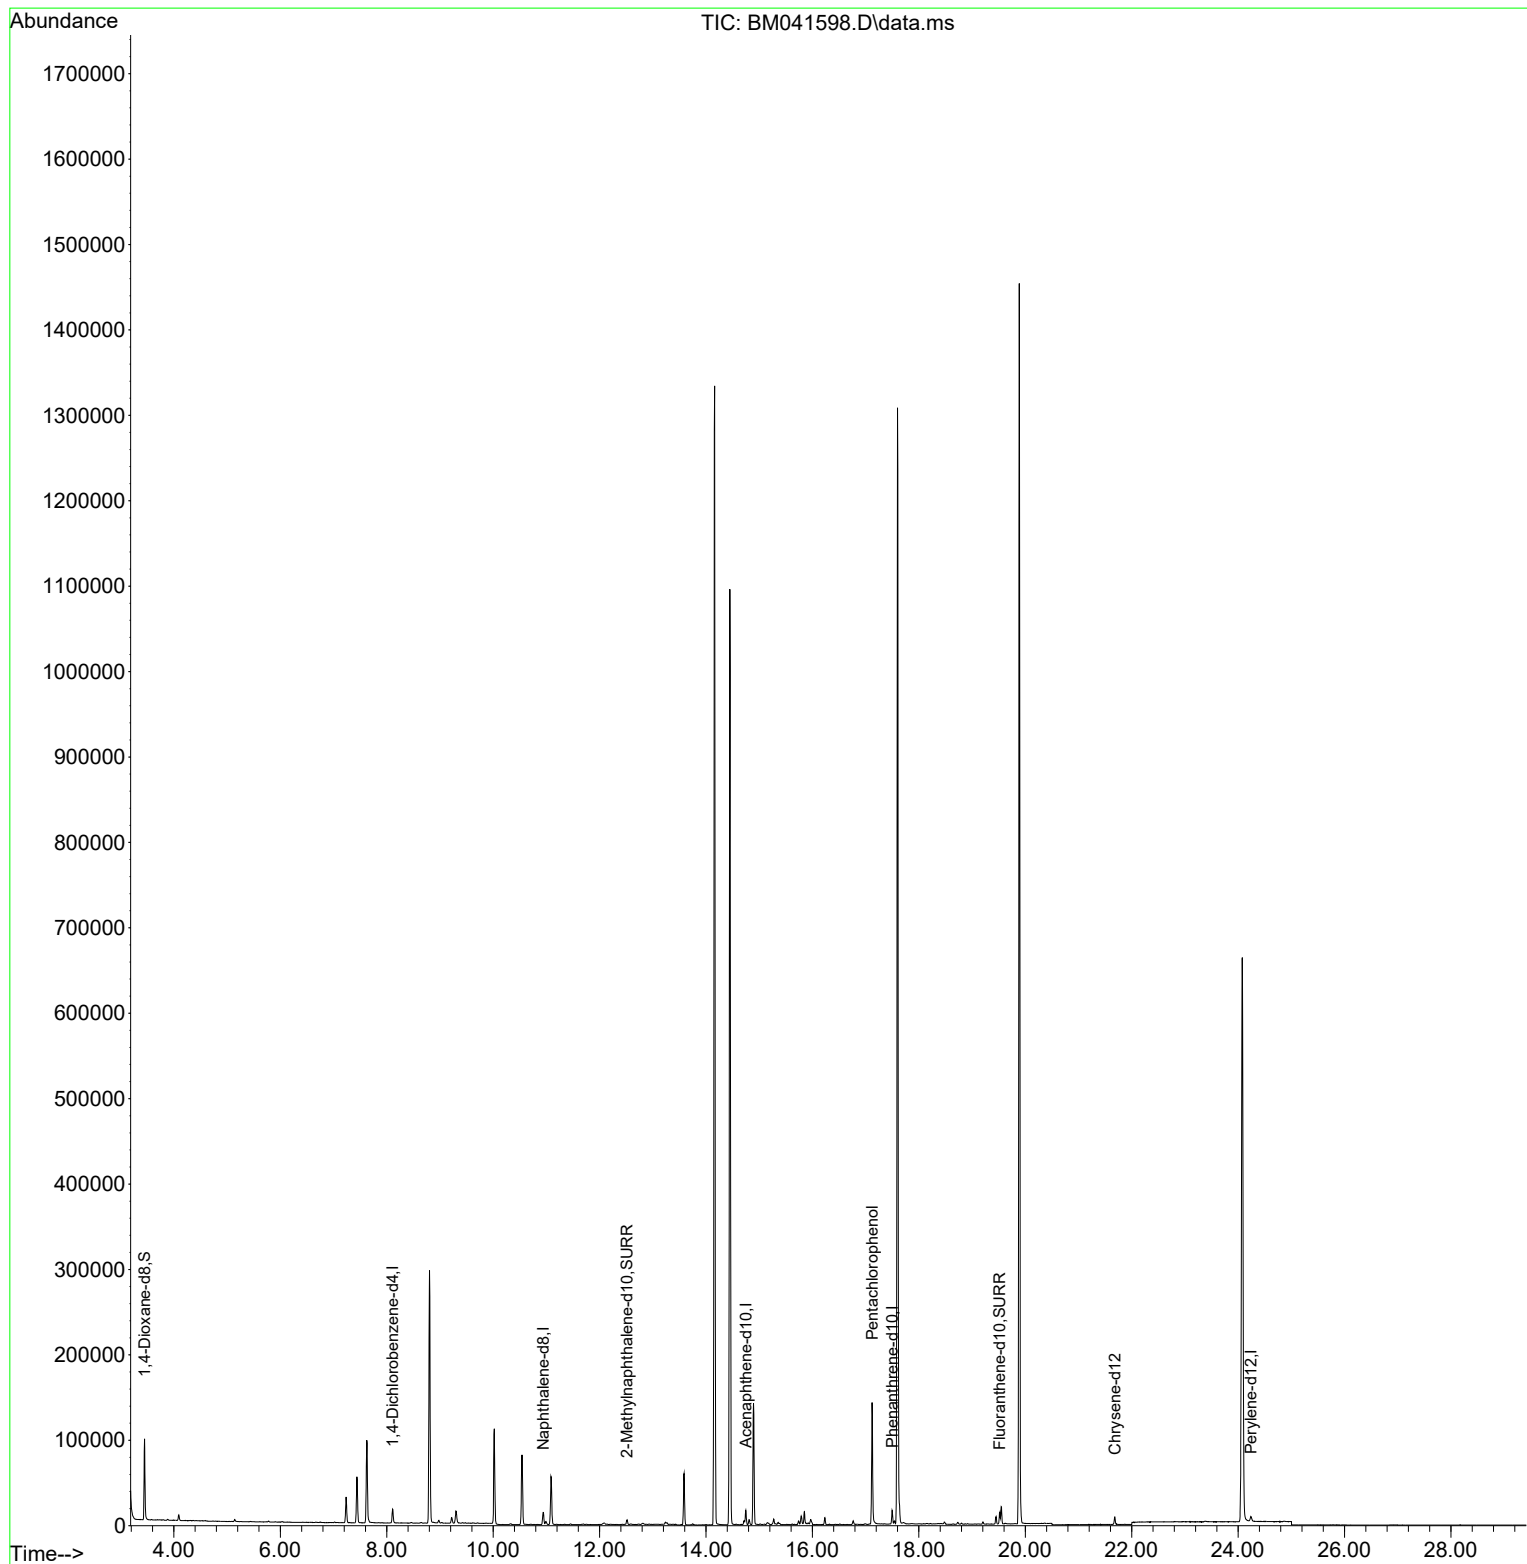

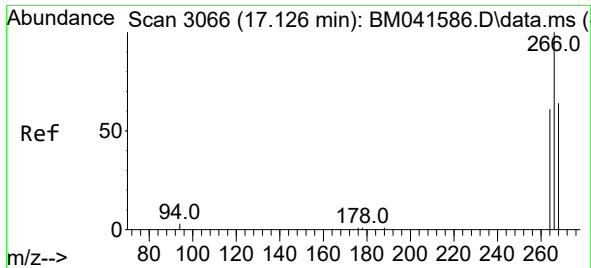

#14
Pentachlorophenol
Concen: 13.913 ng/ul
RT: 17.122 min Scan# 30
Delta R.T. -0.004 min
Lab File: BM041598.D
Acq: 31 Aug 2023 03:25

Instrument :
BNA_M
ClientSampleId :
DCHK4

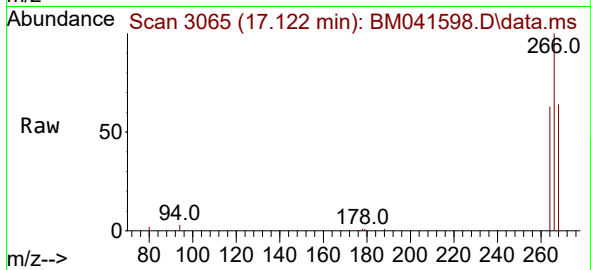

Tgt Ion:266 Resp: 86256
Ion Ratio Lower Upper
266 100
264 62.8 49.3 73.9
268 64.0 50.2 75.4

