

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041600.D
 Acq On : 31 Aug 2023 04:38
 Operator : MA/JU
 Sample : 04134-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHJ6

Quant Time: Aug 31 05:28:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	8986	0.400	ng/ul	0.00
4) Naphthalene-d8	10.939	136	21290	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.745	164	9157	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.498	188	17445	0.400	ng/ul	0.00
17) Chrysene-d12	21.682	240	6662	0.400	ng/ul	0.00
23) Perylene-d12	24.240	264	8840	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	51911	3.914	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	7961	0.310	ng/ul	0.00
18) Fluoranthene-d10	19.520	212	11726	0.357	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.118	266	5371	0.801	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041600.D
Acq On : 31 Aug 2023 04:38
Operator : MA/JU
Sample : 04134-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHJ6


Quant Time: Aug 31 05:28:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

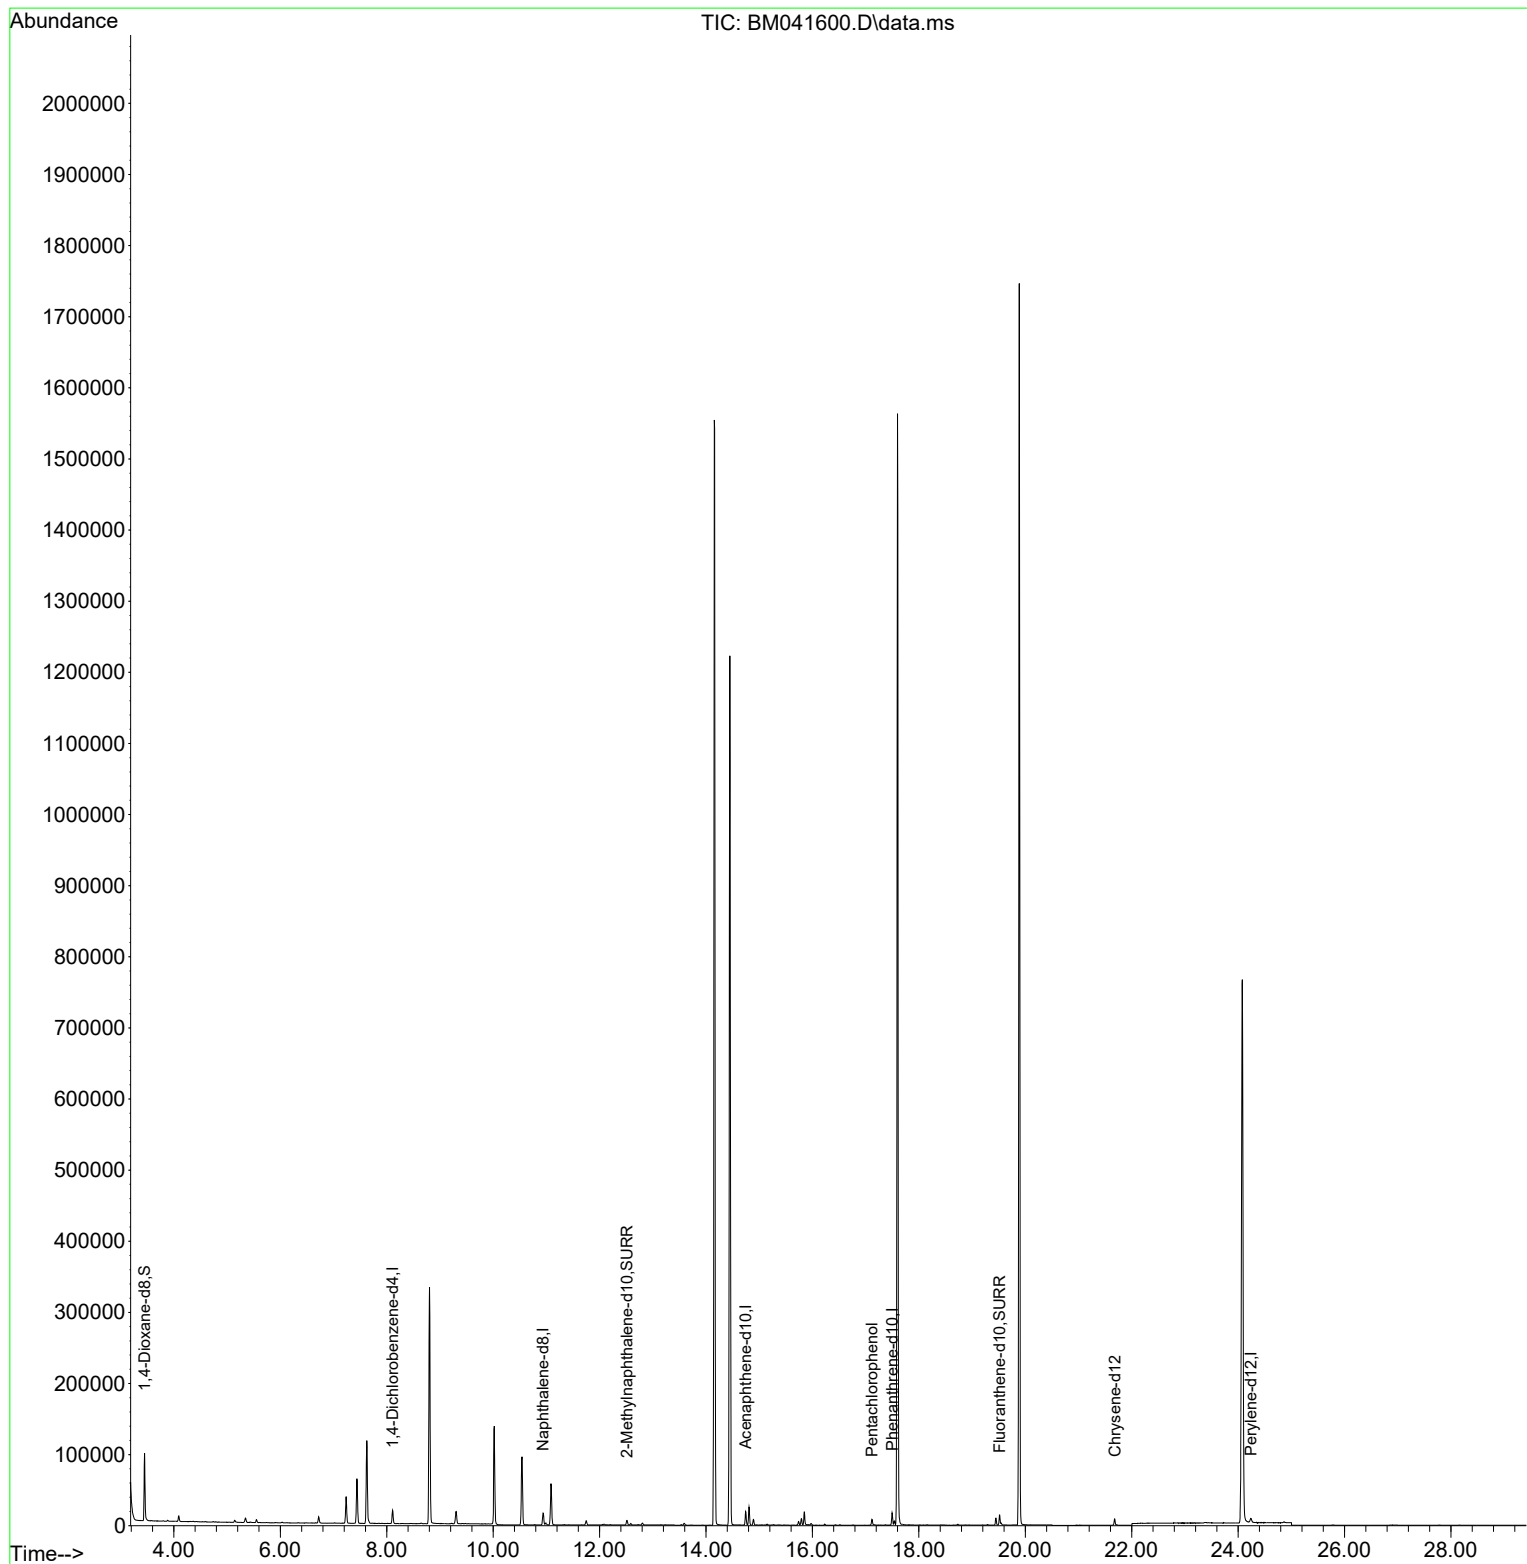

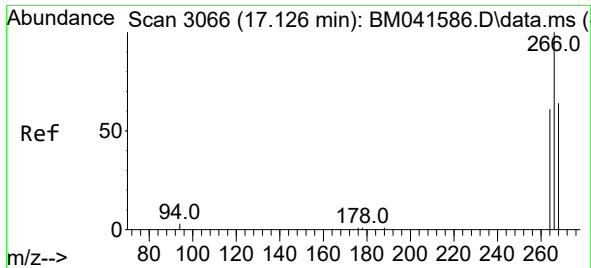

#14
Pentachlorophenol
Concen: 0.801 ng/ul
RT: 17.118 min Scan# 3064
Delta R.T. -0.008 min
Lab File: BM041600.D
Acq: 31 Aug 2023 04:38

Instrument :
BNA_M
ClientSampleId :
DCHJ6

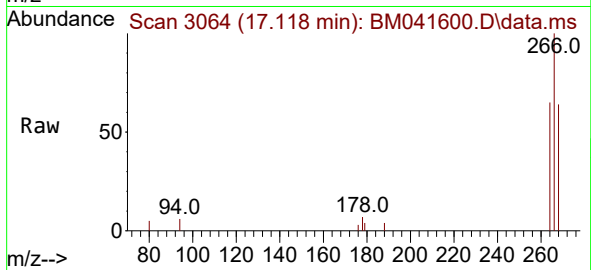

Tgt Ion:	266	Resp:	5371
Ion	Ratio	Lower	Upper
266	100		
264	62.9	49.3	73.9
268	64.4	50.2	75.4

