

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041606.D
 Acq On : 31 Aug 2023 08:53
 Operator : MA/JU
 Sample : 04159-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHJ2

Quant Time: Aug 31 09:22:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	5374	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	12011	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.745	164	5464	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.497	188	9568	0.400	ng/ul	0.00
17) Chrysene-d12	21.679	240	3322	0.400	ng/ul	-0.01
23) Perylene-d12	24.237	264	4207	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	31916	4.024	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	3989	0.275	ng/ul	-0.01
18) Fluoranthene-d10	19.515	212	5264	0.321	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.122	266	34249	9.315	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041606.D
Acq On : 31 Aug 2023 08:53
Operator : MA/JU
Sample : 04159-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHJ2

Quant Time: Aug 31 09:22:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

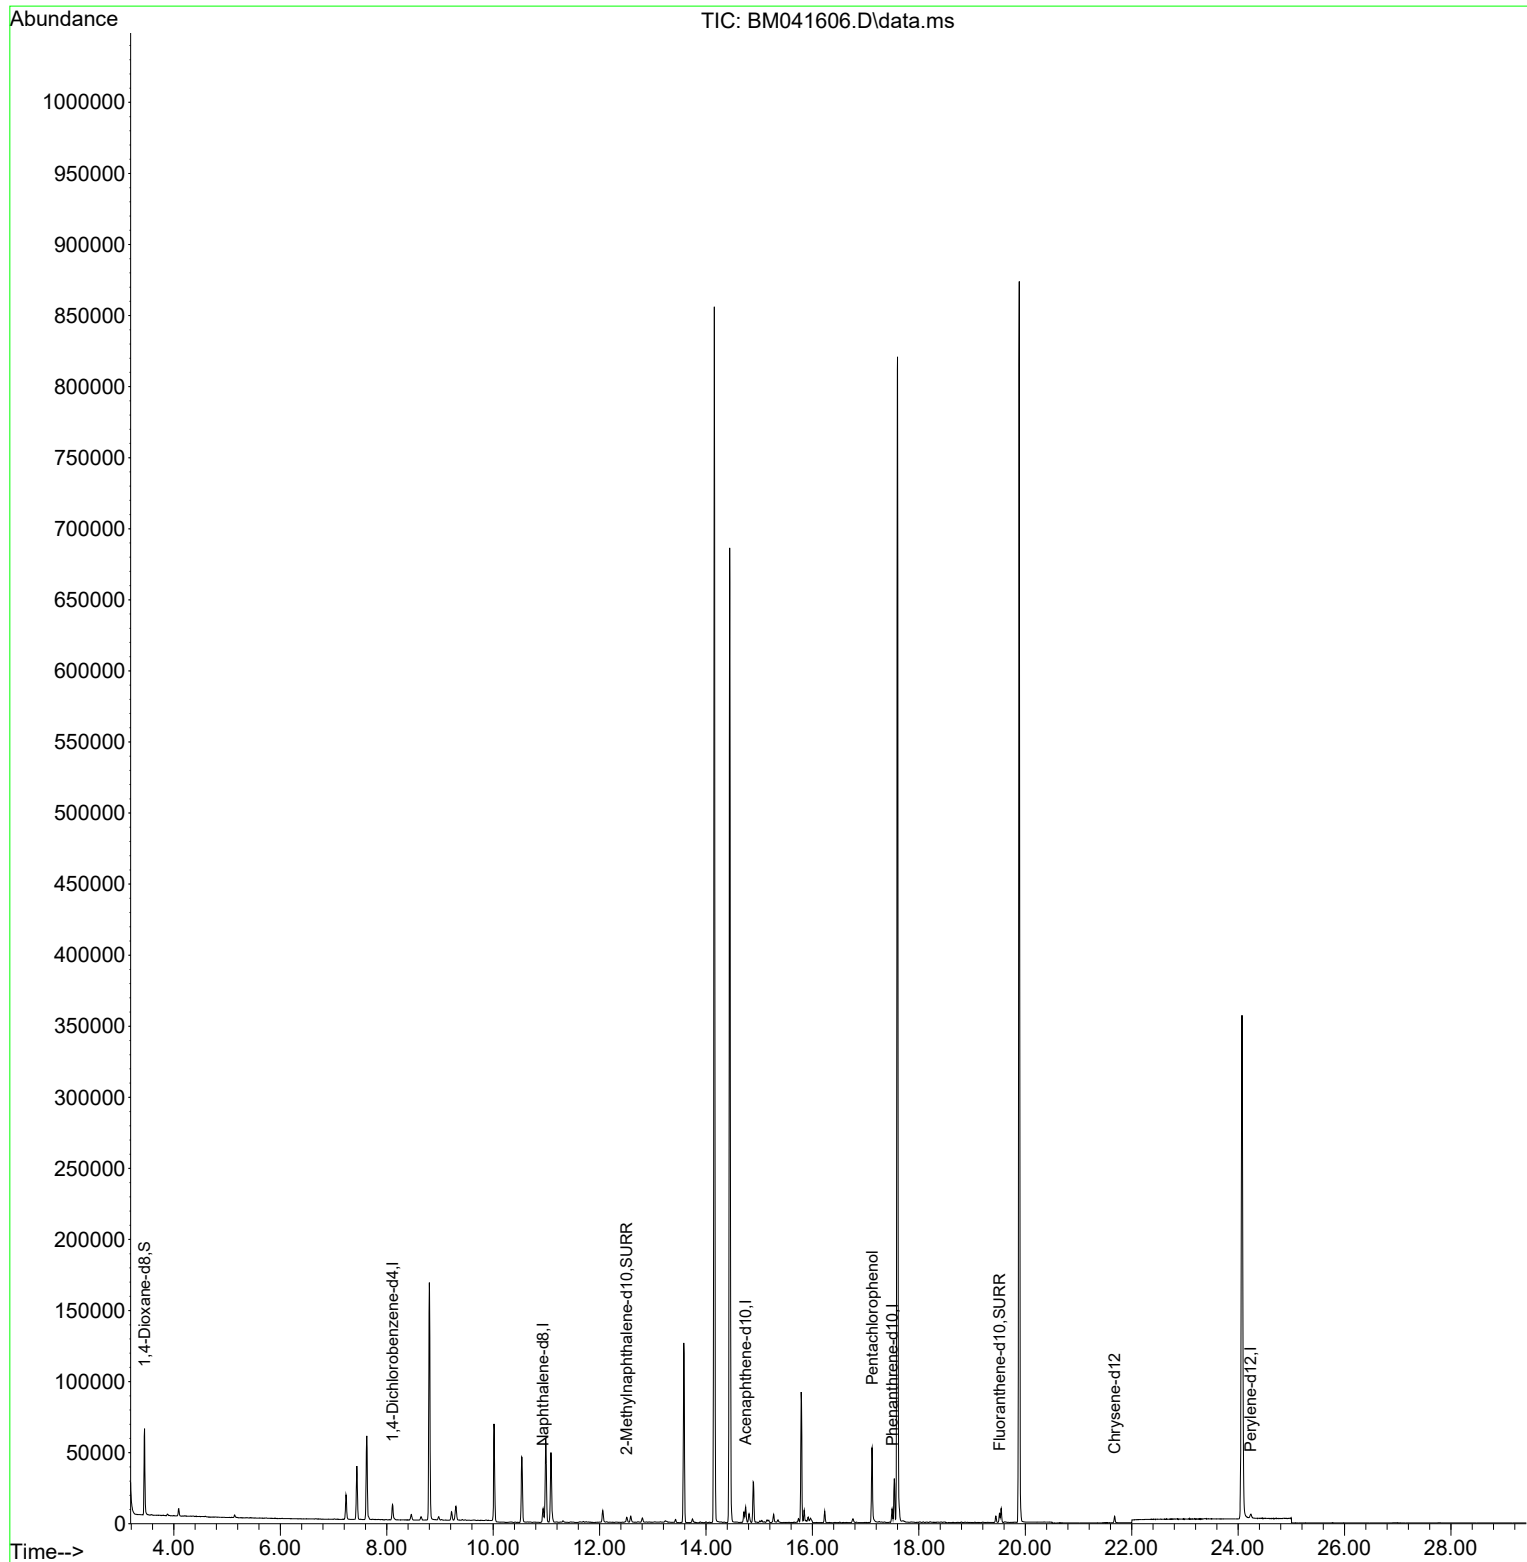

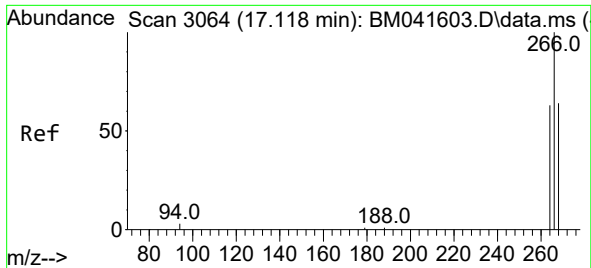

#14
 Pentachlorophenol
 Concen: 9.315 ng/ul
 RT: 17.122 min Scan# 30
 Delta R.T. -0.004 min
 Lab File: BM041606.D
 Acq: 31 Aug 2023 08:53

Instrument :
 BNA_M
 ClientSampleId :
 DCHJ2

Tgt Ion:266 Resp: 34249
 Ion Ratio Lower Upper
 266 100
 264 62.7 49.3 73.9
 268 63.9 50.2 75.4

