

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041610.D
 Acq On : 31 Aug 2023 11:20
 Operator : MA/JU
 Sample : 04159-09
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHK3

Quant Time: Sep 01 02:08:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	7507	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	17014	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.745	164	7207	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.497	188	12847	0.400	ng/ul	0.00
17) Chrysene-d12	21.682	240	4396	0.400	ng/ul	0.00
23) Perylene-d12	24.243	264	5462	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	46463	4.194	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	5345	0.260	ng/ul	-0.01
18) Fluoranthene-d10	19.519	212	7316	0.337	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.117	266	4288	0.869	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041610.D
Acq On : 31 Aug 2023 11:20
Operator : MA/JU
Sample : 04159-09
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHK3


Quant Time: Sep 01 02:08:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

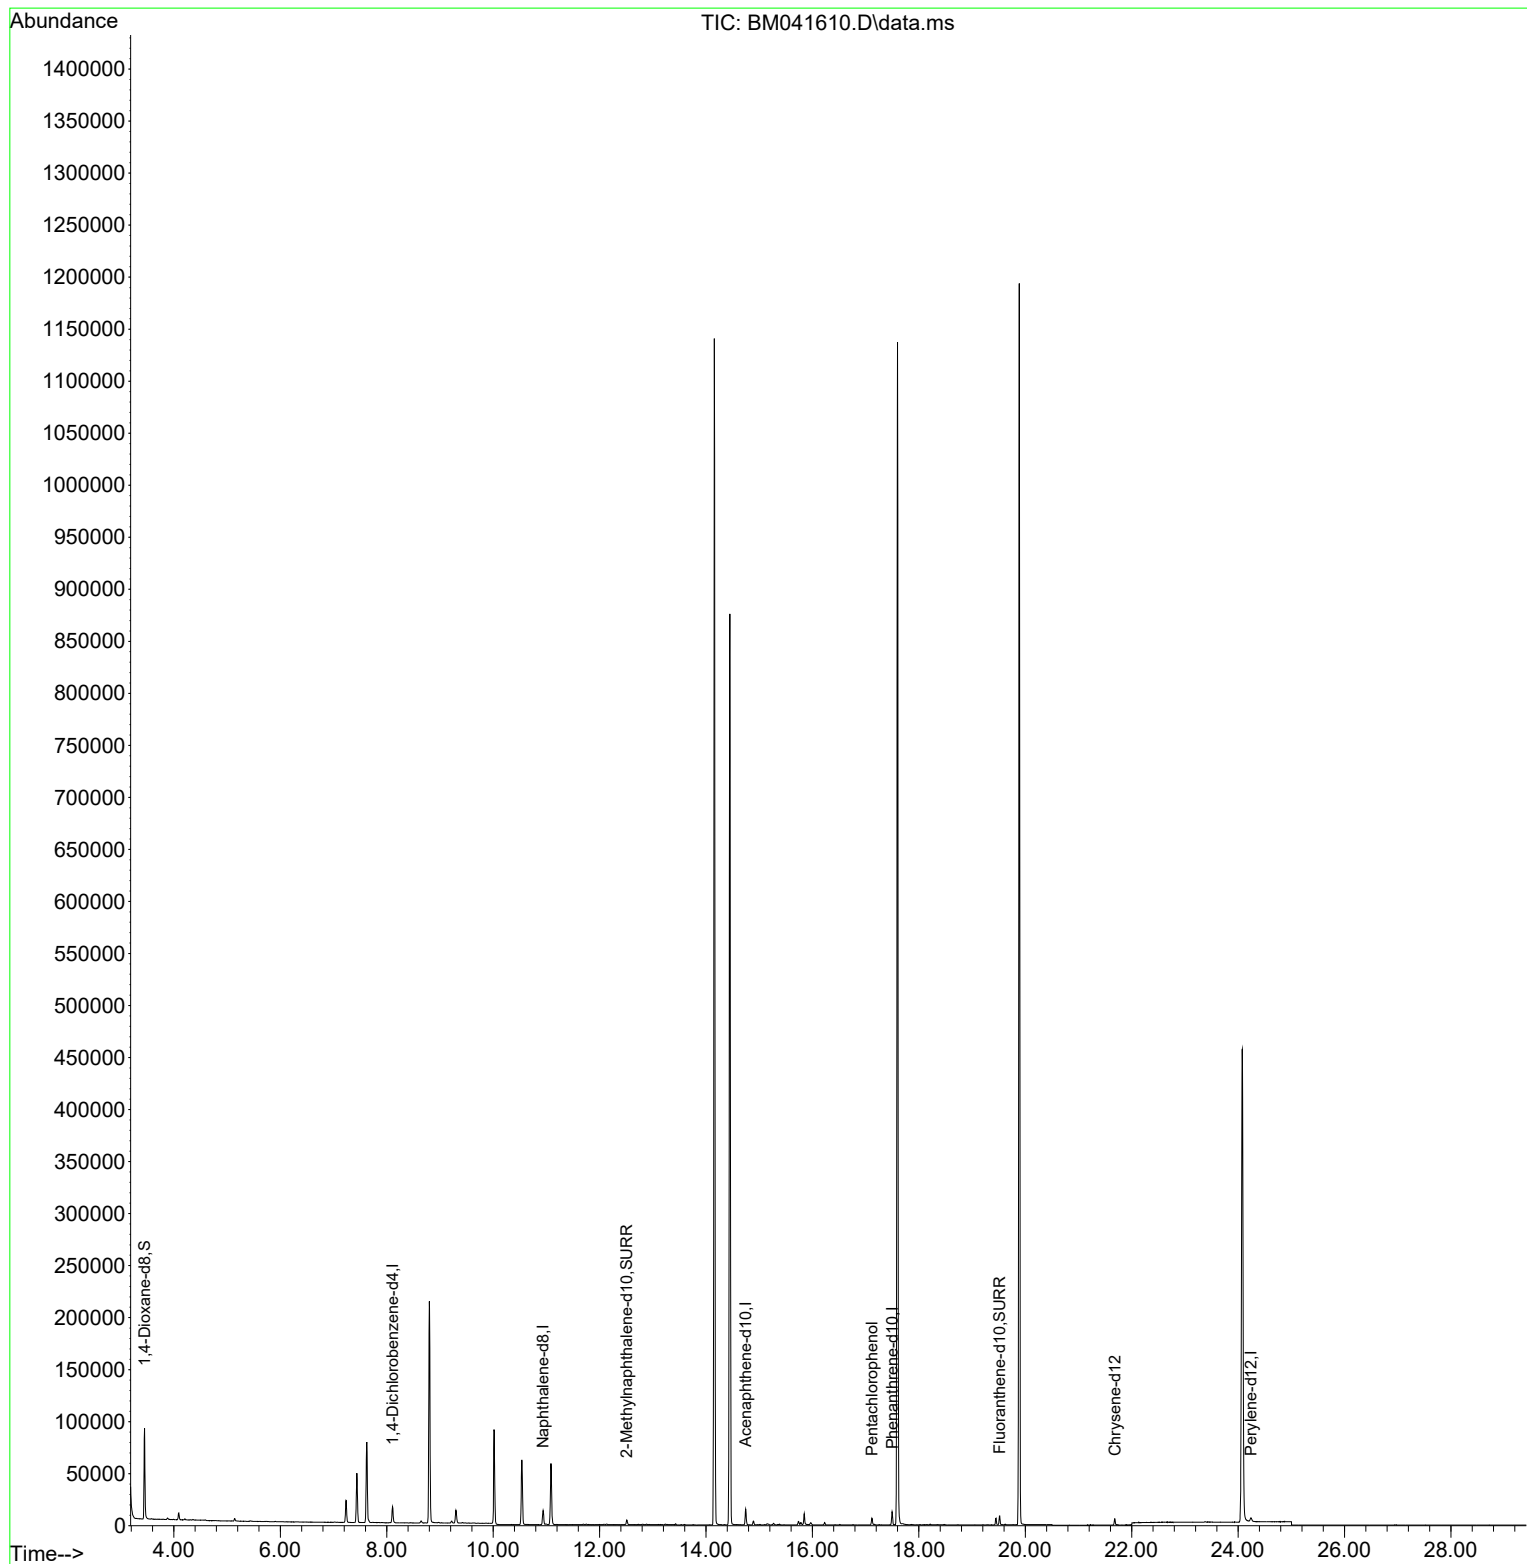

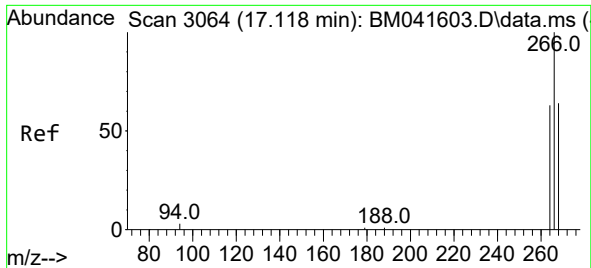

#14
Pentachlorophenol
Concen: 0.869 ng/ul
RT: 17.117 min Scan# 30
Delta R.T. -0.008 min
Lab File: BM041610.D
Acq: 31 Aug 2023 11:20

Instrument :
BNA_M
ClientSampleId :
DCHK3

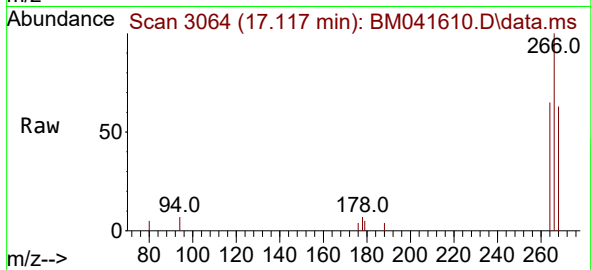

Tgt Ion:266 Resp: 4288
Ion Ratio Lower Upper
266 100
264 62.5 49.3 73.9
268 63.8 50.2 75.4

