

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041611.D
 Acq On : 31 Aug 2023 11:56
 Operator : MA/JU
 Sample : 04159-10
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCHK7

Quant Time: Sep 01 02:08:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	6463	0.400	ng/ul	0.00
4) Naphthalene-d8	10.944	136	16006	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.745	164	7248	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.498	188	15030	0.400	ng/ul	0.00
17) Chrysene-d12	21.685	240	5714	0.400	ng/ul	0.00
23) Perylene-d12	24.243	264	6865	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.452	96	43573	4.568	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	6284	0.325	ng/ul	-0.01
18) Fluoranthene-d10	19.520	212	10708	0.380	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	17.122	266	14383	2.490	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041611.D
Acq On : 31 Aug 2023 11:56
Operator : MA/JU
Sample : 04159-10
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCHK7


Quant Time: Sep 01 02:08:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

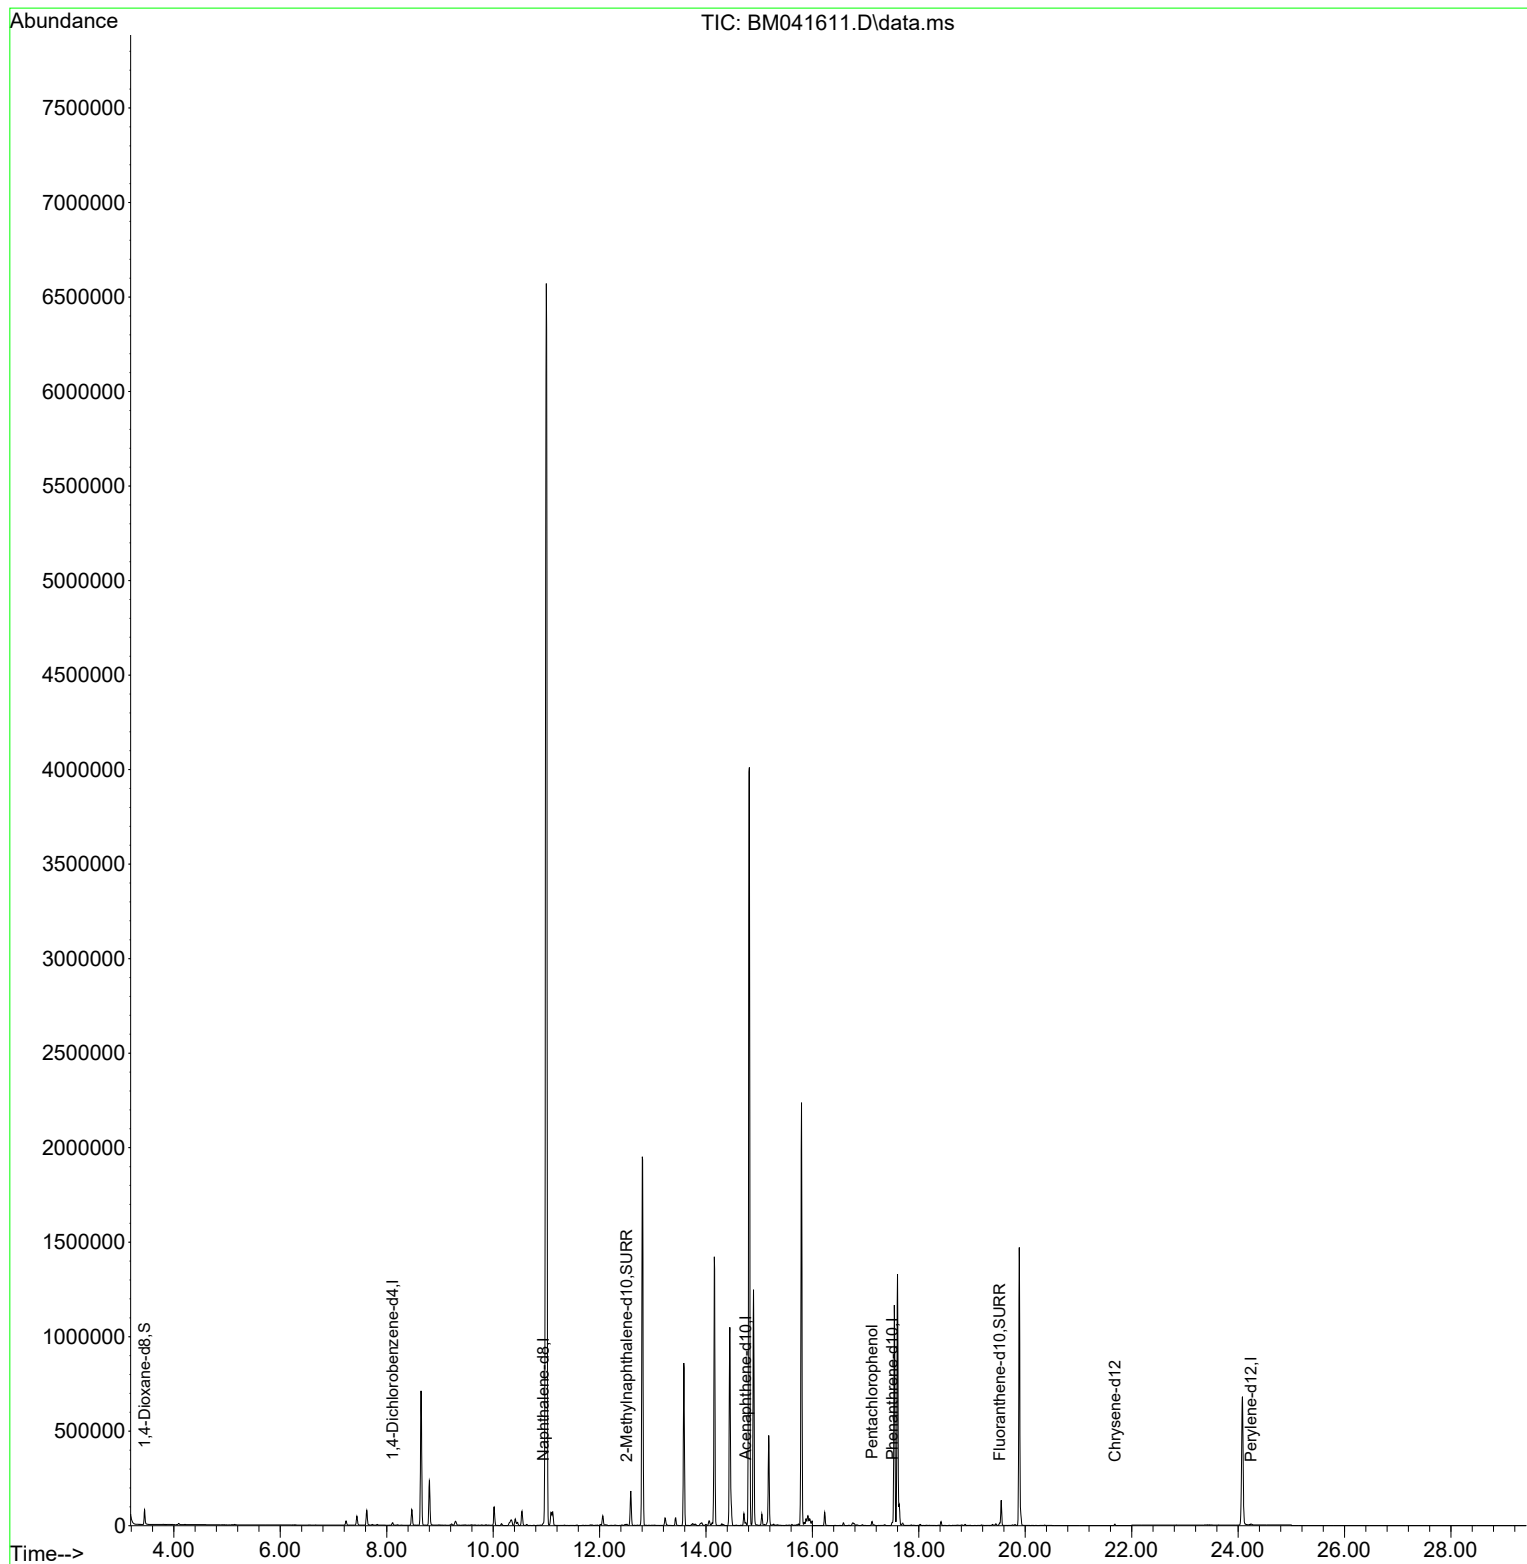

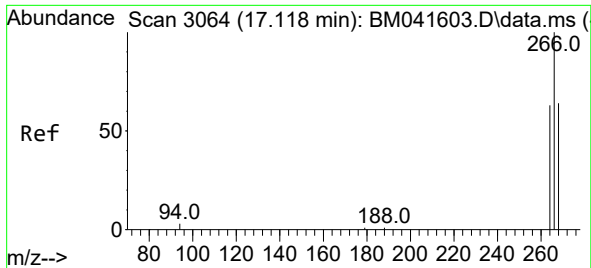

#14
Pentachlorophenol
Concen: 2.490 ng/ul
RT: 17.122 min Scan# 3065
Delta R.T. -0.004 min
Lab File: BM041611.D
Acq: 31 Aug 2023 11:56

Instrument :
BNA_M
ClientSampleId :
DCHK7

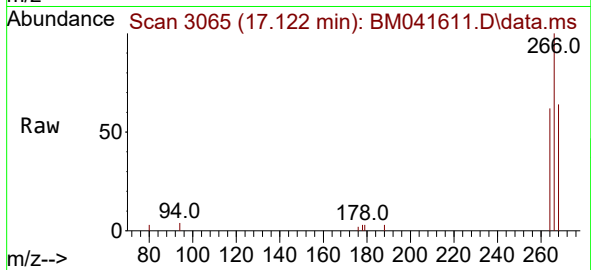

Tgt Ion:	266	Resp:	14383
Ion	Ratio	Lower	Upper
266	100		
264	62.5	49.3	73.9
268	63.7	50.2	75.4

