

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041628.D
 Acq On : 31 Aug 2023 23:02
 Operator : MA/JU
 Sample : 04148-06
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJW3

Quant Time: Sep 01 02:10:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	9232	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	21480	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.745	164	9614	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.497	188	17238	0.400	ng/ul	0.00
17) Chrysene-d12	21.676	240	6776	0.400	ng/ul	-0.01
23) Perylene-d12	24.234	264	8191	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	45675	3.352	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	6646	0.256	ng/ul	-0.01
18) Fluoranthene-d10	19.515	212	9352	0.280	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.486	88	3970	0.273	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041628.D
Acq On : 31 Aug 2023 23:02
Operator : MA/JU
Sample : 04148-06
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJW3


Quant Time: Sep 01 02:10:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

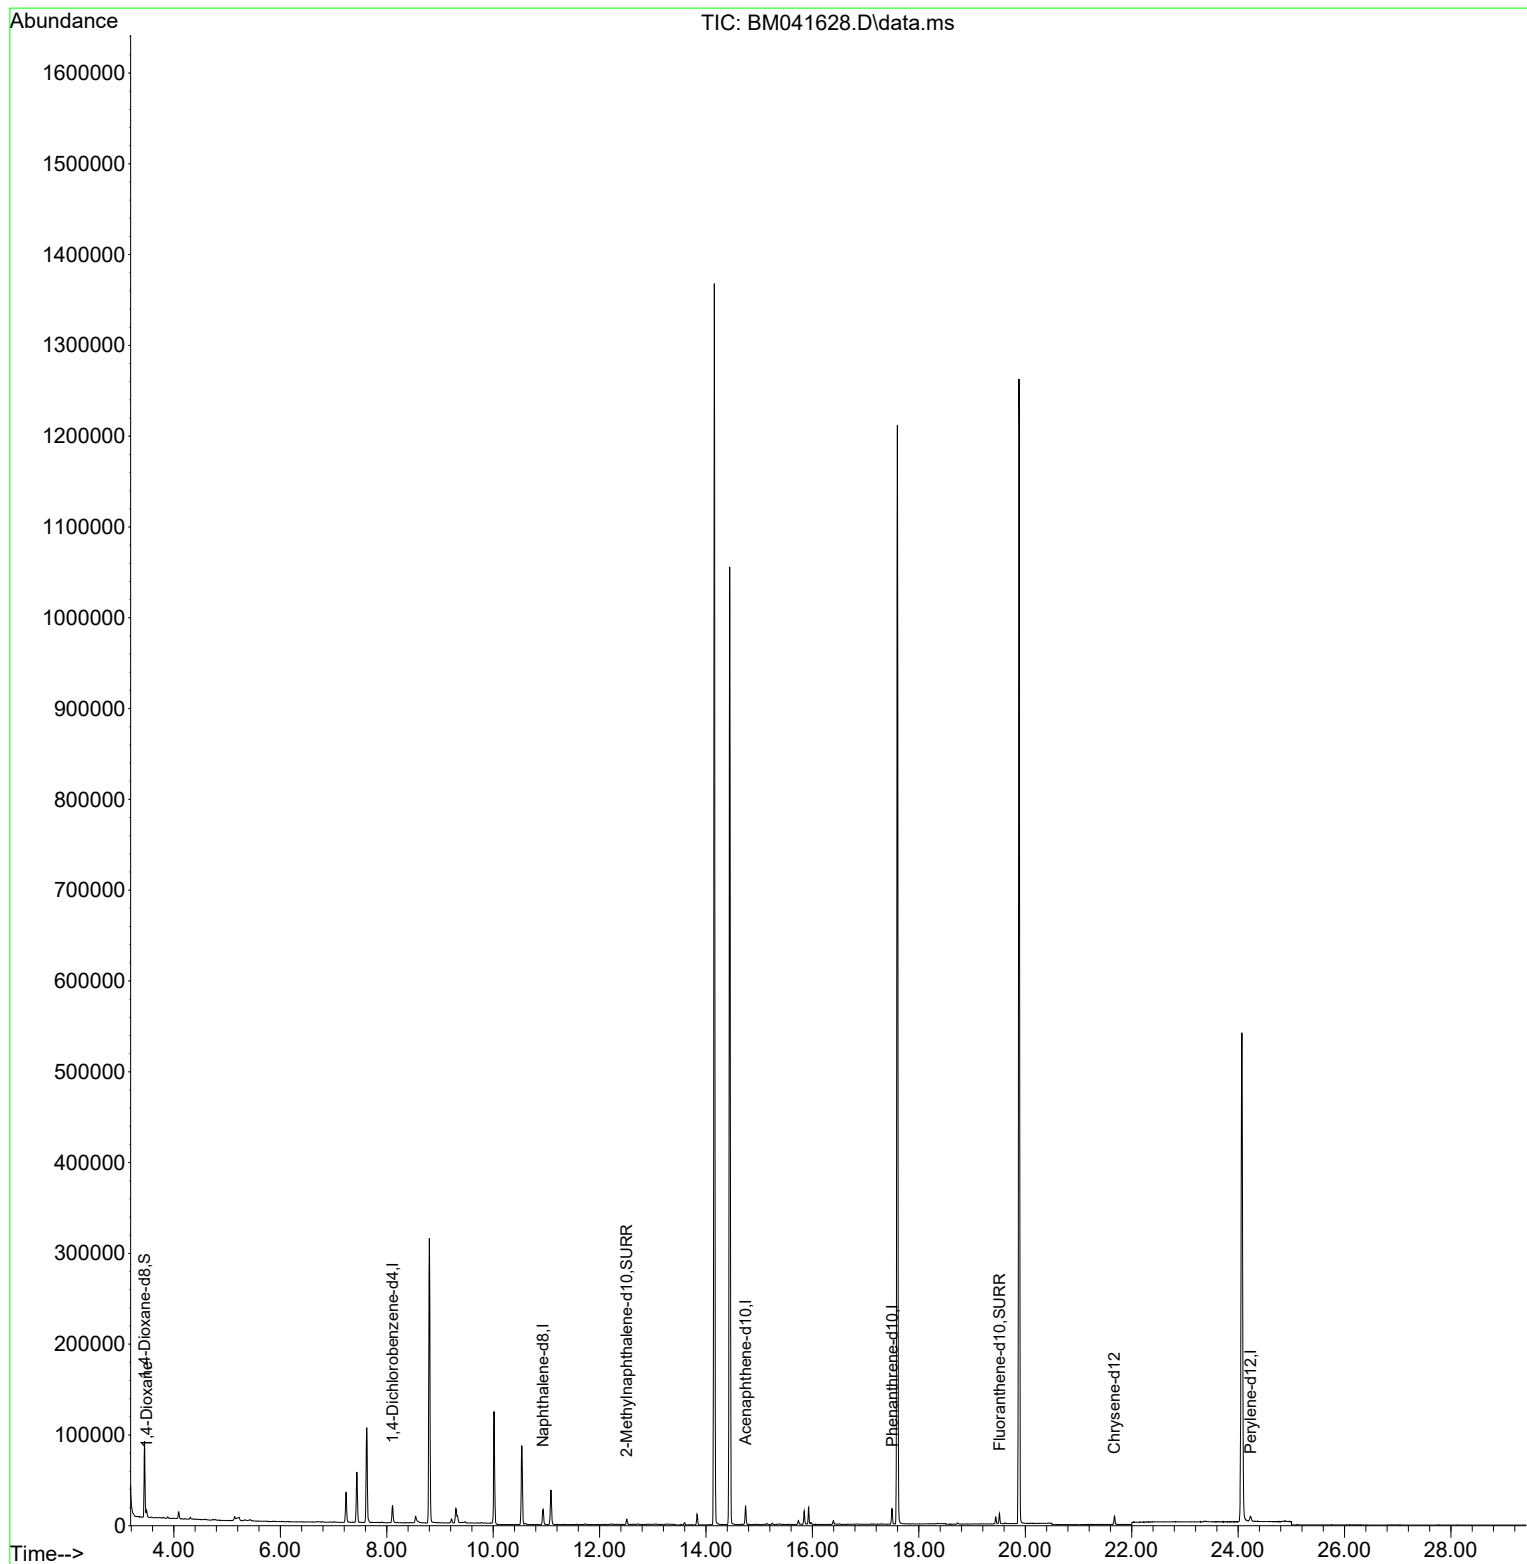


Abundance Scan 72 (3.486 min): BM041620.D\data.ms (-64)

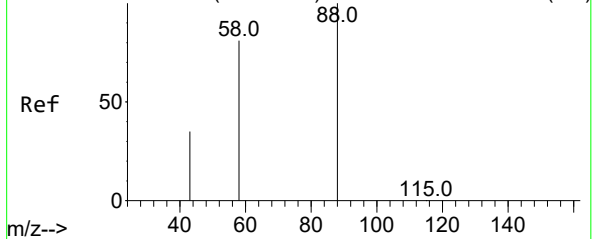

Abundance Scan 72 (3.486 min): BM041628.D\data.ms

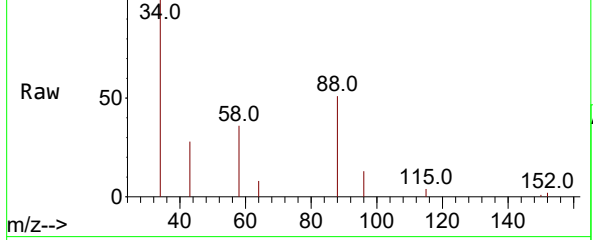

Abundance Scan 72 (3.486 min): BM041628.D\data.ms (-59)

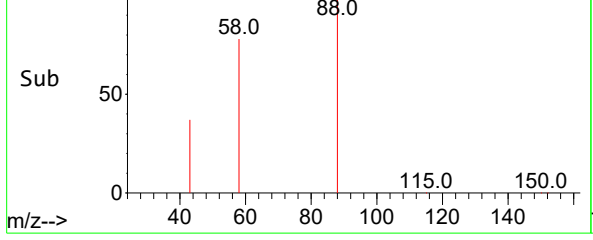

#2
1,4-Dioxane
Concen: 0.273 ng/ul
RT: 3.486 min Scan# 71
Delta R.T. -0.004 min
Lab File: BM041628.D
Acq: 31 Aug 2023 23:02

Instrument :
BNA_M
ClientSampleId :
BBJW3

Tgt Ion:	88	Resp:	3970
Ion	Ratio	Lower	Upper
88	100		
43	55.1	46.2	69.2
58	70.6	58.1	87.1

