

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041632.D
 Acq On : 01 Sep 2023 01:28
 Operator : MA/JU
 Sample : 04148-10
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBKG5

Quant Time: Sep 01 02:11:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	6801	0.400	ng/ul	0.00
4) Naphthalene-d8	10.938	136	14992	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.745	164	6683	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.493	188	12365	0.400	ng/ul	-0.01
17) Chrysene-d12	21.676	240	4939	0.400	ng/ul	-0.01
23) Perylene-d12	24.231	264	6156	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	37519	3.738	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	5819	0.322	ng/ul	-0.01
18) Fluoranthene-d10	19.515	212	9599	0.394	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.486	88	22884	2.137	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041632.D
Acq On : 01 Sep 2023 01:28
Operator : MA/JU
Sample : 04148-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBKG5


Quant Time: Sep 01 02:11:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration

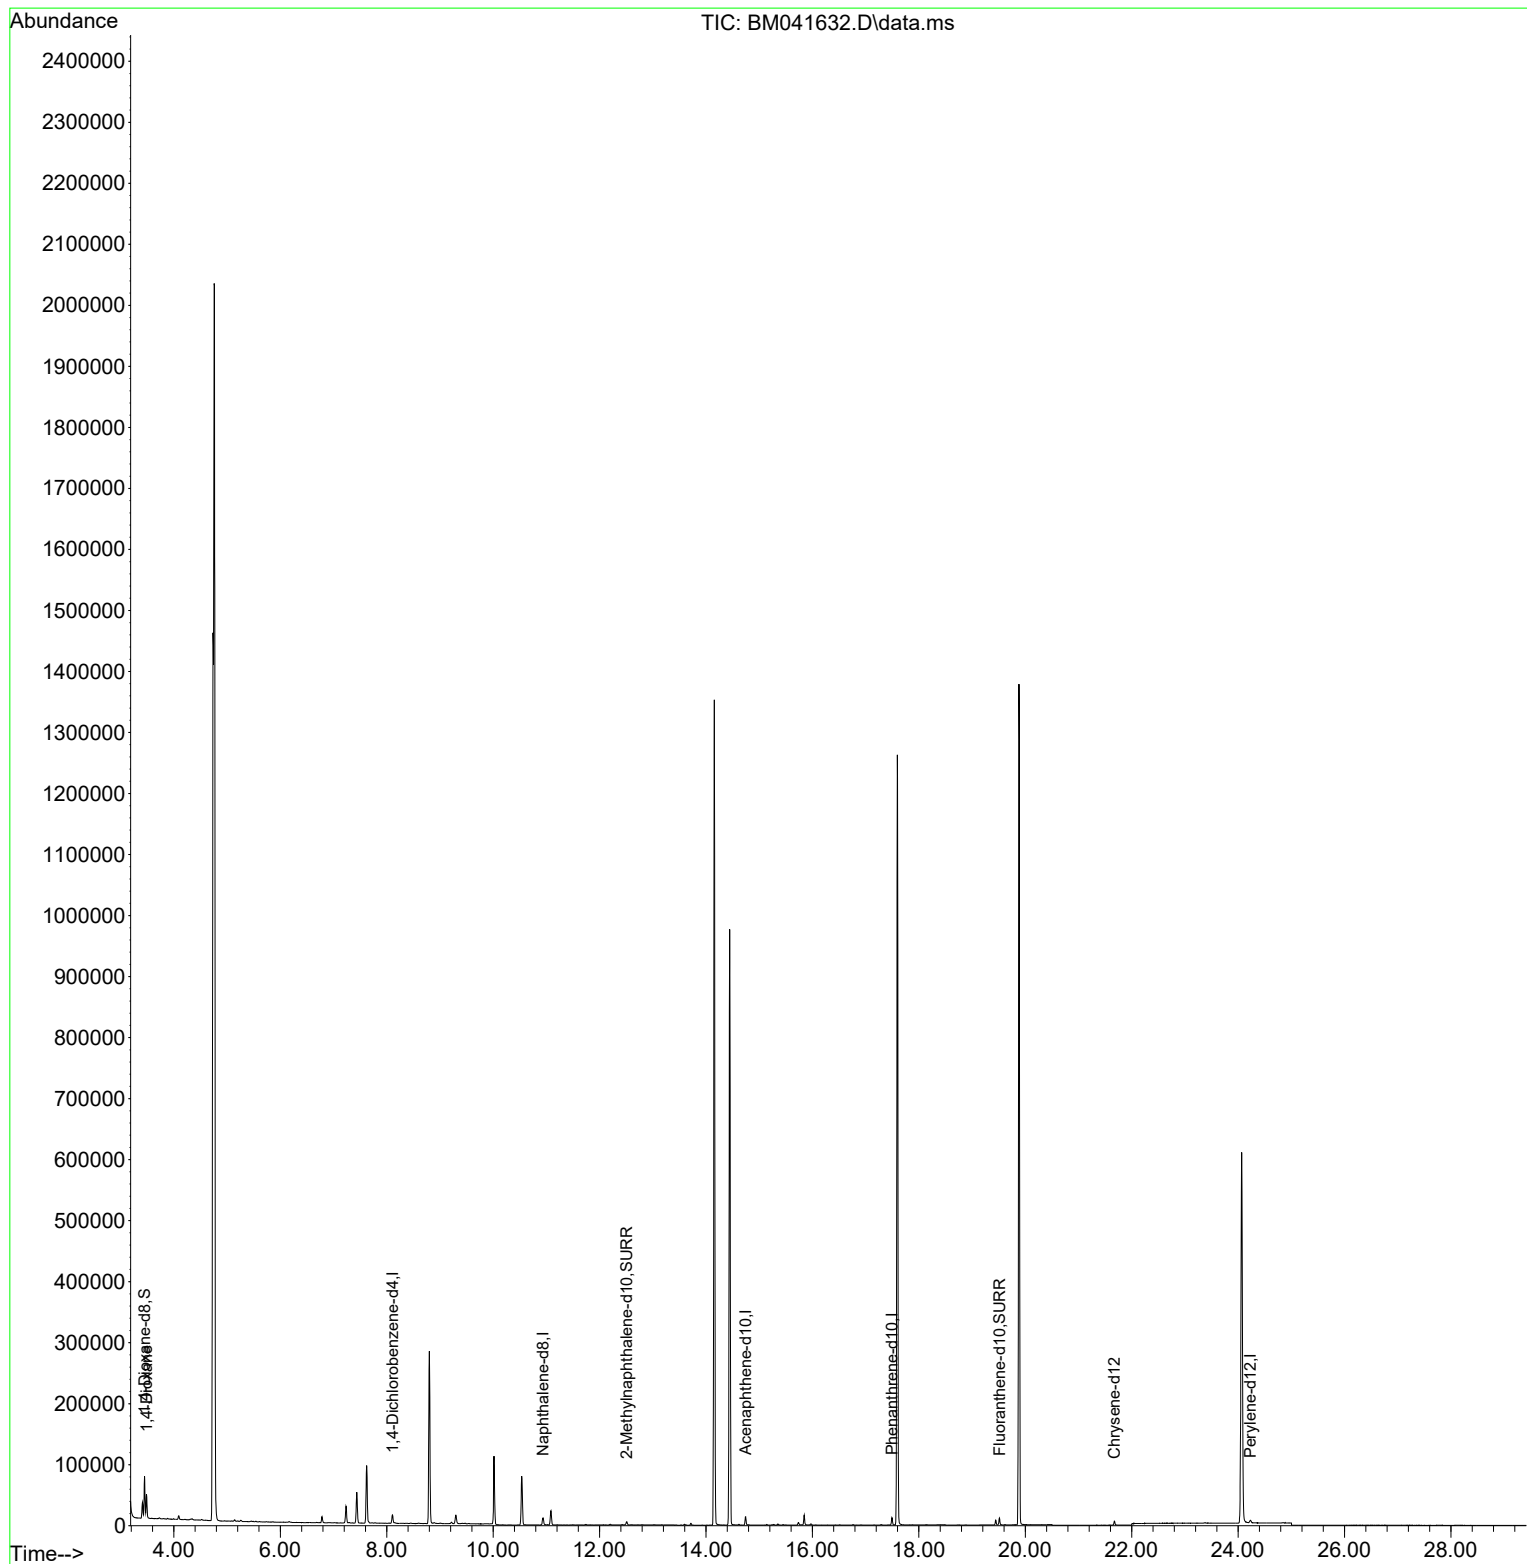


Abundance Scan 72 (3.486 min): BM041620.D\data.ms (-64)

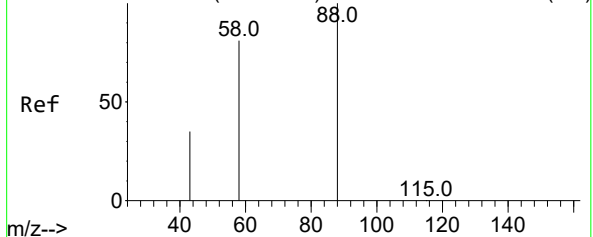

Abundance Scan 72 (3.486 min): BM041632.D\data.ms

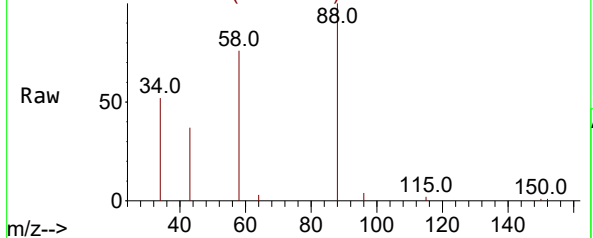

Abundance Scan 72 (3.486 min): BM041632.D\data.ms (-59)

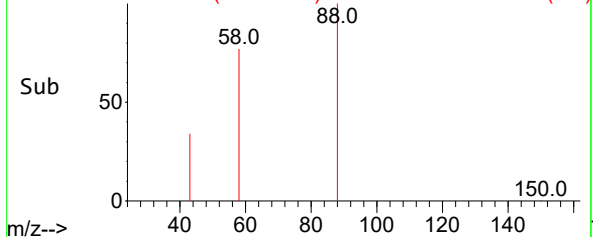

#2
1,4-Dioxane
Concen: 2.137 ng/ul
RT: 3.486 min Scan# 71
Delta R.T. -0.004 min
Lab File: BM041632.D
Acq: 01 Sep 2023 01:28

Instrument :
BNA_M
ClientSampleId :
BBKG5

Tgt Ion: 88 Resp: 22884
Ion Ratio Lower Upper
88 100
43 37.5 46.2 69.2#
58 76.2 58.1 87.1

