

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
 Data File : BM041634.D
 Acq On : 01 Sep 2023 02:41
 Operator : MA/JU
 Sample : 04148-12
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJW5

Quant Time: Sep 01 03:16:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 30 01:50:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.106	152	7112	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.933	136	15832	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.745	164	7008	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.493	188	12945	0.400	ng/ul	-0.01
17) Chrysene-d12	21.676	240	5319	0.400	ng/ul	-0.01
23) Perylene-d12	24.228	264	6643	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	39454	3.759	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.511	152	6386	0.334	ng/ul	-0.01
18) Fluoranthene-d10	19.515	212	9036	0.344	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.486	88	14216	1.270	ng/ul#	87
14) Pentachlorophenol	17.118	266	150	0.030	ng/ul	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082923\
Data File : BM041634.D
Acq On : 01 Sep 2023 02:41
Operator : MA/JU
Sample : 04148-12
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJW5

Quant Time: Sep 01 03:16:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 30 01:50:06 2023
Response via : Initial Calibration




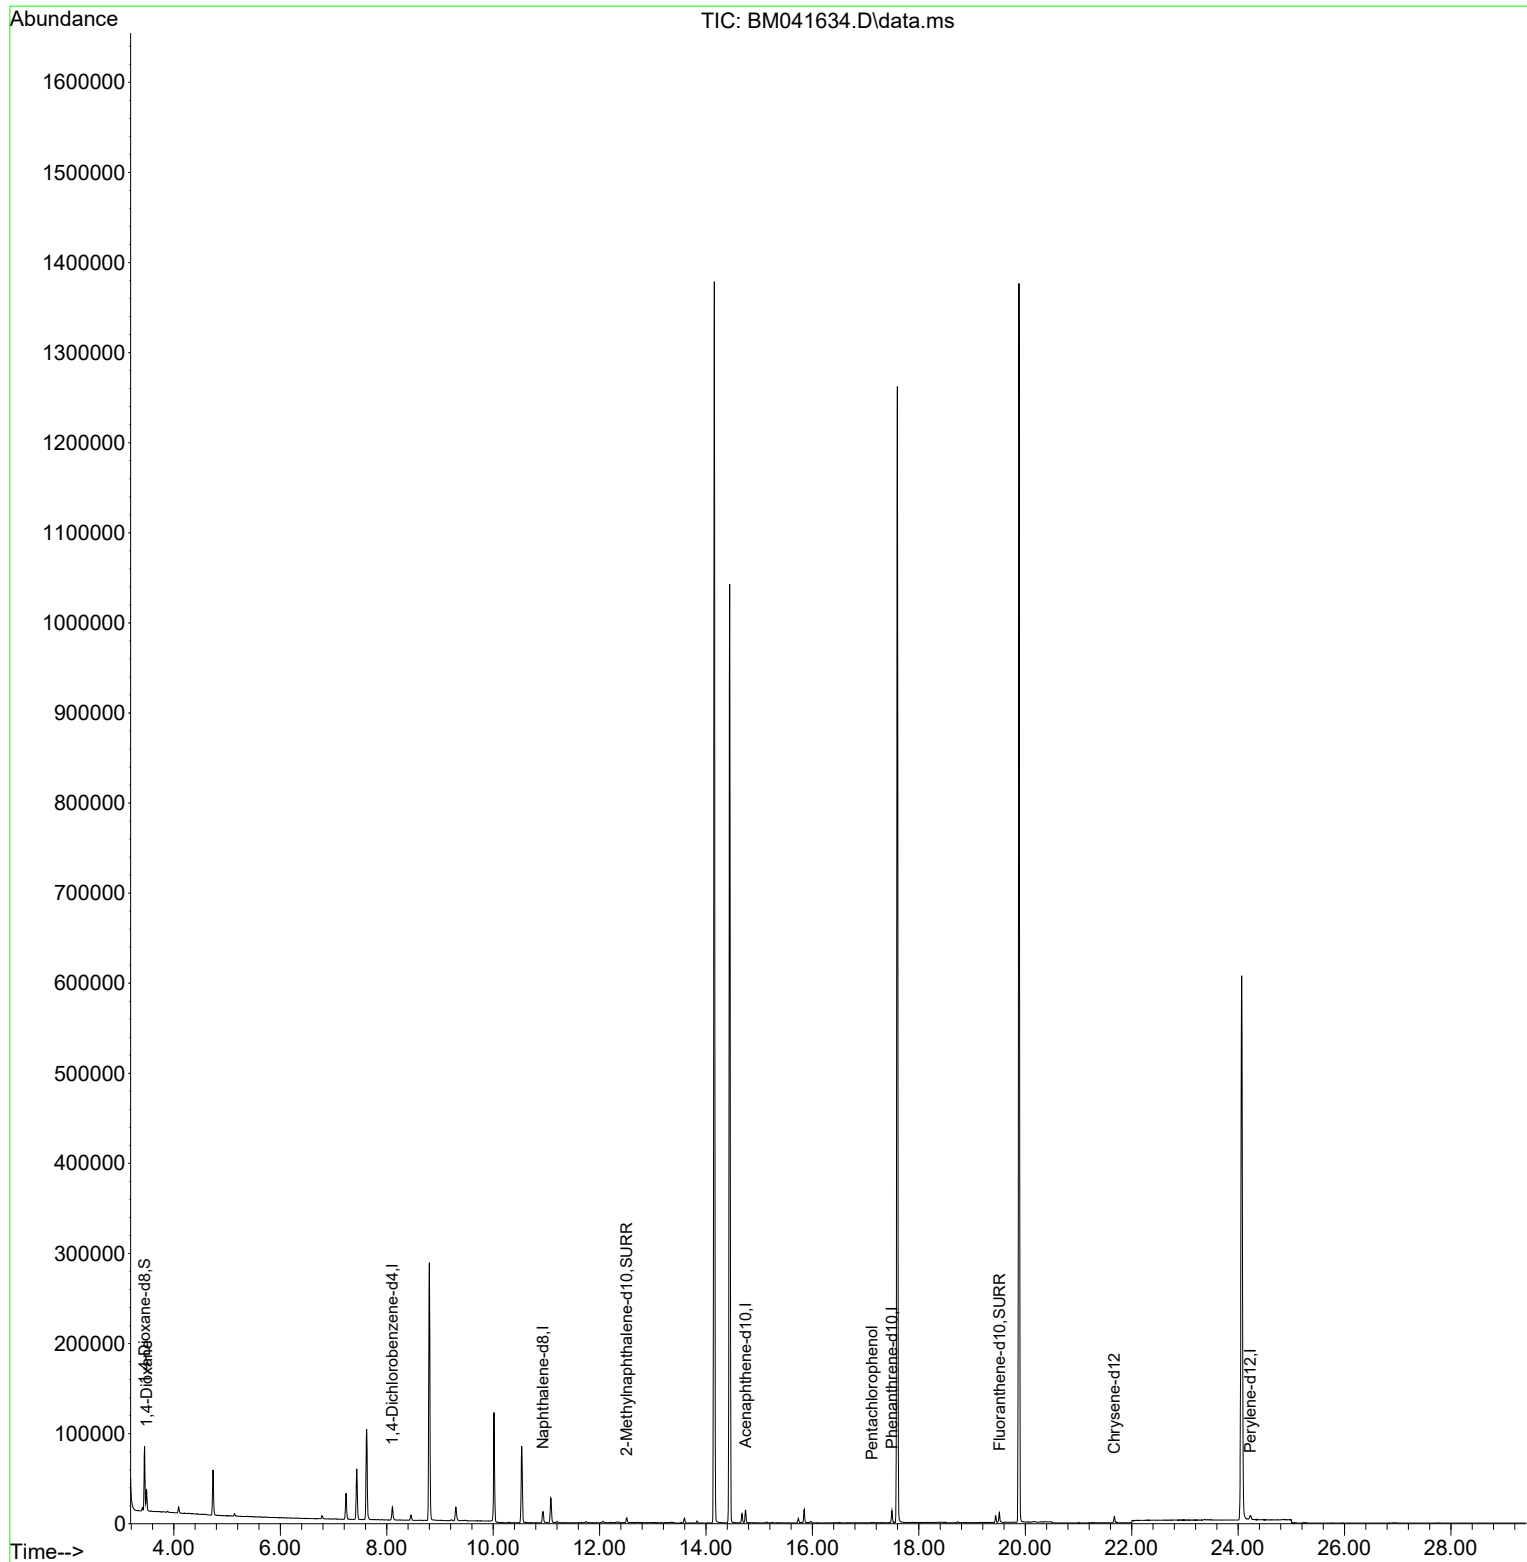


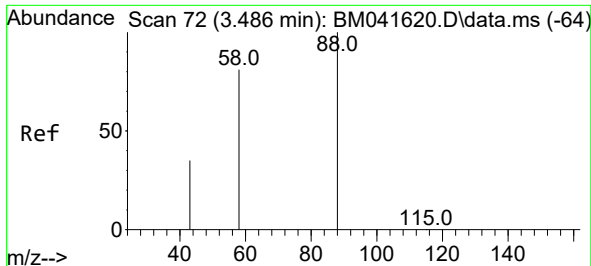

#2
1,4-Dioxane
Concen: 1.270 ng/ul
RT: 3.486 min Scan# 71
Delta R.T. -0.004 min
Lab File: BM041634.D
Acq: 01 Sep 2023 02:41

Instrument :
BNA_M
ClientSampleId :
BBJW5

Tgt Ion: 88 Resp: 14216
Ion Ratio Lower Upper
88 100
43 39.7 46.2 69.2#
58 75.8 58.1 87.1

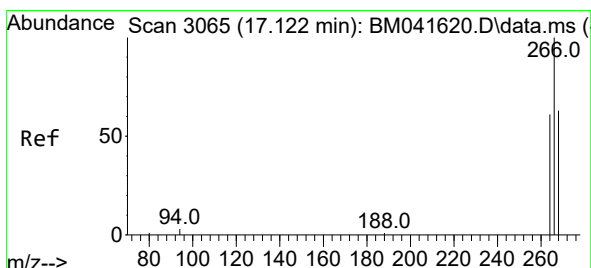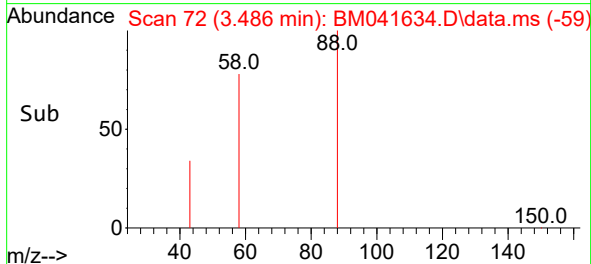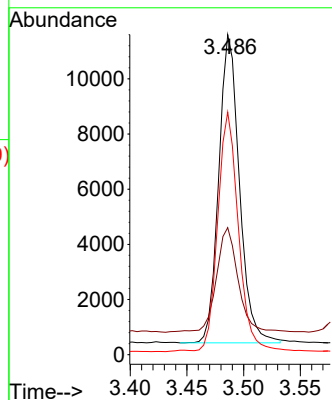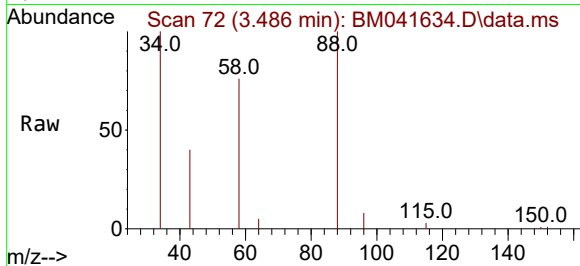

#14
Pentachlorophenol
Concen: 0.030 ng/ul
RT: 17.118 min Scan# 3064
Delta R.T. -0.008 min
Lab File: BM041634.D
Acq: 01 Sep 2023 02:41

Tgt Ion: 266 Resp: 150
Ion Ratio Lower Upper
266 100
264 69.3 49.3 73.9
268 69.3 50.2 75.4

