

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083019\
 Data File : BM022436.D
 Acq On : 30 Aug 2019 11:32
 Operator : HP/JU
 Sample : PB122622BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 30 14:27:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 29 16:51:32 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	21571	20.00	ng	0.00
21) Naphthalene-d8	10.30	136	78805	20.00	ng	0.00
39) Acenaphthene-d10	14.19	164	53598	20.00	ng	0.00
64) Phenanthrene-d10	16.96	188	131281	20.00	ng	0.00
76) Chrysene-d12	21.17	240	176561	20.00	ng	0.00
87) Perylene-d12	23.36	264	196486	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.15	112	172280	140.19	ng	0.00
7) Phenol-d6	6.72	99	223723	136.14	ng	0.00
23) Nitrobenzene-d5	8.70	82	152724	84.89	ng	0.00
42) 2,4,6-Tribromophenol	15.70	330	142935	130.32	ng	0.00
45) 2-Fluorobiphenyl	12.79	172	386846	81.76	ng	0.00
79) Terphenyl-d14	19.60	244	1159270	86.65	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083019\
Data File : BM022436.D
Acq On : 30 Aug 2019 11:32
Operator : HP/JU
Sample : PB122622BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 30 14:27:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 29 16:51:32 2019
Response via : Initial Calibration

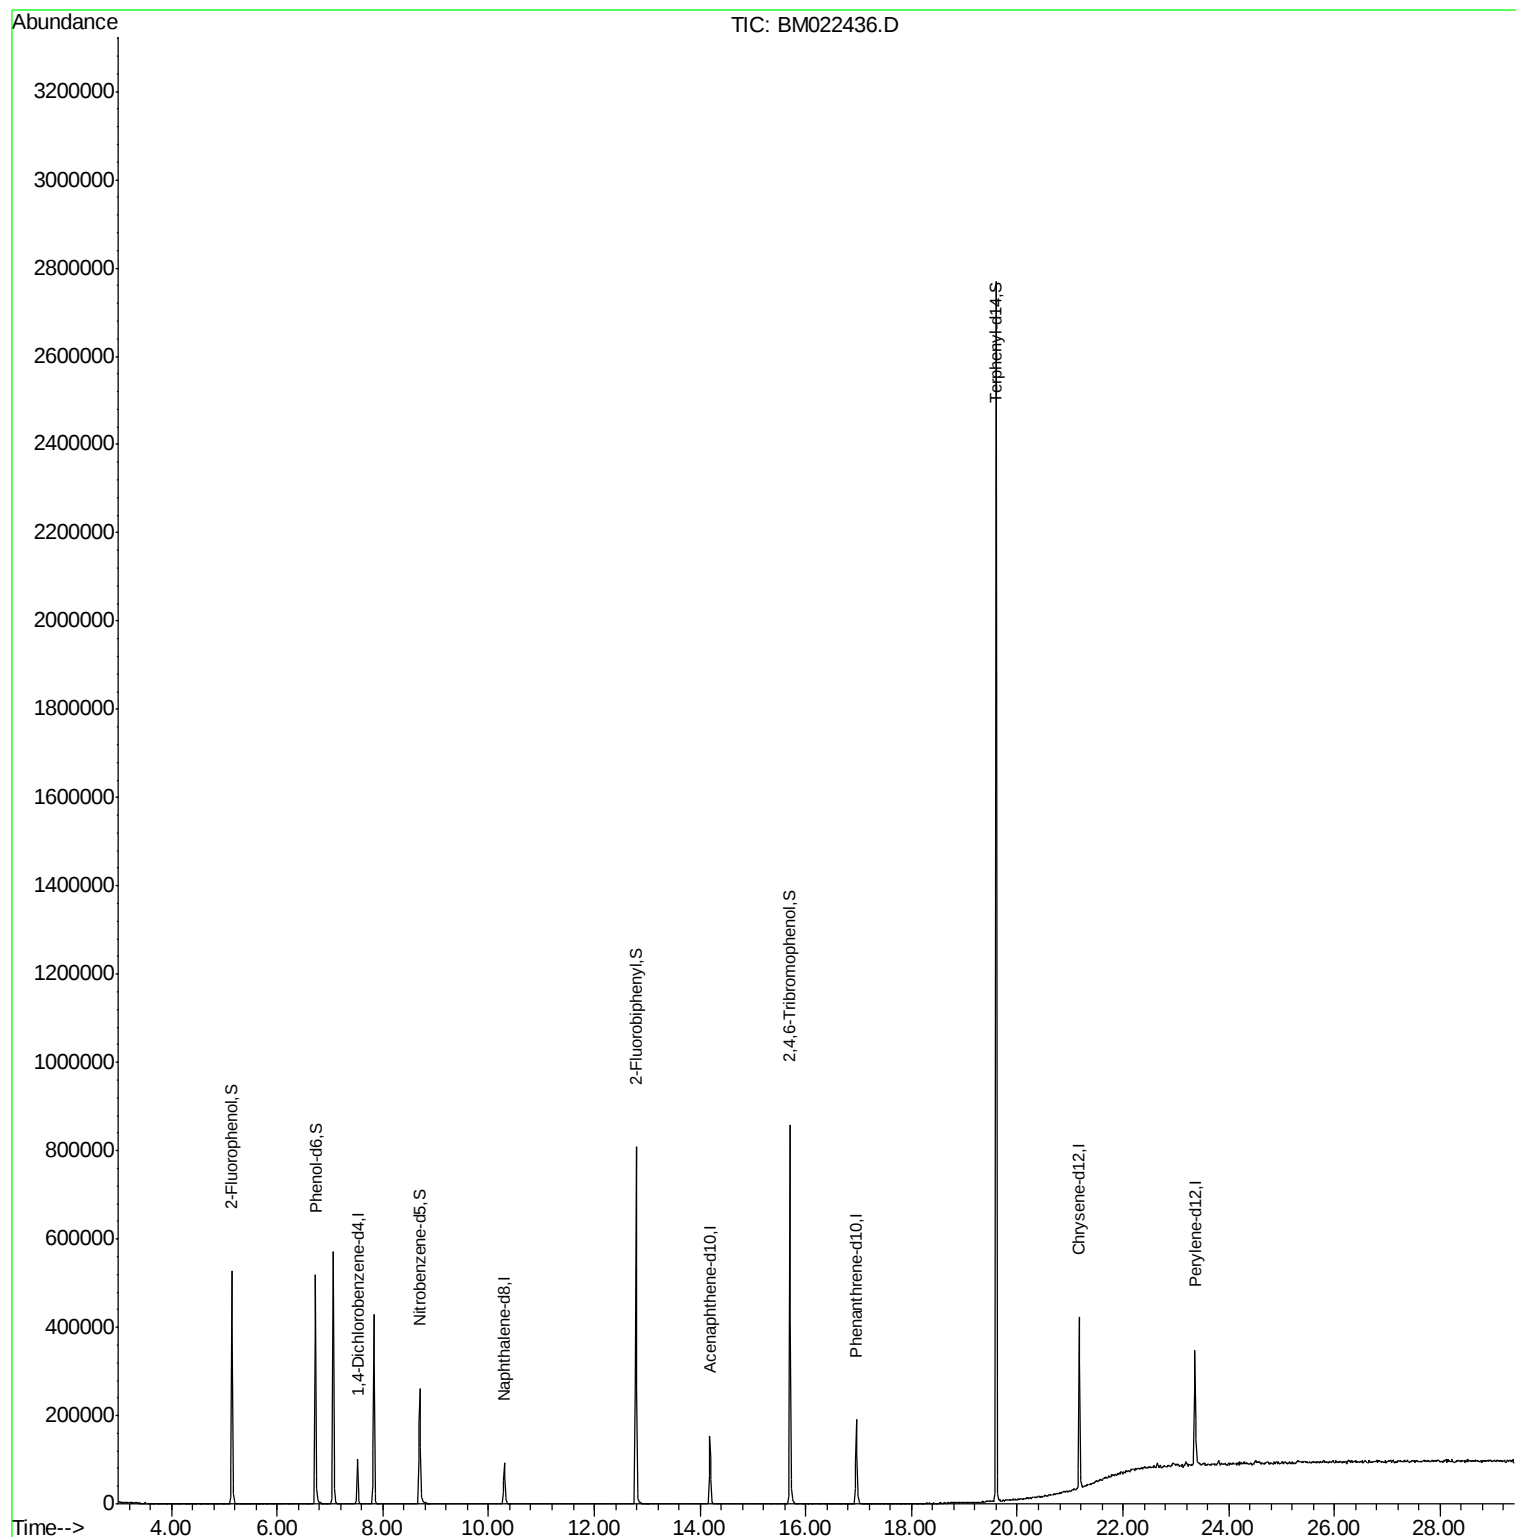




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.52 min Scan# 771
Delta R.T. -0.01 min
Lab File: BM022436.D
Acq: 30 Aug 2019 11:32

Instrument :
BNA_M
ClientSampled :

Tot Ion	Ratio	Lower	Upper
152	100		
150	157.3	125.4	188.0
115	69.0	50.3	75.5

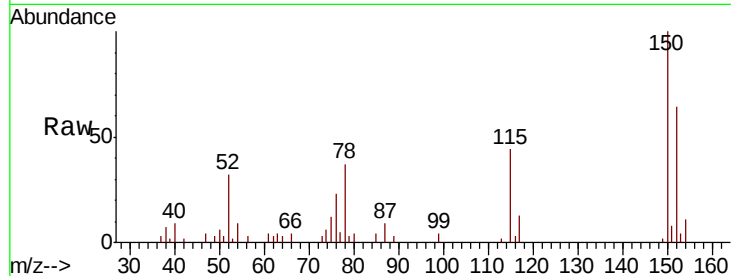


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

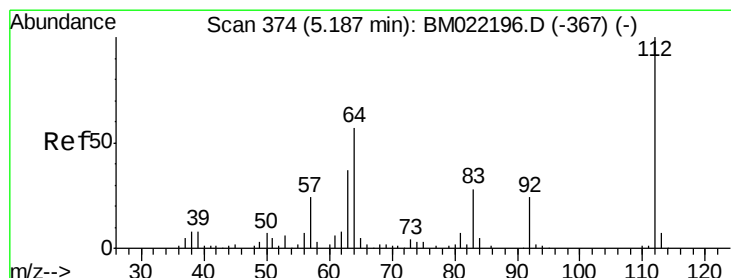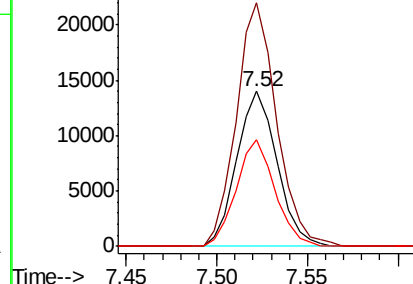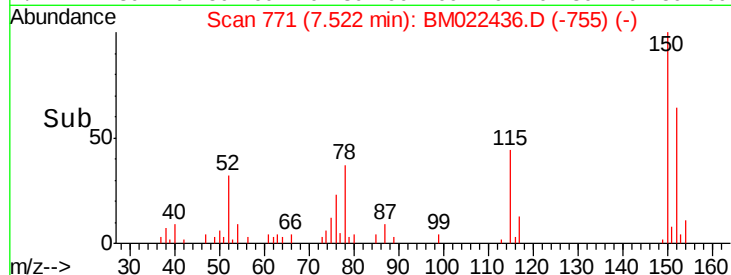



#5


2-Fluorophenol
Concen: 140.192 ng
RT: 5.15 min Scan# 367
Delta R.T. -0.00 min
Lab File: BM022436.D
Acq: 30 Aug 2019 11:32

Tgt Ion	Ratio	Lower	Upper
112	100		
64	60.4	45.4	68.2
63	41.6	34.5	51.7

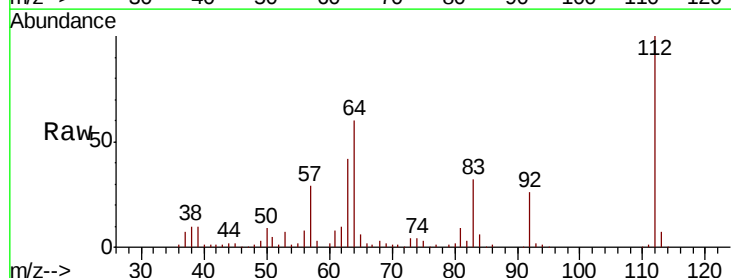

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

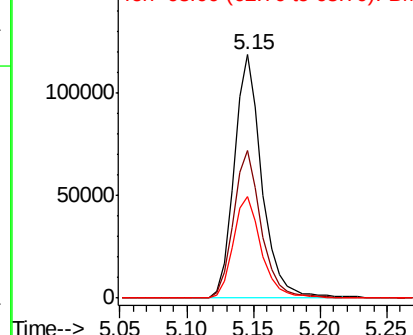

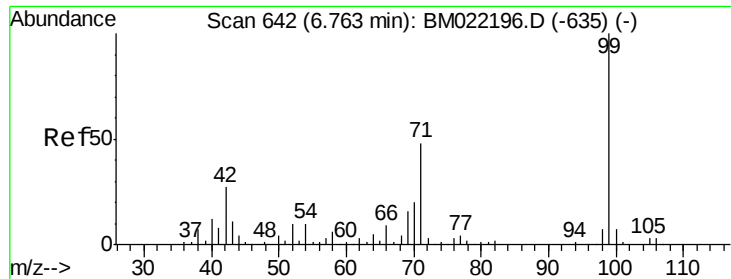

#7

Phenol-d6

Concen: 136.139 ng

RT: 6.72 min Scan# 635

Delta R.T. -0.00 min

Lab File: BM022436.D

Acq: 30 Aug 2019 11:32

Instrument :

BNA_M

ClientSampled :


Tot Ion: 99 Resp: 223723

Ion Ratio Lower Upper

99 100

42 30.2 26.3 39.5




71 54.9 46.6 69.8

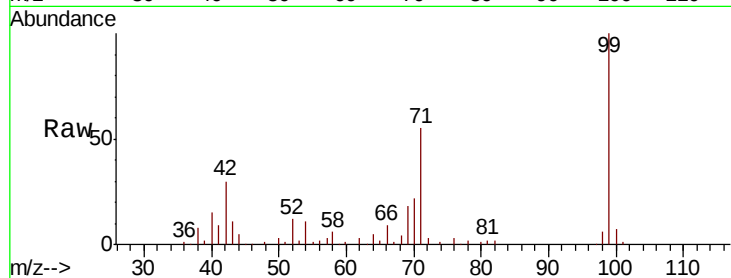

Abundance Ion 99.00 (98.70 to 99.70): BM022436.D (-618) (-)

Ion 42.00 (41.70 to 42.70): BM022436.D (-618) (-)

Ion 71.00 (70.70 to 71.70): BM022436.D (-618) (-)

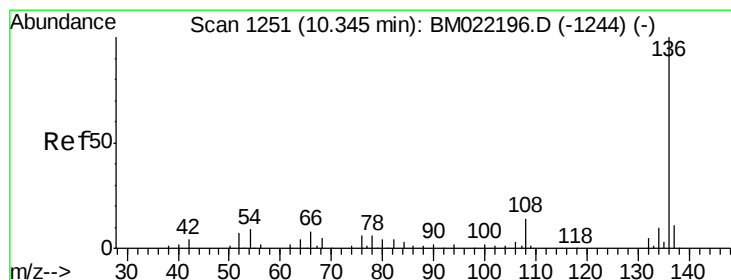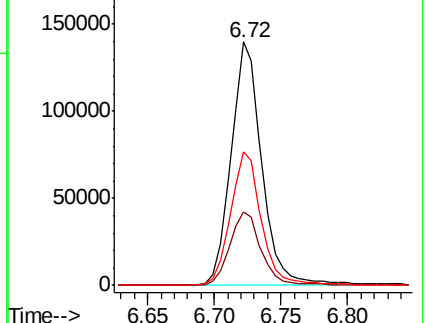

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.30 min Scan# 1243

Delta R.T. -0.00 min

Lab File: BM022436.D

Acq: 30 Aug 2019 11:32

Tgt Ion: 136 Resp: 78805


Ion Ratio Lower Upper

136 100

137 10.6 8.6 13.0

54 8.4 7.0 10.6

68 4.1 2.9 4.3


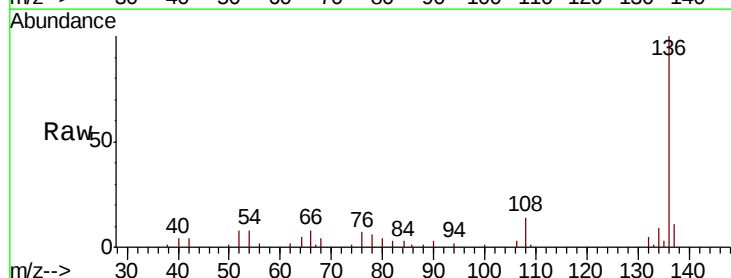



Abundance Ion 136.00 (135.70 to 136.70): BM022436.D (-1226) (-)

Ion 137.00 (136.70 to 137.70): BM022436.D (-1226) (-)

Ion 54.00 (53.70 to 54.70): BM022436.D (-1226) (-)

Ion 68.00 (67.70 to 68.70): BM022436.D (-1226) (-)

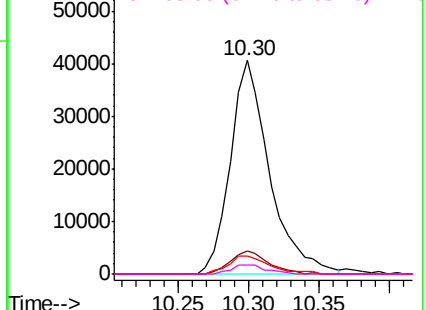


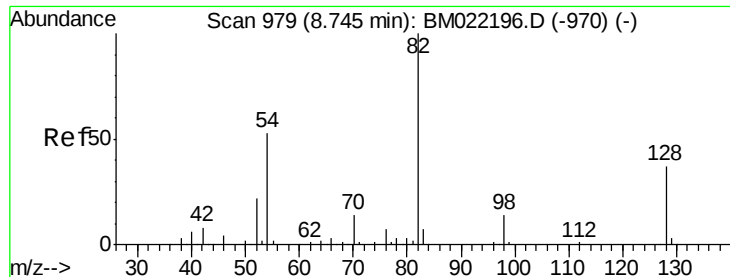




#23
Nitrobenzene-d5
Concen: 84.885 ng
RT: 8.70 min Scan# 971
Delta R.T. -0.00 min
Lab File: BM022436.D
Acq: 30 Aug 2019 11:32

Instrument :
BNA_M
ClientSampled :

Tot Ion: 82 Resp: 152724
Ion Ratio Lower Upper
82 100
128 36.8 27.9 41.9
54 55.6 45.2 67.8

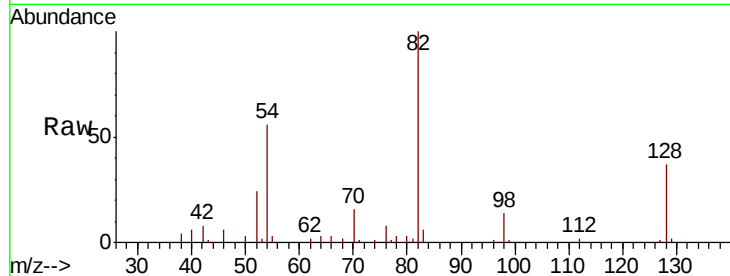


Abundance Ion 82.00 (81.70 to 82.70): BM022436.D (-954) (-)
Ion 128.00 (127.70 to 128.70): BM022436.D (-954) (-)
Ion 54.00 (53.70 to 54.70): BM022436.D (-954) (-)

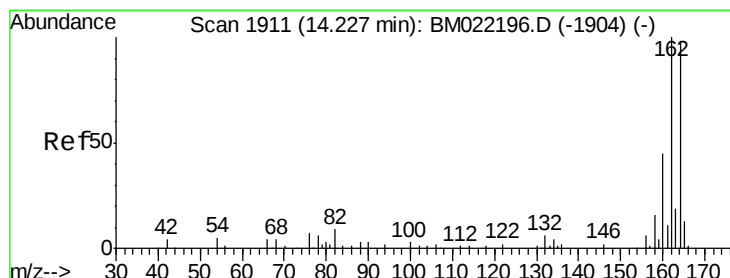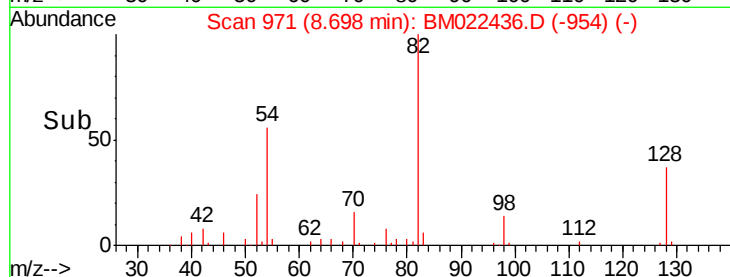
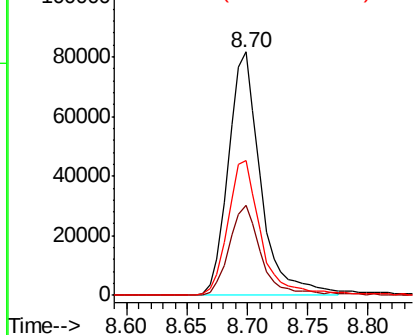



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.19 min Scan# 1904
Delta R.T. -0.00 min
Lab File: BM022436.D
Acq: 30 Aug 2019 11:32

Tgt Ion:164 Resp: 53598
Ion Ratio Lower Upper
164 100
162 106.5 80.6 121.0
160 47.9 37.3 55.9

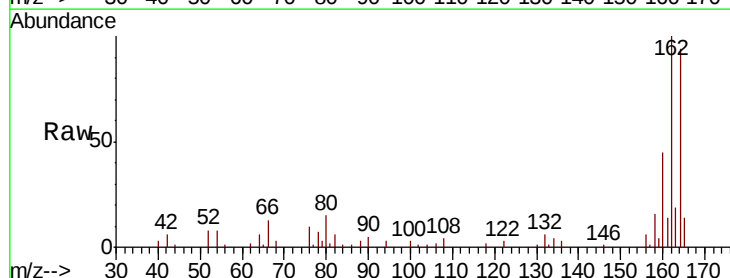

Abundance Ion 164.00 (163.70 to 164.70): BM022436.D (-1887) (-)
Ion 162.00 (161.70 to 162.70): BM022436.D (-1887) (-)
Ion 160.00 (159.70 to 160.70): BM022436.D (-1887) (-)

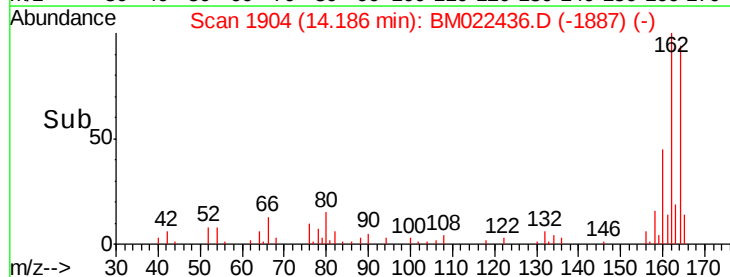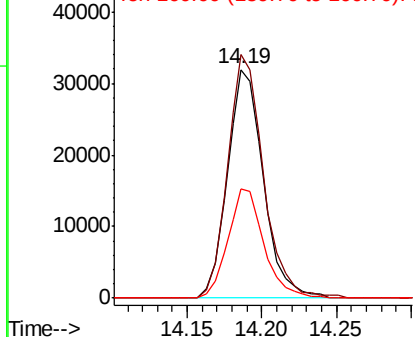


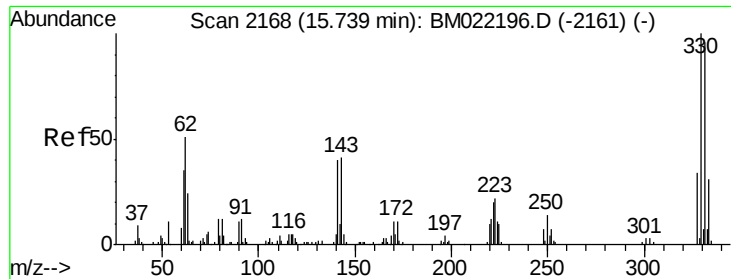

#42
 2,4,6-Tribromophenol
 Concen: 130.324 ng
 RT: 15.70 min Scan# 2161
 Delta R.T. -0.00 min
 Lab File: BM022436.D
 Acq: 30 Aug 2019 11:32

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.0	77.8	116.8
141	43.4	35.6	53.4



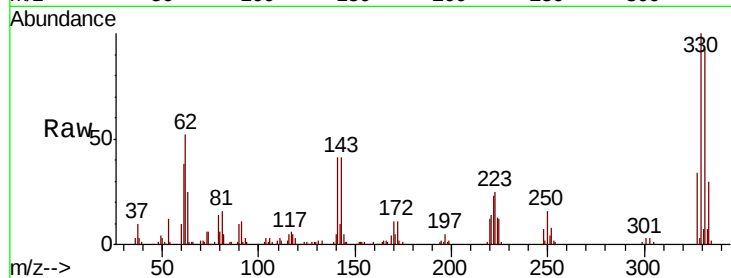


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

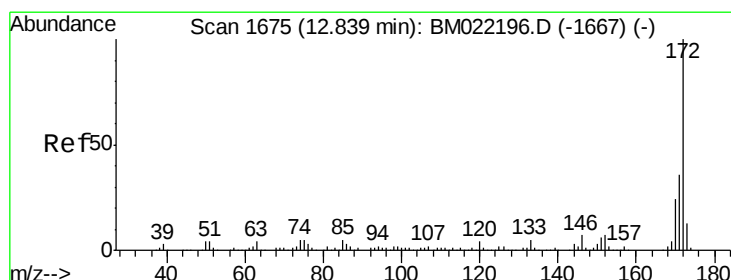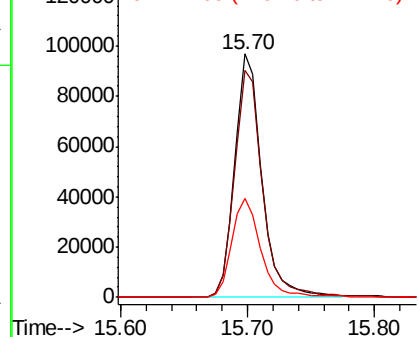

#45
 2-Fluorobiphenyl
 Concen: 81.764 ng
 RT: 12.79 min Scan# 1667
 Delta R.T. -0.00 min
 Lab File: BM022436.D
 Acq: 30 Aug 2019 11:32

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.0	28.5	42.7
170	24.0	18.9	28.3


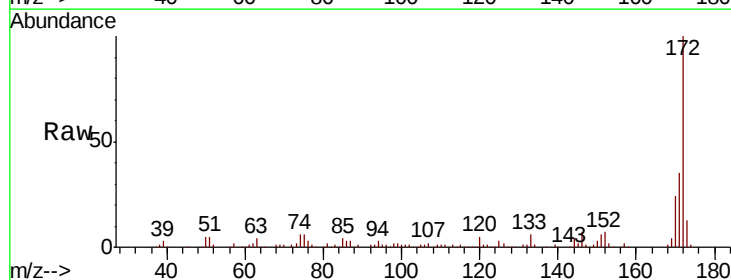



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

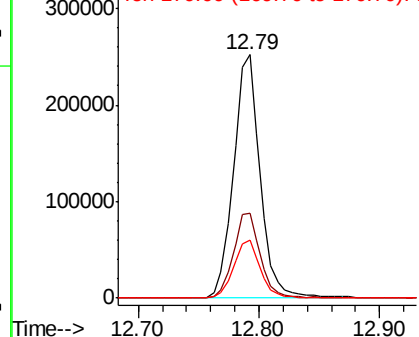


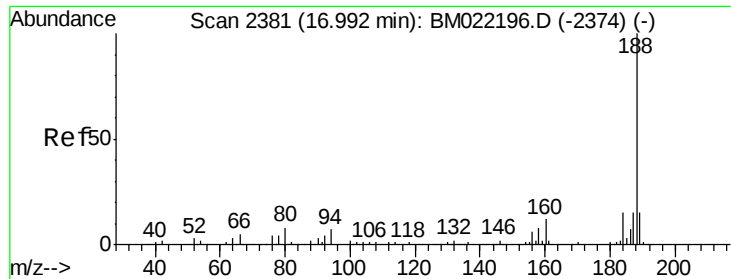




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.96 min Scan# 2375
Delta R.T. 0.01 min
Lab File: BM022436.D
Acq: 30 Aug 2019 11:32

Instrument :
BNA_M
ClientSampleId :

Tot Ion:188 Resp: 131281
Ion Ratio Lower Upper
188 100
94 5.7 4.4 6.6
80 7.1 5.0 7.6

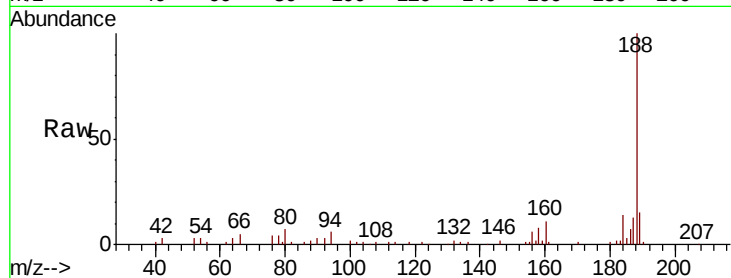


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

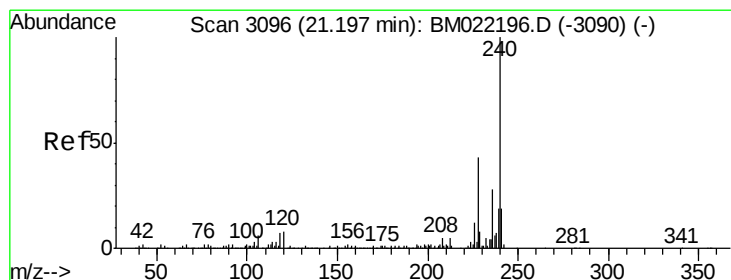
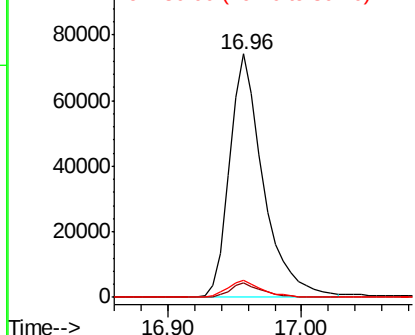



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.17 min Scan# 3092
Delta R.T. -0.00 min
Lab File: BM022436.D
Acq: 30 Aug 2019 11:32

Tgt Ion:240 Resp: 176561
Ion Ratio Lower Upper
240 100
120 4.6 3.9 5.9
236 27.4 21.4 32.2

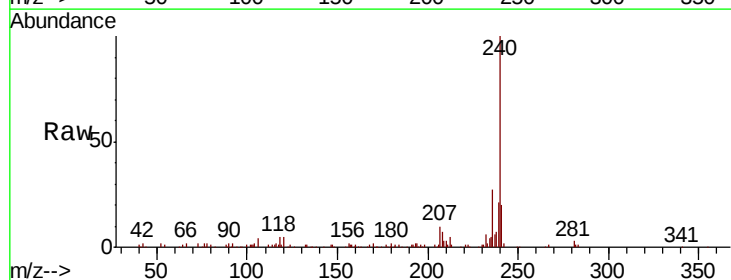

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

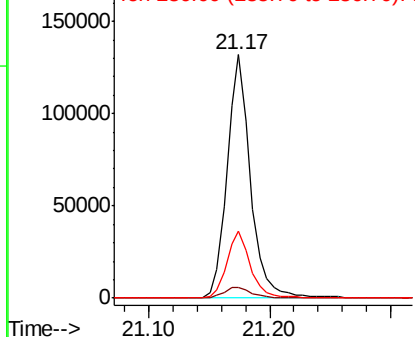




#79
 Terphenyl-d14
 Concen: 86.653 ng
 RT: 19.60 min Scan# 2824
 Delta R.T. -0.01 min
 Lab File: BM022436.D
 Acq: 30 Aug 2019 11:32




Instrument :
 BNA_M
 ClientSampled :

Tot Ion:244 Resp: 1159270

Ion	Ratio	Lower	Upper
244	100		
212	8.4	7.0	10.4
122	5.3	3.9	5.9

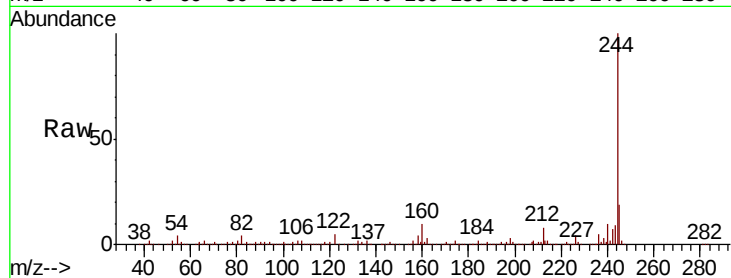


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

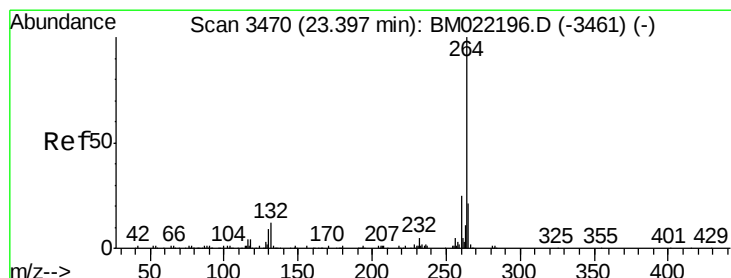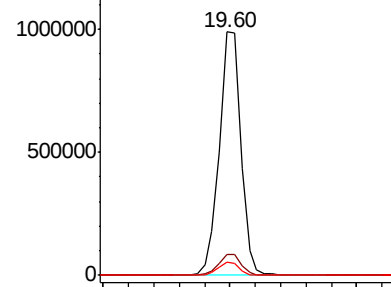

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.36 min Scan# 3464
 Delta R.T. -0.00 min
 Lab File: BM022436.D
 Acq: 30 Aug 2019 11:32

Tgt Ion:264 Resp: 196486

Ion	Ratio	Lower	Upper
264	100		
260	25.7	20.2	30.2
265	21.8	18.2	27.2

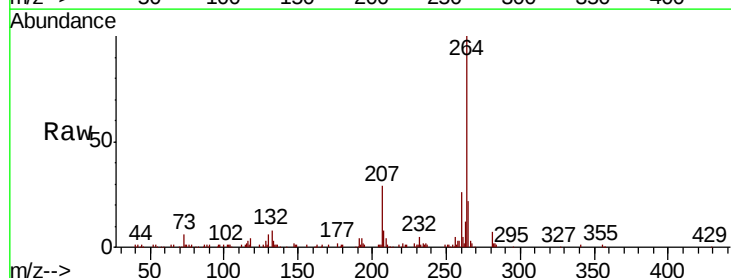

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

