

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083019\
 Data File : BM022438.D
 Acq On : 30 Aug 2019 12:45
 Operator : HP/JU
 Sample : PB122644BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 30 14:27:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 29 16:51:32 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	21808	20.00	ng	0.00
21) Naphthalene-d8	10.30	136	77184	20.00	ng	0.00
39) Acenaphthene-d10	14.19	164	51614	20.00	ng	0.00
64) Phenanthrene-d10	16.96	188	124770	20.00	ng	0.00
76) Chrysene-d12	21.17	240	156051	20.00	ng	0.00
87) Perylene-d12	23.37	264	163692	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.15	112	286631	230.71	ng	0.00
7) Phenol-d6	6.73	99	381248	229.47	ng	0.00
23) Nitrobenzene-d5	8.70	82	253811	144.03	ng	0.00
42) 2,4,6-Tribromophenol	15.70	330	358265	339.21	ng	0.00
45) 2-Fluorobiphenyl	12.79	172	746623	163.87	ng	0.00
79) Terphenyl-d14	19.60	244	2917664	246.75	ng	0.00
Target Compounds						
15) Benzyl Alcohol	7.83	79	5033	3.193	ng	Qvalue # 38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083019\
Data File : BM022438.D
Acq On : 30 Aug 2019 12:45
Operator : HP/JU
Sample : PB122644BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 30 14:27:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 29 16:51:32 2019
Response via : Initial Calibration

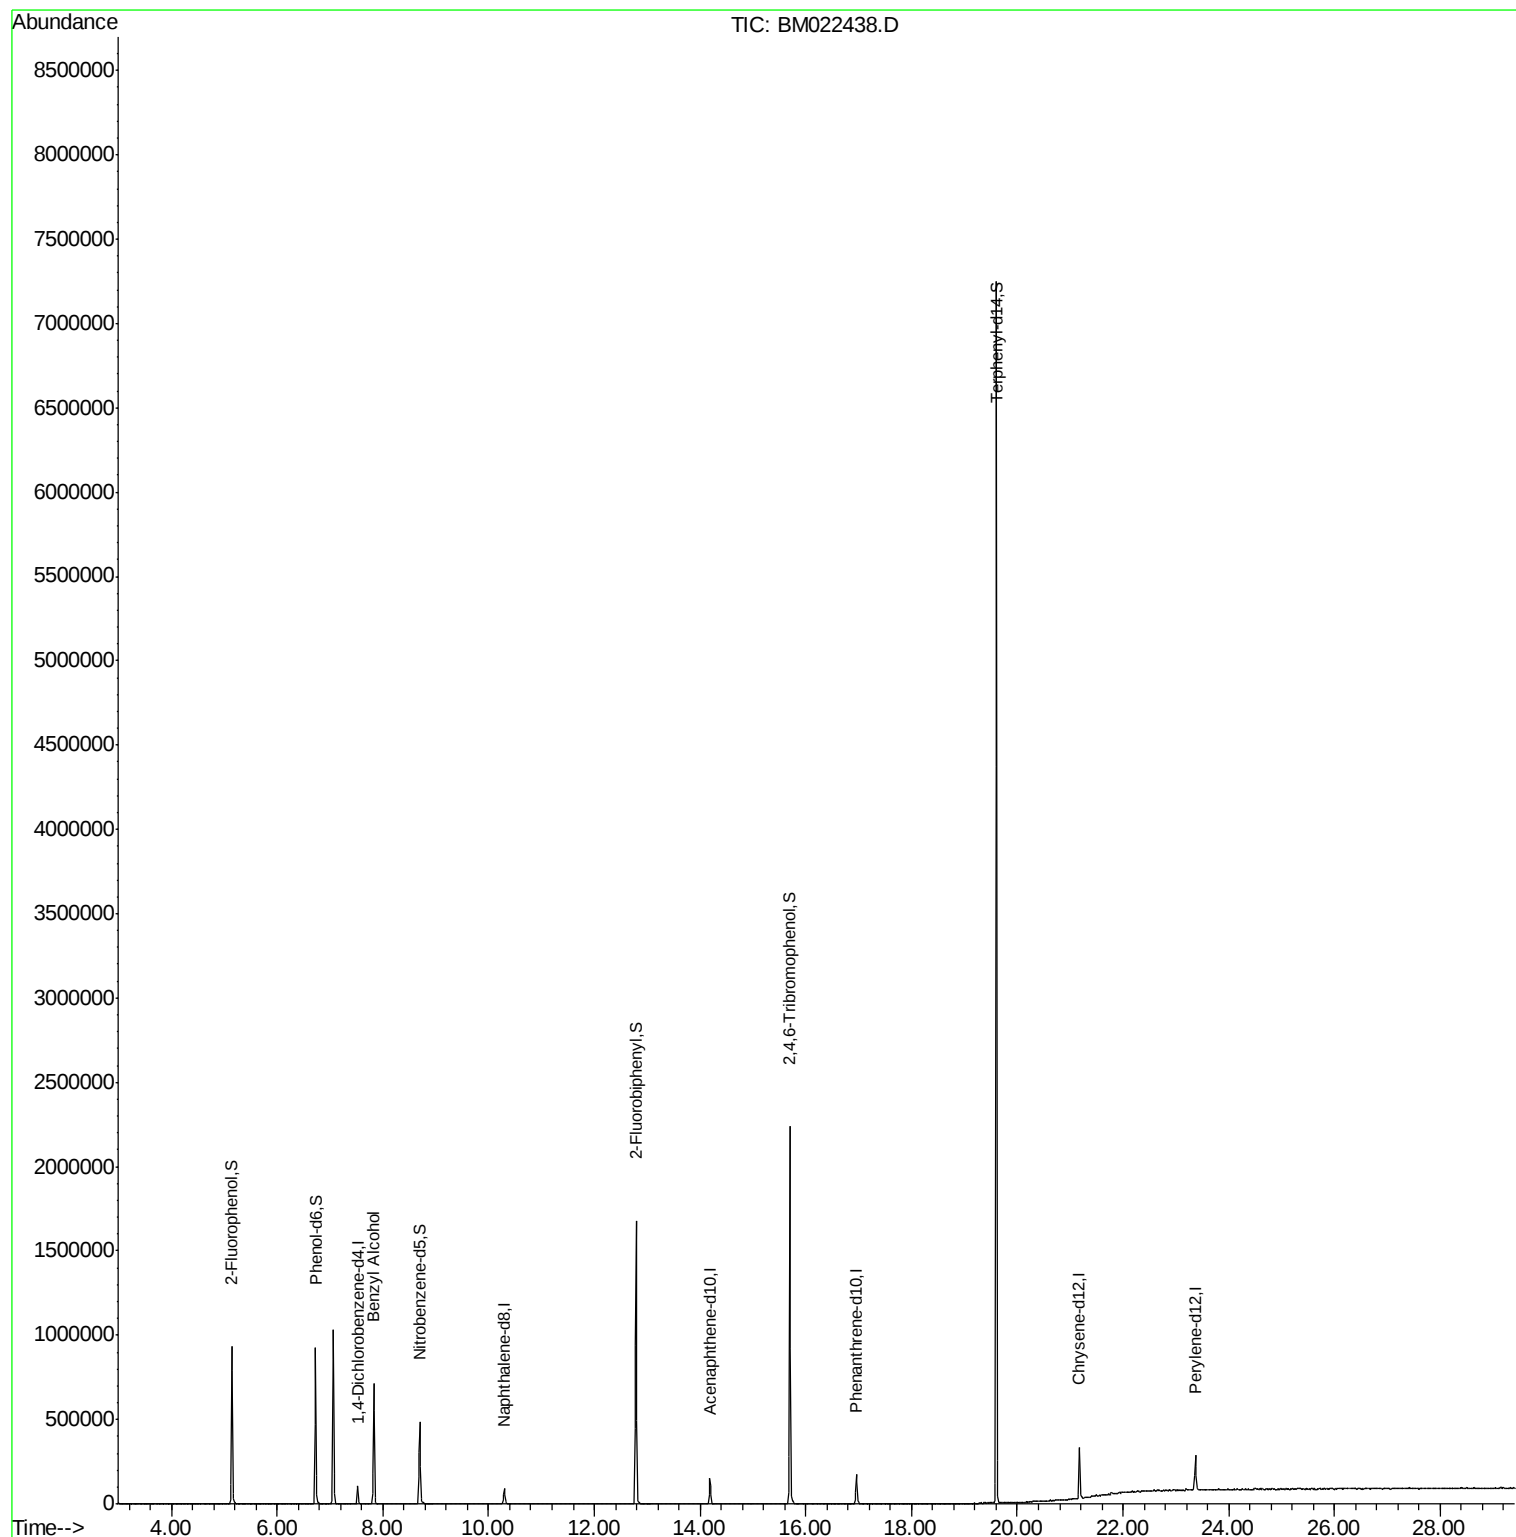







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.52 min Scan# 771
 Delta R.T. -0.01 min
 Lab File: BM022438.D
 Acq: 30 Aug 2019 12:45

Instrument :
 BNA_M
 ClientSampled :

Tot Ion:152 Resp: 21808
 Ion Ratio Lower Upper
 152 100
 150 159.1 125.4 188.0
 115 67.5 50.3 75.5

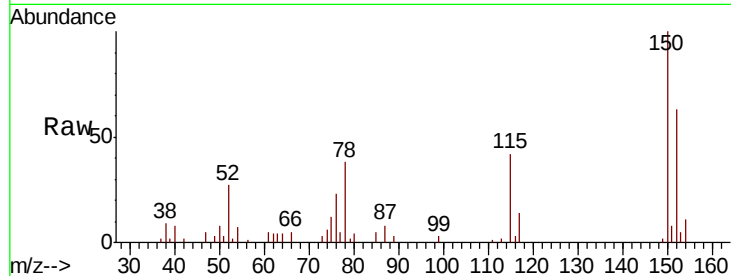


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

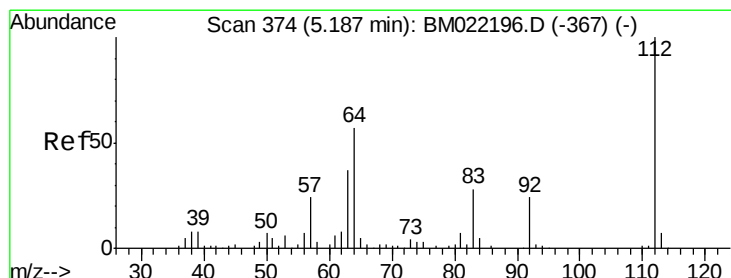
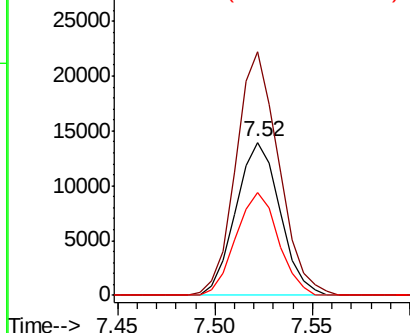



#5
 2-Fluorophenol
 Concen: 230.710 ng
 RT: 5.15 min Scan# 367
 Delta R.T. -0.00 min
 Lab File: BM022438.D
 Acq: 30 Aug 2019 12:45

Tgt Ion:112 Resp: 286631
 Ion Ratio Lower Upper
 112 100
 64 58.9 45.4 68.2
 63 42.7 34.5 51.7

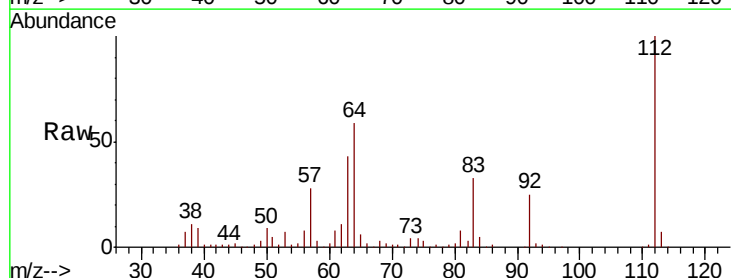

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BM0
 Ion 63.00 (62.70 to 63.70): BM0

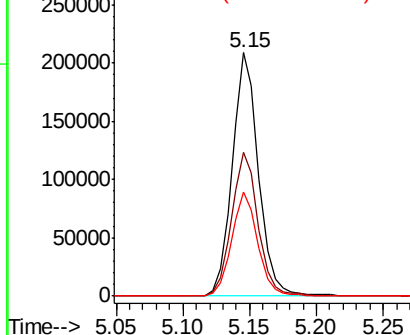

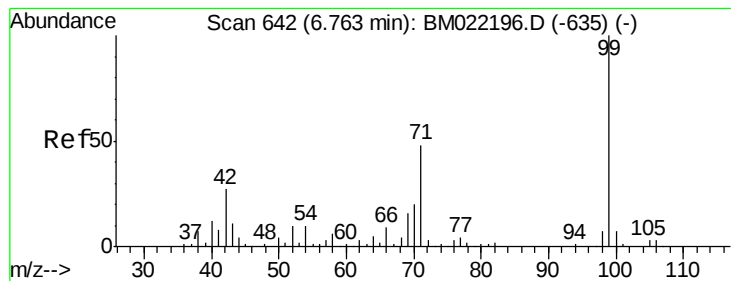

#7

Phenol-d6

Concen: 229.474 ng

RT: 6.73 min Scan# 636

Delta R.T. 0.01 min

Lab File: BM022438.D

Acq: 30 Aug 2019 12:45

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 99 Resp: 381248

Ion Ratio Lower Upper

99 100

42 31.0 26.3 39.5

71 56.8 46.6 69.8



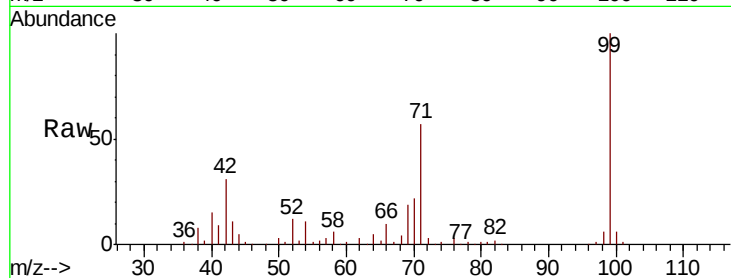


Abundance Ion 99.00 (98.70 to 99.70): BM022196.D (-635) (-)

Ion 42.00 (41.70 to 42.70): BM022196.D (-635) (-)

Ion 71.00 (70.70 to 71.70): BM022196.D (-635) (-)

Time-->

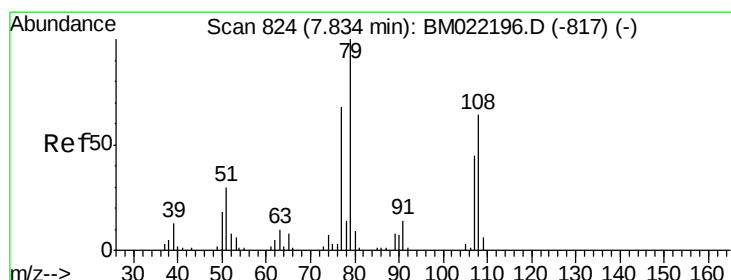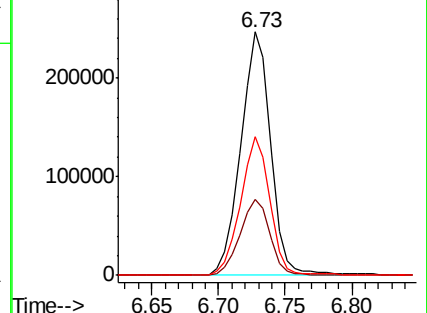

#15

Benzyl Alcohol

Concen: 3.193 ng

RT: 7.83 min Scan# 823

Delta R.T. 0.03 min

Lab File: BM022438.D

Acq: 30 Aug 2019 12:45


Tgt Ion: 79 Resp: 5033

Ion Ratio Lower Upper

79 100

108 78.0 48.2 72.4#

77 149.4 56.6 85.0#


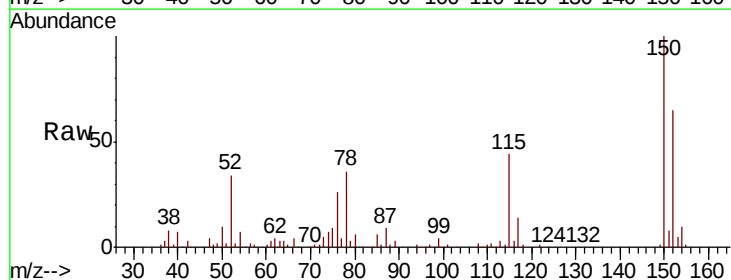



Abundance Ion 79.00 (78.70 to 79.70): BM022196.D (-817) (-)

Ion 108.00 (107.70 to 108.70): BM022196.D (-817) (-)

Ion 77.00 (76.70 to 77.70): BM022196.D (-817) (-)

Time-->

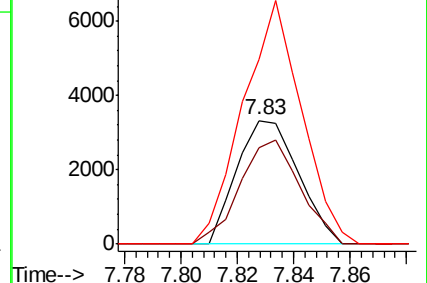

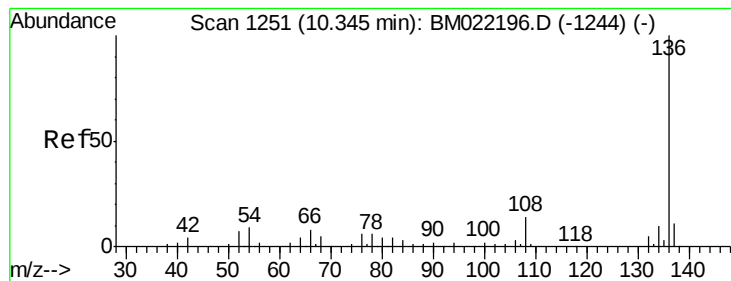

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.30 min Scan# 1243

Delta R.T. -0.00 min

Lab File: BM022438.D

Acq: 30 Aug 2019 12:45

Instrument :

BNA_M

ClientSampleId :

Tot Ion:136 Resp: 77184





Ion Ratio Lower Upper

136 100

137 11.0 8.6 13.0

54 7.3 7.0 10.6

68 4.7 2.9 4.3#

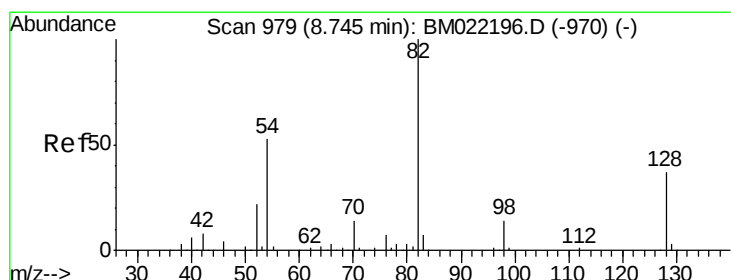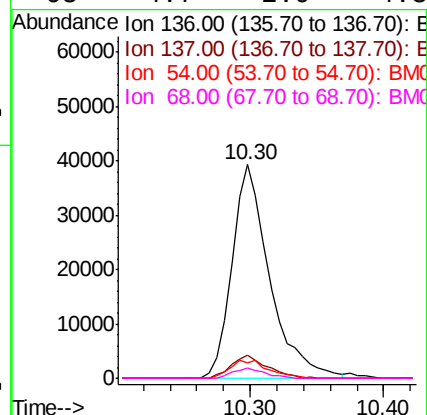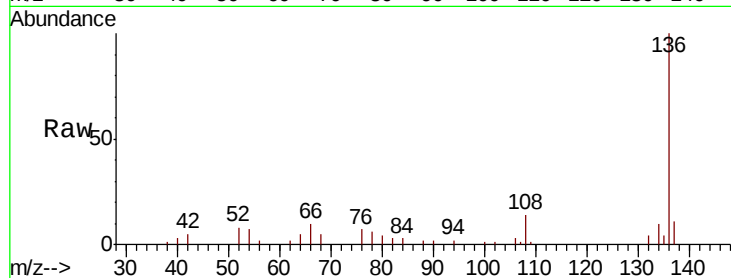

#23

Nitrobenzene-d5

Concen: 144.033 ng

RT: 8.70 min Scan# 971

Delta R.T. -0.00 min

Lab File: BM022438.D

Acq: 30 Aug 2019 12:45




Tgt Ion: 82 Resp: 253811


Ion Ratio Lower Upper

82 100

128 36.2 27.9 41.9

54 56.1 45.2 67.8

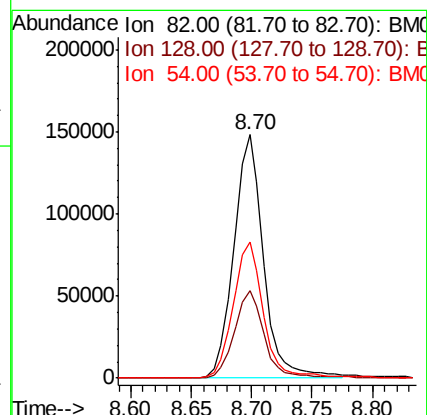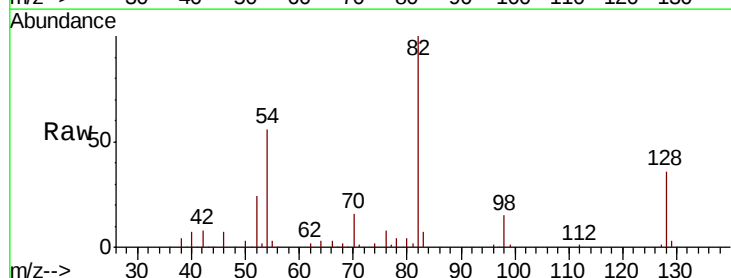







#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.19 min Scan# 1904
 Delta R.T. -0.00 min
 Lab File: BM022438.D
 Acq: 30 Aug 2019 12:45

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:164 Resp: 51614
 Ion Ratio Lower Upper
 164 100
 162 111.0 80.6 121.0
 160 50.3 37.3 55.9

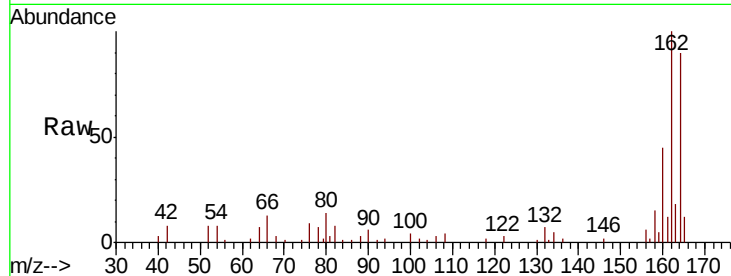


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

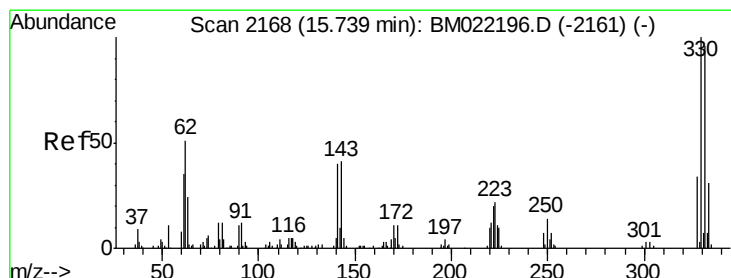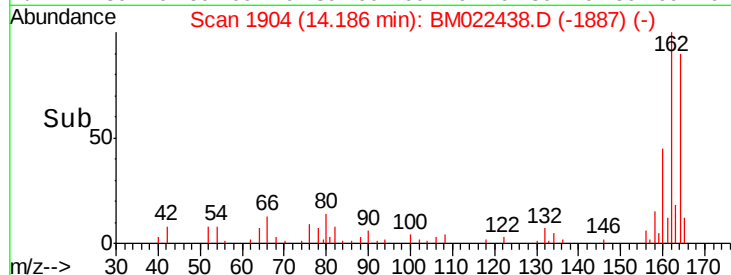
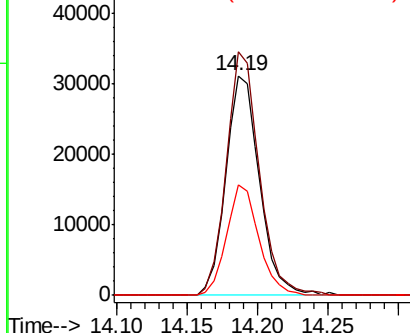



#42
 2,4,6-Tribromophenol
 Concen: 339.213 ng
 RT: 15.70 min Scan# 2161
 Delta R.T. -0.00 min
 Lab File: BM022438.D
 Acq: 30 Aug 2019 12:45

Tgt Ion:330 Resp: 358265
 Ion Ratio Lower Upper
 330 100
 332 96.6 77.8 116.8
 141 38.5 35.6 53.4

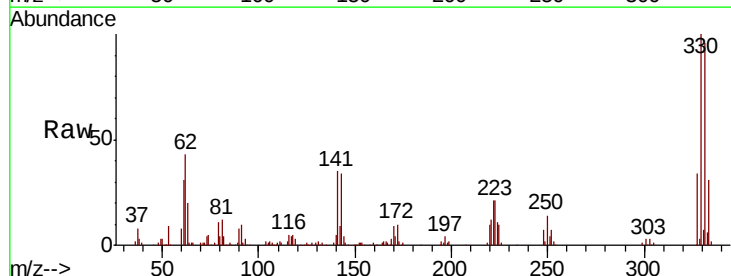

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E




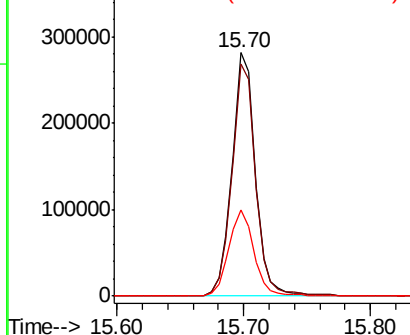


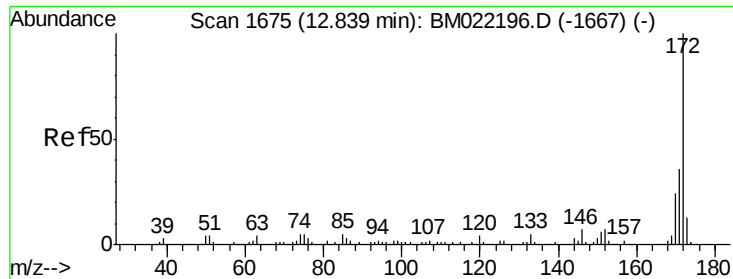

#45
 2-Fluorobiphenyl
 Concen: 163.872 ng
 RT: 12.79 min Scan# 1667
 Delta R.T. -0.00 min
 Lab File: BM022438.D
 Acq: 30 Aug 2019 12:45




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion:172 Resp: 746623
 Ion Ratio Lower Upper
 172 100
 171 35.3 28.5 42.7
 170 24.2 18.9 28.3

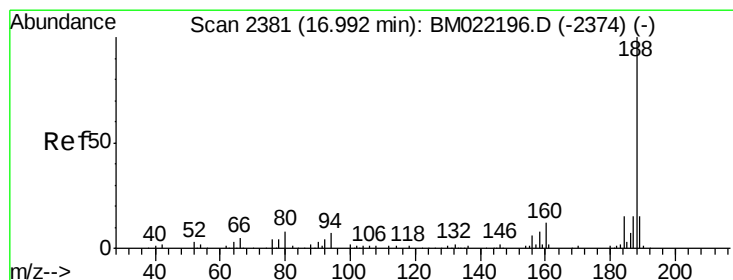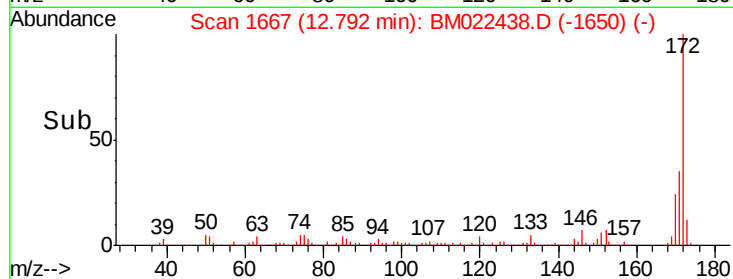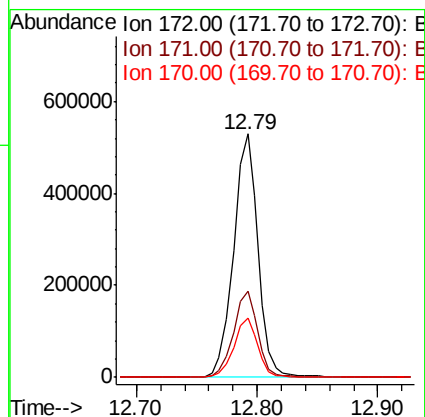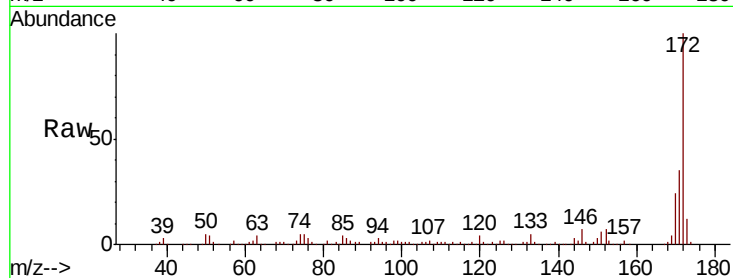

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 16.96 min Scan# 2375
 Delta R.T. 0.01 min
 Lab File: BM022438.D
 Acq: 30 Aug 2019 12:45

Tgt Ion:188 Resp: 124770
 Ion Ratio Lower Upper
 188 100
 94 5.7 4.4 6.6
 80 6.9 5.0 7.6


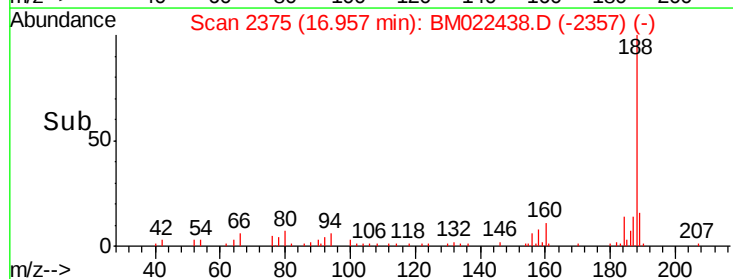
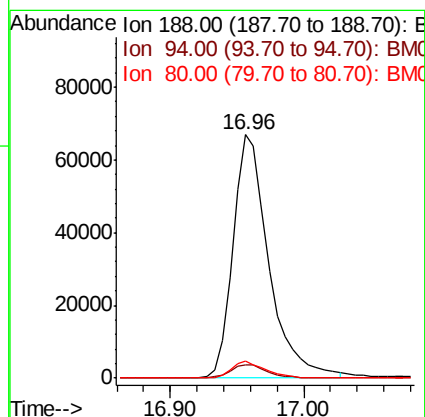
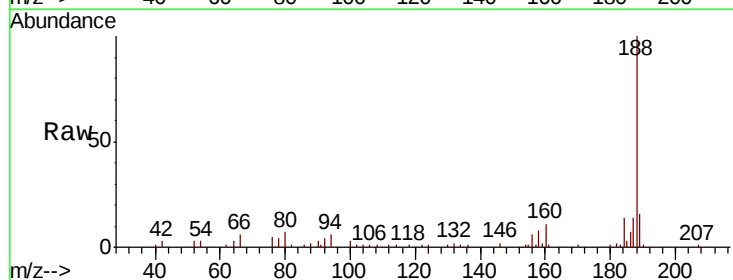


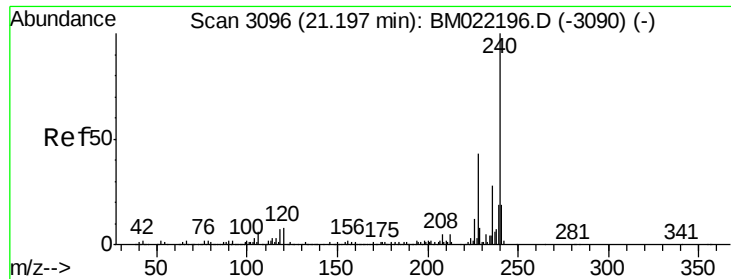

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.17 min Scan# 3092
Delta R.T. -0.00 min
Lab File: BM022438.D
Acq: 30 Aug 2019 12:45




Instrument :
BNA_M
ClientSampled :


Tot Ion:240 Resp: 156051
Ion Ratio Lower Upper
240 100
120 5.5 3.9 5.9
236 28.4 21.4 32.2

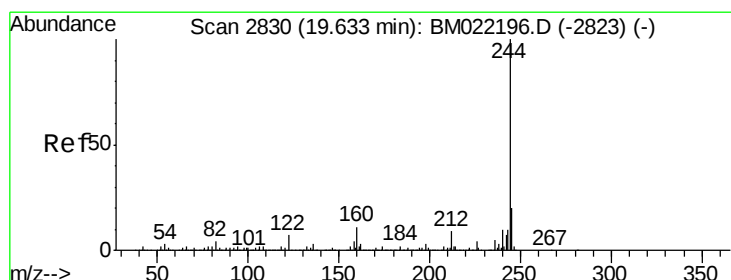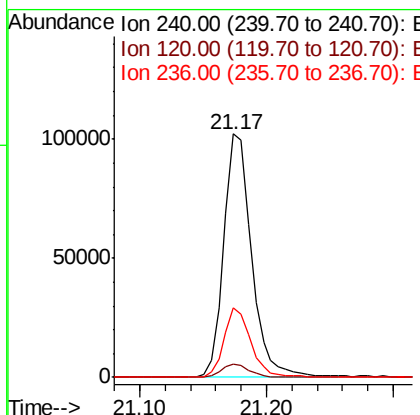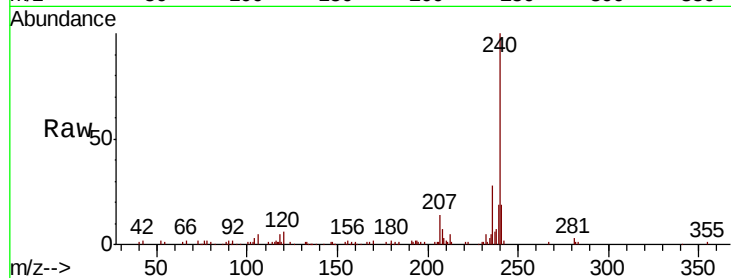

#79
Terphenyl-d14
Concen: 246.752 ng
RT: 19.60 min Scan# 2825
Delta R.T. -0.00 min
Lab File: BM022438.D
Acq: 30 Aug 2019 12:45

Tgt Ion:244 Resp: 2917664
Ion Ratio Lower Upper
244 100
212 7.8 7.0 10.4
122 4.7 3.9 5.9

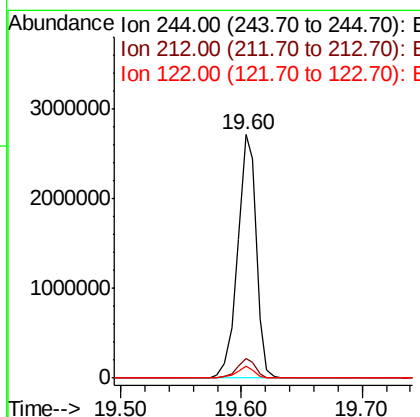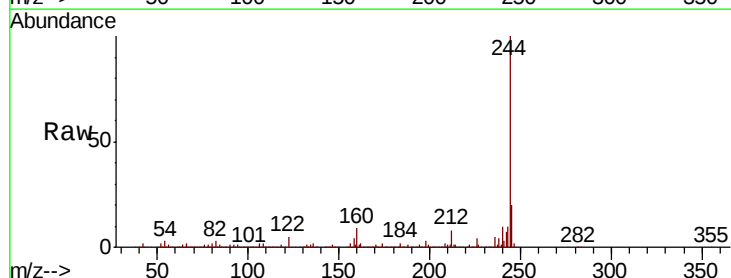


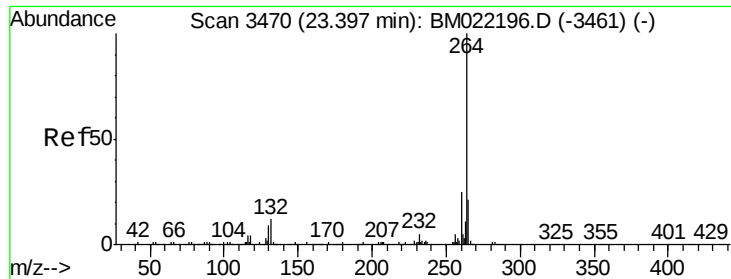

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 23.37 min Scan# 3465
 Delta R.T. 0.01 min
 Lab File: BM022438.D
 Acq: 30 Aug 2019 12:45

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:	264	Resp:	163692
Ion	Ratio	Lower	Upper
264	100		
260	24.6	20.2	30.2
265	22.4	18.2	27.2

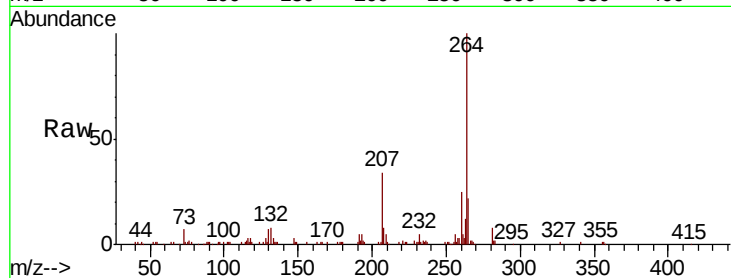

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

