

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083019\
 Data File : BM022439.D
 Acq On : 30 Aug 2019 13:21
 Operator : HP/JU
 Sample : PB122653BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB122653BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.145	361	367	382	rBV	500497	722553	22.60%	6.639%
2	6.722	629	635	646	rBV	497276	790989	24.74%	7.267%
3	7.063	686	693	704	rBV	539212	849780	26.58%	7.808%
4	7.522	766	771	778	rBB	89378	136182	4.26%	1.251%
5	7.834	817	824	833	rBB	418313	635748	19.88%	5.841%
6	8.698	964	971	990	rBV	250325	470090	14.70%	4.319%
7	10.298	1237	1243	1259	rBB	81477	160689	5.03%	1.476%
8	12.792	1660	1667	1685	rBV	763580	1215247	38.00%	11.165%
9	14.186	1899	1904	1915	rBB	137820	231348	7.23%	2.126%
10	15.698	2155	2161	2183	rBB	827676	1255129	39.25%	11.532%
11	16.956	2370	2375	2389	rBV2	170401	302554	9.46%	2.780%
12	19.603	2819	2825	2834	rBV	2741556	3197656	100.00%	29.379%
13	21.174	3087	3092	3102	rBV	335375	472347	14.77%	4.340%
14	23.362	3459	3464	3476	rVB	218997	443732	13.88%	4.077%


Sum of corrected areas: 10884044

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083019\
Data File : BM022439.D
Acq On : 30 Aug 2019 13:21
Operator : HP/JU
Sample : PB122653BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB122653BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

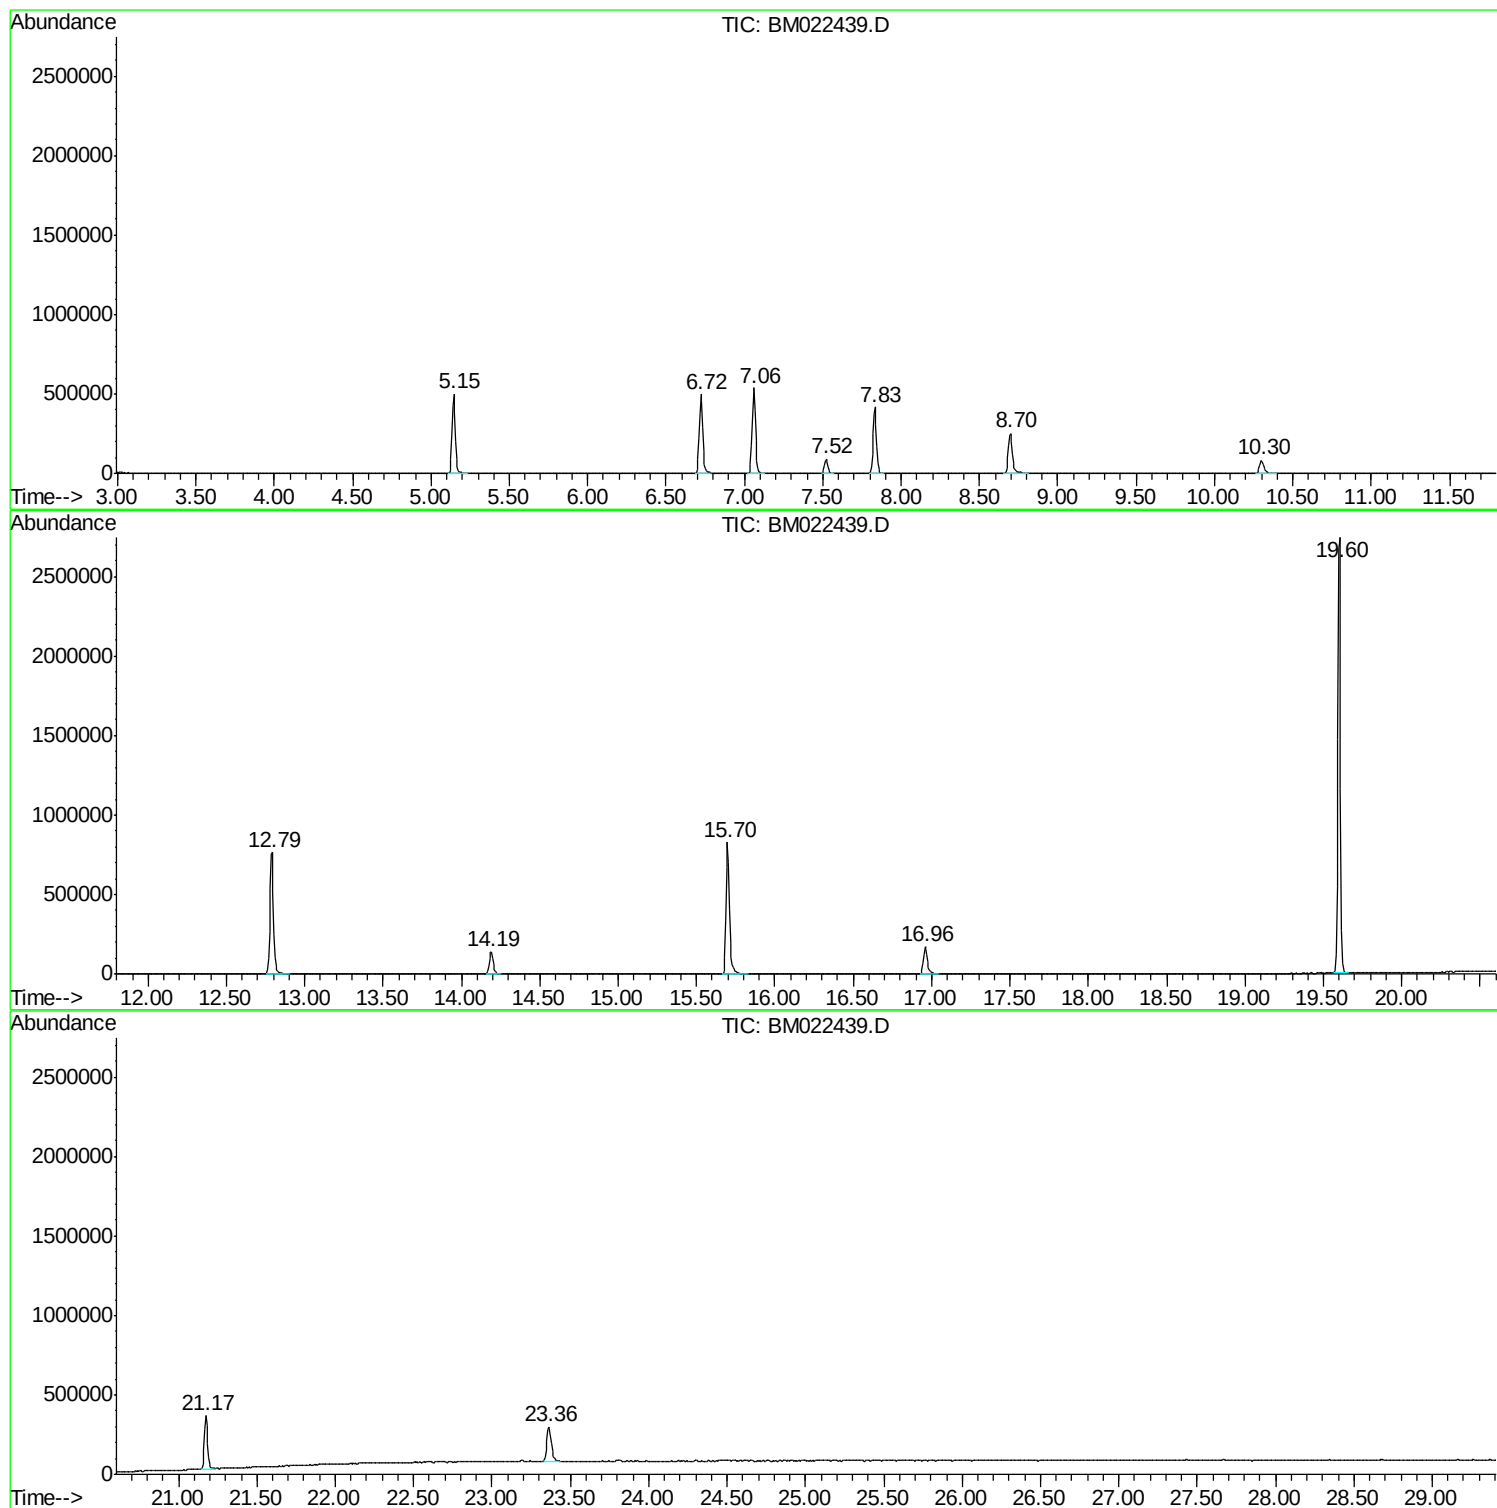

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083019\
Data File : BM022439.D
Acq On : 30 Aug 2019 13:21
Operator : HP/JU
Sample : PB122653BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB122653BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.06 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.06	124.80 ng	849780	1,4-Dichlorobenzene-d4	7.52

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	14
2		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	14
3		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
4		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	12
5		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	10

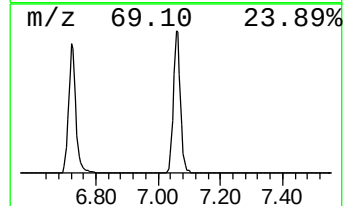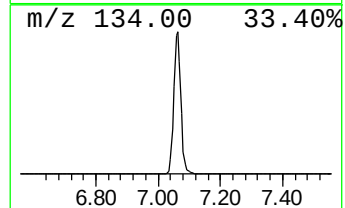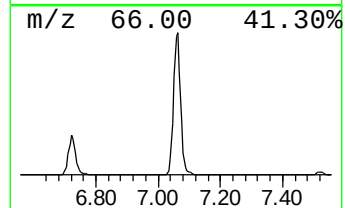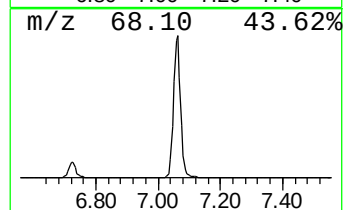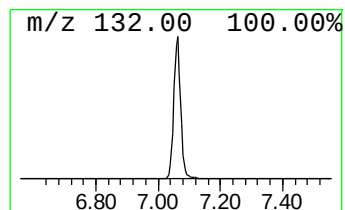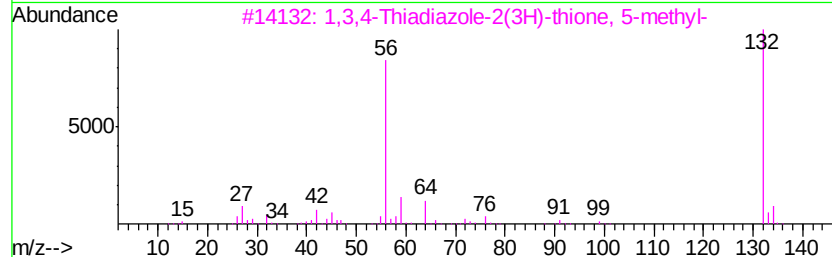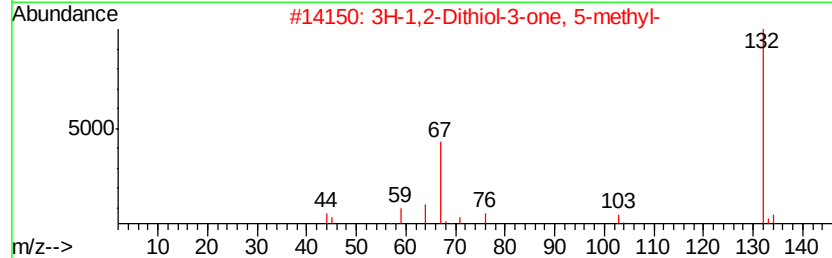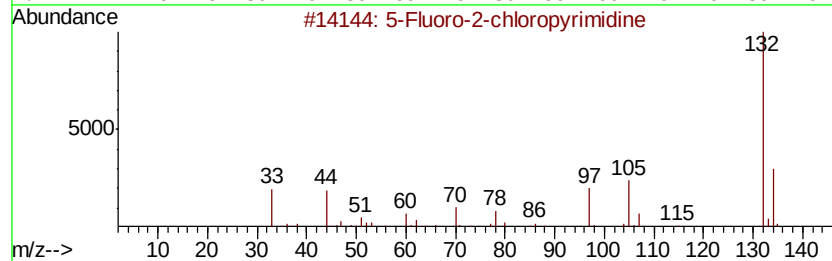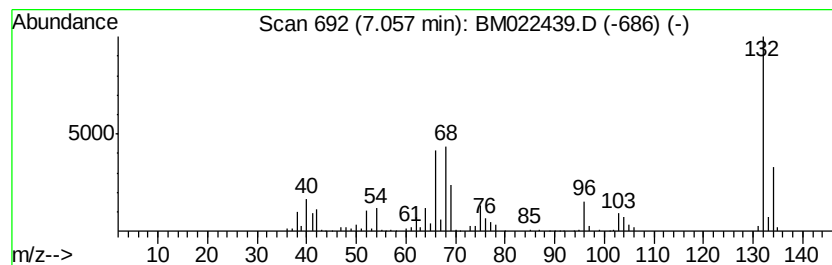

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM083019\
Data File : BM022439.D
Acq On : 30 Aug 2019 13:21
Operator : HP/JU
Sample : PB122653BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB122653BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.06	7.06	124.8	ng	849780	1	7.52	136182	20.0