

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083019\
Data File : BM022454.D
Acq On : 30 Aug 2019 23:10
Operator : HP/JU
Sample : K4562-03 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-02-20-22

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.145	363	367	373	rBV	18039	26556	4.98%	1.369%
2	6.734	633	637	645	rBV3	11091	22793	4.28%	1.175%
3	7.063	688	693	702	rBB3	19149	30606	5.74%	1.578%
4	7.516	765	770	778	rBV	83550	122333	22.95%	6.306%
5	7.828	819	823	830	rBB2	14897	23528	4.41%	1.213%
6	8.710	969	973	979	rBV	6476	11715	2.20%	0.604%
7	10.292	1236	1242	1257	rBV	76607	144323	27.08%	7.440%
8	12.792	1663	1667	1680	rBB	14253	23344	4.38%	1.203%
9	14.180	1898	1903	1916	rBB2	120050	188173	35.30%	9.700%
10	15.709	2158	2163	2170	rBB	14734	22698	4.26%	1.170%
11	16.951	2369	2374	2386	rBV2	147060	235579	44.20%	12.144%
12	17.845	2521	2526	2533	rBV3	5987	10321	1.94%	0.532%
13	19.597	2820	2824	2830	rVB	62972	75249	14.12%	3.879%
14	21.168	3086	3091	3097	rBV	347951	469706	88.12%	24.212%
15	23.362	3457	3464	3470	rBV	279481	533015	100.00%	27.476%


Sum of corrected areas: 1939939

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083019\
Data File : BM022454.D
Acq On : 30 Aug 2019 23:10
Operator : HP/JU
Sample : K4562-03 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-02-20-22

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

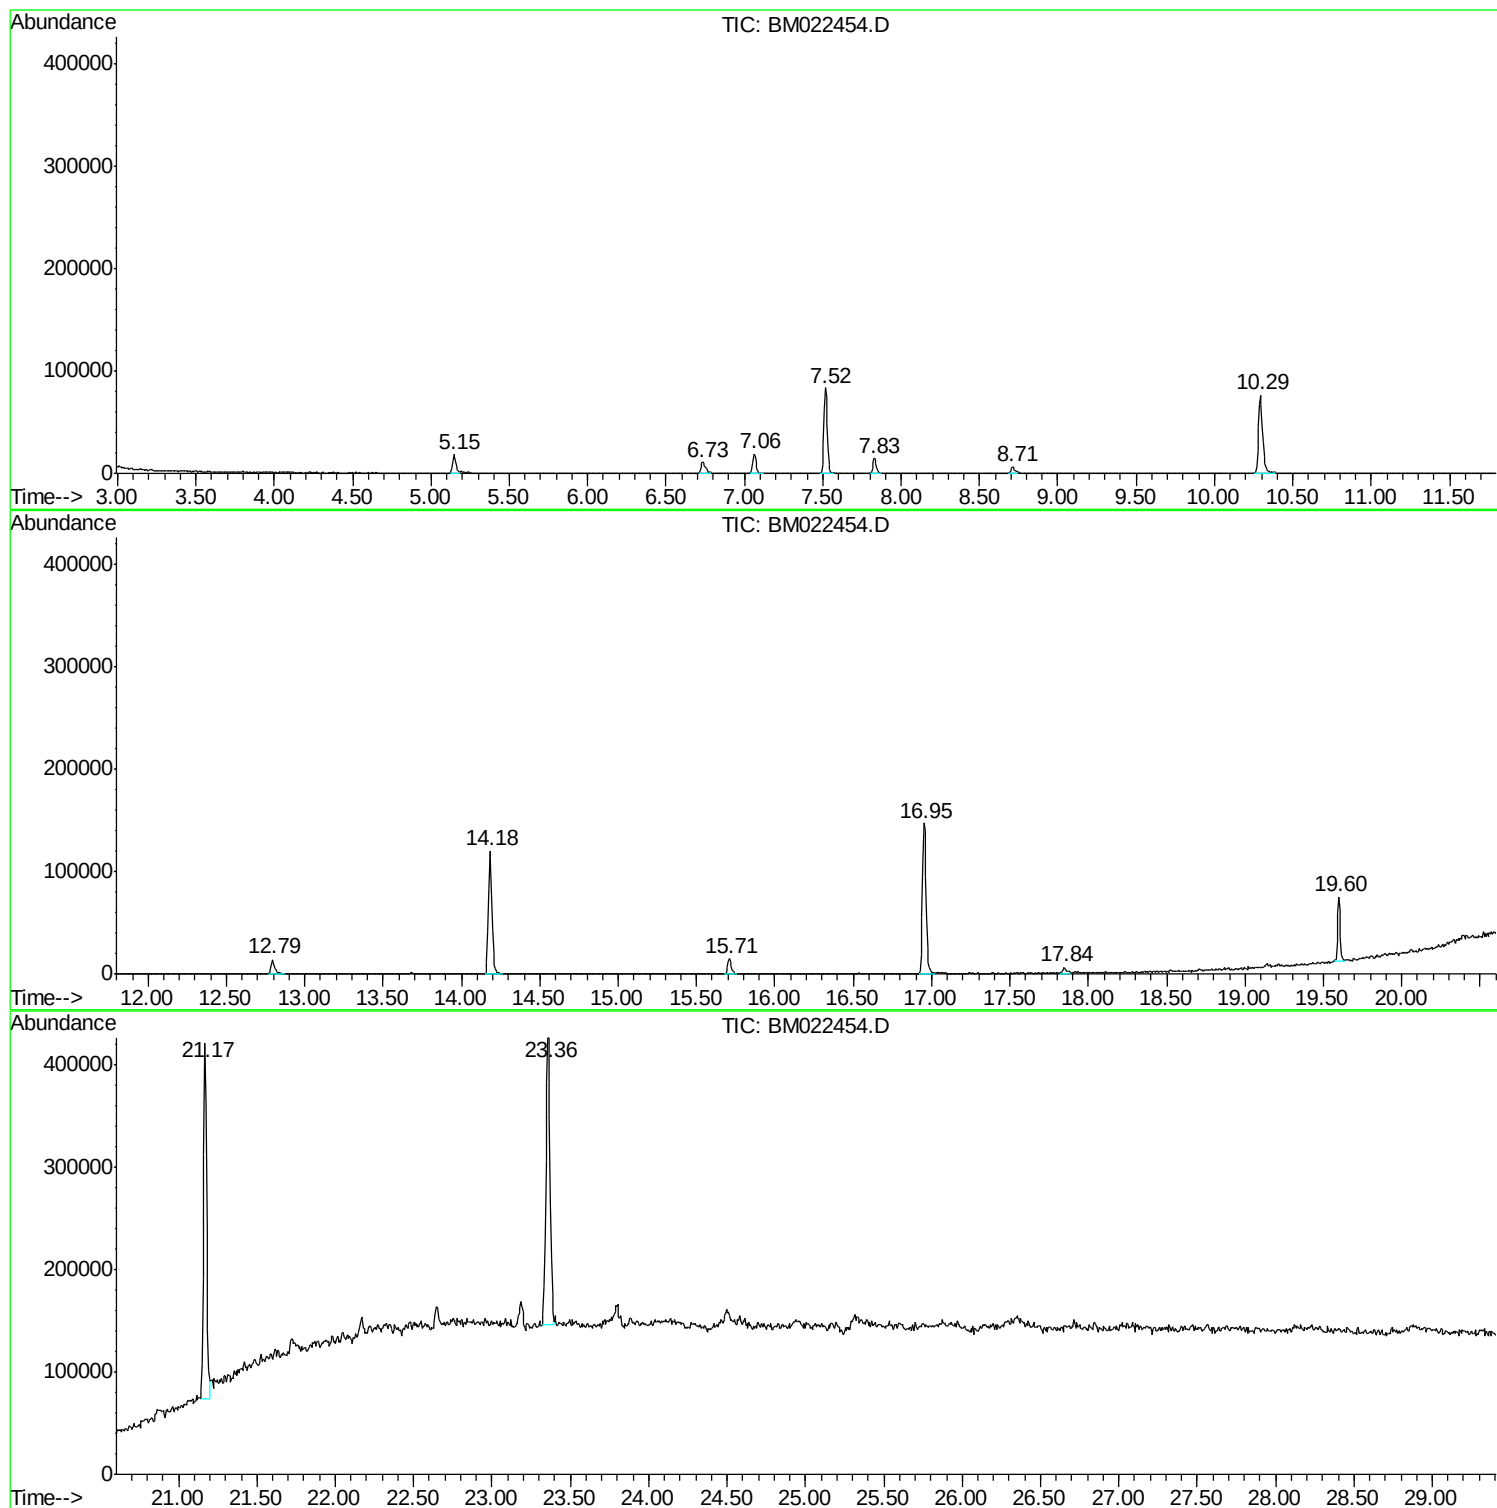

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083019\
Data File : BM022454.D
Acq On : 30 Aug 2019 23:10
Operator : HP/JU
Sample : K4562-03 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-02-20-22










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.06 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.06	5.00 ng	30606	1,4-Dichlorobenzene-d4	7.52

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	22
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	18
3		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	14
4		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	12
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	10

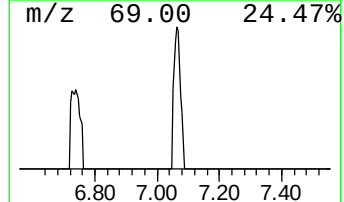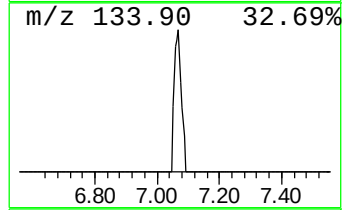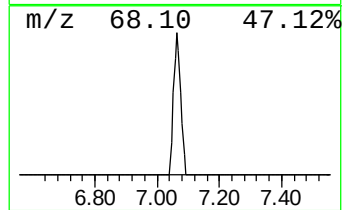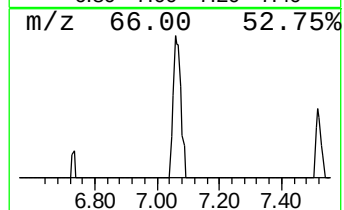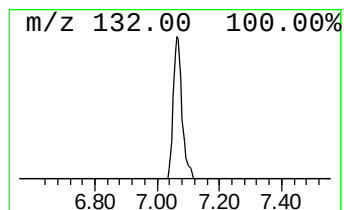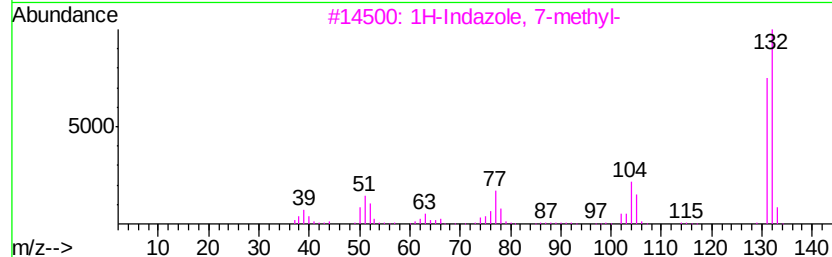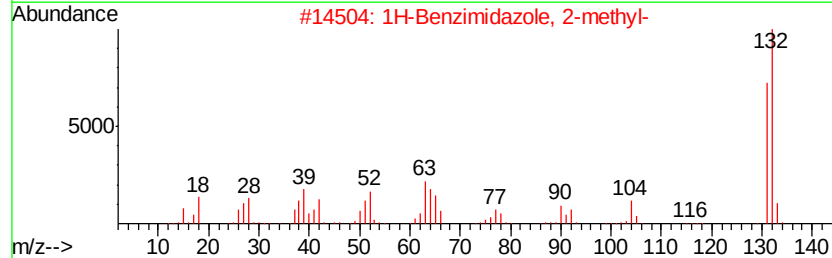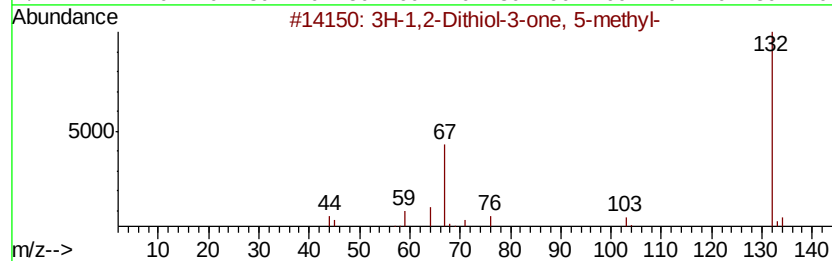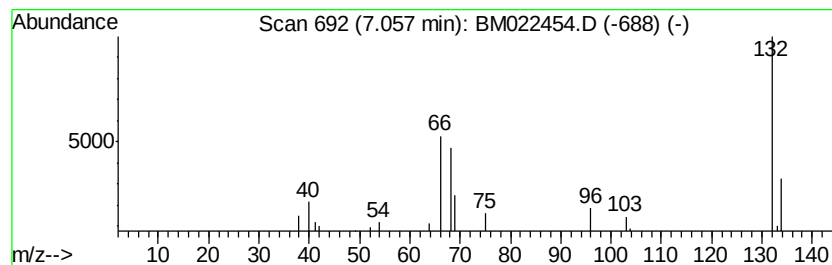

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM083019\
Data File : BM022454.D
Acq On : 30 Aug 2019 23:10
Operator : HP/JU
Sample : K4562-03 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-02-20-22

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.06	7.06	5.0	ng	30606	1	7.52	122333	20.0