


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083019\
 Data File : BM022431.D
 Acq On : 30 Aug 2019 07:55
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 29 16:51:32 2019

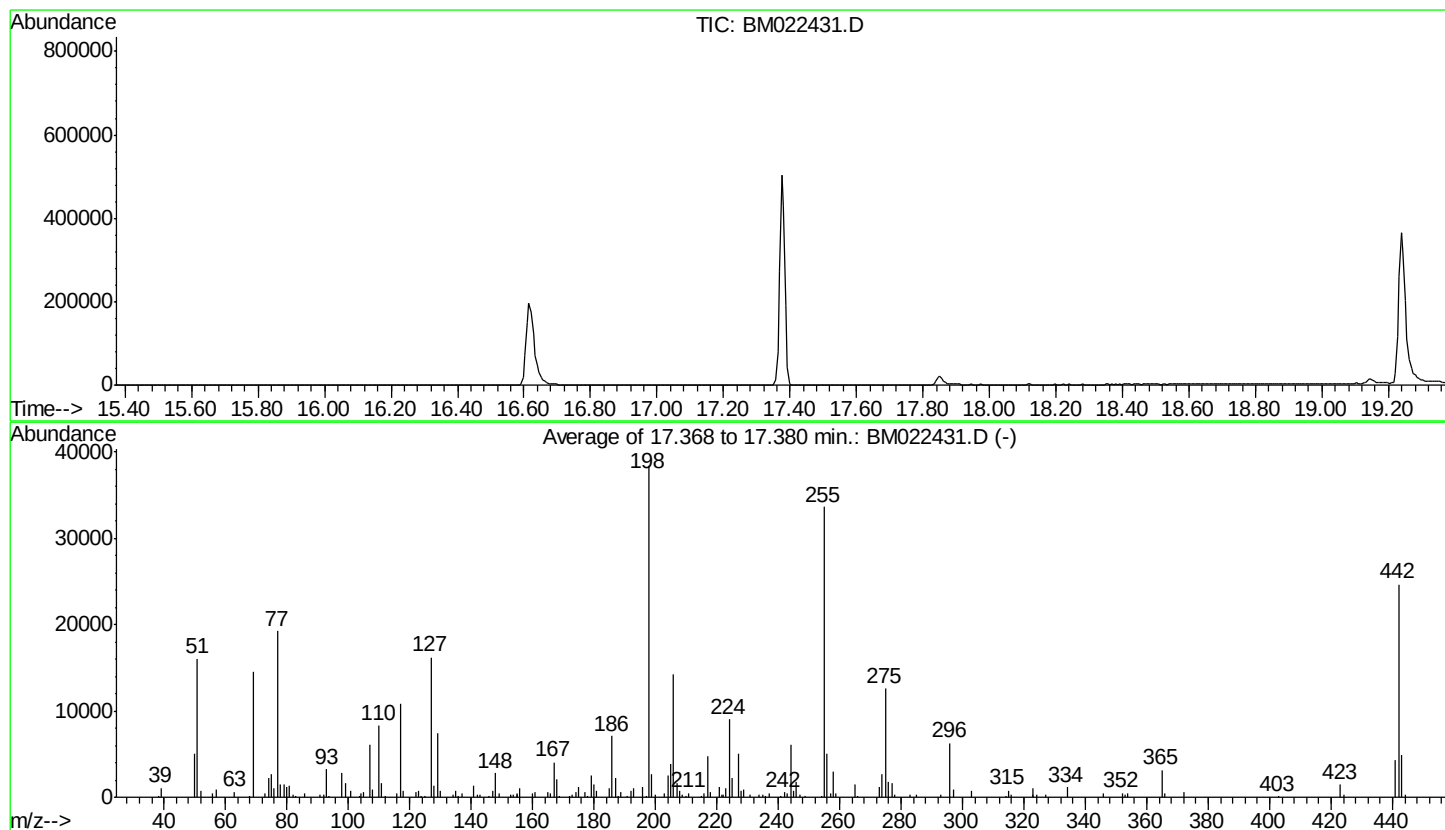

AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	16016	PASS
68	69	0.00	2	0.8	123	PASS
69	198	0.00	100	37.8	14510	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.1	16181	PASS
197	198	0.00	2	0.3	133	PASS
198	198	100	100	100.0	38397	PASS
199	198	5	9	6.9	2667	PASS
275	198	10	60	32.6	12530	PASS
365	198	1	100	8.1	3126	PASS
441	198	0.01	100	11.2	4289	PASS
442	198	50	100	64.1	24624	PASS
443	442	15	24	19.7	4863	PASS