


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM083019\
 Data File : BM022443.D
 Acq On : 30 Aug 2019 15:49
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 29 16:51:32 2019

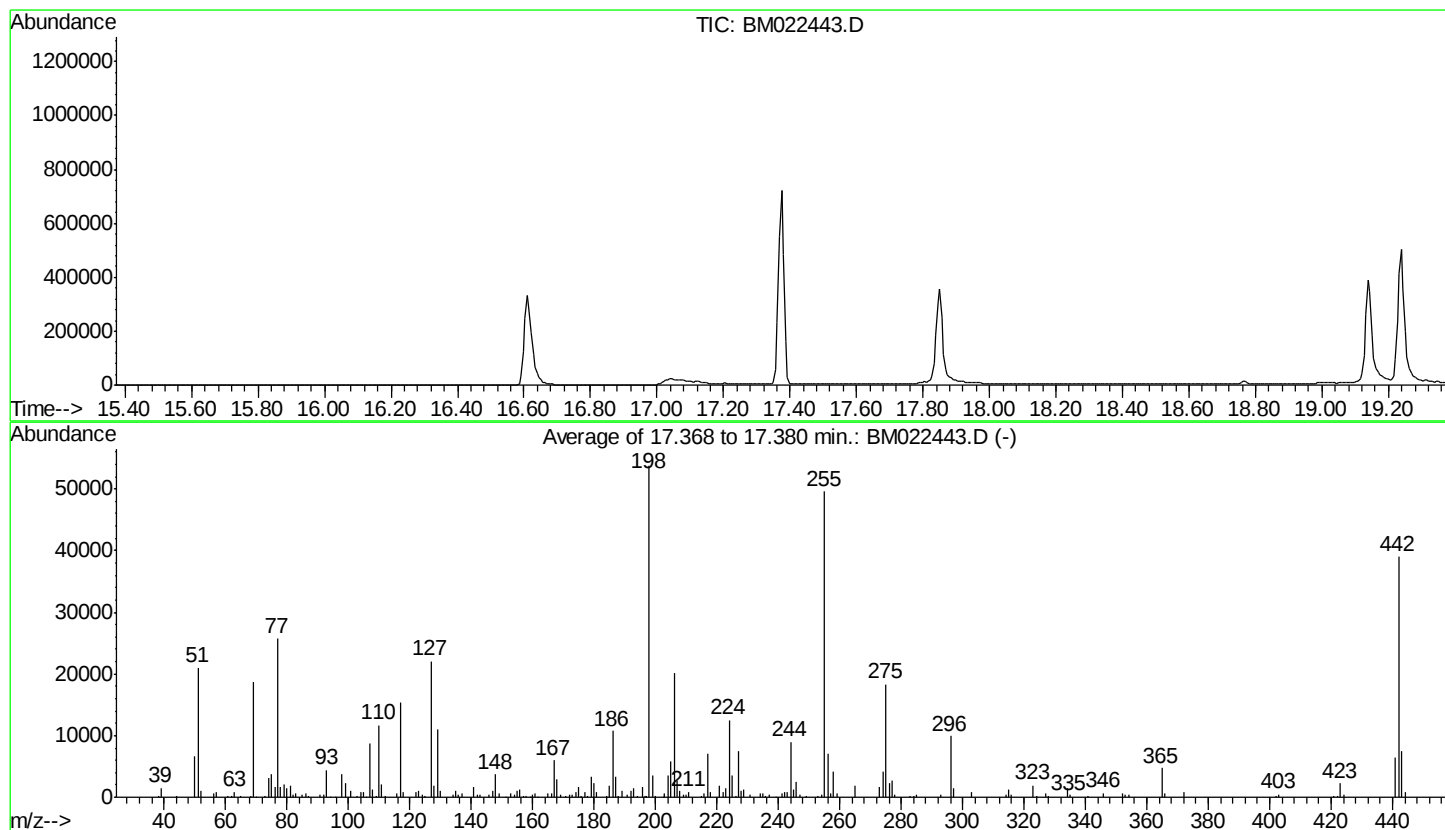

AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	20996	PASS
68	69	0.00	2	1.4	252	PASS
69	198	0.00	100	34.7	18655	PASS
70	69	0.00	2	0.6	104	PASS
127	198	10	80	41.1	22114	PASS
197	198	0.00	2	0.3	153	PASS
198	198	100	100	100.0	53786	PASS
199	198	5	9	6.5	3499	PASS
275	198	10	60	34.0	18308	PASS
365	198	1	100	8.8	4709	PASS
441	198	0.01	100	12.1	6522	PASS
442	198	50	100	72.5	39010	PASS
443	442	15	24	19.1	7460	PASS