

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083122\
 Data File : BM036467.D
 Acq On : 31 Aug 2022 11:06
 Operator : CG/JU
 Sample : PB147325BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	33	rVB	53847	77011	1.56%	0.142%
2	3.557	94	97	122	rBV	631993	1084936	21.92%	1.994%
3	3.875	147	151	162	rVB	15789	29014	0.59%	0.053%
4	6.904	660	666	679	rBV	881196	1413234	28.55%	2.597%
5	7.069	687	694	708	rVB	794092	1209563	24.44%	2.223%
6	7.257	719	726	738	rBV	903605	1401884	28.32%	2.576%
7	7.728	798	806	824	rBV	819672	1290600	26.08%	2.372%
8	8.451	922	929	944	rBV	974687	1581398	31.95%	2.906%
9	8.898	998	1005	1021	rBV	827717	1303944	26.35%	2.396%
10	9.616	1120	1127	1143	rBV	628457	1049394	21.20%	1.929%
11	10.157	1211	1219	1245	rBV	888297	1576077	31.84%	2.897%
12	10.528	1274	1282	1296	rBV	1134988	1837534	37.13%	3.377%
13	10.675	1300	1307	1333	rBV	817973	1555913	31.44%	2.860%
14	12.139	1551	1556	1567	rBV2	12885	28039	0.57%	0.052%
15	12.722	1651	1655	1659	rBV6	3816	7215	0.15%	0.013%
16	13.804	1832	1839	1852	rBV	1917637	2551741	51.56%	4.690%
17	14.074	1877	1885	1899	rBV	2231053	3092401	62.48%	5.683%
18	14.192	1903	1905	1910	rVB4	3296	4957	0.10%	0.009%
19	14.380	1930	1937	1949	rBV	1868147	2585452	52.24%	4.752%
20	14.604	1969	1975	1999	rBV	700354	1250558	25.27%	2.298%
21	14.798	2005	2008	2014	rVB6	6229	10663	0.22%	0.020%
22	15.163	2064	2070	2072	rBV5	4458	5947	0.12%	0.011%
23	15.216	2075	2079	2083	rVB5	4382	7710	0.16%	0.014%
24	15.374	2097	2106	2117	rBV	2933583	3958670	79.98%	7.275%
25	15.510	2123	2129	2143	rBV	766659	1147360	23.18%	2.109%
26	15.616	2143	2147	2155	rVB5	16491	27890	0.56%	0.051%
27	15.786	2171	2176	2181	rVB5	3549	5611	0.11%	0.010%
28	16.092	2223	2228	2236	rBV4	11078	23913	0.48%	0.044%
29	16.145	2236	2237	2245	rVB8	3733	6099	0.12%	0.011%
30	16.263	2253	2257	2263	rBV8	4453	7548	0.15%	0.014%
31	16.433	2280	2286	2294	rBV6	7890	20107	0.41%	0.037%
32	16.498	2294	2297	2301	rVV3	3933	5757	0.12%	0.011%
33	16.551	2303	2306	2309	rBV3	5058	5564	0.11%	0.010%
34	16.592	2309	2313	2321	rVB3	11786	19731	0.40%	0.036%
35	16.668	2321	2326	2329	rBV6	4785	6925	0.14%	0.013%
36	16.886	2360	2363	2366	rBV	13022	17873	0.36%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083122\
 Data File : BM036467.D
 Acq On : 31 Aug 2022 11:06
 Operator : CG/JU
 Sample : PB147325BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK325

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

37	17.127	2397	2404	2412	rBV	2225976	2982414	60.26%	5.481%
38	17.221	2412	2420	2435	rVV	3091037	4355904	88.01%	8.005%
39	17.657	2491	2494	2499	rVB5	6773	11044	0.22%	0.020%
40	18.104	2567	2570	2574	rVB	6950	8301	0.17%	0.015%
41	18.609	2653	2656	2660	rBV6	6893	8296	0.17%	0.015%
42	19.086	2733	2737	2742	rBV2	31839	43062	0.87%	0.079%
43	19.156	2746	2749	2753	rBV	29484	38314	0.77%	0.070%
44	19.521	2805	2811	2823	rBV	3827369	4949453	100.00%	9.096%
45	20.527	2978	2982	2987	rBV	172319	207175	4.19%	0.381%
46	21.315	3111	3116	3128	rBV	2664391	3338242	67.45%	6.135%
47	23.456	3474	3480	3494	rVB2	2670118	4920653	99.42%	9.043%
48	23.609	3499	3506	3518	rVB2	1798318	3340414	67.49%	6.139%




Sum of corrected areas: 54411505

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083122\
Data File : BM036467.D
Acq On : 31 Aug 2022 11:06
Operator : CG/JU
Sample : PB147325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

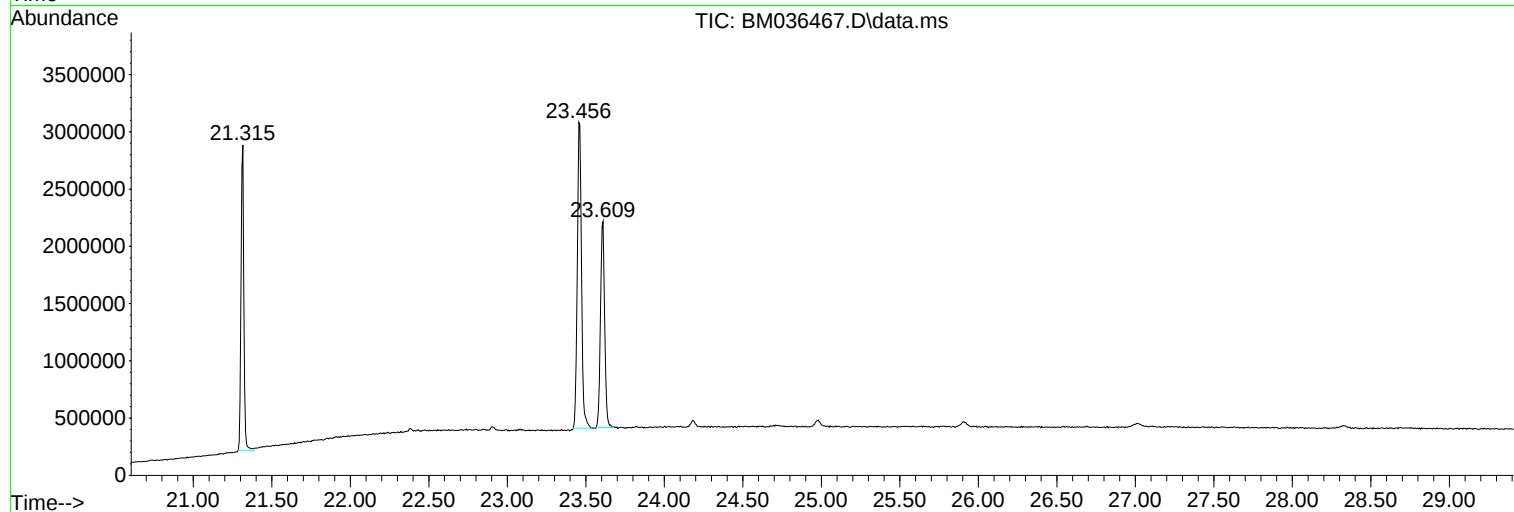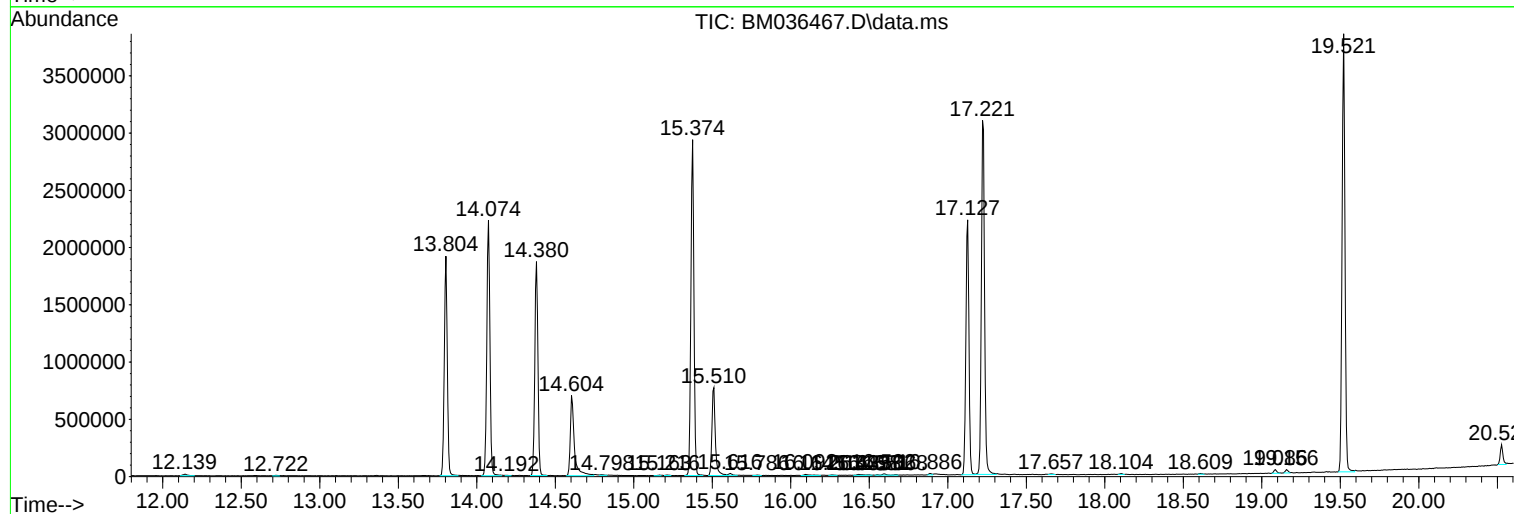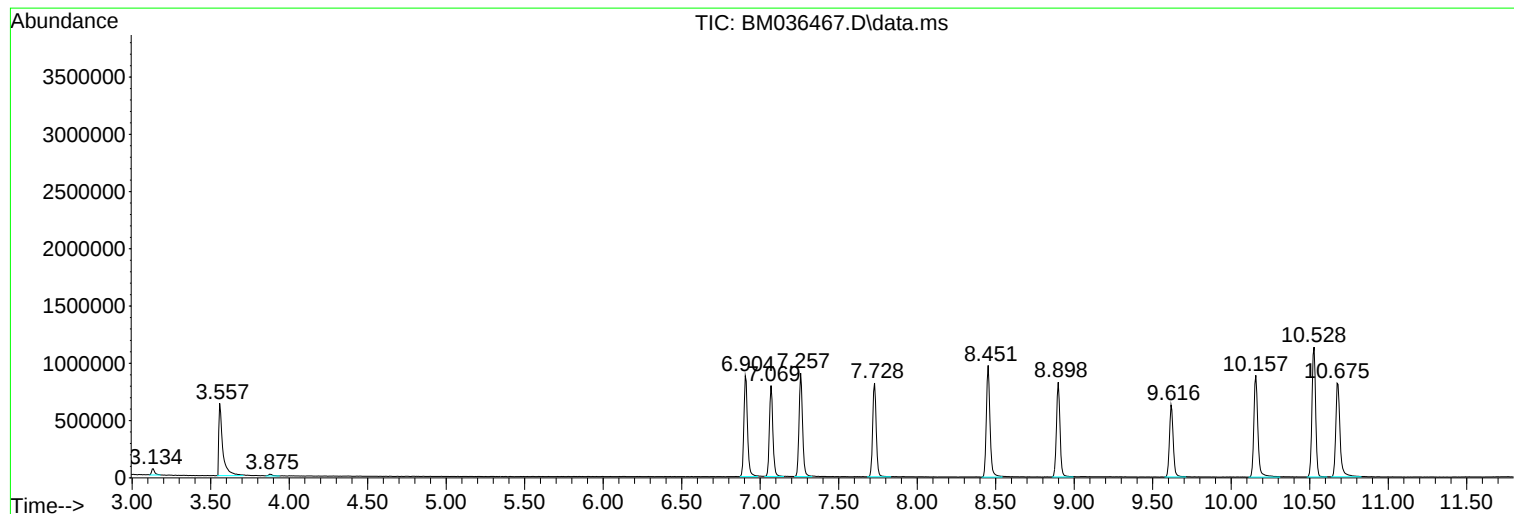

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083122\
Data File : BM036467.D
Acq On : 31 Aug 2022 11:06
Operator : CG/JU
Sample : PB147325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083122\
Data File : BM036467.D
Acq On : 31 Aug 2022 11:06
Operator : CG/JU
Sample : PB147325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc