

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083122\
 Data File : BM036468.D
 Acq On : 31 Aug 2022 11:49
 Operator : CG/JU
 Sample : N4428-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.881	149	152	157	rVB3	13082	18799	0.63%	0.136%
2	7.728	799	806	824	rBV	710230	1167375	39.11%	8.466%
3	9.169	1047	1051	1052	rBV3	2351	3082	0.10%	0.022%
4	10.527	1275	1282	1300	rBV	995255	1699604	56.94%	12.325%
5	12.727	1649	1656	1659	rBV6	3228	4545	0.15%	0.033%
6	13.110	1716	1721	1726	rBV6	2523	4872	0.16%	0.035%
7	13.780	1831	1835	1839	rVB4	2049	3451	0.12%	0.025%
8	14.380	1930	1937	1953	rBV	1539924	2196822	73.60%	15.931%
9	15.162	2067	2070	2076	rBV5	3160	5299	0.18%	0.038%
10	15.233	2076	2082	2085	rVB5	3259	5562	0.19%	0.040%
11	15.345	2096	2101	2104	rBV4	6610	9332	0.31%	0.068%
12	16.092	2225	2228	2233	rBV4	7107	12196	0.41%	0.088%
13	16.268	2254	2258	2265	rVB7	5039	9178	0.31%	0.067%
14	16.433	2282	2286	2290	rBV7	6835	12770	0.43%	0.093%
15	16.504	2294	2298	2300	rVB4	4612	6287	0.21%	0.046%
16	16.551	2303	2306	2309	rBV4	3765	4240	0.14%	0.031%
17	16.598	2309	2314	2318	rBV3	9656	14553	0.49%	0.106%
18	16.668	2323	2326	2329	rVV5	4631	6220	0.21%	0.045%
19	16.892	2360	2364	2366	rBV3	11571	16432	0.55%	0.119%
20	17.127	2397	2404	2412	rBV	1695444	2398739	80.36%	17.395%
21	17.315	2433	2436	2439	rVB4	3320	4753	0.16%	0.034%
22	17.633	2486	2490	2491	rBV3	3798	5345	0.18%	0.039%
23	17.656	2492	2494	2499	rVB6	5566	8222	0.28%	0.060%
24	18.062	2558	2563	2566	rBV6	3096	6349	0.21%	0.046%
25	18.109	2568	2571	2577	rVB2	6615	9266	0.31%	0.067%
26	18.609	2652	2656	2661	rVB6	6153	10087	0.34%	0.073%
27	19.021	2722	2726	2729	rBV5	2406	3925	0.13%	0.028%
28	20.527	2978	2982	2987	rBV	212963	237436	7.95%	1.722%
29	21.315	3111	3116	3125	rBV	2345650	2919718	97.81%	21.174%
30	23.609	3499	3506	3519	rBV2	1541593	2985013	100.00%	21.647%




Sum of corrected areas: 13789472

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083122\
Data File : BM036468.D
Acq On : 31 Aug 2022 11:49
Operator : CG/JU
Sample : N4428-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

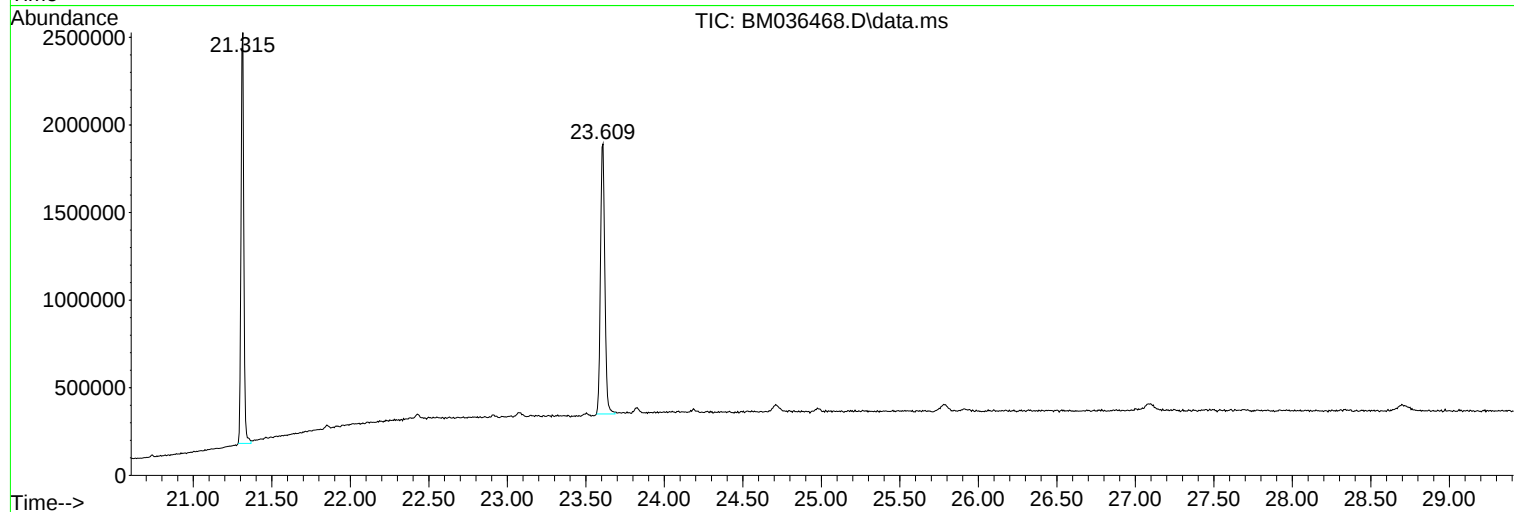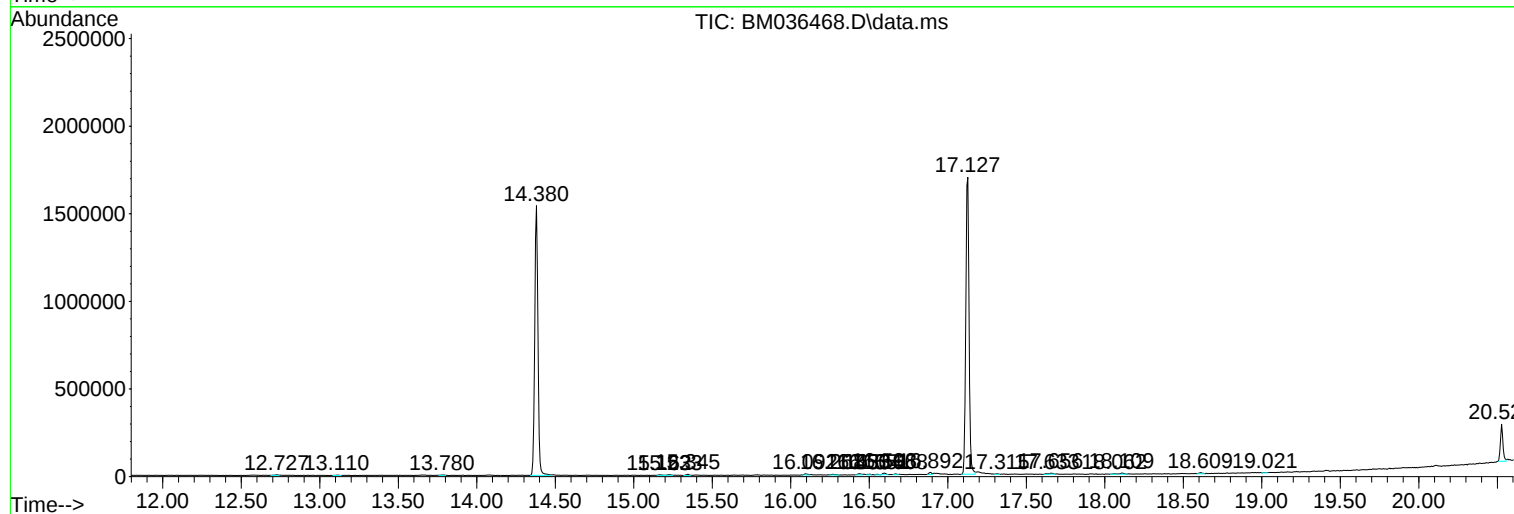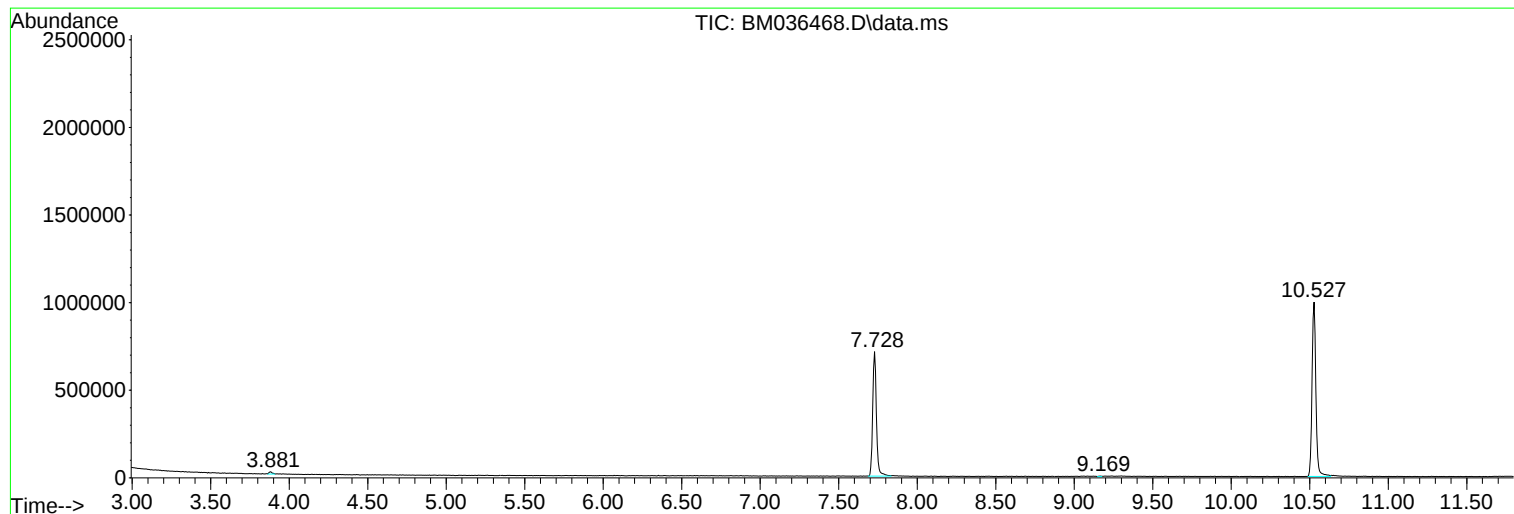

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083122\
Data File : BM036468.D
Acq On : 31 Aug 2022 11:49
Operator : CG/JU
Sample : N4428-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM083122\
Data File : BM036468.D
Acq On : 31 Aug 2022 11:49
Operator : CG/JU
Sample : N4428-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc