

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090221\
 Data File : BM032030.D
 Acq On : 02 Sep 2021 20:37
 Operator : CG/JU
 Sample : PB138856BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB138856BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM032030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.140	342	349	361	rBV	1829012	2625288	47.43%	10.615%
2	6.698	606	614	629	rBV	1706767	2694005	48.67%	10.892%
3	7.492	743	749	757	rBV	336825	523380	9.45%	2.116%
4	8.645	938	945	962	rBV	1015686	1687196	30.48%	6.822%
5	10.251	1211	1218	1231	rBV	394373	688506	12.44%	2.784%
6	12.745	1634	1642	1663	rBV	2687427	4005990	72.37%	16.197%
7	14.133	1872	1878	1889	rBV	603585	941404	17.01%	3.806%
8	15.639	2128	2134	2154	rBV	2126339	2988611	53.99%	12.084%
9	16.892	2341	2347	2360	rBV	689809	1068450	19.30%	4.320%
10	19.545	2792	2798	2806	rBV	4793081	5535586	100.00%	22.381%
11	21.097	3057	3062	3071	rBV	777917	1038515	18.76%	4.199%
12	23.233	3419	3425	3433	rBV2	501531	936043	16.91%	3.785%




Sum of corrected areas: 24732974

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090221\
Data File : BM032030.D
Acq On : 02 Sep 2021 20:37
Operator : CG/JU
Sample : PB138856BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138856BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

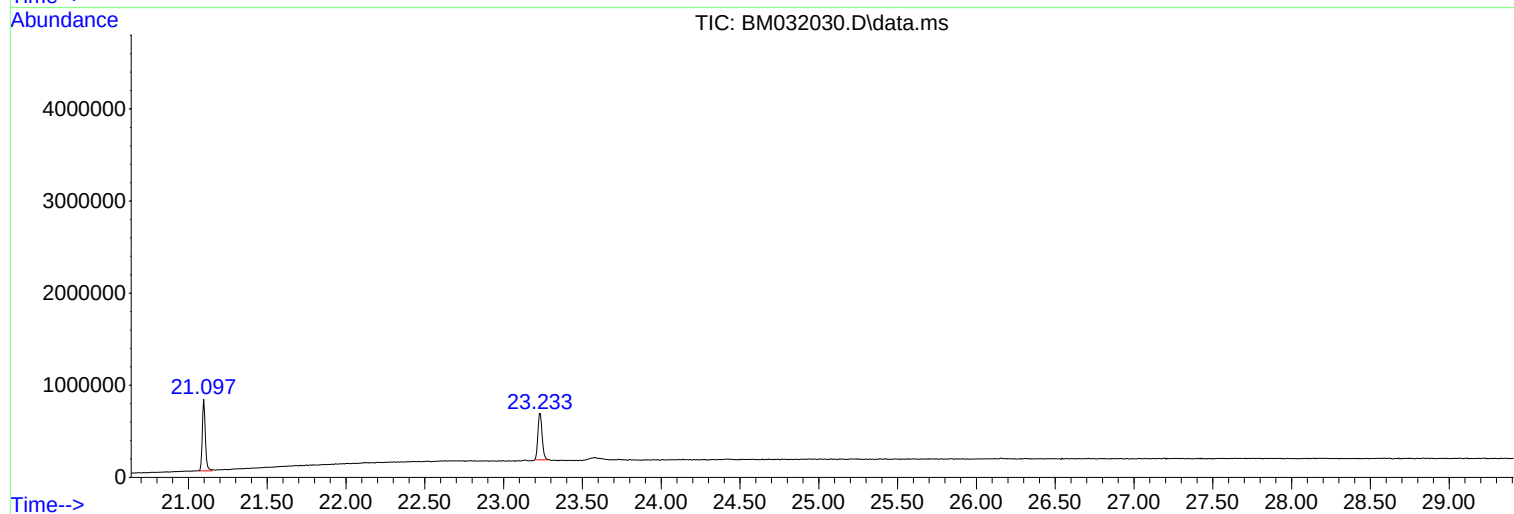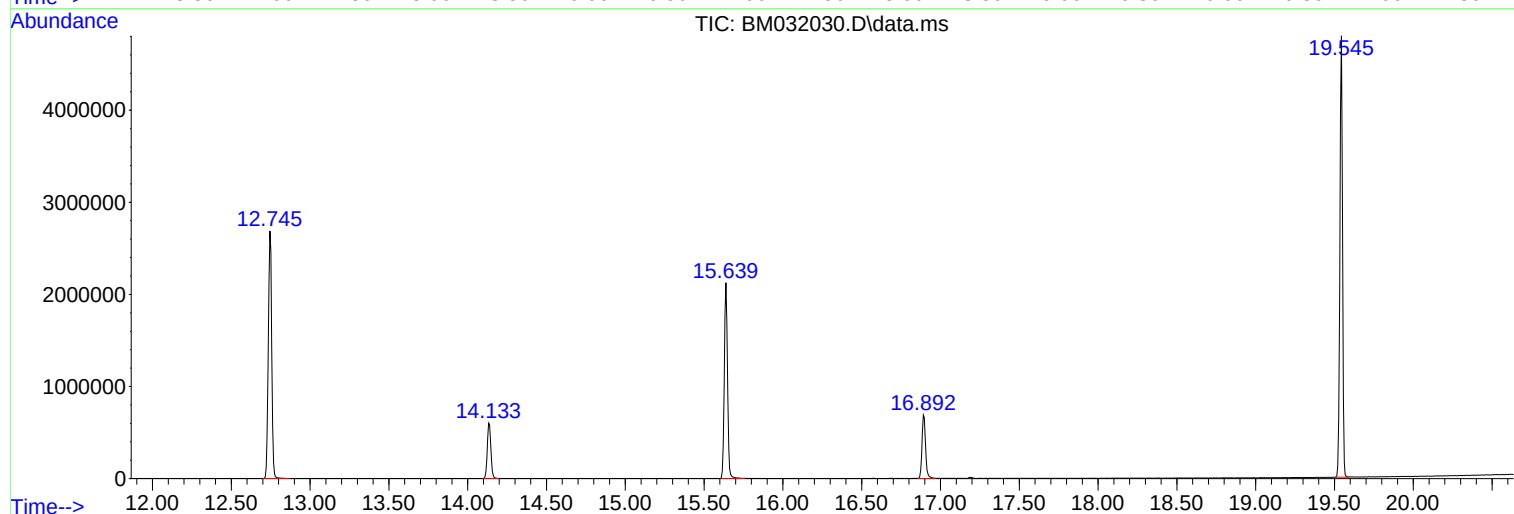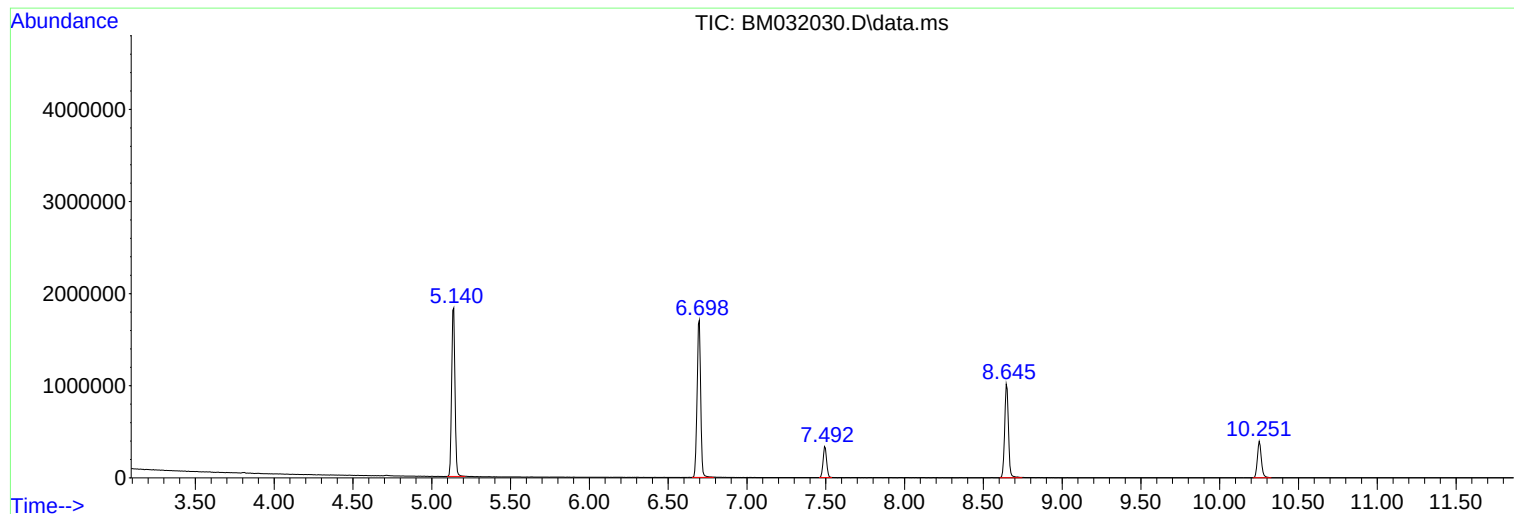

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090221\
Data File : BM032030.D
Acq On : 02 Sep 2021 20:37
Operator : CG/JU
Sample : PB138856BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138856BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090221\
Data File : BM032030.D
Acq On : 02 Sep 2021 20:37
Operator : CG/JU
Sample : PB138856BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138856BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------