

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090221\
 Data File : BM032031.D
 Acq On : 02 Sep 2021 21:14
 Operator : CG/JU
 Sample : PB138876BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB138876BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM032031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.134	342	348	359	rBV	1038847	1443895	30.06%	7.137%
2	6.693	606	613	632	rBV	954955	1462074	30.44%	7.227%
3	7.493	743	749	760	rVB	283695	436087	9.08%	2.156%
4	7.804	795	802	814	rBV	1244915	1929112	40.16%	9.535%
5	8.645	937	945	964	rBV	862474	1442616	30.04%	7.131%
6	10.251	1211	1218	1232	rBV	305048	539524	11.23%	2.667%
7	12.745	1635	1642	1661	rBV	2388986	3358888	69.93%	16.602%
8	14.133	1872	1878	1888	rBV	465413	721968	15.03%	3.569%
9	15.639	2128	2134	2152	rBV	1052172	1530350	31.86%	7.564%
10	16.892	2341	2347	2360	rBV	533154	817230	17.01%	4.039%
11	19.545	2792	2798	2811	rBV	4095149	4803082	100.00%	23.741%
12	21.098	3057	3062	3070	rBV	624107	864611	18.00%	4.274%
13	23.233	3419	3425	3434	rVB	468816	881882	18.36%	4.359%




Sum of corrected areas: 20231319

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090221\
Data File : BM032031.D
Acq On : 02 Sep 2021 21:14
Operator : CG/JU
Sample : PB138876BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138876BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

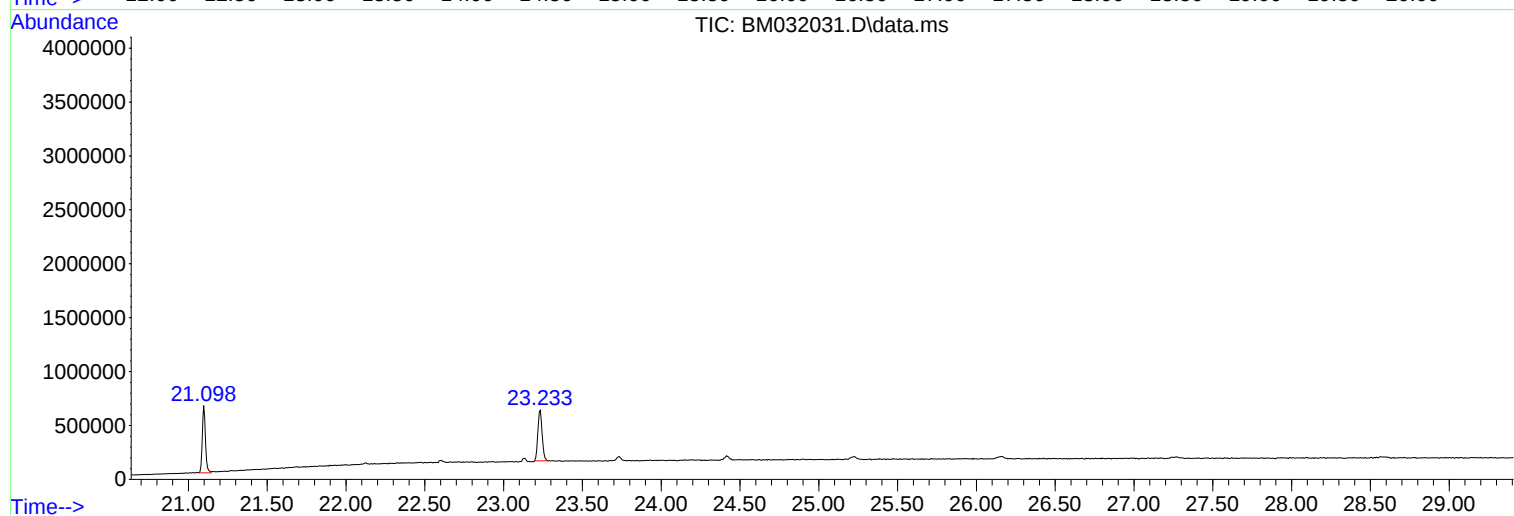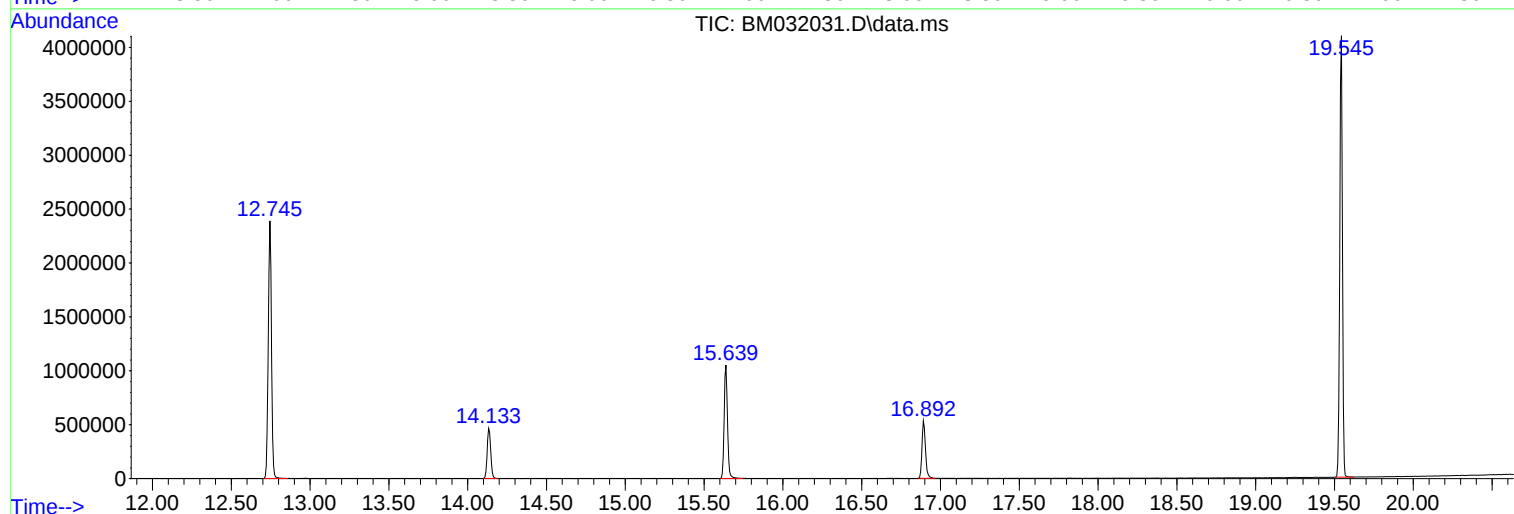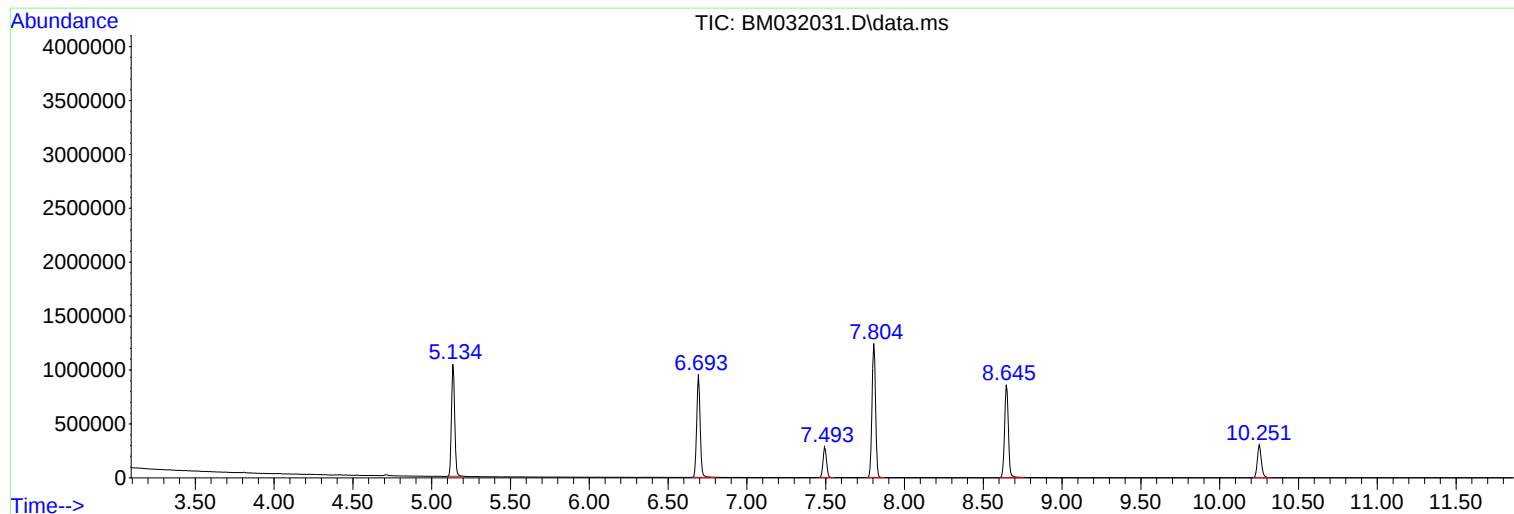

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090221\
Data File : BM032031.D
Acq On : 02 Sep 2021 21:14
Operator : CG/JU
Sample : PB138876BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138876BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090221\
Data File : BM032031.D
Acq On : 02 Sep 2021 21:14
Operator : CG/JU
Sample : PB138876BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138876BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------