


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090221\
 Data File : BM032021.D
 Acq On : 02 Sep 2021 14:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 02 19:37:10 2021

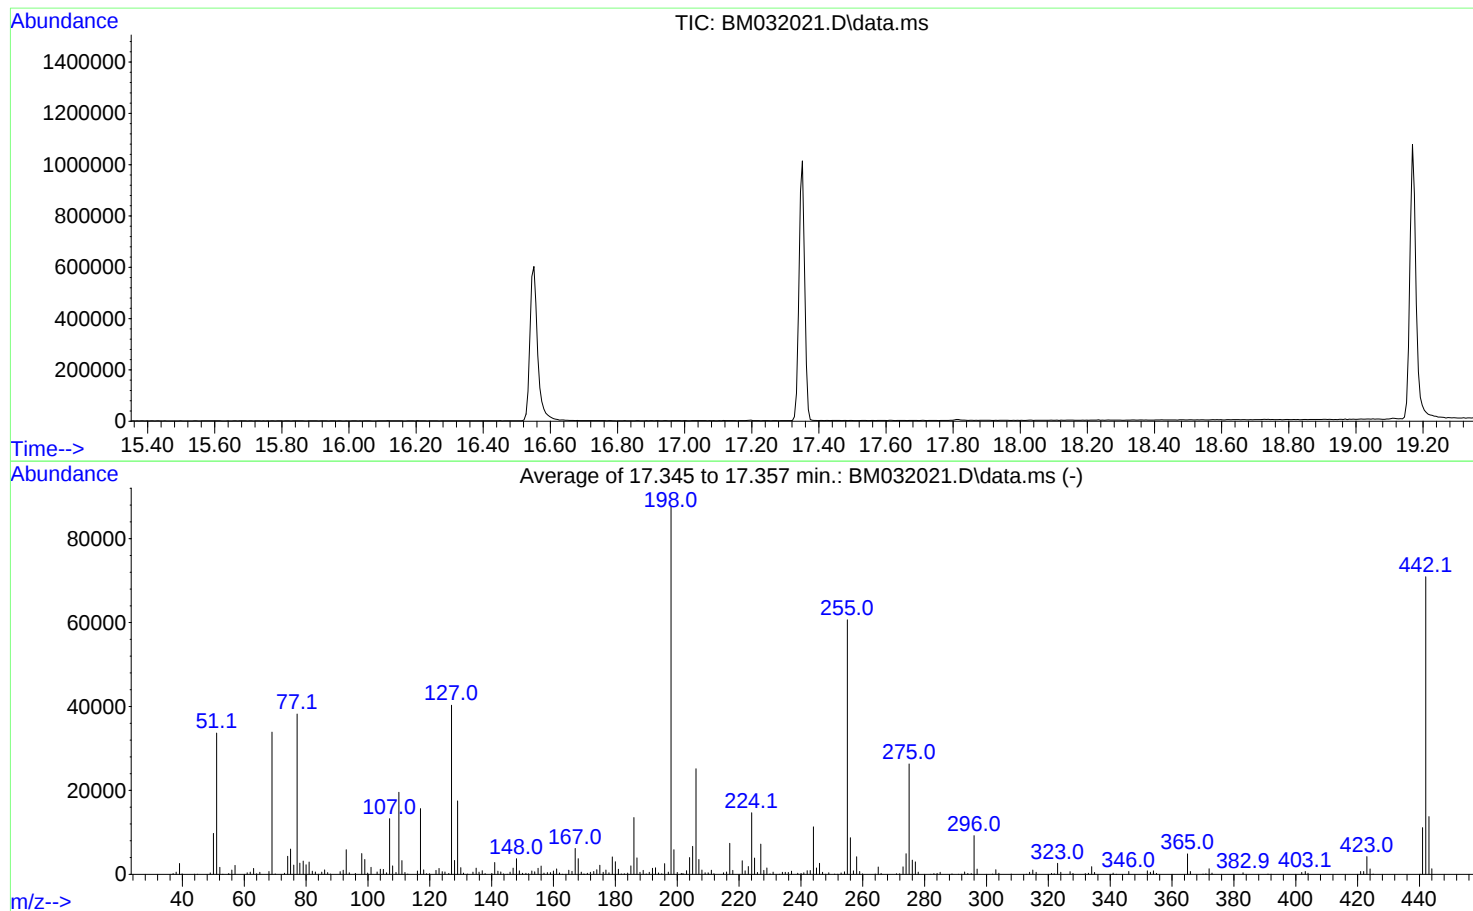




AutoFind: Scans 2424, 2425, 2426; Background Corrected with Scan 2417

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	33661	PASS
68	69	0.00	2	2.1	695	PASS
69	198	0.00	100	38.7	33885	PASS
70	69	0.00	2	0.4	135	PASS
127	198	10	80	46.0	40293	PASS
197	198	0.00	2	0.6	538	PASS
198	198	100	100	100.0	87661	PASS
199	198	5	9	6.7	5883	PASS
275	198	10	60	30.0	26323	PASS
365	198	1	100	5.6	4885	PASS
441	198	0.01	100	12.7	11116	PASS
442	442	50	100	100.0	70909	PASS
443	442	15	24	19.4	13783	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090221\
Data File : BM032021.D
Acq On : 02 Sep 2021 14:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 02 16:18:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 02 15:16:12 2021
Response via : Initial Calibration

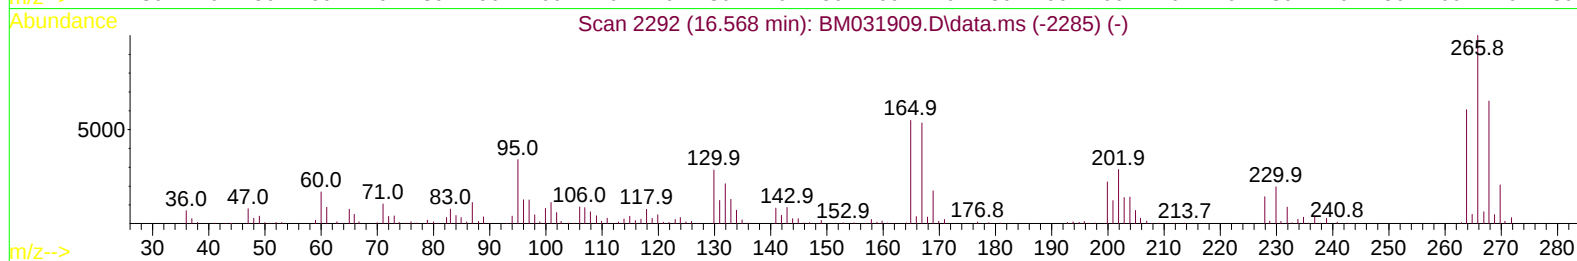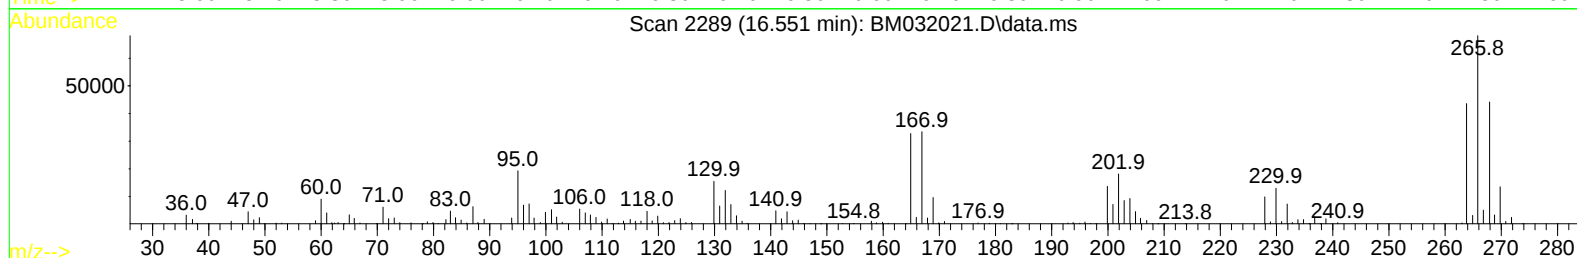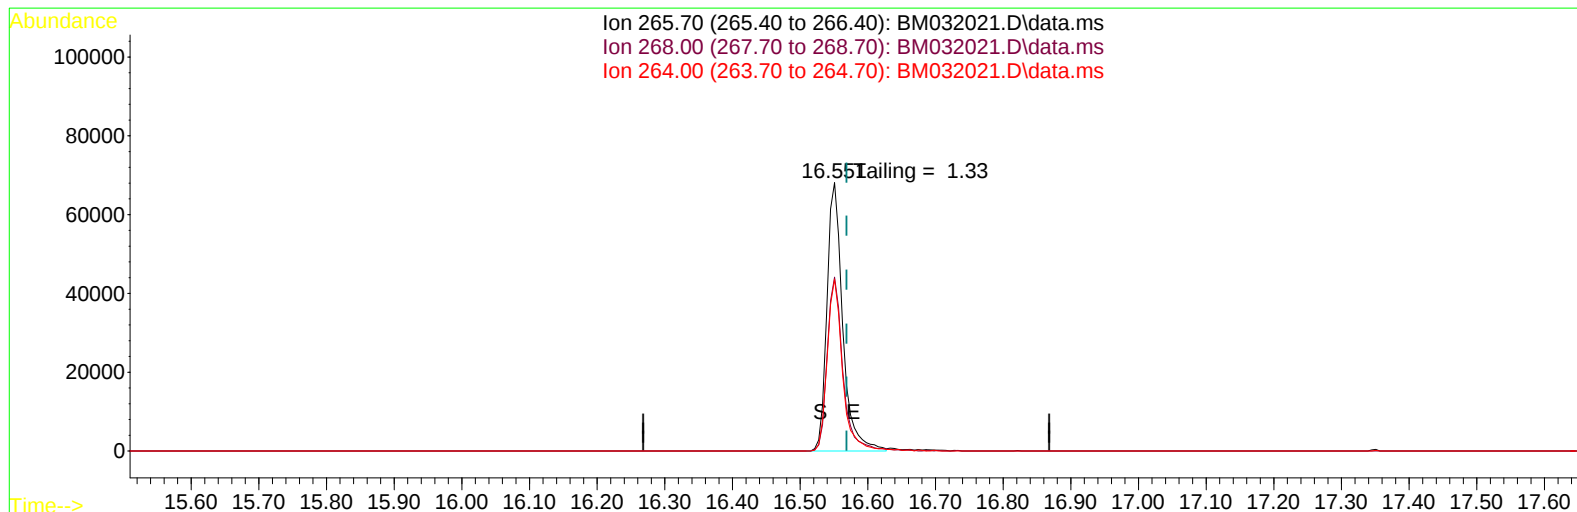

TIC: BM032021.D\data.ms

(70) Pentachlorophenol (C)

16.551min (-0.018) 0.00 ng




response 110954

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.83
264.00	65.10	64.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090221\
Data File : BM032021.D
Acq On : 02 Sep 2021 14:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 02 16:18:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 02 15:16:12 2021
Response via : Initial Calibration

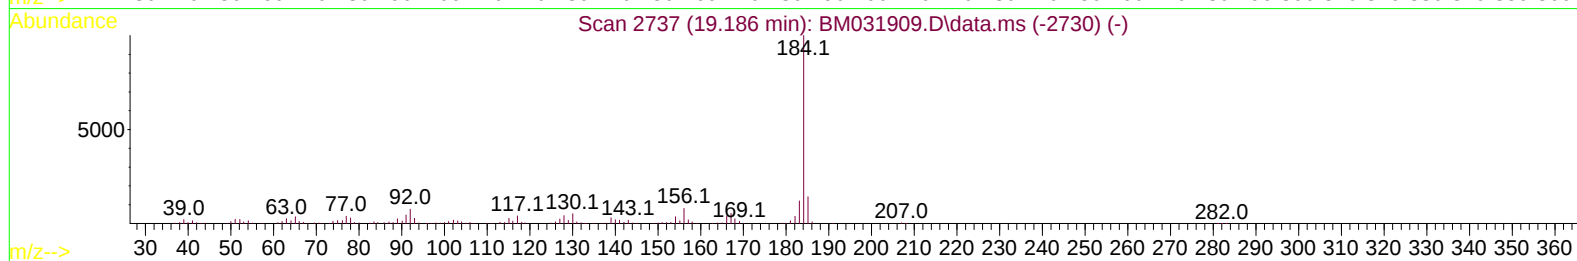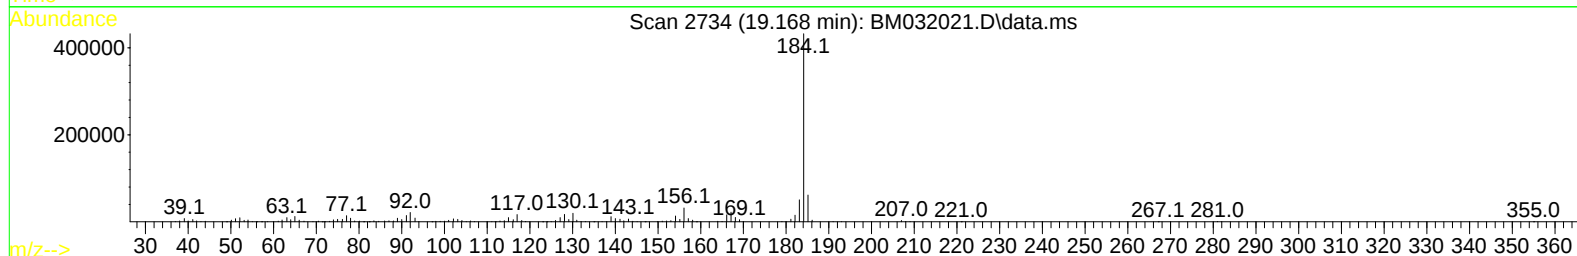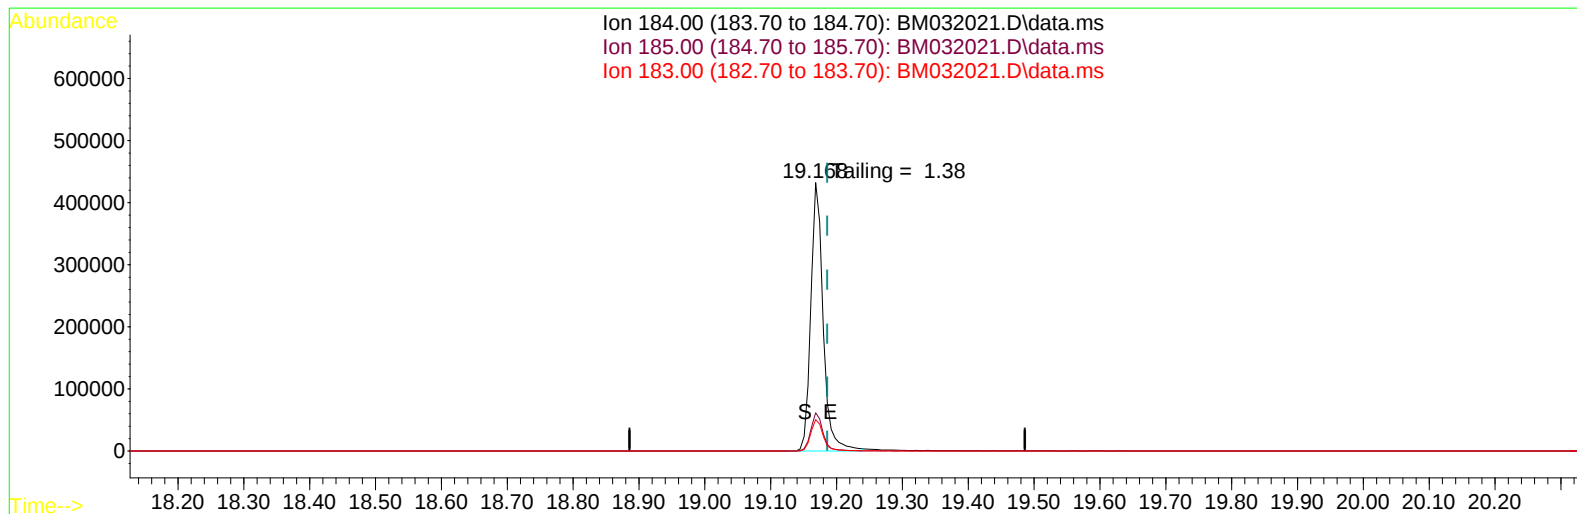

TIC: BM032021.D\data.ms

(77) Benzidine

19.168min (-0.018) 0.00 ng

response 571208

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.26
183.00	11.20	11.69
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/2/2021	BNA_M	<u>BM032021.D</u>
Compound Name	Response	Retention Time
DDT	311146	20.4
DDD	708	19.96
DDE	398	19.45
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1106	312252	0.35

Instrument :
BNA_M
ClientSampleId :
DFTPP