

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
 Data File : BM036488.D
 Acq On : 02 Sep 2022 13:07
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020167

Quant Time: Sep 02 23:16:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 02 01:33:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.716	152	236278	20.000	ng/u1	0.00
20) Naphthalene-d8	10.516	136	1228429	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.374	164	784801	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.115	188	1602897	20.000	ng/u1	0.00
79) Chrysene-d12	21.309	240	1611413	20.000	ng/u1	0.00
88) Perylene-d12	23.603	264	1531194	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.128	96	47255	7.622	ng/uL	0.00
4) Pyridine-d5	3.551	84	324278	18.967	ng/u1	0.00
7) Phenol-d5	6.898	99	354820	17.593	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	235793	18.574	ng/u1	0.00
11) 2-Chlorophenol-d4	7.251	132	283525	17.892	ng/u1	0.00
15) 4-Methylphenol-d8	8.445	113	299228	19.871	ng/u1	0.00
21) Nitrobenzene-d5	8.886	128	169747	18.225	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.610	143	174908	18.514	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.145	165	316880	18.772	ng/u1	0.00
31) 4-Chloroaniline-d4	10.669	131	498418	19.046	ng/u1	0.00
46) Dimethylphthalate-d6	13.798	166	947704	19.088	ng/u1	0.00
49) Acenaphthylene-d8	14.063	160	1157413	18.690	ng/u1	0.00
54) 4-Nitrophenol-d4	14.598	143	178463	18.970	ng/u1	0.00
60) Fluorene-d10	15.368	176	861569	19.204	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.504	200	148510	18.022	ng/u1	0.00
73) Anthracene-d10	17.215	188	1338224	18.776	ng/u1	0.00
81) Pyrene-d10	19.515	212	1509270	18.056	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.456	264	1399746	18.645	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.163	88	48594	7.442	ng/uL	94
5) Pyridine	3.569	79	338099	19.143	ng/u1	97
6) Benzaldehyde	6.863	77	188501	22.754	ng/u1	90
8) Phenol	6.922	94	368616	17.579	ng/u1	94
10) Bis(2-Chloroethyl)ether	7.151	93	302826	18.056	ng/u1	98
12) 2-Chlorophenol	7.281	128	298274	18.000	ng/u1	98
13) 2-Methylphenol	8.175	108	299059	19.348	ng/u1	96
14) 2,2'-oxybis(1-Chloropr...	8.251	45	305693	13.623	ng/u1	99
16) Acetophenone	8.551	105	518366	21.402	ng/u1	96
17) N-Nitroso-di-n-propyla...	8.539	70	264192	21.915	ng/u1	99
18) 4-Methylphenol	8.504	108	333967	20.185	ng/u1	99
19) Hexachloroethane	8.786	117	145071	20.926	ng/u1	88
22) Nitrobenzene	8.933	77	414441	18.780	ng/u1	99
23) Isophorone	9.457	82	767753	19.591	ng/u1	96
25) 2-Nitrophenol	9.639	139	197443	18.759	ng/u1	95
26) 2,4-Dimethylphenol	9.704	107	394397	18.737	ng/u1	96
27) Bis(2-Chloroethoxy)met...	9.945	93	490844	19.239	ng/u1	99
29) 2,4-Dichlorophenol	10.169	162	327297	18.951	ng/u1	98
30) Naphthalene	10.569	128	1181418	18.324	ng/u1	99
32) 4-Chloroaniline	10.692	127	510438	19.177	ng/u1	99
33) Hexachlorobutadiene	10.845	225	201318	18.555	ng/u1	99
34) Caprolactam	11.486	113	51474	9.947	ng/u1	95
35) 4-Chloro-3-methylphenol	11.827	107	358041	20.504	ng/u1	99
36) 2-Methylnaphthalene	12.186	142	794733	19.646	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
 Data File : BM036488.D
 Acq On : 02 Sep 2022 13:07
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 SSTD020167


Quant Time: Sep 02 23:16:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 02 01:33:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.404	142	805013	19.760	ng/ul#	99
39) 1,2,4,5-Tetrachloroben...	12.557	216	377310	17.394	ng/ul	99
40) Hexachlorocyclopentadiene	12.527	237	312985	24.321	ng/ul	96
41) 2,4,6-Trichlorophenol	12.804	196	247895	18.161	ng/ul	97
42) 2,4,5-Trichlorophenol	12.880	196	273961	18.922	ng/ul	98
43) 1,1'-Biphenyl	13.204	154	1064386	18.033	ng/ul	99
44) 2-Chloronaphthalene	13.245	162	801653	17.699	ng/ul	99
45) 2-Nitroaniline	13.468	65	236544	19.286	ng/ul	94
47) Dimethylphthalate	13.845	163	976472	19.106	ng/ul	99
48) 2,6-Dinitrotoluene	13.968	165	192385	19.951	ng/ul#	86
50) Acenaphthylene	14.092	152	1354275	18.545	ng/ul	100
51) 3-Nitroaniline	14.298	138	205377	19.476	ng/ul	98
52) Acenaphthene	14.433	153	883306	18.558	ng/ul	98
53) 2,4-Dinitrophenol	14.510	184	118503	22.550	ng/ul	91
55) 4-Nitrophenol	14.615	109	145258	19.542	ng/ul	84
56) Dibenzofuran	14.774	168	1235115	18.701	ng/ul	97
57) 2,4-Dinitrotoluene	14.757	165	282575	20.663	ng/ul#	86
58) 2,3,4,6-Tetrachlorophenol	15.004	232	219138	19.934	ng/ul#	93
59) Diethylphthalate	15.204	149	1032070	20.486	ng/ul	99
61) Fluorene	15.421	166	1020743	19.486	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.421	204	477952	19.532	ng/ul	98
63) 4-Nitroaniline	15.462	138	180124	18.311	ng/ul#	87
66) 4,6-Dinitro-2-methylph...	15.515	198	150127	18.019	ng/ul	92
67) N-Nitrosodiphenylamine	15.639	169	831975	18.155	ng/ul	98
68) 4-Bromophenyl-phenylether	16.315	248	273578	18.433	ng/ul	98
69) Hexachlorobenzene	16.415	284	326245	18.138	ng/ul	94
70) Atrazine	16.598	200	291846	18.639	ng/ul	98
71) Pentachlorophenol	16.768	266	214160	21.597	ng/ul	99
72) Phenanthrene	17.162	178	1565794	18.582	ng/ul	99
74) Anthracene	17.251	178	1602008	18.963	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.168	216	389630	16.200	ng/ul	97
76) Pentachlorobenzene	14.686	250	387961	17.276	ng/ul	98
77) Carbazole	17.533	167	1462368	18.488	ng/ul	99
78) Di-n-butylphthalate	18.098	149	1796321	20.763	ng/ul	99
80) Fluoranthene	19.180	202	1830043	18.115	ng/ul	99
82) Pyrene	19.545	202	1910851	18.126	ng/ul	98
83) Butylbenzylphthalate	20.456	149	777228	19.707	ng/ul	95
84) 3,3'-Dichlorobenzidine	21.233	252	568730	17.139	ng/ul	98
85) Benzo(a)anthracene	21.297	228	1826268	18.859	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.233	149	1208190	22.187	ng/ul	99
87) Chrysene	21.350	228	1751653	18.409	ng/ul	100
89) Di-n-octyl phthalate	22.121	149	1958377	21.515	ng/ul	100
90) Benzo(b)fluoranthene	22.903	252	1771322	18.974	ng/ul	98
91) Benzo(k)fluoranthene	22.950	252	1718631	19.350	ng/ul	98
93) Benzo(a)pyrene	23.503	252	1725699	18.790	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	25.968	276	1773531	16.425	ng/ul	96
95) Dibenzo(a,h)anthracene	25.979	278	1529674	16.445	ng/ul	98
96) Benzo(g,h,i)perylene	26.691	276	1459440	15.805	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 02 23:16:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 02 01:33:23 2022
Response via : Initial Calibration









#2
1,4-Dioxane
Concen: 7.442 ng/uL
RT: 3.163 min Scan# 30
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion: 88 Resp: 48594
Ion Ratio Lower Upper
88 100
43 30.7 27.8 41.8
58 71.9 61.8 92.8



#5
Pyridine
Concen: 19.143 ng/uL
RT: 3.569 min Scan# 99
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion: 79 Resp: 338099
Ion Ratio Lower Upper
79 100
52 82.7 67.8 101.6
51 36.8 31.4 47.0









#6
Benzaldehyde
Concen: 22.754 ng/ul
RT: 6.863 min Scan# 61
Delta R.T. -0.012 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion: 77 Resp: 188501
Ion Ratio Lower Upper
77 100
105 93.7 84.6 127.0
106 92.0 80.3 120.5



#8
Phenol
Concen: 17.579 ng/ul
RT: 6.922 min Scan# 669
Delta R.T. -0.012 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion: 94 Resp: 368616
Ion Ratio Lower Upper
94 100
65 29.4 21.3 31.9
66 37.9 27.4 41.0





#10

Bis(2-Chloroethyl)ether

Concen: 18.056 ng/ul

RT: 7.151 min Scan# 709

Delta R.T. -0.006 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07

Instrument :

BNA_M

ClientSampleId :

SSTD020167





Tgt Ion: 93 Resp: 302826

Ion Ratio Lower Upper

93 100

63 78.5 64.0 96.0

95 32.7 25.8 38.6

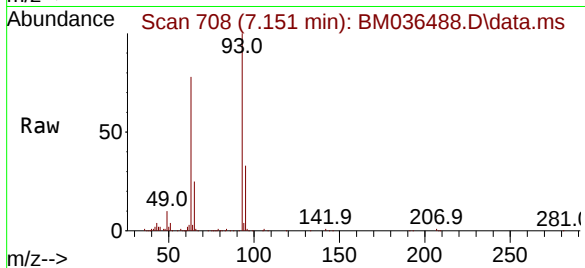

#12

2-Chlorophenol

Concen: 18.000 ng/ul

RT: 7.281 min Scan# 730

Delta R.T. -0.006 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07




Tgt Ion:128 Resp: 298274


Ion Ratio Lower Upper

128 100

64 47.8 36.9 55.3

130 33.1 25.6 38.4




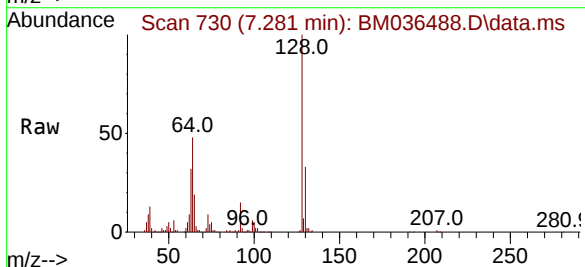


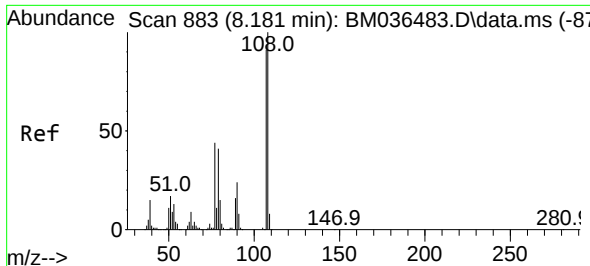

#13
2-Methylphenol
Concen: 19.348 ng/ul
RT: 8.175 min Scan# 882
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:108 Resp: 299059
Ion Ratio Lower Upper
108 100
107 89.5 75.0 112.4

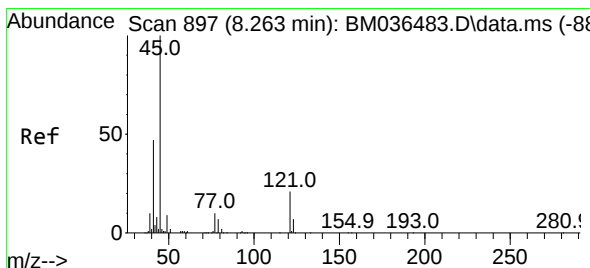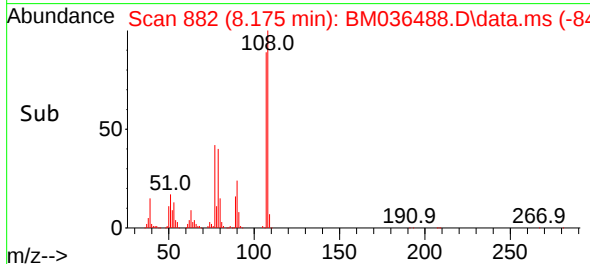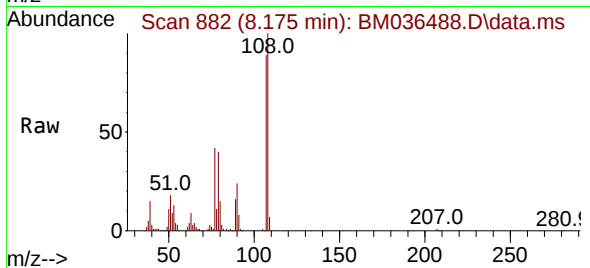

#14
2,2'-oxybis(1-Chloropropane)
Concen: 13.623 ng/ul
RT: 8.251 min Scan# 895
Delta R.T. -0.012 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion: 45 Resp: 305693
Ion Ratio Lower Upper
45 100
77 13.7 10.6 15.8
79 9.8 8.3 12.5


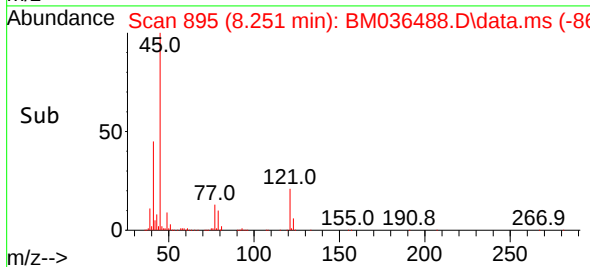

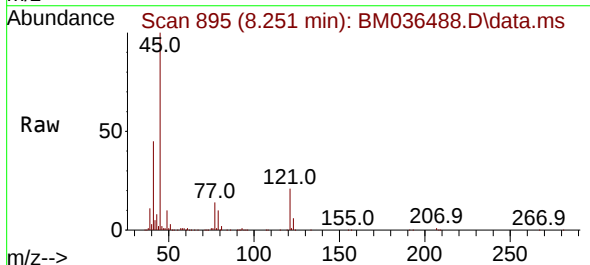




#16
Acetophenone
Concen: 21.402 ng/ul
RT: 8.551 min Scan# 947
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:105 Resp: 518366
Ion Ratio Lower Upper
105 100
77 78.8 59.8 89.6
51 29.4 22.1 33.1



#17
N-Nitroso-di-n-propylamine
Concen: 21.915 ng/ul
RT: 8.539 min Scan# 944
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion: 70 Resp: 264192
Ion Ratio Lower Upper
70 100
42 62.2 49.6 74.4
101 9.2 8.1 12.1
130 20.9 18.4 27.6





#18

4-Methylphenol

Concen: 20.185 ng/ul

RT: 8.504 min Scan# 91

Delta R.T. -0.012 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07

Instrument :

BNA_M

ClientSampleId :





SSTD020167

Tgt Ion:108 Resp: 333967

Ion Ratio Lower Upper

108 100

107 114.0 90.3 135.5

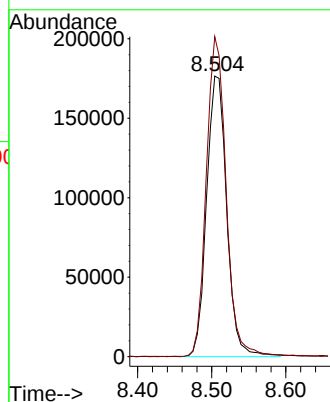

#19

Hexachloroethane

Concen: 20.926 ng/ul

RT: 8.786 min Scan# 986

Delta R.T. -0.006 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07




Tgt Ion:117 Resp: 145071


Ion Ratio Lower Upper

117 100

201 90.1 81.8 122.6

199 54.7 51.6 77.4









#22
 Nitrobenzene
 Concen: 18.780 ng/ul
 RT: 8.933 min Scan# 1100
 Delta R.T. -0.006 min
 Lab File: BM036488.D
 Acq: 02 Sep 2022 13:07




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020167


Tgt Ion: 77 Resp: 414441
 Ion Ratio Lower Upper
 77 100
 123 46.2 37.4 56.0
 65 13.6 10.8 16.2



#23
 Isophorone
 Concen: 19.591 ng/ul
 RT: 9.457 min Scan# 1100
 Delta R.T. -0.006 min
 Lab File: BM036488.D
 Acq: 02 Sep 2022 13:07

Tgt Ion: 82 Resp: 767753
 Ion Ratio Lower Upper
 82 100
 95 6.6 5.5 8.3
 138 16.9 15.3 22.9







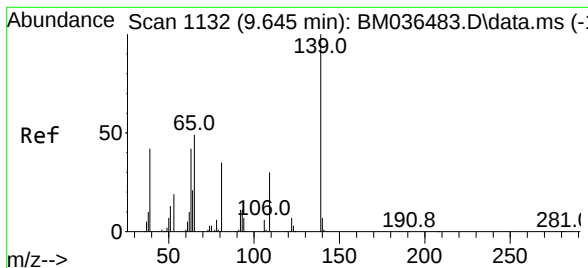

#25
2-Nitrophenol
Concen: 18.759 ng/ul
RT: 9.639 min Scan# 1131
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:139 Resp: 197443
Ion Ratio Lower Upper
139 100
65 51.6 39.8 59.6
109 32.2 22.2 33.4

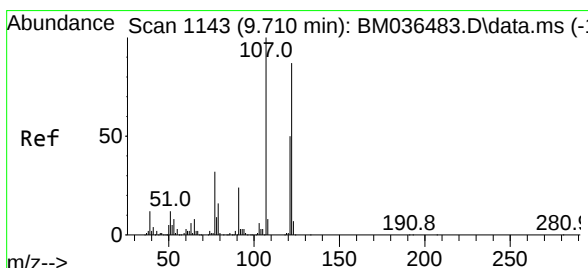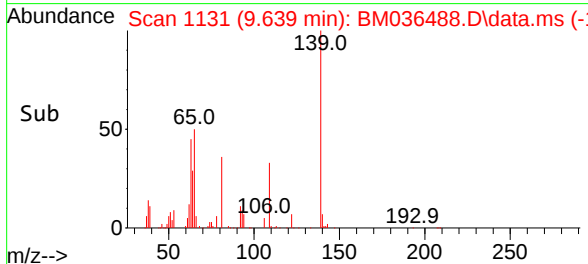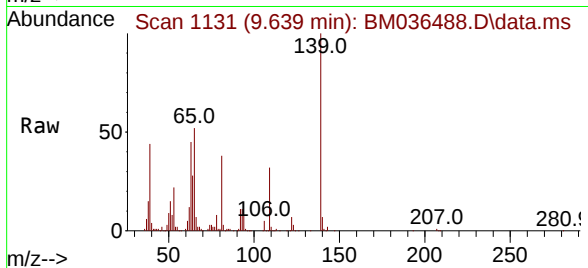

#26
2,4-Dimethylphenol
Concen: 18.737 ng/ul
RT: 9.704 min Scan# 1142
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:107 Resp: 394397
Ion Ratio Lower Upper
107 100
121 50.0 42.7 64.1
122 86.5 71.5 107.3


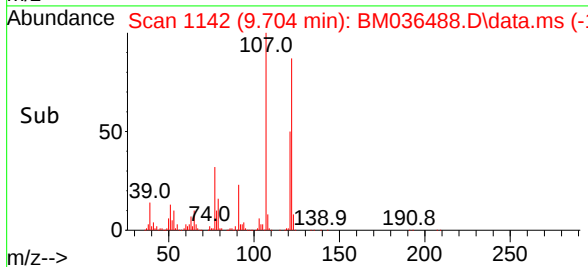

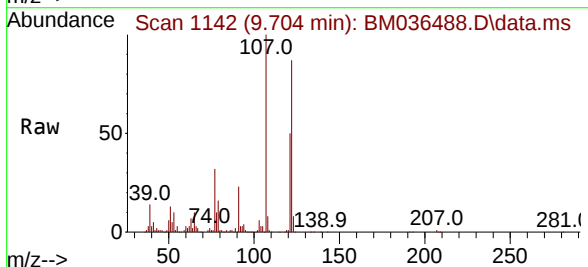




#27
 Bis(2-Chloroethoxy)methane
 Concen: 19.239 ng/ul
 RT: 9.945 min Scan# 1183
 Delta R.T. -0.006 min
 Lab File: BM036488.D
 Acq: 02 Sep 2022 13:07




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020167


Tgt Ion: 93 Resp: 490844
 Ion Ratio Lower Upper
 93 100
 95 31.5 26.1 39.1
 123 11.7 9.4 14.0

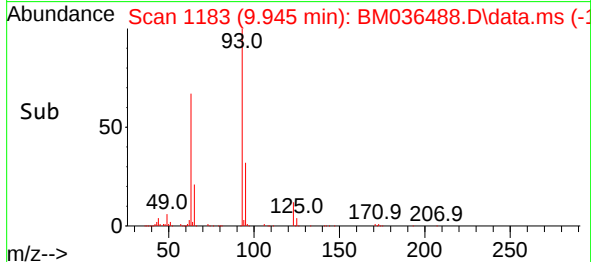

#29
 2,4-Dichlorophenol
 Concen: 18.951 ng/ul
 RT: 10.169 min Scan# 1221
 Delta R.T. -0.012 min
 Lab File: BM036488.D
 Acq: 02 Sep 2022 13:07

Tgt Ion: 162 Resp: 327297
 Ion Ratio Lower Upper
 162 100
 164 64.1 51.8 77.6
 98 34.7 29.5 44.3




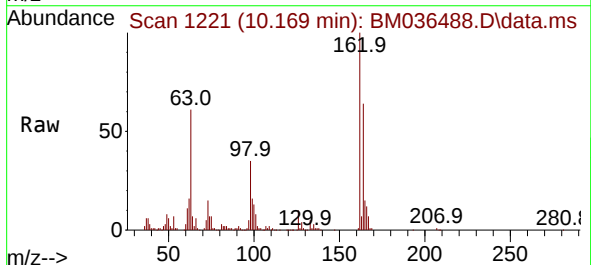




#30
Naphthalene
Concen: 18.324 ng/ul
RT: 10.569 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:128 Resp: 1181418
Ion Ratio Lower Upper
128 100
129 10.9 8.8 13.2
127 12.8 10.6 16.0



#32
4-Chloroaniline
Concen: 19.177 ng/ul
RT: 10.692 min Scan# 1310
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:127 Resp: 510438
Ion Ratio Lower Upper
127 100
129 31.9 25.3 37.9









#33
Hexachlorobutadiene
Concen: 18.555 ng/ul
RT: 10.845 min Scan# 1336
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:225 Resp: 201318
Ion Ratio Lower Upper
225 100
223 62.0 50.0 75.0
227 63.3 49.9 74.9

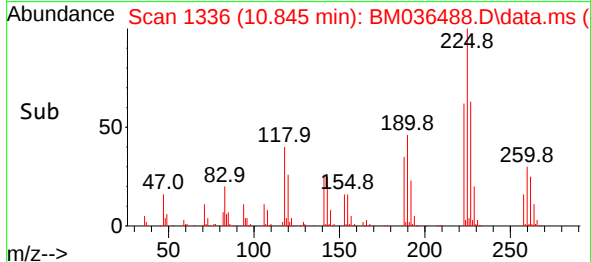

#34
Caprolactam
Concen: 9.947 ng/ul
RT: 11.486 min Scan# 1445
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:113 Resp: 51474
Ion Ratio Lower Upper
113 100
55 192.7 150.2 225.4
56 137.1 102.1 153.1




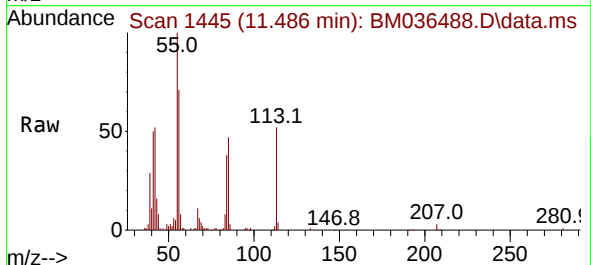




#35
4-Chloro-3-methylphenol
Concen: 20.504 ng/ul
RT: 11.827 min Scan# 1503
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:107 Resp: 358041
Ion Ratio Lower Upper
107 100
144 25.9 20.3 30.5
142 81.8 64.4 96.6

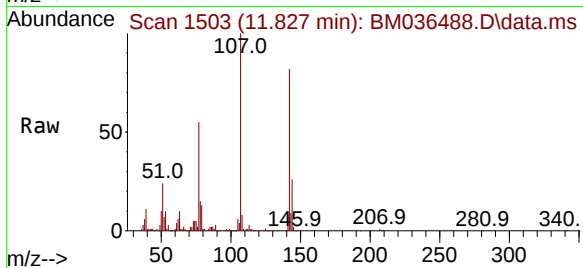

#36
2-Methylnaphthalene
Concen: 19.646 ng/ul
RT: 12.186 min Scan# 1564
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:142 Resp: 794733
Ion Ratio Lower Upper
142 100
141 89.4 70.7 106.1

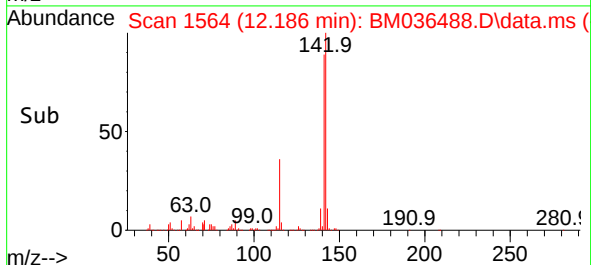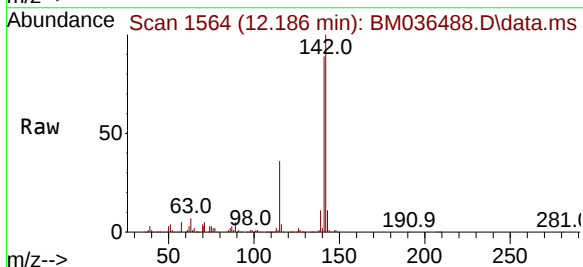



#37

1-Methylnaphthalene

Concen: 19.760 ng/ul

RT: 12.404 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07

Instrument :

BNA_M

ClientSampleId :

SSTD020167





Tgt Ion:142 Resp: 805013

Ion Ratio Lower Upper

142 100

141 92.9 75.2 112.8

116 4.2 2.6 3.8#

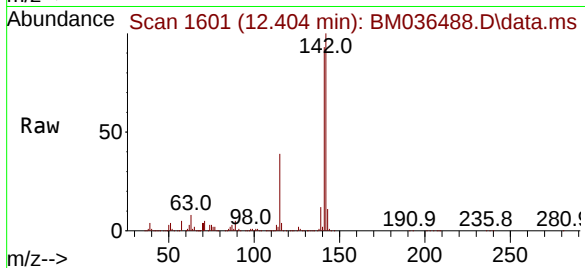

#39

1,2,4,5-Tetrachlorobenzene

Concen: 17.394 ng/ul

RT: 12.557 min Scan# 1627

Delta R.T. -0.006 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07

Tgt Ion:216 Resp: 377310




Ion Ratio Lower Upper


216 100

214 78.1 62.4 93.6

179 21.9 17.3 25.9

108 19.4 14.0 21.0



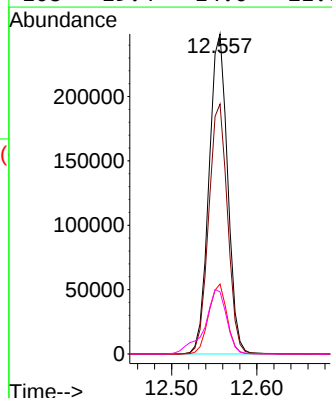
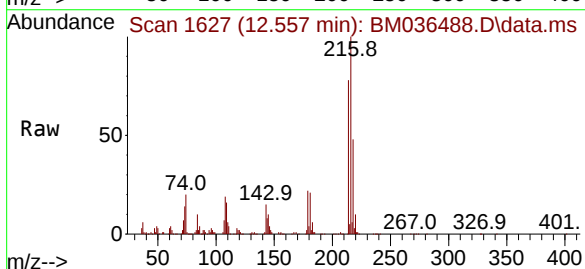




#40
Hexachlorocyclopentadiene
Concen: 24.321 ng/ul
RT: 12.527 min Scan# 1
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:237 Resp: 312985
Ion Ratio Lower Upper
237 100
235 63.4 48.4 72.6
272 12.9 11.6 17.4



#41
2,4,6-Trichlorophenol
Concen: 18.161 ng/ul
RT: 12.804 min Scan# 1669
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:196 Resp: 247895
Ion Ratio Lower Upper
196 100
198 93.9 77.8 116.6
200 30.1 25.0 37.6









#42
2,4,5-Trichlorophenol
Concen: 18.922 ng/ul
RT: 12.880 min Scan# 1
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:196 Resp: 273961
Ion Ratio Lower Upper
196 100
198 94.3 76.8 115.2
200 30.1 24.9 37.3

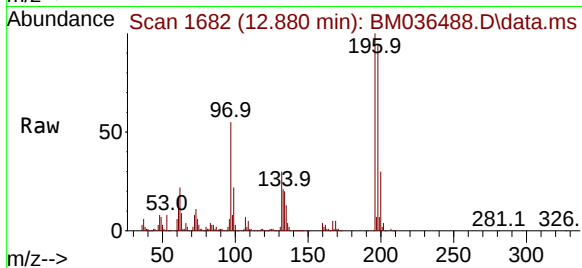

#43
1,1'-Biphenyl
Concen: 18.033 ng/ul
RT: 13.204 min Scan# 1737
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:154 Resp: 1064386
Ion Ratio Lower Upper
154 100
153 40.1 32.4 48.6
76 14.1 10.1 15.1

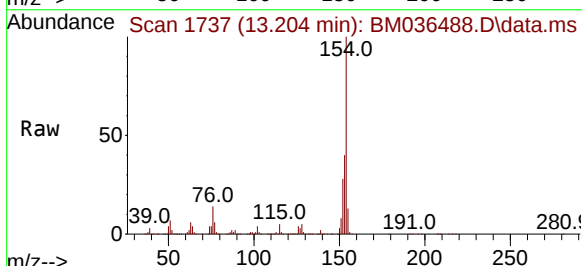



#44

2-Chloronaphthalene

Concen: 17.699 ng/ul

RT: 13.245 min Scan# 1744

Delta R.T. -0.006 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07

Instrument :

BNA_M

ClientSampleId :

SSTD020167





Tgt Ion:162 Resp: 801653

Ion Ratio Lower Upper

162 100

164 32.6 25.4 38.0

127 40.3 31.6 47.4

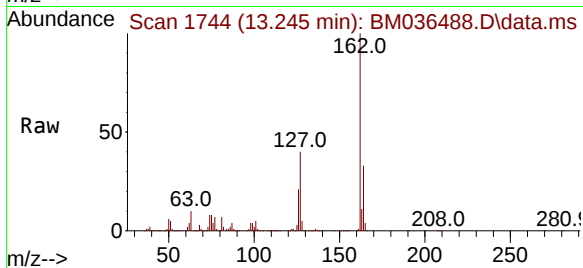

#45

2-Nitroaniline

Concen: 19.286 ng/ul

RT: 13.468 min Scan# 1782

Delta R.T. -0.006 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07




Tgt Ion: 65 Resp: 236544


Ion Ratio Lower Upper

65 100

92 66.4 54.5 81.7

138 105.6 91.2 136.8




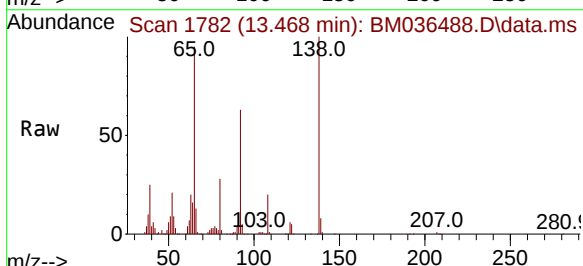




#47
Dimethylphthalate
Concen: 19.106 ng/ul
RT: 13.845 min Scan# 1846
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:163 Resp: 976472
Ion Ratio Lower Upper
163 100
194 3.7 3.2 4.8
164 9.8 7.9 11.9

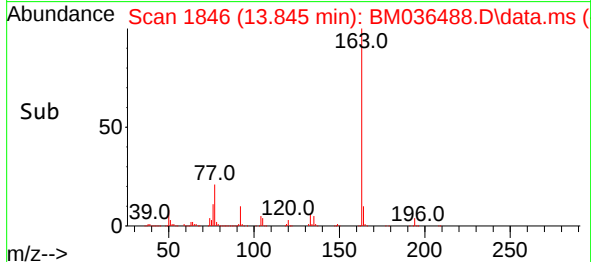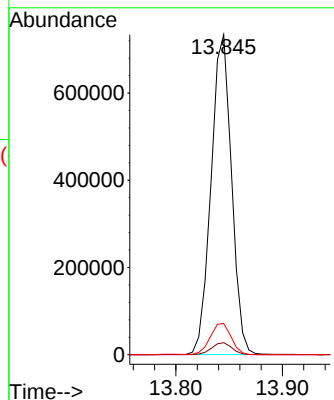

#48
2,6-Dinitrotoluene
Concen: 19.951 ng/ul
RT: 13.968 min Scan# 1867
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:165 Resp: 192385
Ion Ratio Lower Upper
165 100
89 66.0 42.5 63.7#
121 24.0 17.2 25.8



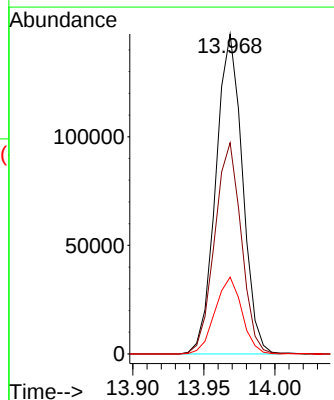
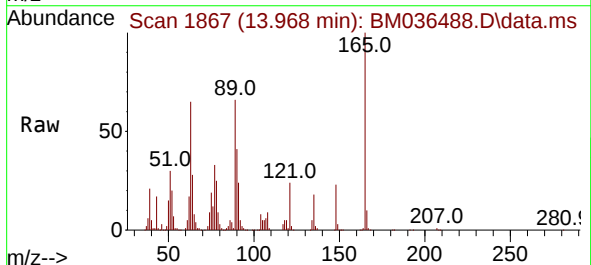




#50
Acenaphthylene
Concen: 18.545 ng/ul
RT: 14.092 min Scan# 1888
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:152 Resp: 1354275
Ion Ratio Lower Upper
152 100
151 20.1 16.1 24.1
153 13.2 10.6 15.8



#51
3-Nitroaniline
Concen: 19.476 ng/ul
RT: 14.298 min Scan# 1923
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:138 Resp: 205377
Ion Ratio Lower Upper
138 100
108 9.7 8.1 12.1
92 115.5 90.4 135.6





#52

Acenaphthene

Concen: 18.558 ng/ul

RT: 14.433 min Scan# 1946

Delta R.T. -0.006 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07

Instrument :

BNA_M

ClientSampleId :

SSTD020167





Tgt Ion:153 Resp: 883306

Ion Ratio Lower Upper

153 100

152 48.2 37.1 55.7

154 88.0 71.3 106.9

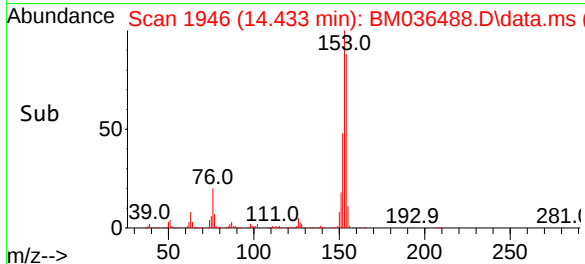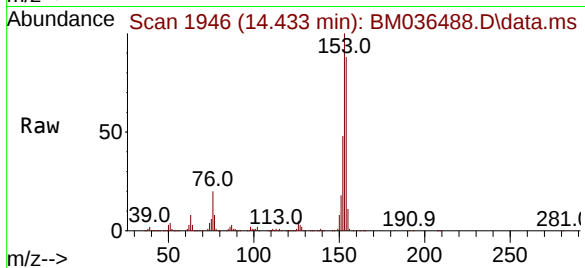

#53

2,4-Dinitrophenol

Concen: 22.550 ng/ul

RT: 14.510 min Scan# 1959

Delta R.T. -0.006 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07




Tgt Ion:184 Resp: 118503


Ion Ratio Lower Upper

184 100

63 75.6 54.2 81.4

154 67.6 49.3 73.9


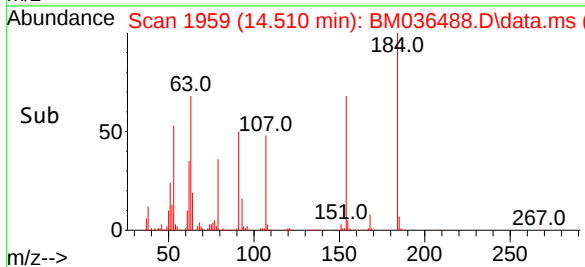

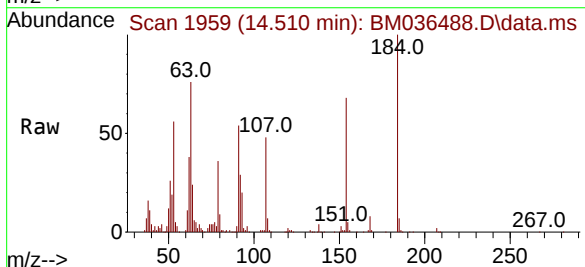




#55
4-Nitrophenol
Concen: 19.542 ng/ul
RT: 14.615 min Scan# 1977
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:109 Resp: 145258
Ion Ratio Lower Upper
109 100
139 134.5 124.9 187.3
65 132.0 122.2 183.4

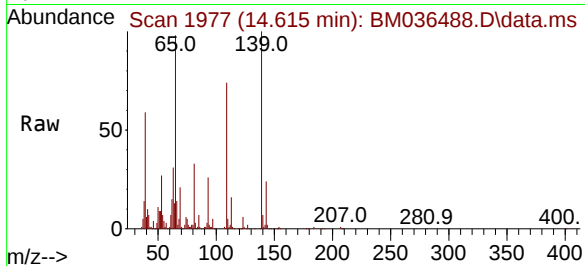

#56
Dibenzofuran
Concen: 18.701 ng/ul
RT: 14.774 min Scan# 2004
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:168 Resp: 1235115
Ion Ratio Lower Upper
168 100
139 39.1 30.1 45.1




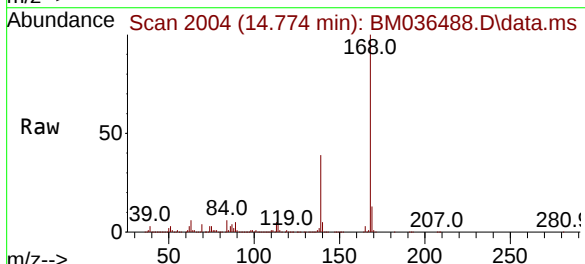




#57
2,4-Dinitrotoluene
Concen: 20.663 ng/ul
RT: 14.757 min Scan# 2001
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:165 Resp: 282575
Ion Ratio Lower Upper
165 100
63 54.9 35.9 53.9#
182 2.6 2.5 3.7

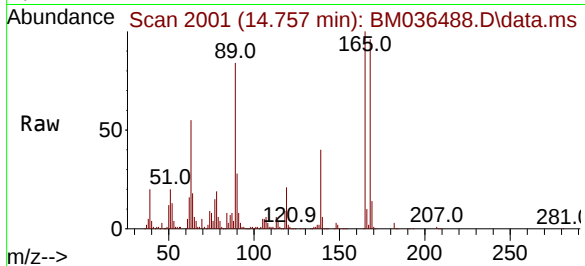

#58
2,3,4,6-Tetrachlorophenol
Concen: 19.934 ng/ul
RT: 15.004 min Scan# 2043
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:232 Resp: 219138
Ion Ratio Lower Upper
232 100
131 53.2 36.7 55.1
130 2.6 1.7 2.5#
166 31.9 24.4 36.6




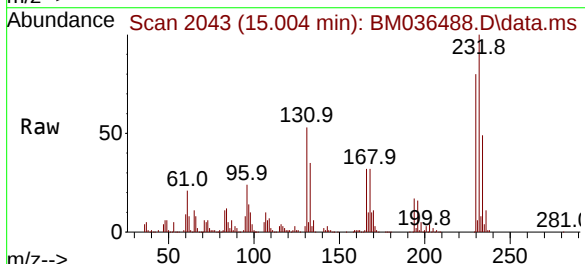




#59
Diethylphthalate
Concen: 20.486 ng/ul
RT: 15.204 min Scan# 2077
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:149 Resp: 1032070
Ion Ratio Lower Upper
149 100
177 20.5 16.8 25.2
150 12.4 10.2 15.4

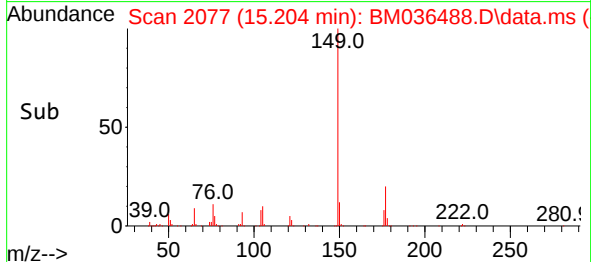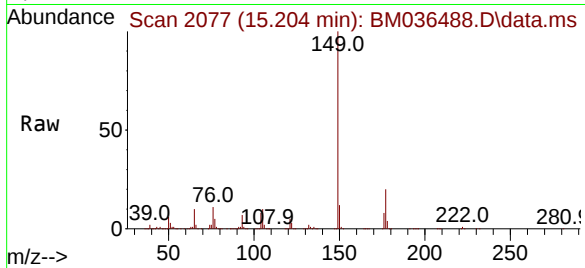

#61
Fluorene
Concen: 19.486 ng/ul
RT: 15.421 min Scan# 2114
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:166 Resp: 1020743
Ion Ratio Lower Upper
166 100
165 98.4 77.2 115.8
167 13.5 11.0 16.4




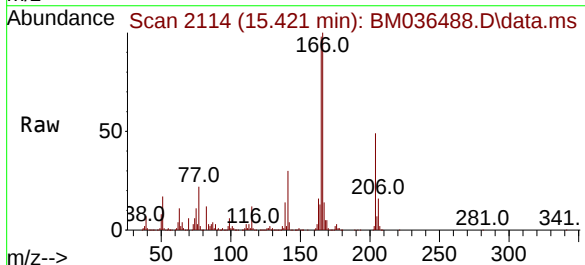




#62
4-Chlorophenyl-phenylether
Concen: 19.532 ng/ul
RT: 15.421 min Scan# 2114
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:204 Resp: 477952
Ion Ratio Lower Upper
204 100
206 32.7 25.9 38.9
141 61.5 50.6 75.8

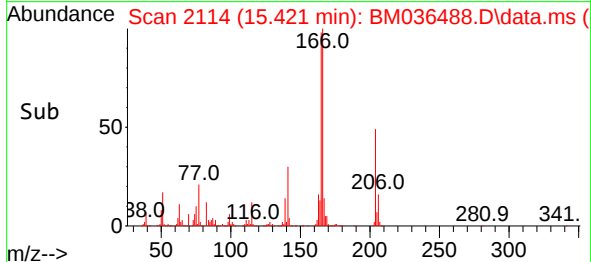

#63
4-Nitroaniline
Concen: 18.311 ng/ul
RT: 15.462 min Scan# 2121
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:138 Resp: 180124
Ion Ratio Lower Upper
138 100
92 50.8 39.2 58.8
108 80.9 51.6 77.4#




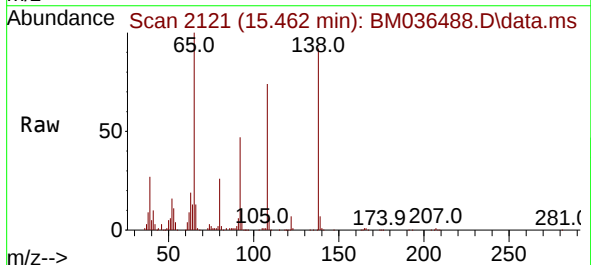




#66
4,6-Dinitro-2-methylphenol
Concen: 18.019 ng/ul
RT: 15.515 min Scan# 2130
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:198 Resp: 150127
Ion Ratio Lower Upper
198 100
182 4.8 4.2 6.4
77 29.5 19.9 29.9



#67
N-Nitrosodiphenylamine
Concen: 18.155 ng/ul
RT: 15.639 min Scan# 2151
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:169 Resp: 831975
Ion Ratio Lower Upper
169 100
168 68.3 53.8 80.6
167 38.1 28.7 43.1









#68
4-Bromophenyl-phenylether
Concen: 18.433 ng/ul
RT: 16.315 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:248 Resp: 273578
Ion Ratio Lower Upper
248 100
250 97.1 77.3 115.9
141 77.4 59.8 89.8

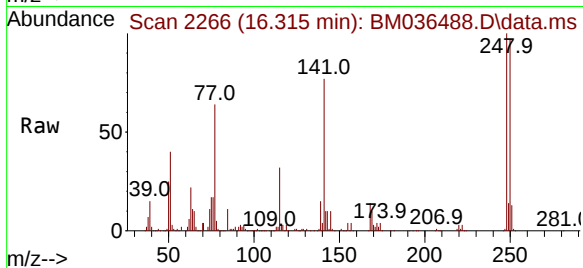

#69
Hexachlorobenzene
Concen: 18.138 ng/ul
RT: 16.415 min Scan# 2283
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:284 Resp: 326245
Ion Ratio Lower Upper
284 100
142 42.2 28.6 42.8
249 30.2 24.6 37.0

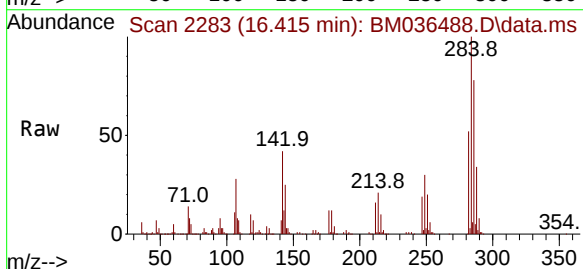



#70

Atrazine

Concen: 18.639 ng/ul

RT: 16.598 min Scan# 21

Delta R.T. -0.000 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07

Instrument :

BNA_M

ClientSampleId :

SSTD020167





Tgt Ion:200 Resp: 291846

Ion Ratio Lower Upper

200 100

173 26.7 21.3 31.9

215 47.2 39.0 58.6

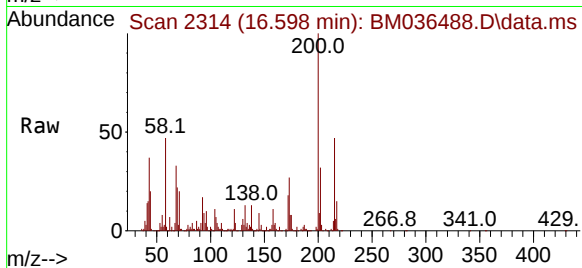

#71

Pentachlorophenol

Concen: 21.597 ng/ul

RT: 16.768 min Scan# 2343

Delta R.T. -0.006 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07




Tgt Ion:266 Resp: 214160


Ion Ratio Lower Upper

266 100

264 63.3 49.5 74.3

268 62.9 51.0 76.4

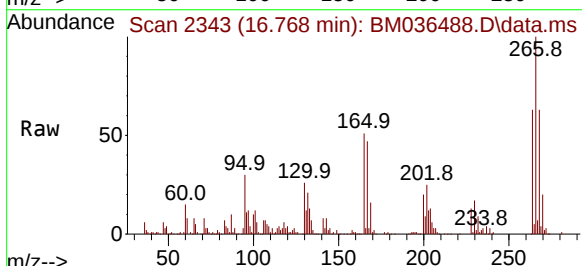



#72

Phenanthrene

Concen: 18.582 ng/ul

RT: 17.162 min Scan# 2410

Delta R.T. -0.000 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07

Instrument :

BNA_M

ClientSampleId :

SSTD020167





Tgt Ion:178 Resp: 1565794

Ion Ratio Lower Upper

178 100

179 15.2 12.2 18.2

176 19.7 14.9 22.3



#74

Anthracene

Concen: 18.963 ng/ul

RT: 17.251 min Scan# 2425

Delta R.T. -0.006 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07




Tgt Ion:178 Resp: 1602008


Ion Ratio Lower Upper

178 100

179 15.7 12.2 18.2

176 19.2 14.4 21.6


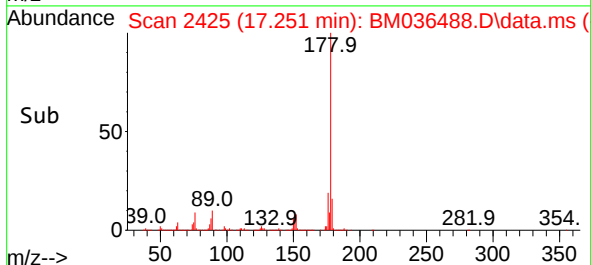
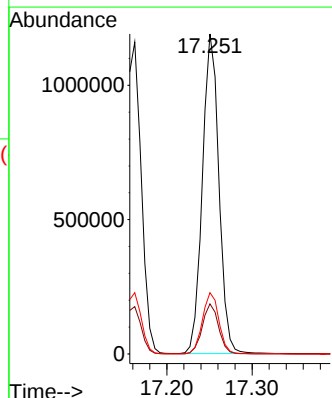





#75
1,2,3,4-Tetrachlorobenzene
Concen: 16.200 ng/uL
RT: 13.168 min Scan# 1731
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:216 Resp: 389630
Ion Ratio Lower Upper
216 100
214 79.0 60.9 91.3
218 48.5 37.5 56.3

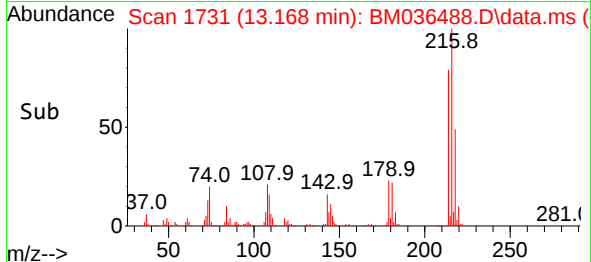

#76
Pentachlorobenzene
Concen: 17.276 ng/uL
RT: 14.686 min Scan# 1989
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:250 Resp: 387961
Ion Ratio Lower Upper
250 100
248 63.8 50.4 75.6
252 62.3 51.1 76.7


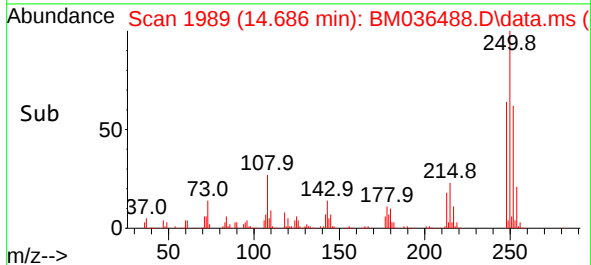






#77
 Carbazole
 Concen: 18.488 ng/ul
 RT: 17.533 min Scan# 2473
 Delta R.T. -0.000 min
 Lab File: BM036488.D
 Acq: 02 Sep 2022 13:07




Instrument :
 BNA_M
 ClientSampleId :
 SST020167


Tgt Ion:167 Resp: 1462368
 Ion Ratio Lower Upper
 167 100
 166 21.6 17.4 26.0
 139 13.7 10.1 15.1

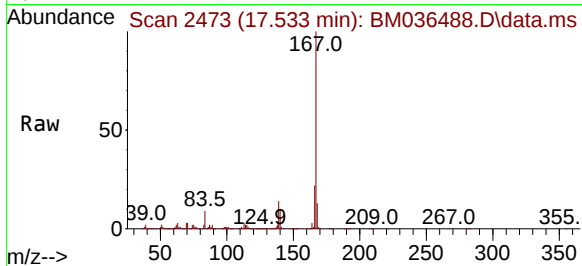

#78
 Di-n-butylphthalate
 Concen: 20.763 ng/ul
 RT: 18.098 min Scan# 2569
 Delta R.T. -0.000 min
 Lab File: BM036488.D
 Acq: 02 Sep 2022 13:07

Tgt Ion:149 Resp: 1796321
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.3 10.9
 104 5.1 3.7 5.5




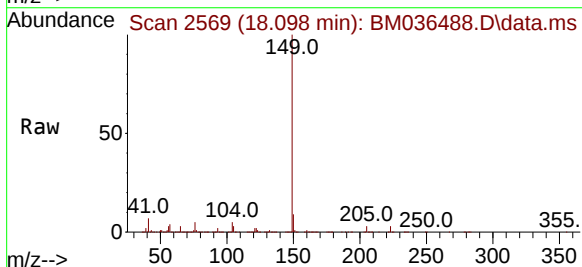




#80
Fluoranthene
Concen: 18.115 ng/ul
RT: 19.180 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:202 Resp: 1830043
Ion Ratio Lower Upper
202 100
101 12.0 10.1 15.1
100 9.4 7.8 11.6



#82
Pyrene
Concen: 18.126 ng/ul
RT: 19.545 min Scan# 2815
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:202 Resp: 1910851
Ion Ratio Lower Upper
202 100
101 13.9 11.9 17.9
100 11.8 10.2 15.4









#83
Butylbenzylphthalate
Concen: 19.707 ng/ul
RT: 20.456 min Scan# 2969
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:149 Resp: 777228
Ion Ratio Lower Upper
149 100
91 71.0 53.2 79.8
206 18.3 16.0 24.0

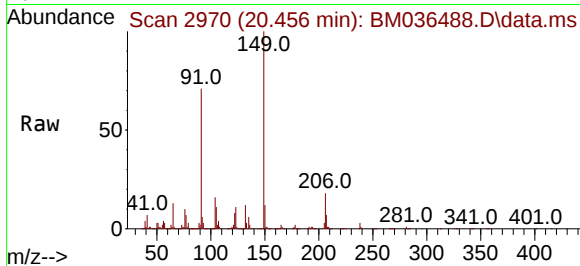

#84
3,3'-Dichlorobenzidine
Concen: 17.139 ng/ul
RT: 21.233 min Scan# 3102
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:252 Resp: 568730
Ion Ratio Lower Upper
252 100
254 63.6 52.4 78.6
126 13.9 10.8 16.2




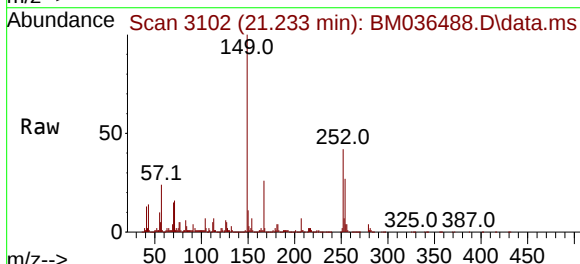




#85
Benzo(a)anthracene
Concen: 18.859 ng/ul
RT: 21.297 min Scan# 3112
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:228 Resp: 1826268
Ion Ratio Lower Upper
228 100
229 19.7 15.6 23.4
226 27.5 21.7 32.5

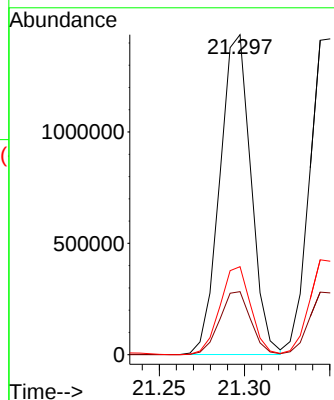

#86
Bis(2-ethylhexyl)phthalate
Concen: 22.187 ng/ul
RT: 21.233 min Scan# 3102
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:149 Resp: 1208190
Ion Ratio Lower Upper
149 100
167 26.2 21.5 32.3
279 3.8 3.4 5.2



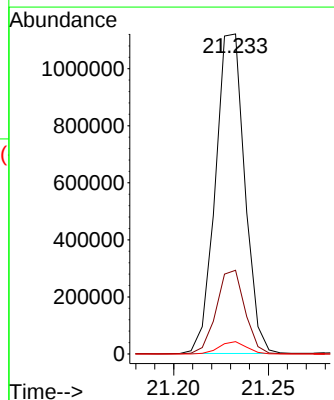





#87
Chrysene
Concen: 18.409 ng/u1
RT: 21.350 min Scan# 3121
Delta R.T. 0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:228 Resp: 1751653
Ion Ratio Lower Upper
228 100
226 29.6 23.7 35.5
229 19.6 15.5 23.3

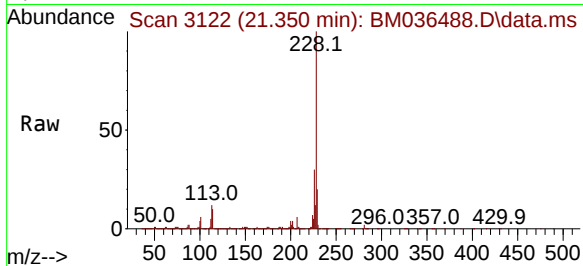

#89
Di-n-octyl phthalate
Concen: 21.515 ng/u1
RT: 22.121 min Scan# 3253
Delta R.T. -0.000 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:149 Resp: 1958377




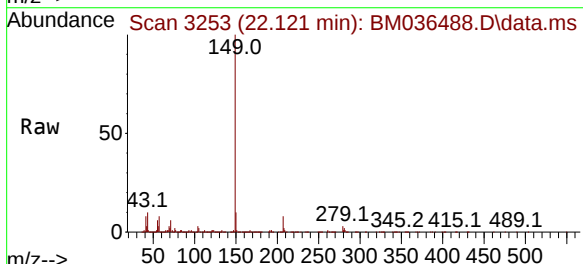




#90
Benzo(b)fluoranthene
Concen: 18.974 ng/ul
RT: 22.903 min Scan# 3386
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07




Instrument :
BNA_M
ClientSampleId :
SSTD020167


Tgt Ion:252 Resp: 1771322
Ion Ratio Lower Upper
252 100
253 22.5 17.5 26.3
125 12.1 10.7 16.1



#91
Benzo(k)fluoranthene
Concen: 19.350 ng/ul
RT: 22.950 min Scan# 3394
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:252 Resp: 1718631
Ion Ratio Lower Upper
252 100
253 21.9 17.4 26.0
125 11.8 10.6 15.8





#93

Benzo(a)pyrene

Concen: 18.790 ng/ul

RT: 23.503 min Scan# 34

Delta R.T. -0.000 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07

Instrument :

BNA_M

ClientSampleId :

SSTD020167





Tgt Ion:252 Resp: 1725699

Ion Ratio Lower Upper

252 100

253 21.6 17.3 25.9

125 12.6 11.8 17.8

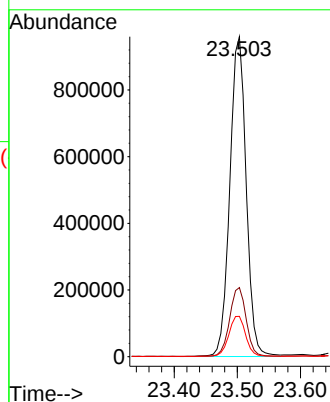

#94

Indeno(1,2,3-cd)pyrene

Concen: 16.425 ng/ul

RT: 25.968 min Scan# 3907

Delta R.T. -0.000 min

Lab File: BM036488.D

Acq: 02 Sep 2022 13:07




Tgt Ion:276 Resp: 1773531


Ion Ratio Lower Upper

276 100

138 28.4 25.6 38.4

277 25.2 20.1 30.1









#95
Dibenzo(a,h)anthracene
Concen: 16.445 ng/ul
RT: 25.979 min Scan# 3909
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Instrument :
BNA_M
ClientSampleId :
SSTD020167

Tgt Ion:278 Resp: 1529674
Ion Ratio Lower Upper
278 100
139 18.4 16.2 24.2
279 23.6 18.7 28.1



#96
Benzo(g,h,i)perylene
Concen: 15.805 ng/ul
RT: 26.691 min Scan# 4030
Delta R.T. -0.006 min
Lab File: BM036488.D
Acq: 02 Sep 2022 13:07

Tgt Ion:276 Resp: 1459440
Ion Ratio Lower Upper
276 100
138 24.6 21.3 31.9
277 23.8 18.6 28.0

