

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
 Data File : BM036485.D
 Acq On : 02 Sep 2022 10:59
 Operator : CG/JU
 Sample : N4441-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN58

Quant Time: Sep 02 23:15:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 02 01:33:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	192525	20.000	ng/u1	0.00
20) Naphthalene-d8	10.522	136	880211	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.374	164	537368	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.121	188	1093881	20.000	ng/u1	0.00
79) Chrysene-d12	21.303	240	1064842	20.000	ng/u1	0.00
88) Perylene-d12	23.591	264	1034508	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.128	96	30521	6.042	ng/uL	0.00
4) Pyridine-d5	3.563	84	155866	11.188	ng/u1	0.00
7) Phenol-d5	6.904	99	161427	9.823	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	510465	49.348	ng/u1	0.00
11) 2-Chlorophenol-d4	7.251	132	464483	35.973	ng/u1	0.00
15) 4-Methylphenol-d8	8.445	113	299257	24.389	ng/u1	0.00
21) Nitrobenzene-d5	8.892	128	311236	46.637	ng/u1	0.00
24) 2-Nitrophenol-d4	9.610	143	305103	45.071	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.151	165	484766	40.078	ng/u1	0.00
31) 4-Chloroaniline-d4	10.675	131	512541	27.334	ng/u1	0.00
46) Dimethylphthalate-d6	13.798	166	1721264	50.631	ng/u1	0.00
49) Acenaphthylene-d8	14.069	160	2068916	48.793	ng/u1	0.00
54) 4-Nitrophenol-d4	14.604	143	42284	6.564	ng/u1	0.00
60) Fluorene-d10	15.368	176	1590335	51.769	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.504	200	229796	40.861	ng/u1	0.00
73) Anthracene-d10	17.221	188	2602086	53.498	ng/u1	0.00
81) Pyrene-d10	19.515	212	2979204	53.934	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.450	264	2714040	53.509	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.163	88	10267	1.930 ng/uL	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
Data File : BM036485.D
Acq On : 02 Sep 2022 10:59
Operator : CG/JU
Sample : N4441-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN58

Quant Time: Sep 02 23:15:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 02 01:33:23 2022
Response via : Initial Calibration

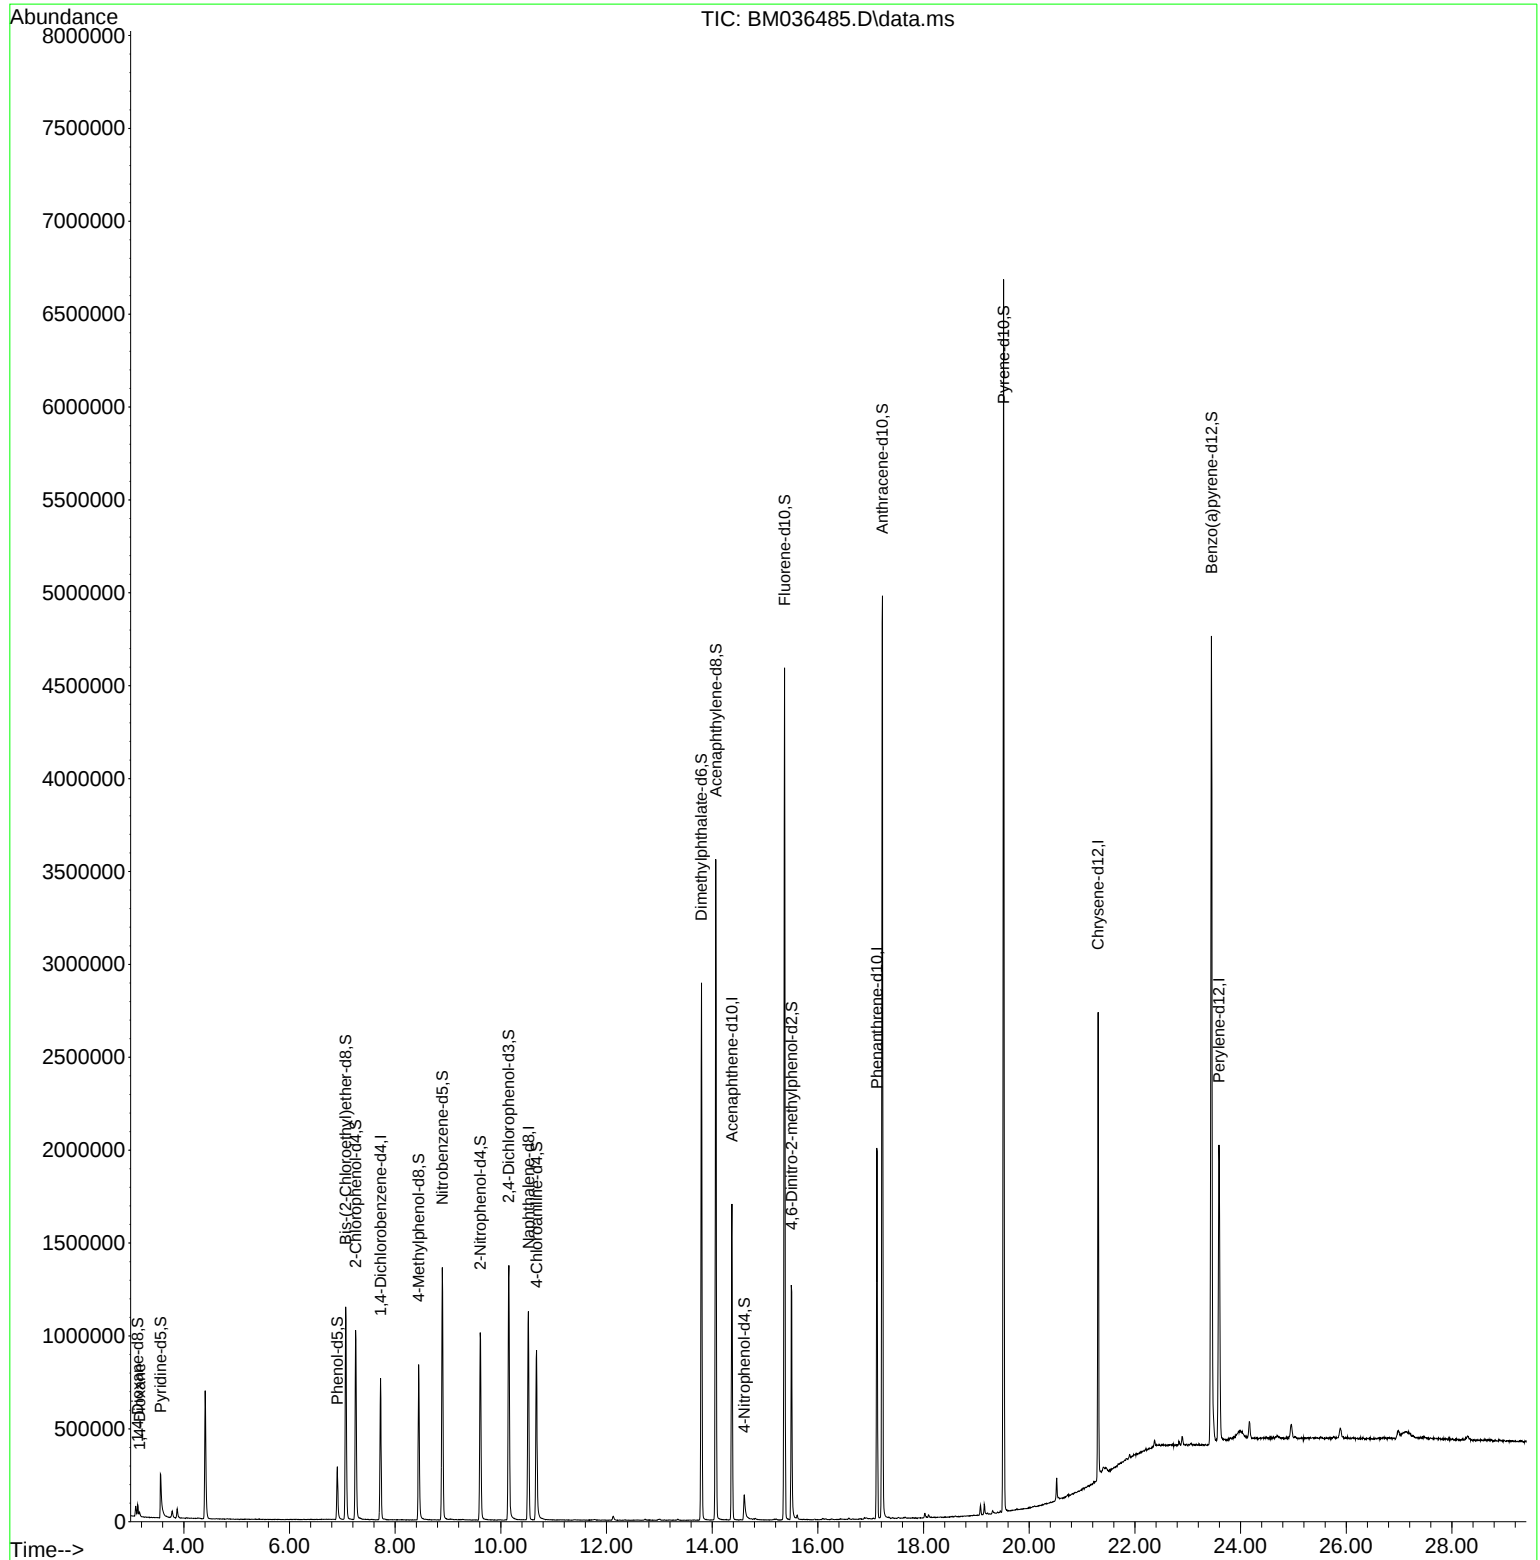

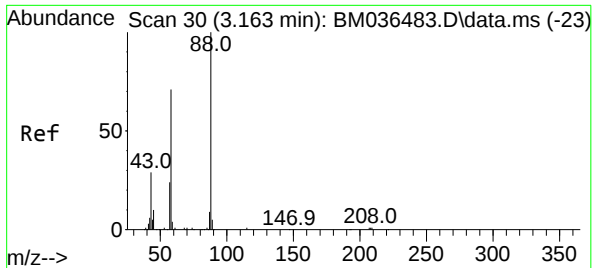

1,4-Dioxane
 Concen: 1.930 ng/uL
 RT: 3.163 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BM036485.D
 Acq: 02 Sep 2022 10:59

Instrument :
 BNA_M
 ClientSampleId :
 BGN58

Tgt Ion:	88	Resp:	10267
Ion	Ratio	Lower	Upper
88	100		
43	36.3	27.8	41.8
58	68.1	61.8	92.8

