

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
 Data File : BM036484.D
 Acq On : 02 Sep 2022 10:23
 Operator : CG/JU
 Sample : PB147414BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK414

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	32	rVB	53145	73954	1.49%	0.155%
2	3.558	93	97	116	rBV	534548	991022	20.02%	2.074%
3	3.875	148	151	157	rVB	13650	17458	0.35%	0.037%
4	6.457	585	590	594	rBV6	2840	5444	0.11%	0.011%
5	6.904	659	666	682	rBV	702092	1165534	23.55%	2.440%
6	7.063	687	693	709	rVB	612654	965570	19.51%	2.021%
7	7.251	719	725	746	rVB	722898	1183967	23.92%	2.478%
8	7.722	798	805	814	rBV	601748	934719	18.88%	1.957%
9	8.445	921	928	948	rBV	895560	1452228	29.34%	3.040%
10	8.892	997	1004	1018	rBV	732685	1185986	23.96%	2.482%
11	9.610	1118	1126	1140	rBV	580550	955097	19.29%	1.999%
12	10.151	1210	1218	1238	rBV	817148	1444683	29.19%	3.024%
13	10.522	1273	1281	1292	rVB	885897	1467937	29.65%	3.073%
14	10.675	1300	1307	1330	rBV	767544	1406141	28.41%	2.943%
15	11.769	1492	1493	1500	rVB6	3672	5231	0.11%	0.011%
16	12.133	1547	1555	1561	rBV3	11004	24378	0.49%	0.051%
17	13.798	1831	1838	1852	rBV	1635228	2177404	43.99%	4.558%
18	14.069	1877	1884	1894	rBV	1950726	2724481	55.04%	5.703%
19	14.374	1927	1936	1947	rBV	1395189	1977435	39.95%	4.139%
20	14.598	1969	1974	1995	rBV	587109	1059469	21.40%	2.218%
21	15.369	2097	2105	2116	rBV	2589037	3483707	70.38%	7.292%
22	15.498	2122	2127	2142	rBV	654635	984751	19.89%	2.061%
23	15.610	2142	2146	2151	rVB4	11964	19454	0.39%	0.041%
24	16.586	2308	2312	2318	rBV4	5533	9498	0.19%	0.020%
25	16.886	2356	2363	2364	rBV4	6234	8563	0.17%	0.018%
26	16.904	2364	2366	2374	rVB8	4766	10480	0.21%	0.022%
27	17.115	2396	2402	2412	rBV	1741332	2359681	47.67%	4.939%
28	17.215	2412	2419	2438	rVV	2841854	3921369	79.22%	8.208%
29	17.657	2490	2494	2496	rBV4	4872	5095	0.10%	0.011%
30	19.080	2732	2736	2741	rBV3	29866	42267	0.85%	0.088%
31	19.151	2744	2748	2754	rVV2	29524	41789	0.84%	0.087%
32	19.515	2804	2810	2823	rBV	3627682	4602738	92.98%	9.634%
33	20.521	2977	2981	2987	rBV	147175	195322	3.95%	0.409%
34	21.309	3110	3115	3123	rBV	2418139	3043193	61.48%	6.370%
35	23.450	3472	3479	3493	rBV2	2606923	4950054	100.00%	10.361%
36	23.597	3498	3504	3516	rVB2	1515206	2878672	58.15%	6.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
Data File : BM036484.D
Acq On : 02 Sep 2022 10:23
Operator : CG/JU
Sample : PB147414BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK414

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Title : SVOA CALIBRATION




Sum of corrected areas: 47774771

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
Data File : BM036484.D
Acq On : 02 Sep 2022 10:23
Operator : CG/JU
Sample : PB147414BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

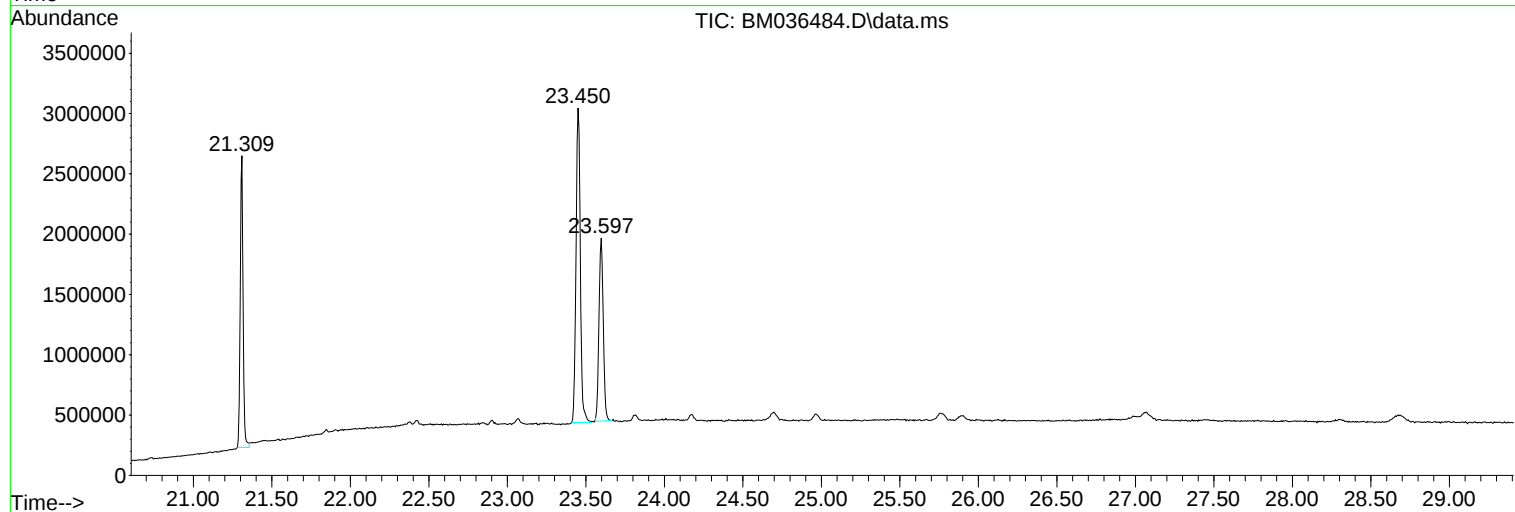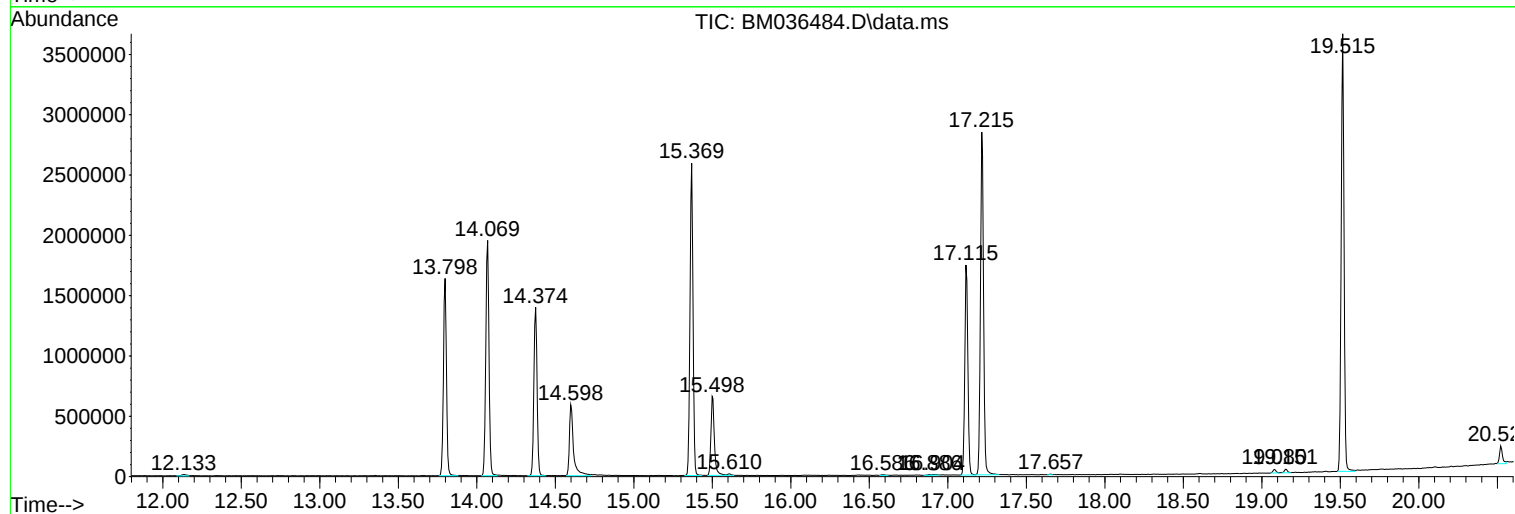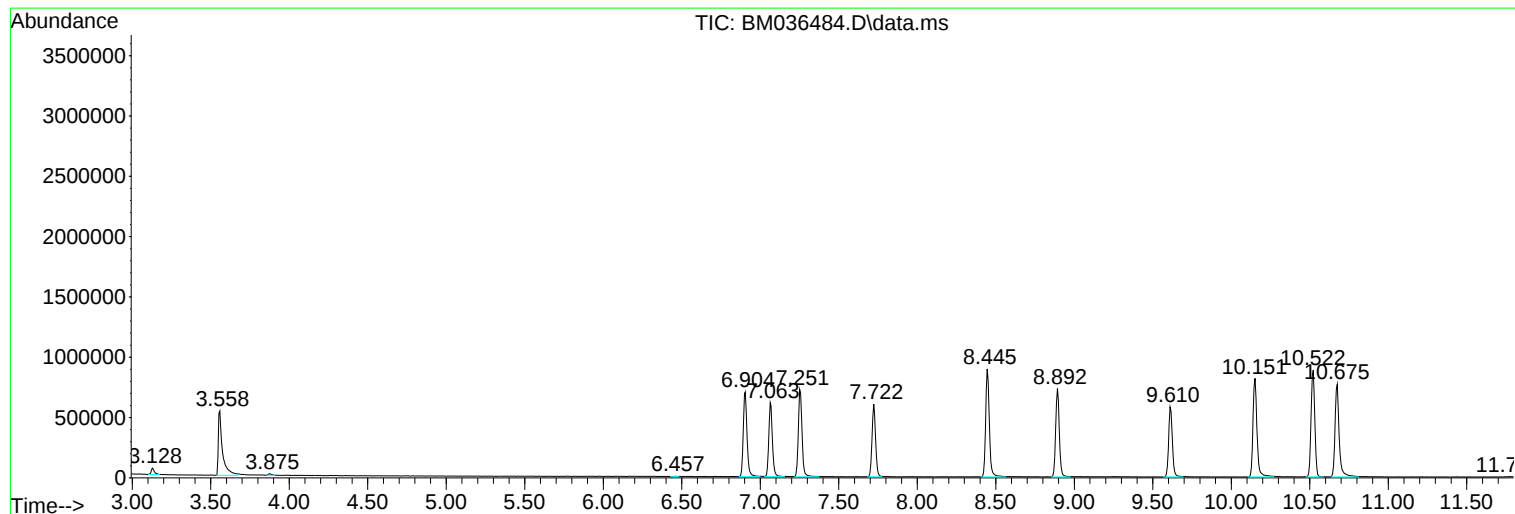

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
Data File : BM036484.D
Acq On : 02 Sep 2022 10:23
Operator : CG/JU
Sample : PB147414BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
Data File : BM036484.D
Acq On : 02 Sep 2022 10:23
Operator : CG/JU
Sample : PB147414BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc