

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
 Data File : BM036485.D
 Acq On : 02 Sep 2022 10:59
 Operator : CG/JU
 Sample : N4441-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	14	18	21	rBV	53229	76941	0.96%	0.111%
2	3.128	21	24	28	rVV	64071	86392	1.08%	0.124%
3	3.163	28	30	41	rVB	25814	35401	0.44%	0.051%
4	3.557	94	97	116	rBV	237541	464010	5.79%	0.668%
5	3.781	130	135	144	rVB	37271	64303	0.80%	0.093%
6	3.875	146	151	156	rBV	49545	71132	0.89%	0.102%
7	4.404	235	241	256	rVB	688810	1051525	13.11%	1.513%
8	6.904	660	666	683	rBV	284387	472178	5.89%	0.679%
9	7.063	687	693	705	rVV	1143482	1784083	22.24%	2.567%
10	7.251	717	725	737	rBV	1019663	1652064	20.60%	2.377%
11	7.334	737	739	746	rVB5	8192	13803	0.17%	0.020%
12	7.722	798	805	814	rBV	762215	1179780	14.71%	1.697%
13	8.445	922	928	941	rBV	836530	1345101	16.77%	1.935%
14	8.892	996	1004	1015	rBV	1358667	2174298	27.11%	3.128%
15	9.610	1119	1126	1143	rBV	1010249	1676493	20.90%	2.412%
16	10.151	1211	1218	1235	rBV	1370031	2353514	29.34%	3.386%
17	10.522	1273	1281	1291	rBV	1121568	1825811	22.76%	2.627%
18	10.675	1299	1307	1336	rBV	912473	1680022	20.95%	2.417%
19	11.769	1491	1493	1501	rVB6	4366	9877	0.12%	0.014%
20	12.127	1548	1554	1566	rVB	21618	45295	0.56%	0.065%
21	12.727	1650	1656	1661	rBV6	5791	9103	0.11%	0.013%
22	13.010	1696	1704	1709	rVB8	5358	14852	0.19%	0.021%
23	13.798	1831	1838	1852	rBV	2890972	3823329	47.67%	5.501%
24	14.069	1877	1884	1902	rBV	3555585	4911315	61.23%	7.066%
25	14.374	1929	1936	1944	rBV	1700373	2393968	29.85%	3.444%
26	14.610	1970	1976	1996	rBV	133971	320648	4.00%	0.461%
27	14.816	2009	2011	2017	rVB6	6708	8993	0.11%	0.013%
28	15.210	2075	2078	2085	rVB6	5752	9687	0.12%	0.014%
29	15.368	2094	2105	2115	rBV	4587603	6135287	76.49%	8.827%
30	15.498	2121	2127	2142	rBV	1262384	1788382	22.30%	2.573%
31	15.610	2142	2146	2156	rVB2	23184	40128	0.50%	0.058%
32	16.098	2224	2229	2235	rBV8	5785	13659	0.17%	0.020%
33	16.586	2308	2312	2316	rBV3	7103	9818	0.12%	0.014%
34	16.880	2359	2362	2365	rBV5	8305	11148	0.14%	0.016%
35	17.115	2396	2402	2411	rBV	1996478	2749012	34.27%	3.955%
36	17.221	2413	2420	2436	rVV	4962239	6909065	86.14%	9.941%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
 Data File : BM036485.D
 Acq On : 02 Sep 2022 10:59
 Operator : CG/JU
 Sample : N4441-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

37	17.527	2468	2472	2478	rVB7	5335	9275	0.12%	0.013%
38	18.021	2550	2556	2564	rBV5	26069	50888	0.63%	0.073%
39	18.092	2566	2568	2573	rVV	14235	18510	0.23%	0.027%
40	18.598	2652	2654	2660	rVB7	5380	8153	0.10%	0.012%
41	19.080	2731	2736	2740	rBV2	55194	74579	0.93%	0.107%
42	19.151	2744	2748	2753	rBV	56784	75157	0.94%	0.108%
43	19.309	2771	2775	2778	rBV5	16595	23907	0.30%	0.034%
44	19.451	2797	2799	2804	rBV6	8448	9396	0.12%	0.014%
45	19.515	2804	2810	2818	rBV	6635020	8020805	100.00%	11.540%
46	20.521	2977	2981	2985	rBV	115723	133423	1.66%	0.192%
47	21.303	3109	3114	3121	rBV	2521559	3123272	38.94%	4.494%
48	23.450	3472	3479	3492	rVB2	4330697	7749126	96.61%	11.149%
49	23.591	3497	3503	3517	rVB2	1589953	2995864	37.35%	4.310%




Sum of corrected areas: 69502772

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
Data File : BM036485.D
Acq On : 02 Sep 2022 10:59
Operator : CG/JU
Sample : N4441-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN58

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

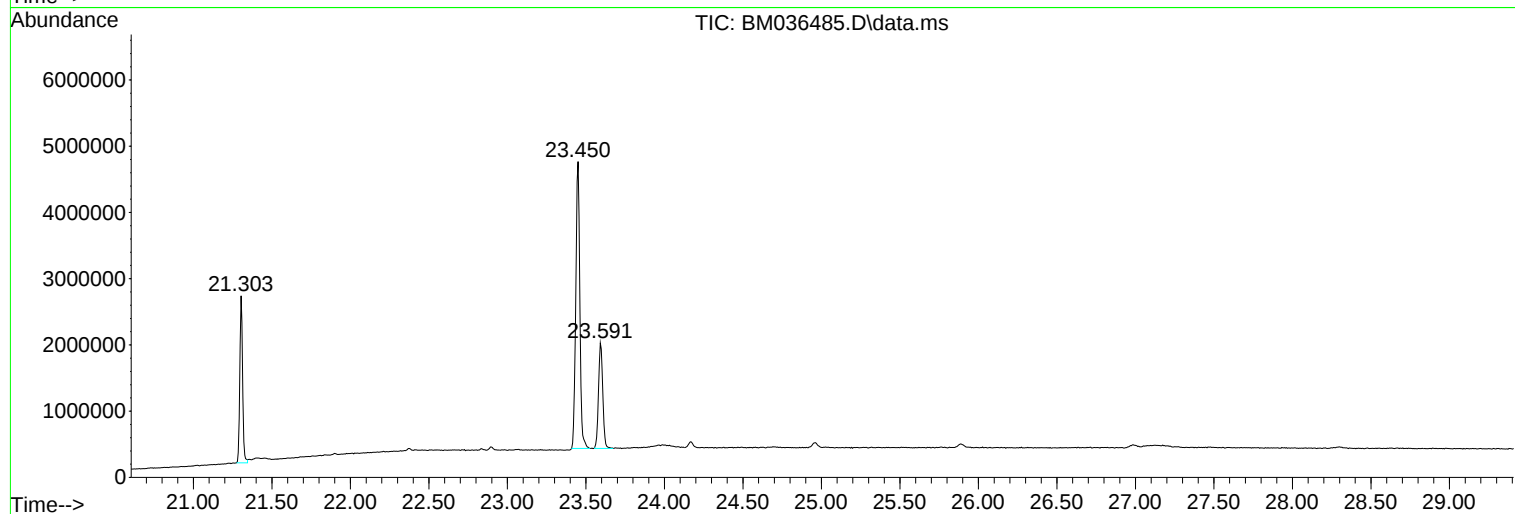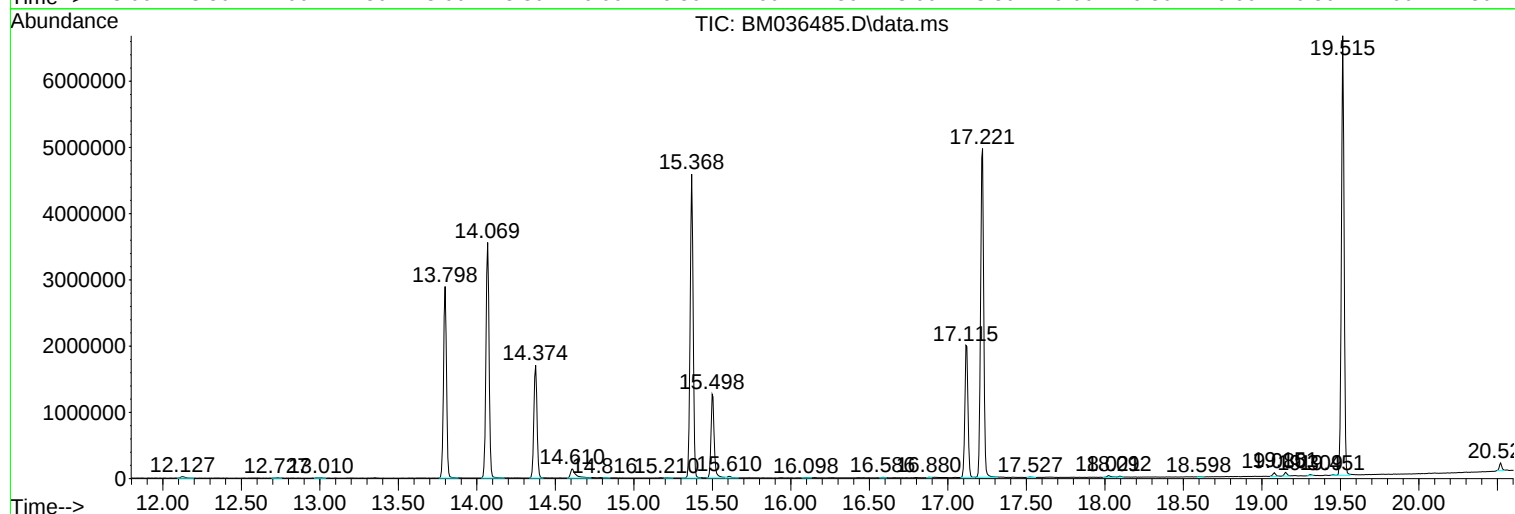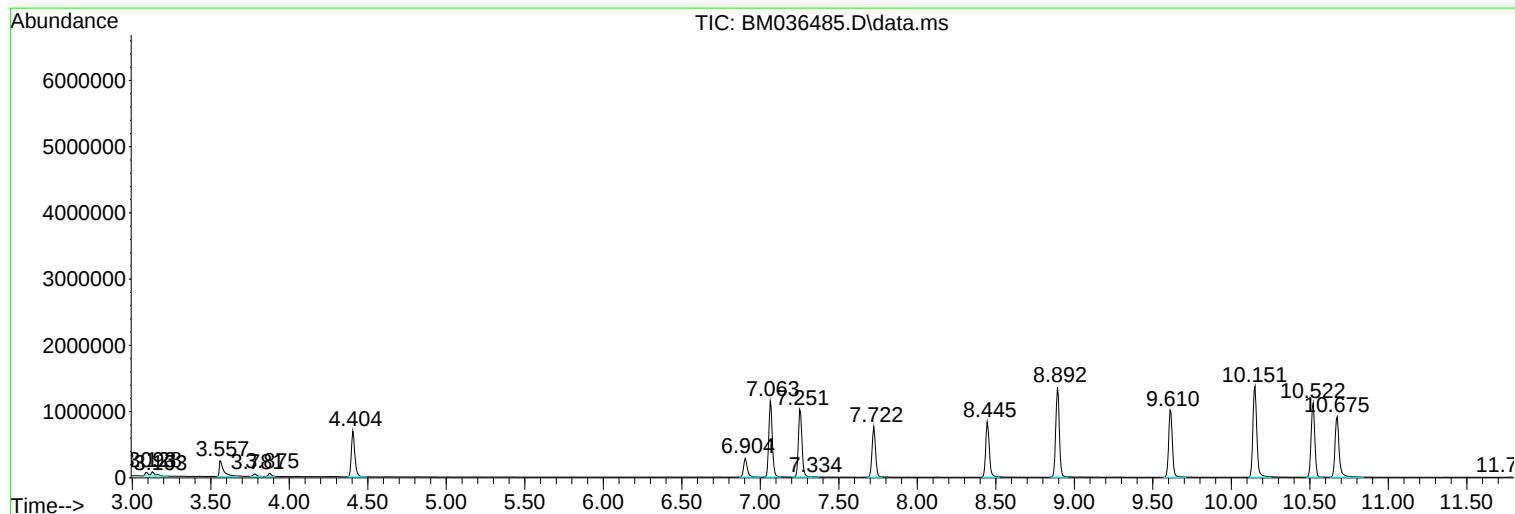

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
Data File : BM036485.D
Acq On : 02 Sep 2022 10:59
Operator : CG/JU
Sample : N4441-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN58










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.404	17.83 ng/ul	1051530	1,4-Dichlorobenzene-d4	7.722

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

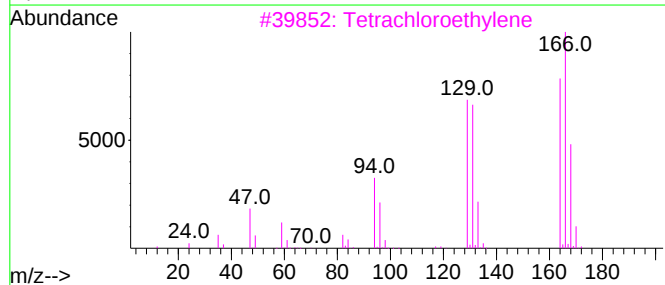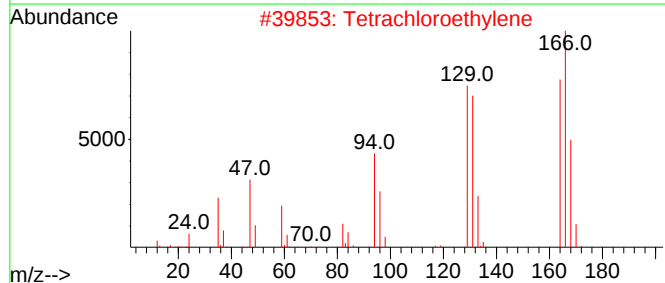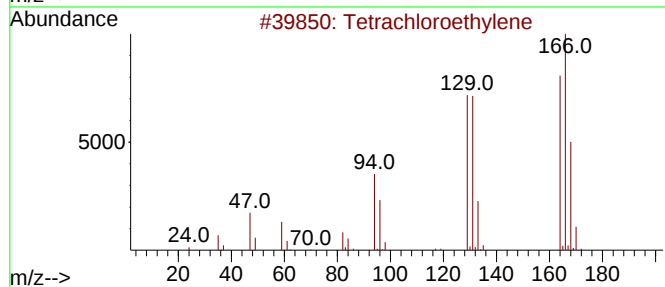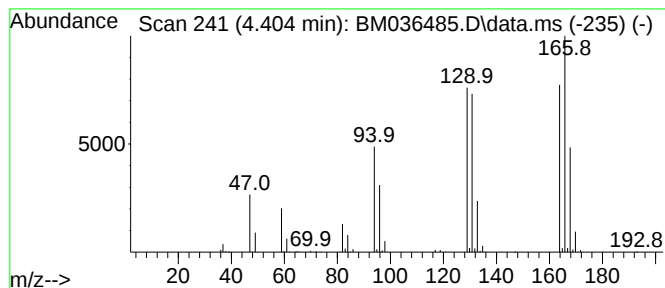

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090222\
Data File : BM036485.D
Acq On : 02 Sep 2022 10:59
Operator : CG/JU
Sample : N4441-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN58

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.404	17.8	ng/ul	1051530	1	7.722	1179780	20.0