

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090322\
 Data File : BM036492.D
 Acq On : 02 Sep 2022 15:36
 Operator : CG/JU
 Sample : N4441-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN58

Quant Time: Sep 02 16:07:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM083022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 29 17:45:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.733	152	3967	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.523	136	15428	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.376	164	9161	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.123	188	19620	0.400	ng/ul	0.00
17) Chrysene-d12	21.318	240	18158	0.400	ng/ul	# 0.00
23) Perylene-d12	23.607	264	18161	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	33957	5.892	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.134	152	10797	0.449	ng/ul	0.00
18) Fluoranthene-d10	19.154	212	26848	0.475	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.168	88	9714	1.774	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090322\
Data File : BM036492.D
Acq On : 02 Sep 2022 15:36
Operator : CG/JU
Sample : N4441-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN58

Quant Time: Sep 02 16:07:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM083022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 29 17:45:20 2022
Response via : Initial Calibration

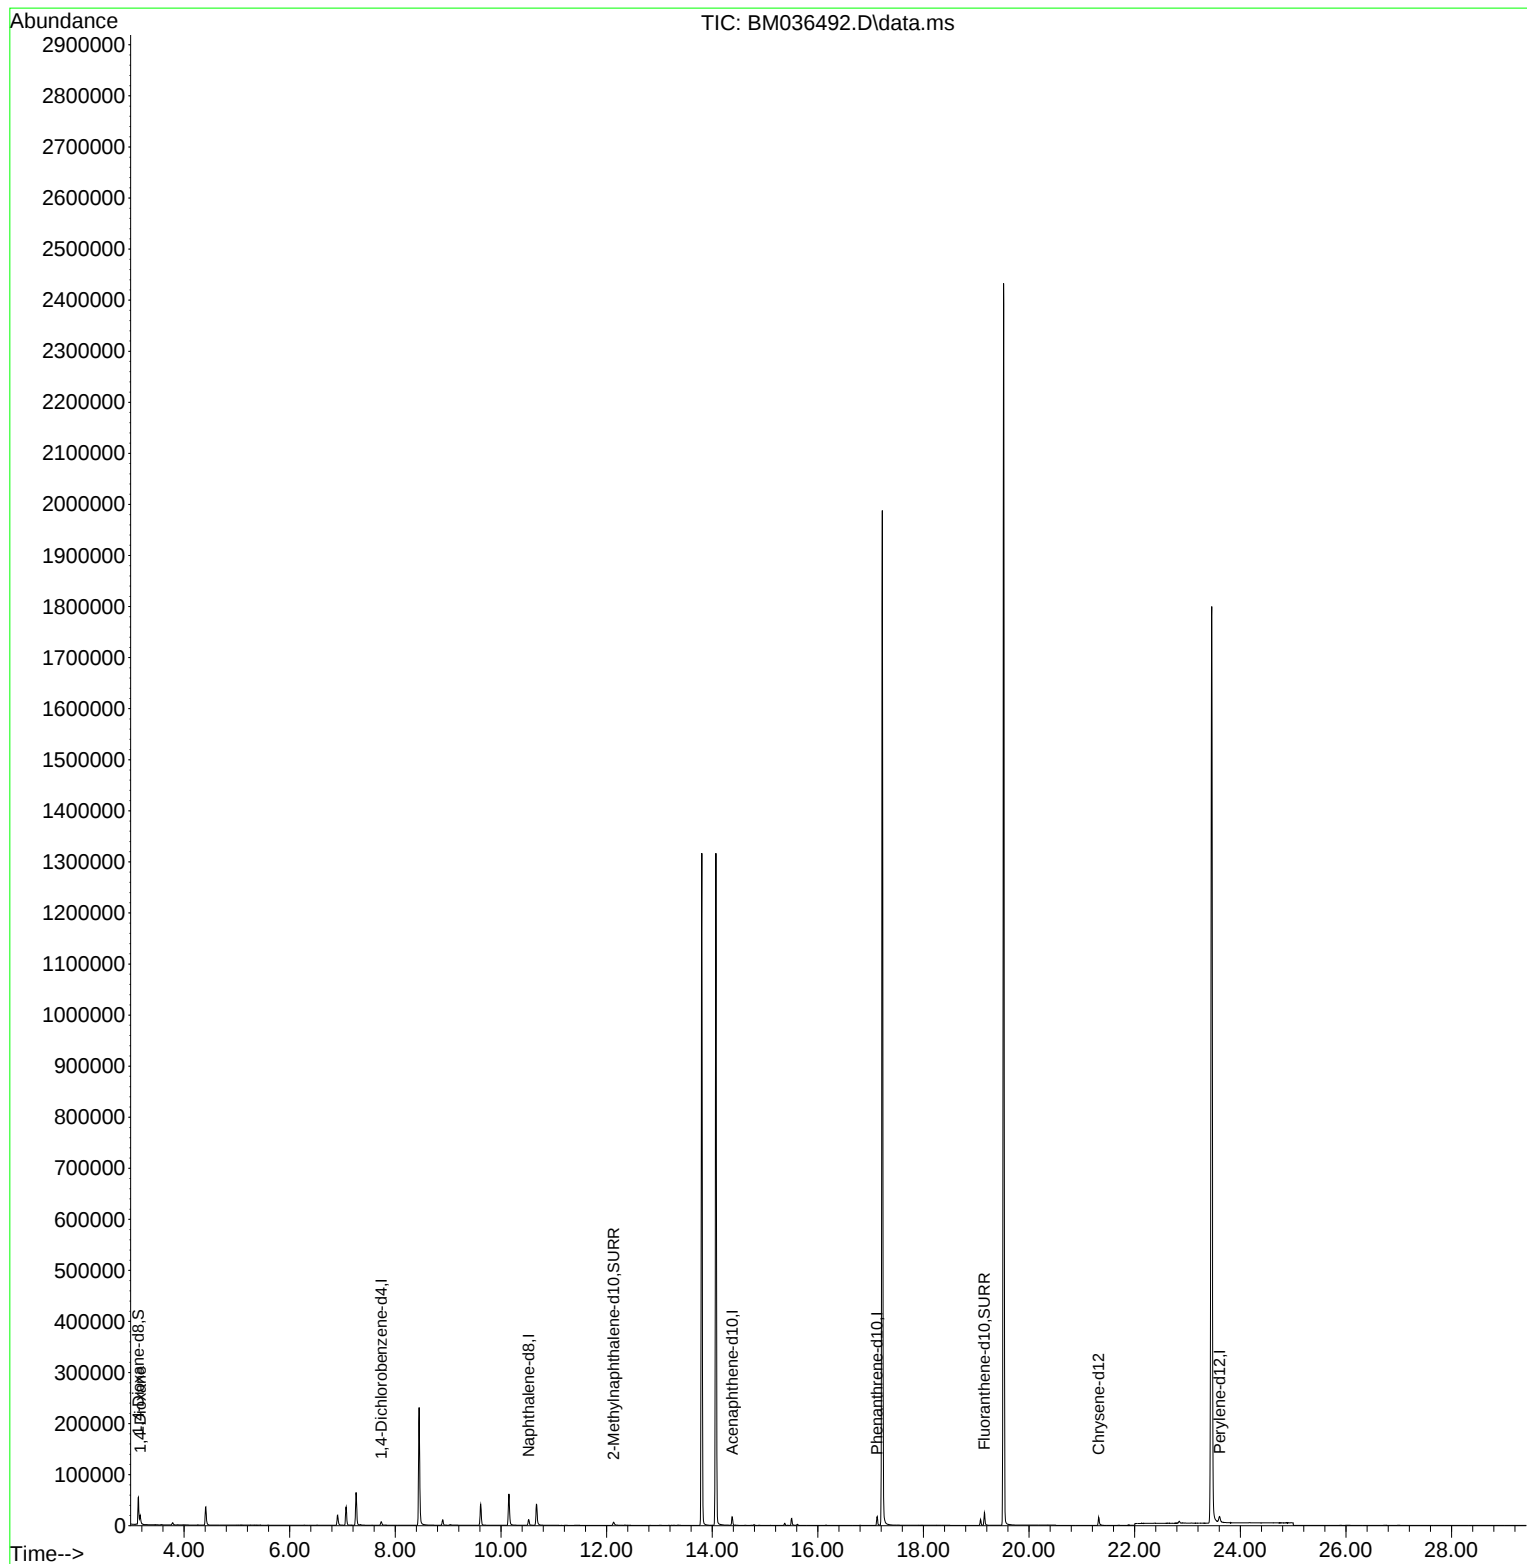

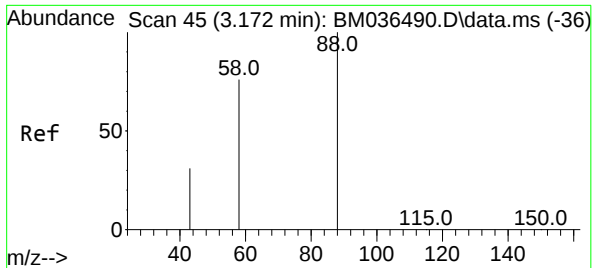

#2
 1,4-Dioxane
 Concen: 1.774 ng/ul
 RT: 3.168 min Scan# 44
 Delta R.T. -0.013 min
 Lab File: BM036492.D
 Acq: 02 Sep 2022 15:36

Instrument :
 BNA_M
 ClientSampleId :
 BGN58

Tgt Ion: 88 Resp: 9714

Ion	Ratio	Lower	Upper
88	100		
43	34.2	37.8	56.6#
58	67.8	42.6	63.8#

