
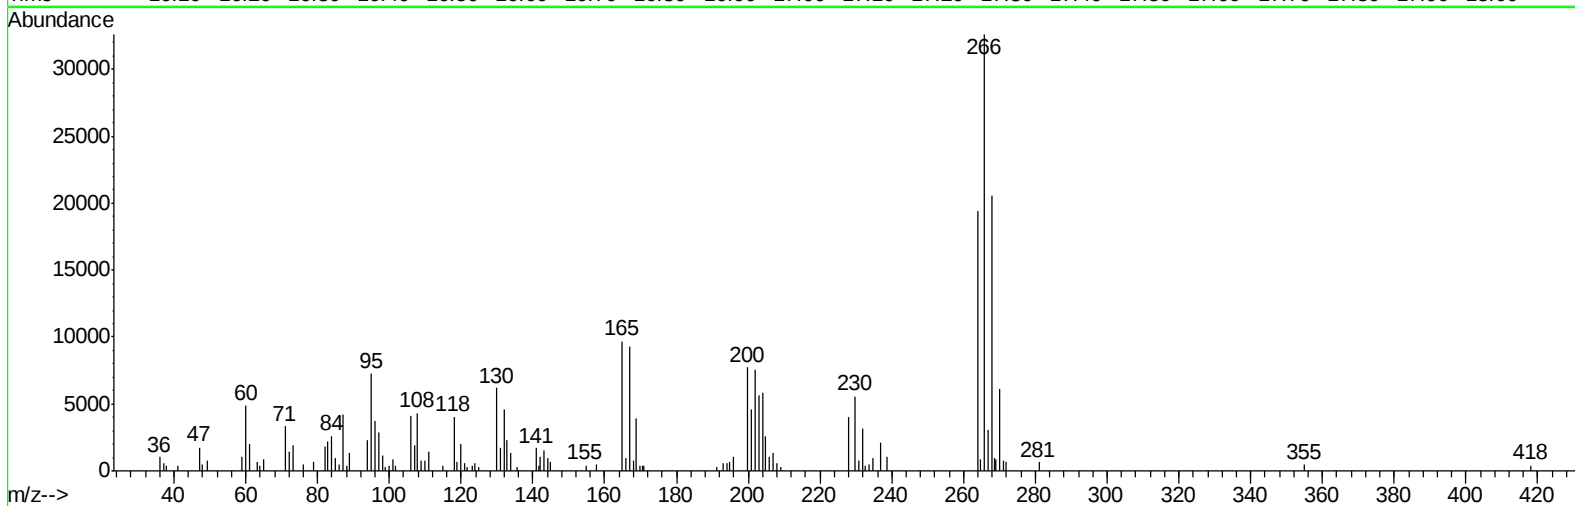


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090418\
Data File : BM016661.D
Acq On : 05 Sep 2018 03:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 08:49:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 27 13:01:22 2018
Response via : Initial Calibration

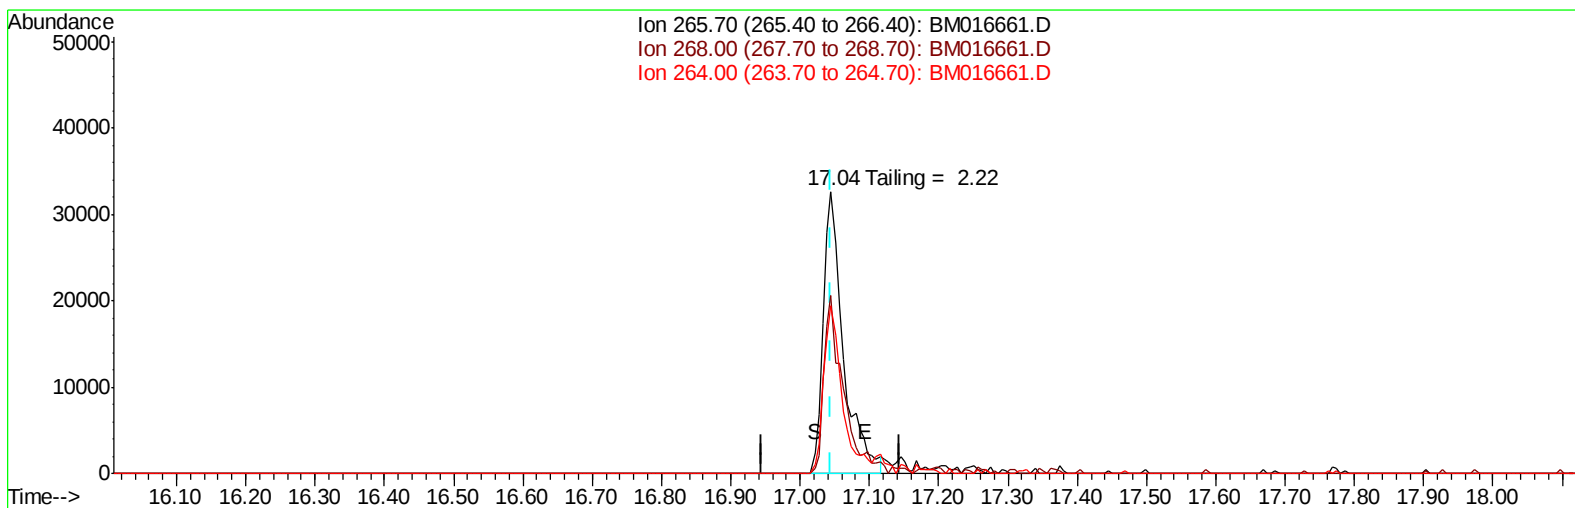

TIC: BM016661.D

(69) Pentachlorophenol (C)



17.045min (-0.000) 0.00ng

response 65810

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	65.96
264.00	61.20	62.23
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090418\
Data File : BM016661.D
Acq On : 05 Sep 2018 03:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 08:49:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 27 13:01:22 2018
Response via : Initial Calibration

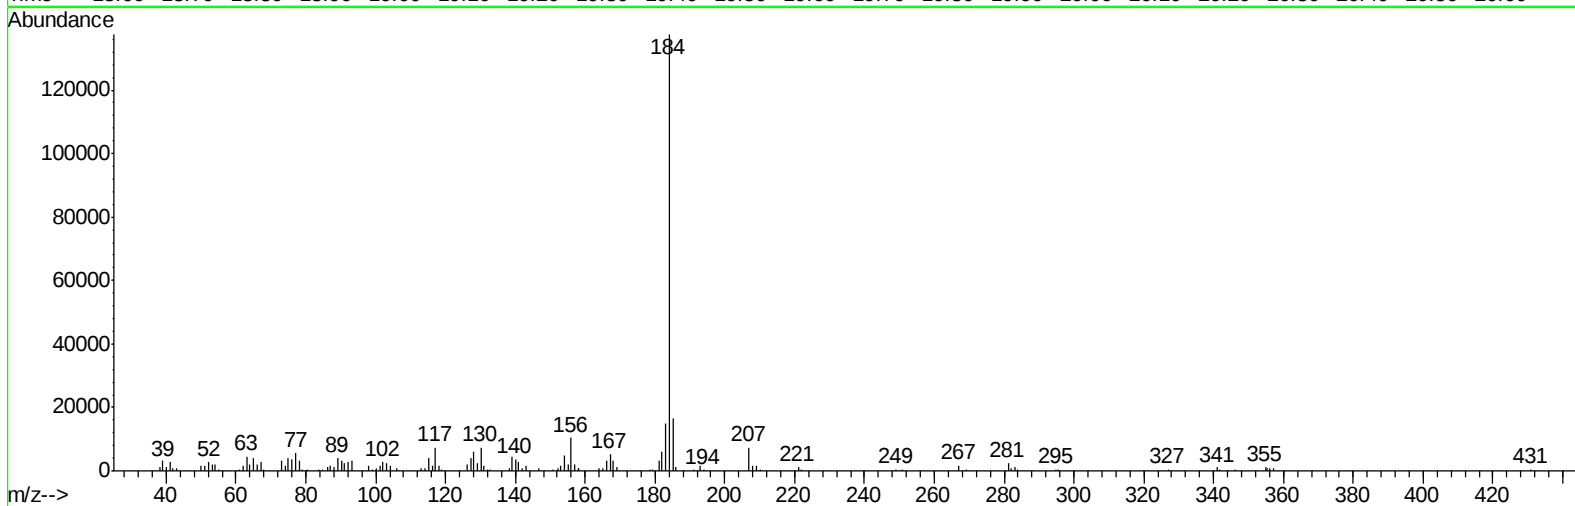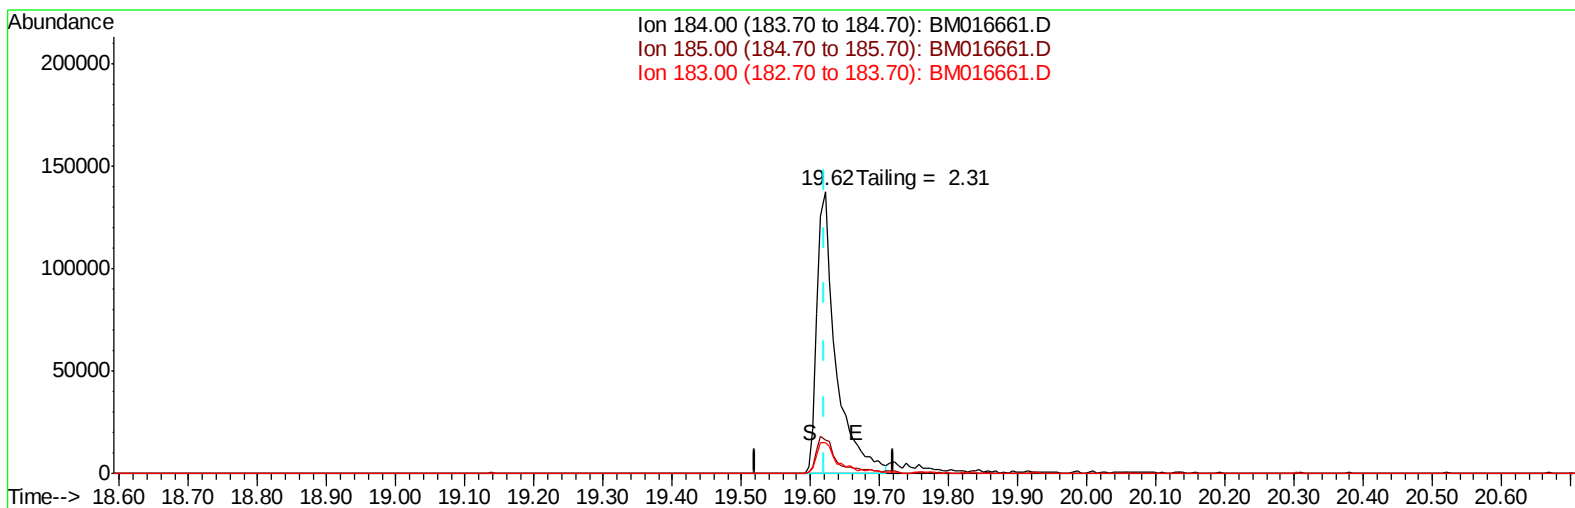

TIC: BM016661.D

(76) Benzidine

19.621min (-0.000) 77001.52ng

response 257663

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	11.98
183.00	11.10	10.83
0.00	0.00	0.00