

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090418\
 Data File : BM016646.D
 Acq On : 04 Sep 2018 15:05
 Operator : SJ/JU
 Sample : PB112537BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB112537BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	378	383	402	rBV	1124533	1817052	24.54%	6.143%
2	7.175	655	661	682	rBV	1075106	1814711	24.51%	6.135%
3	7.522	714	720	742	rBV	1332746	2274933	30.73%	7.691%
4	7.998	795	801	814	rBV	279311	506882	6.85%	1.714%
5	8.310	847	854	871	rBV	1215586	2060035	27.82%	6.964%
6	9.181	996	1002	1019	rBV	637300	1202553	16.24%	4.065%
7	10.804	1270	1278	1291	rBV	287364	547636	7.40%	1.851%
8	13.251	1688	1694	1710	rBV	2519372	3631633	49.05%	12.277%
9	14.639	1924	1930	1941	rBV3	415888	697721	9.42%	2.359%
10	16.133	2176	2184	2203	rBV	2294444	3541600	47.83%	11.973%
11	17.386	2389	2397	2408	rBV	608676	1023650	13.83%	3.461%
12	19.968	2831	2836	2845	rBV	6253778	7404094	100.00%	25.030%
13	21.527	3097	3101	3114	rBV	1011657	1478790	19.97%	4.999%
14	23.803	3483	3488	3500	rBV2	720611	1579637	21.33%	5.340%


Sum of corrected areas: 29580927

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090418\
Data File : BM016646.D
Acq On : 04 Sep 2018 15:05
Operator : SJ/JU
Sample : PB112537BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112537BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

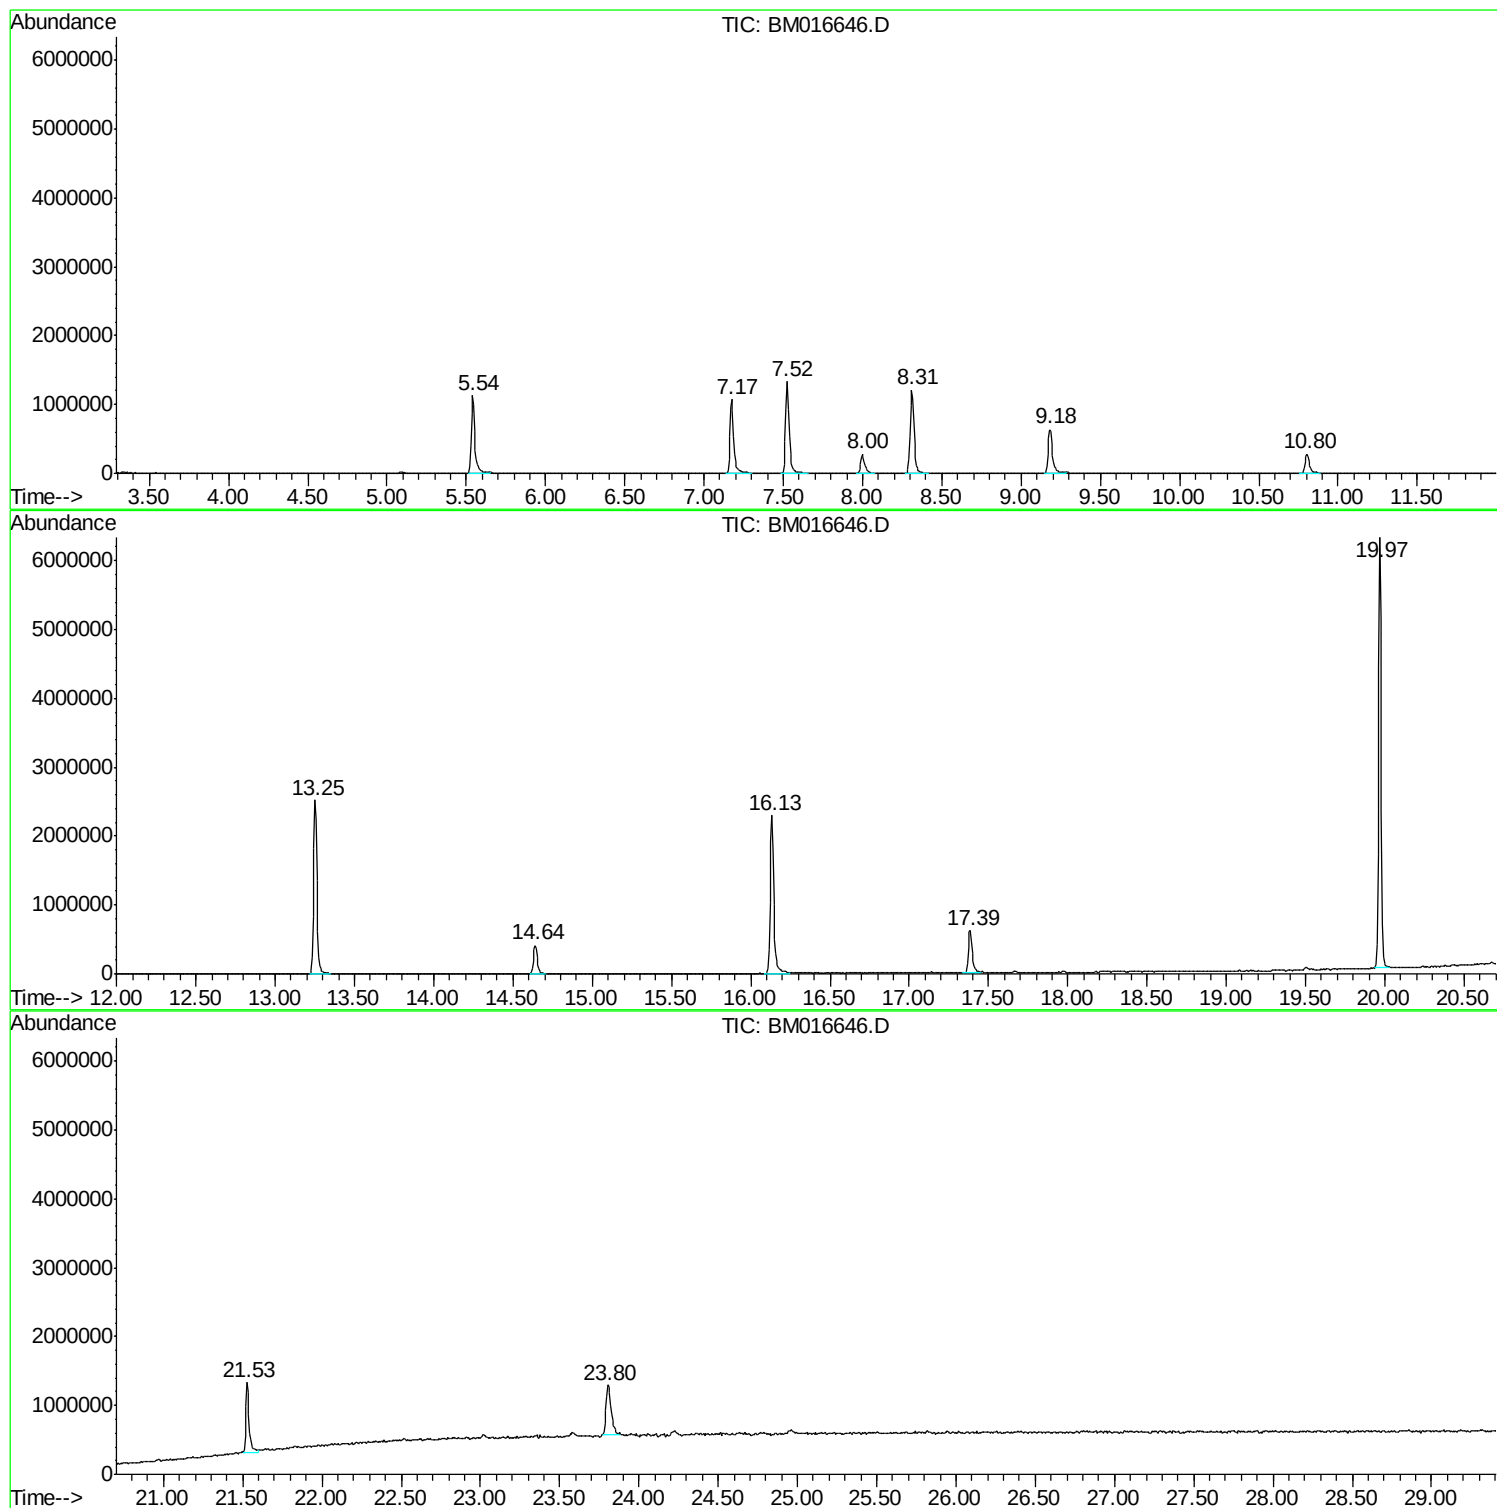

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090418\
Data File : BM016646.D
Acq On : 04 Sep 2018 15:05
Operator : SJ/JU
Sample : PB112537BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112537BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.52	89.76 ng	2274930	1,4-Dichlorobenzene-d4	8.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Tetrazaborole, 5-chloro-4,5-d...	132	C2H6BClN4	021960-49-6	27
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	22
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		Tricyclo[4.2.1.0<2,5>]non-3-ene	120	C9H12	007078-40-2	16
5		1-Penten-3-yne	66	C5H6	000646-05-9	16

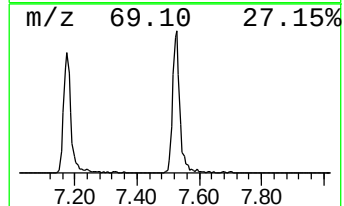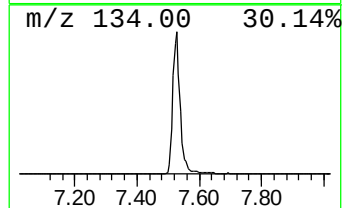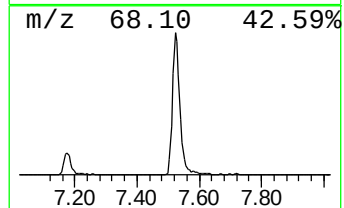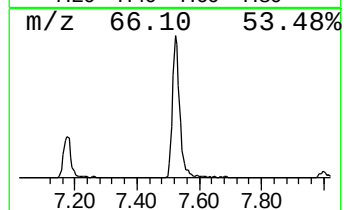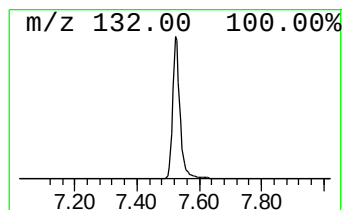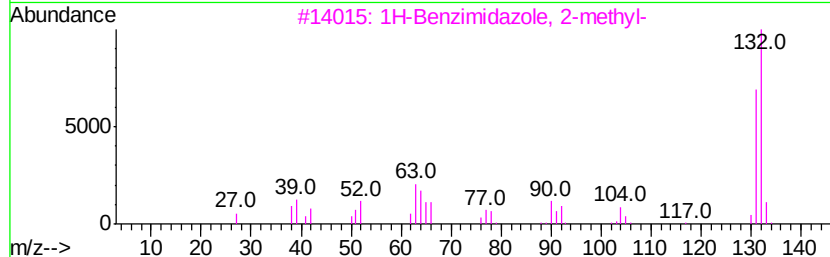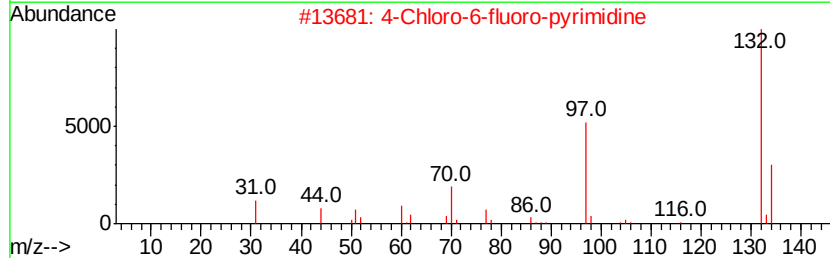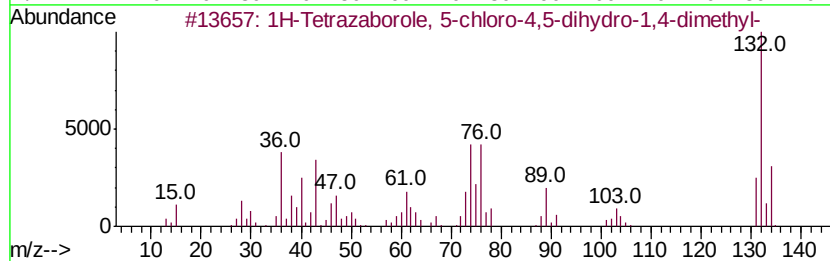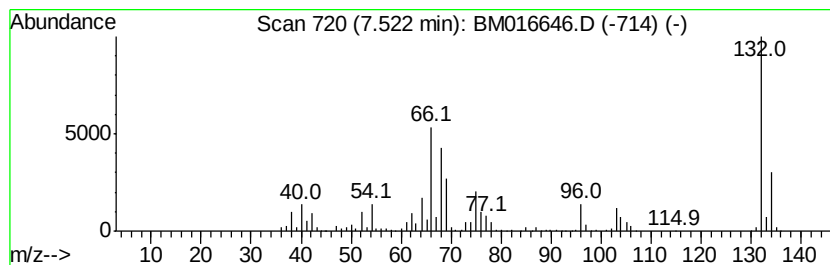

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090418\
Data File : BM016646.D
Acq On : 04 Sep 2018 15:05
Operator : SJ/JU
Sample : PB112537BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112537BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.52	7.52	89.8	ng	2274930	1	8.00	506882	20.0