

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090418\
 Data File : BM016651.D
 Acq On : 04 Sep 2018 18:06
 Operator : SJ/JU
 Sample : PB112568BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB112568BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	378	383	400	rBV	1262530	2004142	28.22%	6.597%
2	7.175	655	661	674	rBV	1198721	1942678	27.35%	6.394%
3	7.522	714	720	738	rBV	1453025	2463620	34.69%	8.109%
4	7.998	794	801	813	rBV2	275008	540735	7.61%	1.780%
5	8.310	848	854	872	rBV	1294839	2205094	31.05%	7.258%
6	9.181	996	1002	1016	rBV	675183	1276995	17.98%	4.203%
7	10.804	1272	1278	1291	rBV	316224	588451	8.29%	1.937%
8	13.251	1688	1694	1710	rBV	2816439	4010287	56.47%	13.200%
9	14.639	1923	1930	1948	rBV	456928	751250	10.58%	2.473%
10	16.133	2178	2184	2196	rBV	2465743	3748204	52.78%	12.337%
11	17.386	2392	2397	2410	rBV	597678	1011328	14.24%	3.329%
12	19.968	2831	2836	2847	rBV	6312280	7102127	100.00%	23.377%
13	21.527	3097	3101	3110	rBV	849556	1314533	18.51%	4.327%
14	23.809	3484	3489	3503	rVB	642915	1421618	20.02%	4.679%


Sum of corrected areas: 30381062

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090418\
Data File : BM016651.D
Acq On : 04 Sep 2018 18:06
Operator : SJ/JU
Sample : PB112568BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112568BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

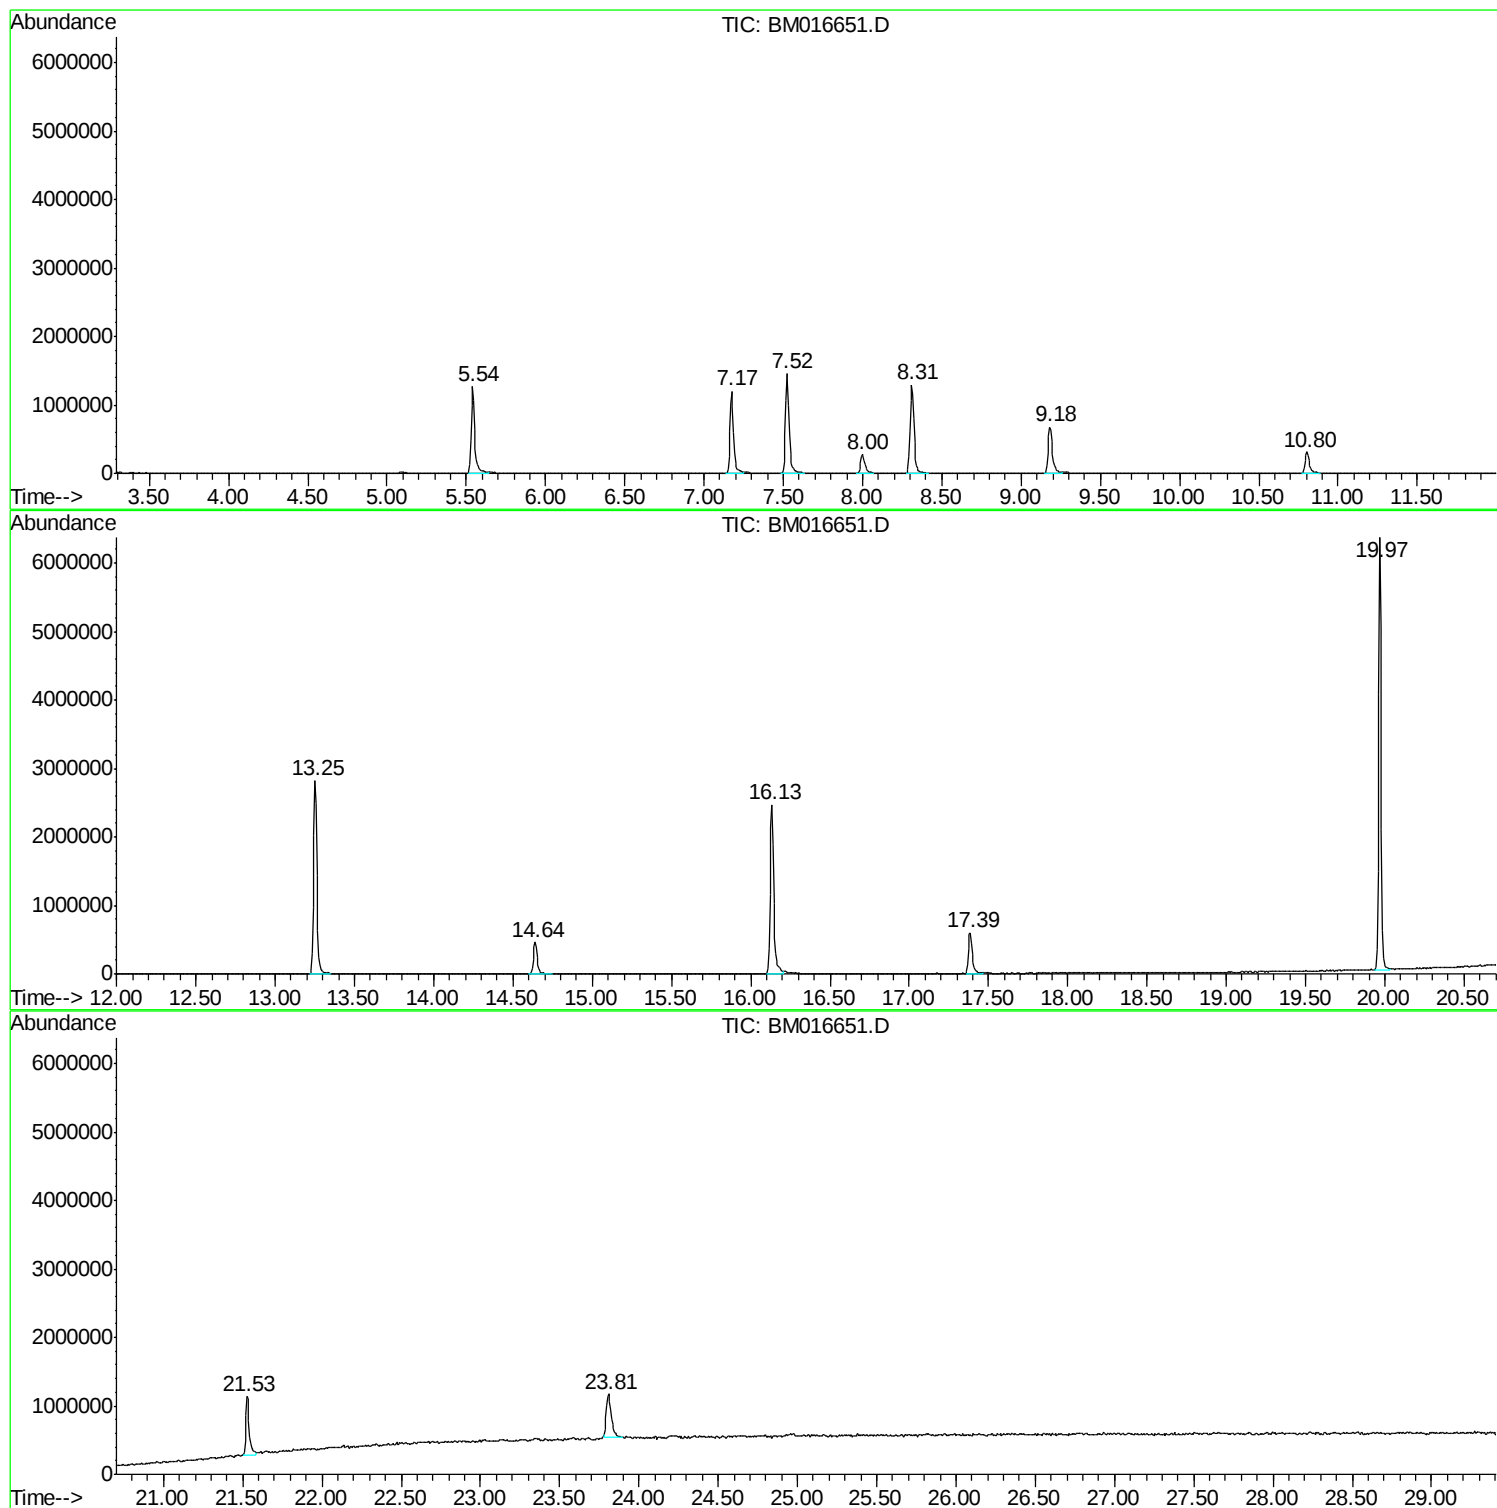

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090418\
Data File : BM016651.D
Acq On : 04 Sep 2018 18:06
Operator : SJ/JU
Sample : PB112568BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112568BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.52	91.12 ng	2463620	1,4-Dichlorobenzene-d4	8.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	The first isomer tricvclopentadiene	198	C15H18	1000222-21-0	38
2		3-Penten-1-yne, (Z)-	66	C5H6	001574-40-9	16
3		1,3-Cyclopentadiene	66	C5H6	000542-92-7	16
4		Silane, bicyclo[2.2.1]hept-5-en-...	226	C7H9Cl3Si	014319-64-3	16
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	14

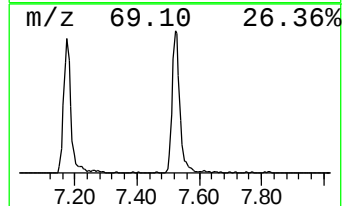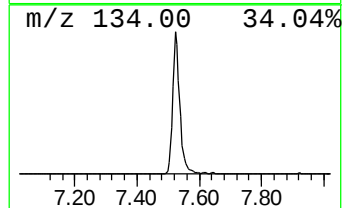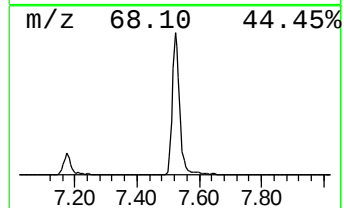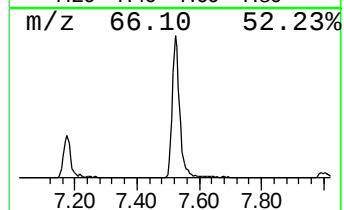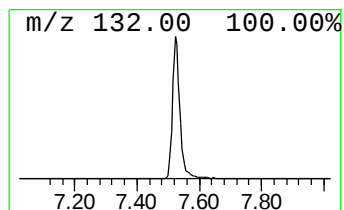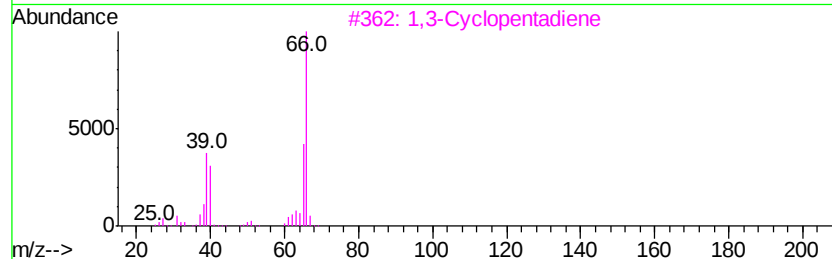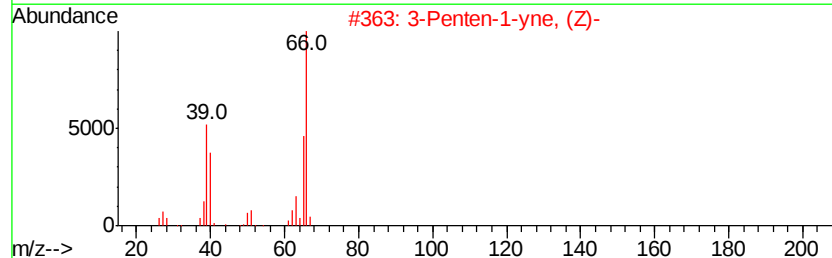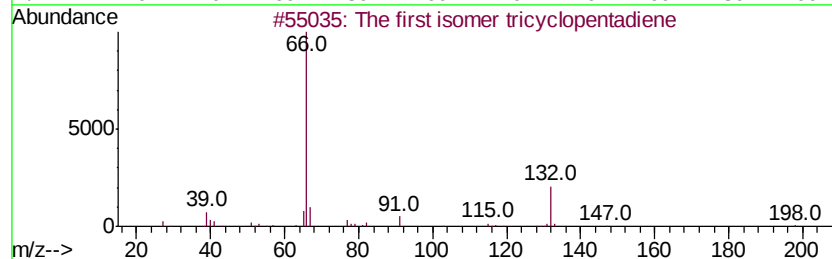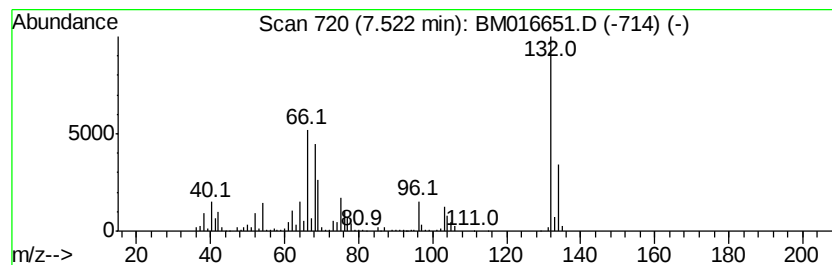

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090418\
Data File : BM016651.D
Acq On : 04 Sep 2018 18:06
Operator : SJ/JU
Sample : PB112568BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112568BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.52	7.52	91.1	ng	2463620	1	8.00	540735	20.0