


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090418\
 Data File : BM016642.D
 Acq On : 04 Sep 2018 12:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 27 13:01:22 2018

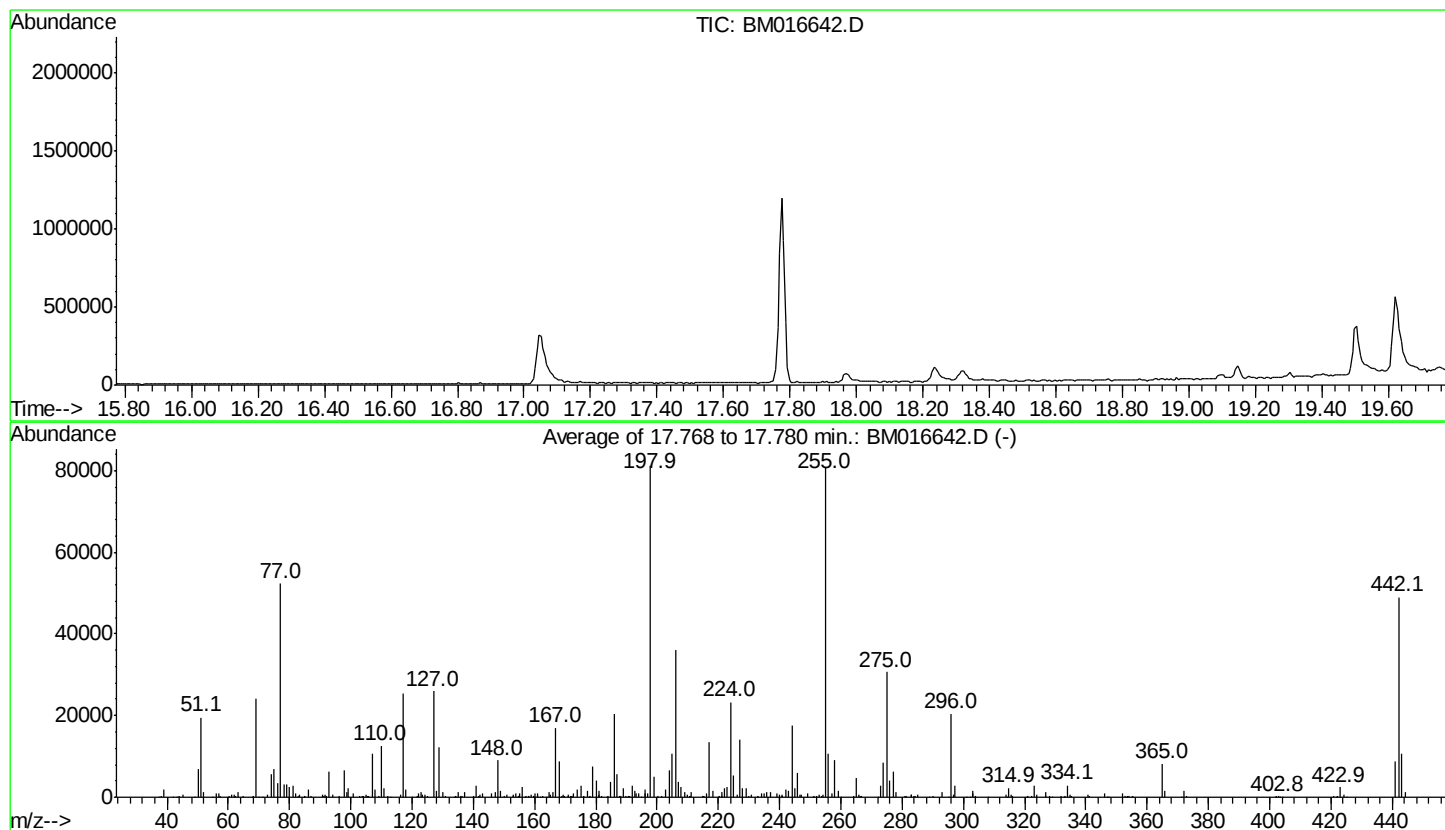

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.9	19450	PASS
68	69	0.00	2	1.5	351	PASS
69	198	0.00	100	29.7	24141	PASS
70	69	0.00	2	0.6	152	PASS
127	198	10	80	31.9	25938	PASS
197	198	0.00	2	1.1	915	PASS
198	198	100	100	100.0	81229	PASS
199	198	5	9	6.0	4904	PASS
275	198	10	60	37.8	30698	PASS
365	198	1	100	10.2	8270	PASS
441	198	0.01	100	10.8	8782	PASS
442	198	50	100	60.4	49066	PASS
443	442	15	24	21.5	10560	PASS