

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090419\
 Data File : BM022517.D
 Acq On : 04 Sep 2019 00:27
 Operator : HP/JU
 Sample : K4606-02
 Misc : GCMS CONFIRMATION
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 04 01:21:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 30 01:29:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	18347	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.28	136	68128	20.00	ng/ul	-0.02
35) Acenaphthene-d10	14.16	164	43925	20.00	ng/ul	-0.03
61) Phenanthrene-d10	16.94	188	85954	20.00	ng/ul	-0.02
77) Chrysene-d12	21.16	240	86693	20.00	ng/ul	-0.02
85) Perylene-d12	23.34	264	88947	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	0.00	176	0	0.00	ng/ul	
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.04	188	303	0.07	ng/ul	-0.01
78) Pyrene-d10	0.00	212	0	0.00	ng/ul	
89) Benzo(a)pyrene-d12	23.34	264	82457	16.87	ng/ul	0.12

Target Compounds


				Ovalue	
69) Phenanthrene	16.98	178	27556	5.359	ng/ul 95
71) Anthracene	16.98	178	27556	5.150	ng/ul 95
76) Fluoranthene	19.01	202	31184	4.024	ng/ul 98
82) Benzo(a)anthracene	21.19	228	14277	2.188	ng/ul 95
84) Chrysene	21.19	228	14277	2.340	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090419\
Data File : BM022517.D
Acq On : 04 Sep 2019 00:27
Operator : HP/JU
Sample : K4606-02
Misc : GCMS CONFIRMATION
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 04 01:21:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 30 01:29:39 2019
Response via : Initial Calibration

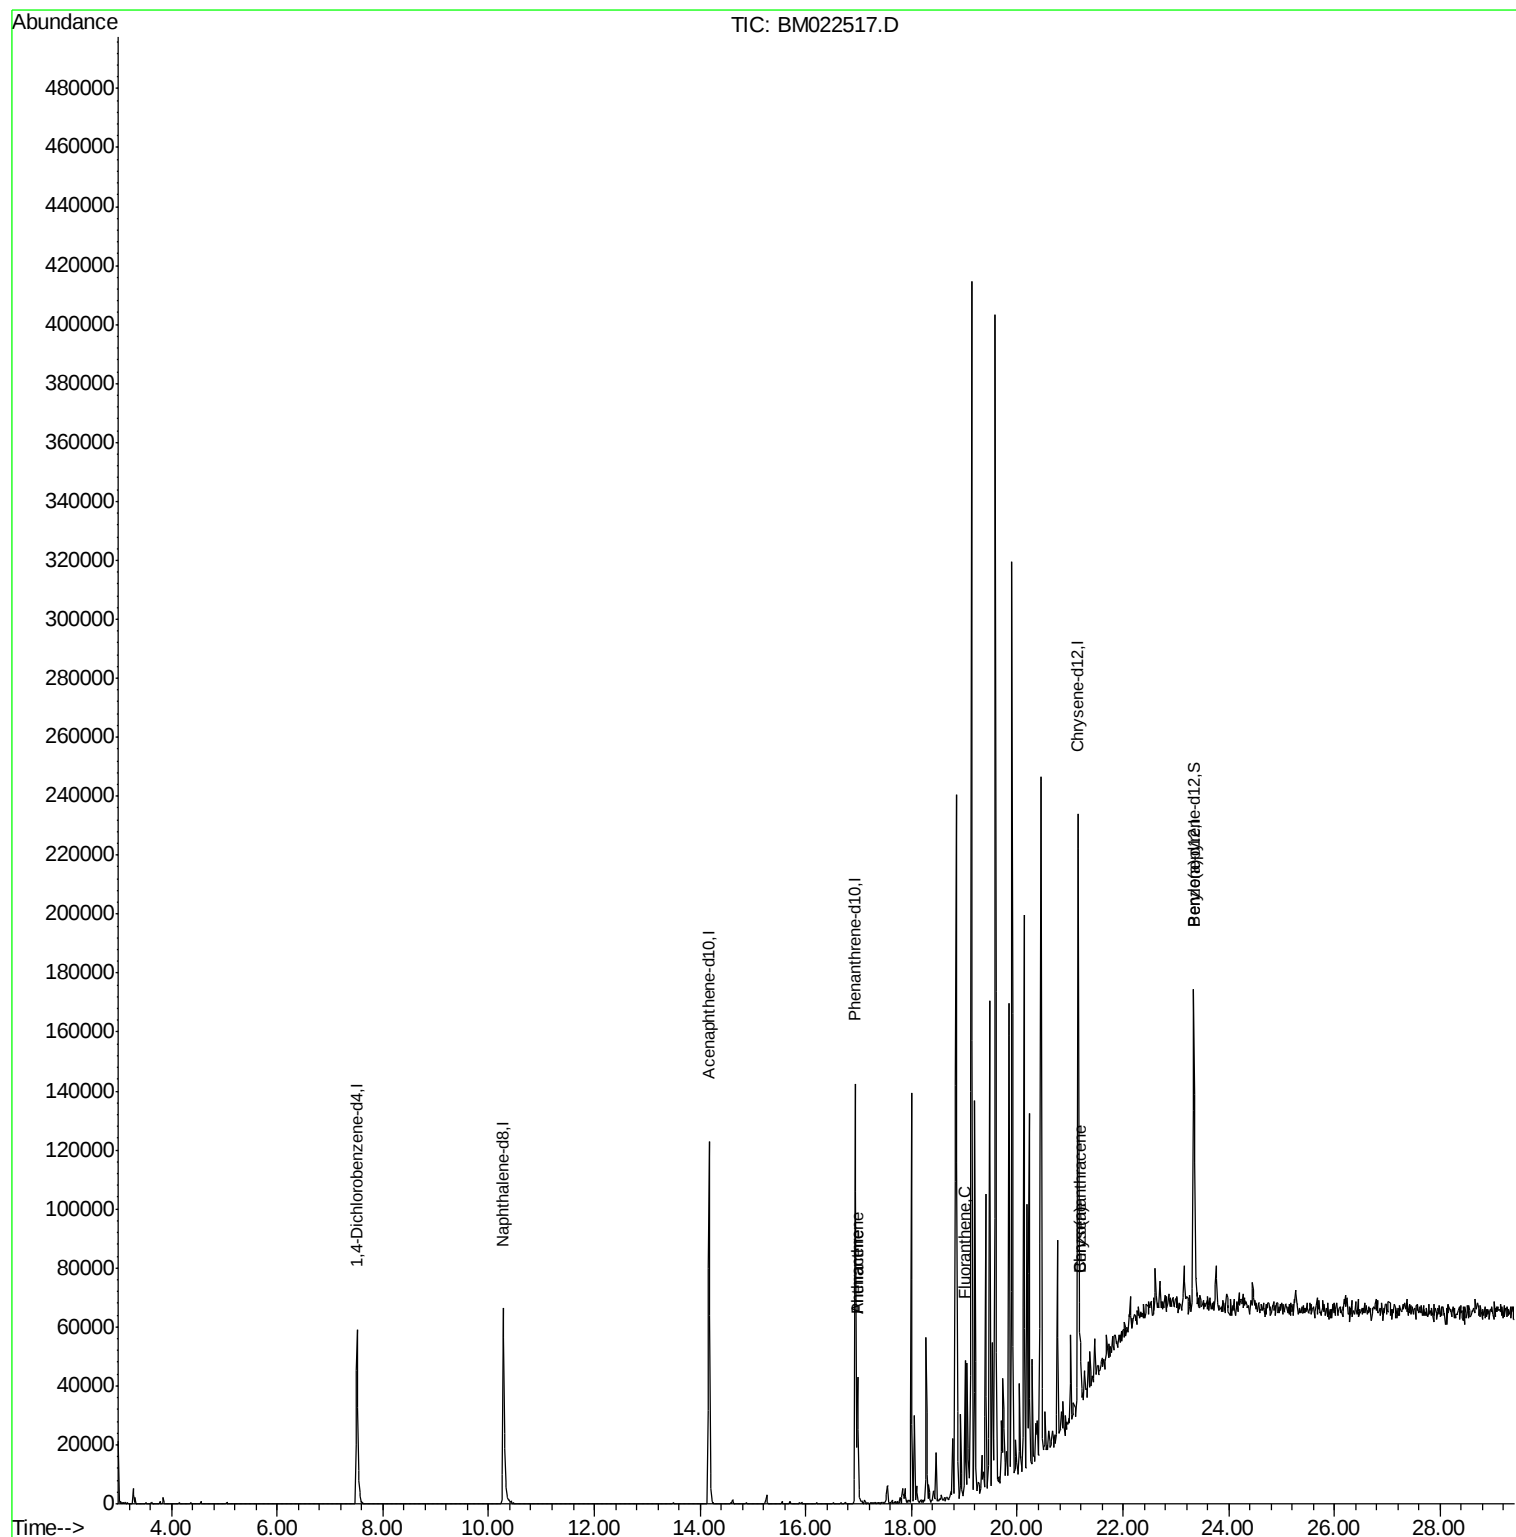

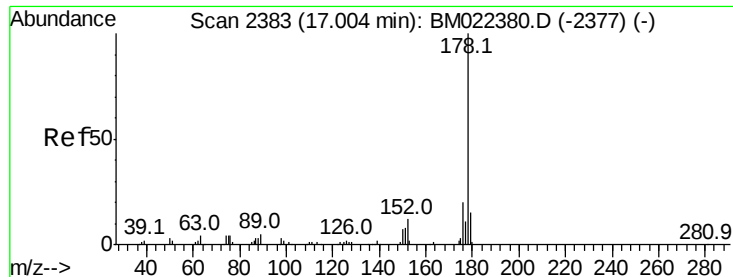

#69

Phenanthrene

Concen: 5.359 ng/ul

RT: 16.98 min Scan# 2379

Delta R.T. -0.02 min

Lab File: BM022517.D

Acq: 04 Sep 2019 00:27



Instrument :

BNA_M


ClientSampleId :

Tot Ion:178 Resp: 27556

Ion	Ratio	Lower	Upper
178	100		
179	18.3	12.4	18.6
176	21.2	15.4	23.0

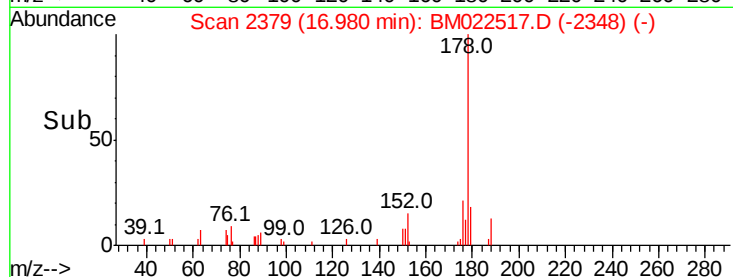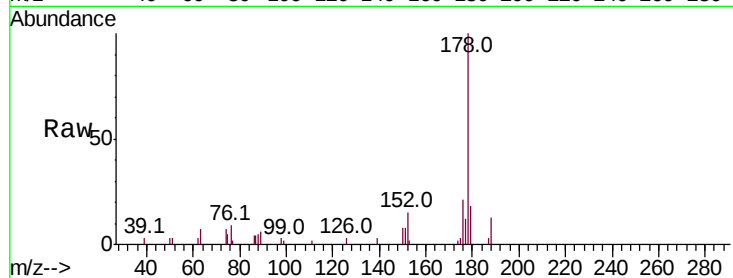

Time-->

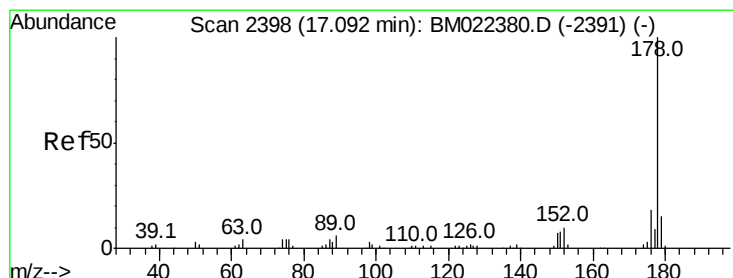

#71

Anthracene

Concen: 5.150 ng/ul

RT: 16.98 min Scan# 2379



Delta R.T. -0.11 min

Lab File: BM022517.D


Acq: 04 Sep 2019 00:27

Tgt Ion:178 Resp: 27556

Ion	Ratio	Lower	Upper
178	100		
179	18.3	12.3	18.5
176	21.2	15.5	23.3

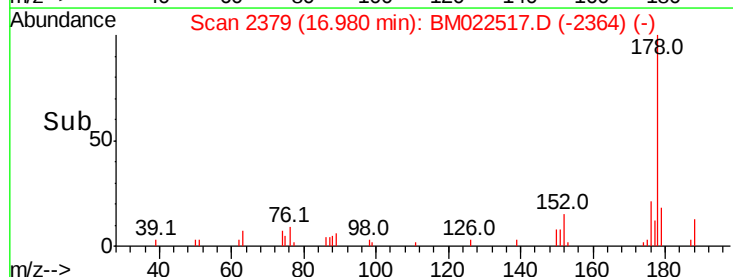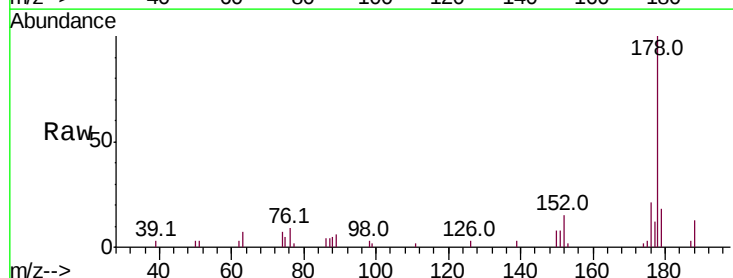

Time-->

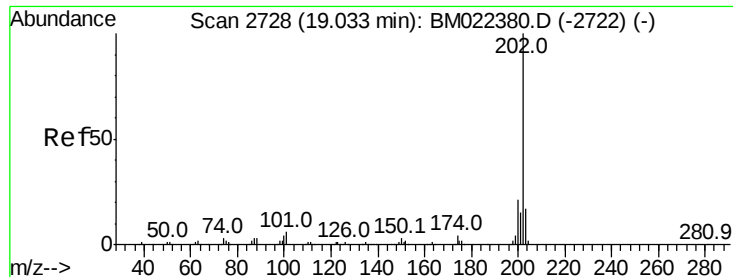

#76

Fluoranthene

Concen: 4.024 ng/ul

RT: 19.01 min Scan# 2724

Delta R.T. -0.02 min

Lab File: BM022517.D

Acq: 04 Sep 2019 00:27

Instrument :

BNA_M

ClientSampled :


Tot Ion:202 Resp: 31184

Ion Ratio Lower Upper

202 100

101 7.0 5.3 7.9




100 4.9 4.6 6.8

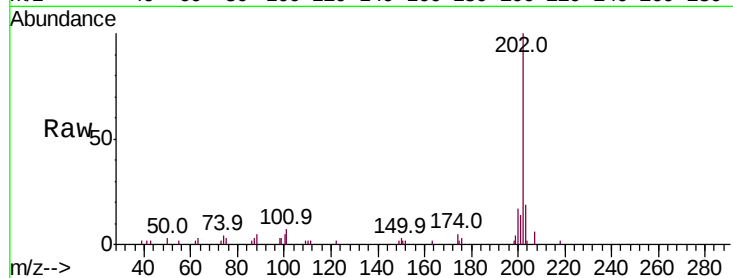

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

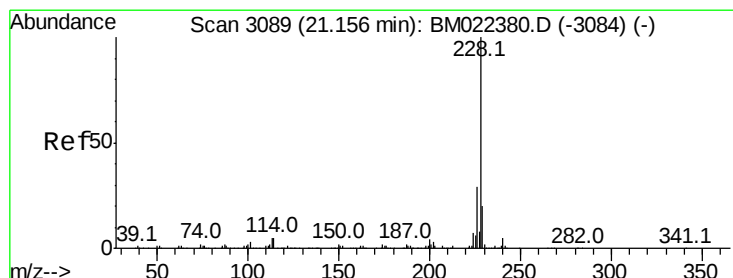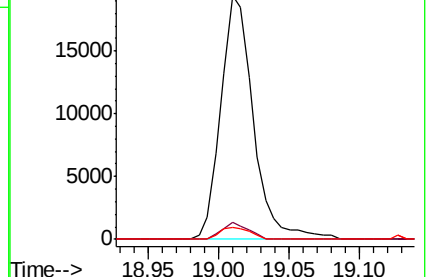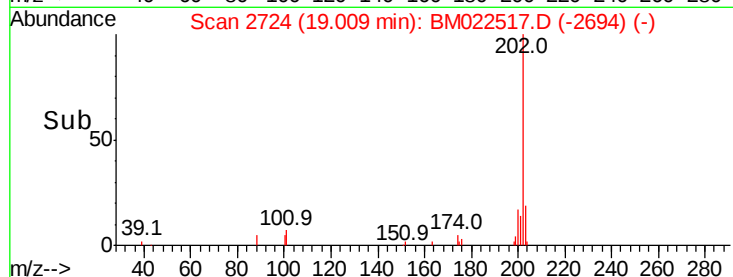

#82

Benzo(a)anthracene

Concen: 2.188 ng/ul

RT: 21.19 min Scan# 3095

Delta R.T. 0.04 min

Lab File: BM022517.D

Acq: 04 Sep 2019 00:27


Tgt Ion:228 Resp: 14277

Ion Ratio Lower Upper

228 100

229 21.3 15.2 22.8



226 30.2 22.3 33.5



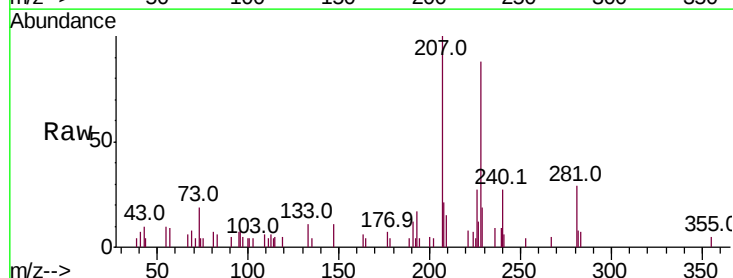


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

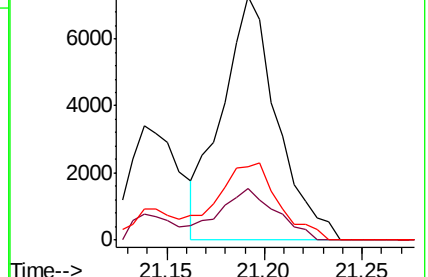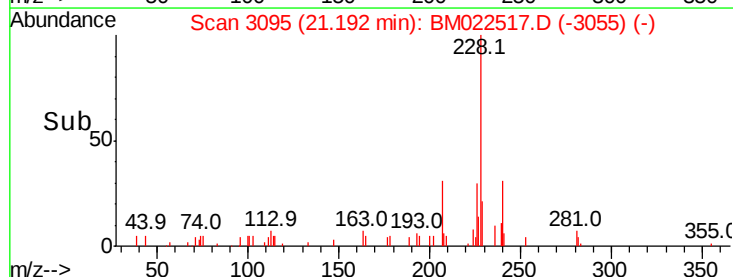

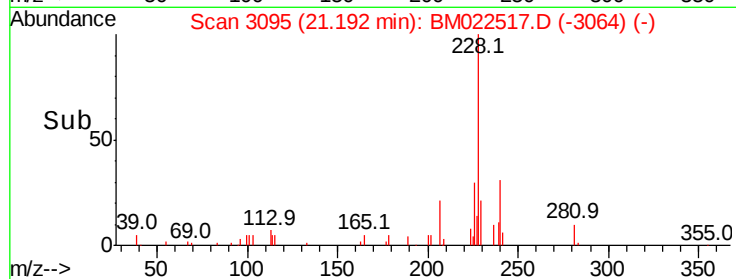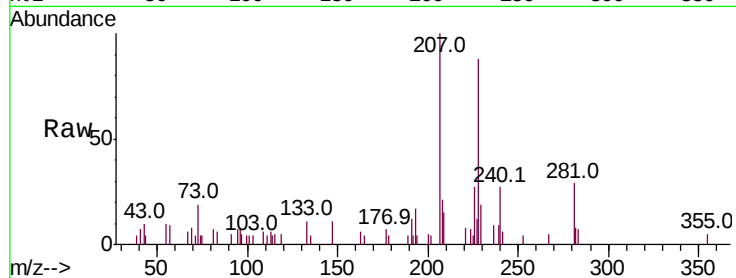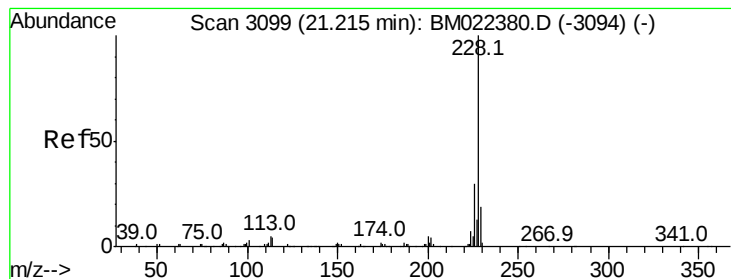

#84

Chrysene

Concen: 2.340 ng/ul

RT: 21.19 min Scan# 3095

Delta R.T. -0.02 min

Lab File: BM022517.D

Acq: 04 Sep 2019 00:27

Instrument :

BNA_M

ClientSampleId :

Tot Ion:228 Resp: 14277

Ion Ratio Lower Upper

228 100

226 30.2 24.7 37.1

229 21.3 15.7 23.5

