

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090419\
 Data File : BM022515.D
 Acq On : 03 Sep 2019 23:13
 Operator : HP/JU
 Sample : PB122681BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	5	7	8	rVB	901	525	0.28%	0.053%
2	3.046	8	10	12	rVV	645	493	0.26%	0.050%
3	3.063	12	13	16	rVV2	634	681	0.36%	0.069%
4	3.110	19	21	22	rVB	453	317	0.17%	0.032%
5	3.122	22	23	26	rBV2	408	436	0.23%	0.044%
6	3.181	29	33	34	rVB	541	401	0.21%	0.041%
7	3.299	52	53	56	rBV	486	337	0.18%	0.034%
8	3.381	66	67	71	rBV	403	354	0.19%	0.036%
9	3.604	101	105	108	rBV	252	347	0.18%	0.035%
10	3.652	111	113	116	rVB	480	568	0.30%	0.058%
11	3.693	118	120	122	rBB	470	484	0.25%	0.049%
12	3.716	122	124	127	rBV	505	691	0.36%	0.070%
13	3.763	129	132	134	rVV	314	437	0.23%	0.044%
14	3.799	134	138	140	rVB	446	710	0.37%	0.072%
15	3.834	141	144	145	rBV	423	478	0.25%	0.048%
16	3.863	148	149	152	rVB	410	394	0.21%	0.040%
17	3.946	162	163	166	rBB	361	376	0.20%	0.038%
18	4.199	203	206	207	rBB	332	336	0.18%	0.034%
19	4.357	230	233	235	rBB	401	392	0.21%	0.040%
20	7.504	763	768	785	rBV	51260	108216	57.01%	10.969%
21	10.281	1234	1240	1253	rBV	50448	124209	65.43%	12.590%
22	10.363	1253	1254	1259	rVB	1965	1339	0.71%	0.136%
23	10.463	1269	1271	1273	rVB	533	504	0.27%	0.051%
24	14.174	1896	1902	1919	rBV	86913	172077	90.65%	17.441%
25	16.945	2368	2373	2397	rBV2	81042	189829	100.00%	19.241%
26	17.104	2399	2400	2403	rVB	546	531	0.28%	0.054%
27	17.133	2403	2405	2408	rBB	621	582	0.31%	0.059%
28	17.233	2419	2422	2423	rBB	401	363	0.19%	0.037%
29	17.592	2480	2483	2485	rBB	683	611	0.32%	0.062%
30	17.768	2510	2513	2515	rBB	482	527	0.28%	0.053%
31	17.815	2520	2521	2524	rBB	342	335	0.18%	0.034%
32	17.845	2525	2526	2529	rBB	407	374	0.20%	0.038%
33	17.874	2529	2531	2532	rBV	945	555	0.29%	0.056%
34	17.909	2534	2537	2540	rVB	669	852	0.45%	0.086%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090419\
 Data File : BM022515.D
 Acq On : 03 Sep 2019 23:13
 Operator : HP/JU
 Sample : PB122681BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	17.939	2540	2542	2543	rBV	360	358	0.19%	0.036%
36	18.033	2556	2558	2561	rVB	517	631	0.33%	0.064%
37	18.057	2561	2562	2564	rBV	426	387	0.20%	0.039%
38	18.121	2570	2573	2575	rBB	450	552	0.29%	0.056%
39	18.145	2575	2577	2578	rBV	475	457	0.24%	0.046%
40	18.157	2578	2579	2583	rVB	429	343	0.18%	0.035%
41	18.198	2584	2586	2588	rVB	490	446	0.23%	0.045%
42	18.221	2588	2590	2591	rBV	448	426	0.22%	0.043%
43	18.262	2596	2597	2601	rVB	531	663	0.35%	0.067%
44	18.315	2603	2606	2608	rBV	540	782	0.41%	0.079%
45	18.562	2644	2648	2649	rBV	305	358	0.19%	0.036%
46	18.715	2673	2674	2676	rBV	540	437	0.23%	0.044%
47	18.774	2682	2684	2688	rVV	343	439	0.23%	0.044%
48	18.815	2690	2691	2694	rBV	583	375	0.20%	0.038%
49	18.839	2694	2695	2699	rBV	766	431	0.23%	0.044%
50	18.892	2701	2704	2707	rBV	501	378	0.20%	0.038%
51	18.921	2707	2709	2710	rBV	484	326	0.17%	0.033%
52	18.968	2714	2717	2720	rVB	452	422	0.22%	0.043%
53	19.009	2722	2724	2725	rBV	578	546	0.29%	0.055%
54	19.062	2731	2733	2736	rVB	551	492	0.26%	0.050%
55	19.127	2742	2744	2746	rBV	785	741	0.39%	0.075%
56	19.151	2746	2748	2752	rBV	663	801	0.42%	0.081%
57	19.198	2754	2756	2757	rVB	716	480	0.25%	0.049%
58	19.209	2757	2758	2759	rBV	665	324	0.17%	0.033%
59	19.227	2759	2761	2764	rVB	659	613	0.32%	0.062%
60	19.262	2764	2767	2768	rBV	522	418	0.22%	0.042%
61	19.274	2768	2769	2774	rVB2	1111	1186	0.62%	0.120%
62	19.321	2774	2777	2778	rBV	662	624	0.33%	0.063%
63	19.333	2778	2779	2781	rVB	1217	673	0.35%	0.068%
64	19.362	2781	2784	2785	rBV	1108	922	0.49%	0.093%
65	19.386	2785	2788	2791	rBV2	1270	1378	0.73%	0.140%
66	19.409	2791	2792	2794	rBV	455	345	0.18%	0.035%
67	19.451	2797	2799	2801	rVB2	617	469	0.25%	0.048%
68	19.480	2803	2804	2806	rBV	726	440	0.23%	0.045%
69	19.498	2806	2807	2810	rVB	910	574	0.30%	0.058%
70	19.521	2810	2811	2812	rBV	827	383	0.20%	0.039%
71	19.551	2814	2816	2817	rBV	728	390	0.21%	0.040%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090419\
 Data File : BM022515.D
 Acq On : 03 Sep 2019 23:13
 Operator : HP/JU
 Sample : PB122681BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

72	19.568	2817	2819	2822	rBV2	810	830	0.44%	0.084%
73	19.603	2823	2825	2828	rVB2	1097	815	0.43%	0.083%
74	19.656	2832	2834	2835	rVB	672	342	0.18%	0.035%
75	19.703	2840	2842	2843	rBV2	765	643	0.34%	0.065%
76	19.721	2843	2845	2847	rVB2	942	556	0.29%	0.056%
77	19.745	2847	2849	2850	rVB2	578	388	0.20%	0.039%
78	19.768	2850	2853	2854	rBV2	1047	707	0.37%	0.072%
79	19.815	2858	2861	2862	rBV2	736	848	0.45%	0.086%
80	19.833	2862	2864	2865	rBV2	715	587	0.31%	0.059%
81	19.845	2865	2866	2869	rVB2	939	722	0.38%	0.073%
82	19.874	2869	2871	2873	rVB2	842	541	0.28%	0.055%
83	19.915	2877	2878	2881	rBV2	1639	1125	0.59%	0.114%
84	19.939	2881	2882	2883	rBV	918	448	0.24%	0.045%
85	19.980	2886	2889	2891	rVB3	1398	1415	0.75%	0.143%
86	20.003	2891	2893	2894	rBV	1003	716	0.38%	0.073%
87	20.021	2894	2896	2898	rBV3	672	699	0.37%	0.071%
88	20.039	2898	2899	2901	rVV3	1238	718	0.38%	0.073%
89	20.074	2904	2905	2906	rVB	1233	435	0.23%	0.044%
90	20.103	2909	2910	2912	rBV	2423	1634	0.86%	0.166%
91	20.139	2914	2916	2918	rVV3	1173	1160	0.61%	0.118%
92	20.180	2920	2923	2924	rBV2	1330	1256	0.66%	0.127%
93	20.221	2929	2930	2931	rBV	1727	887	0.47%	0.090%
94	20.239	2931	2933	2934	rVV	1480	724	0.38%	0.073%
95	20.280	2938	2940	2941	rBV2	1400	720	0.38%	0.073%
96	20.368	2953	2955	2956	rBV2	1401	971	0.51%	0.098%
97	20.462	2968	2971	2973	rBV4	1367	1432	0.75%	0.145%
98	20.797	3026	3028	3029	rBV2	1766	1173	0.62%	0.119%
99	21.162	3086	3090	3099	rBV	106452	183849	96.85%	18.635%
100	23.350	3456	3462	3473	rVB	66413	150593	79.33%	15.264%


Sum of corrected areas: 986605

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090419\
Data File : BM022515.D
Acq On : 03 Sep 2019 23:13
Operator : HP/JU
Sample : PB122681BL
Misc : GCMS CONFIRMATION
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK81

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

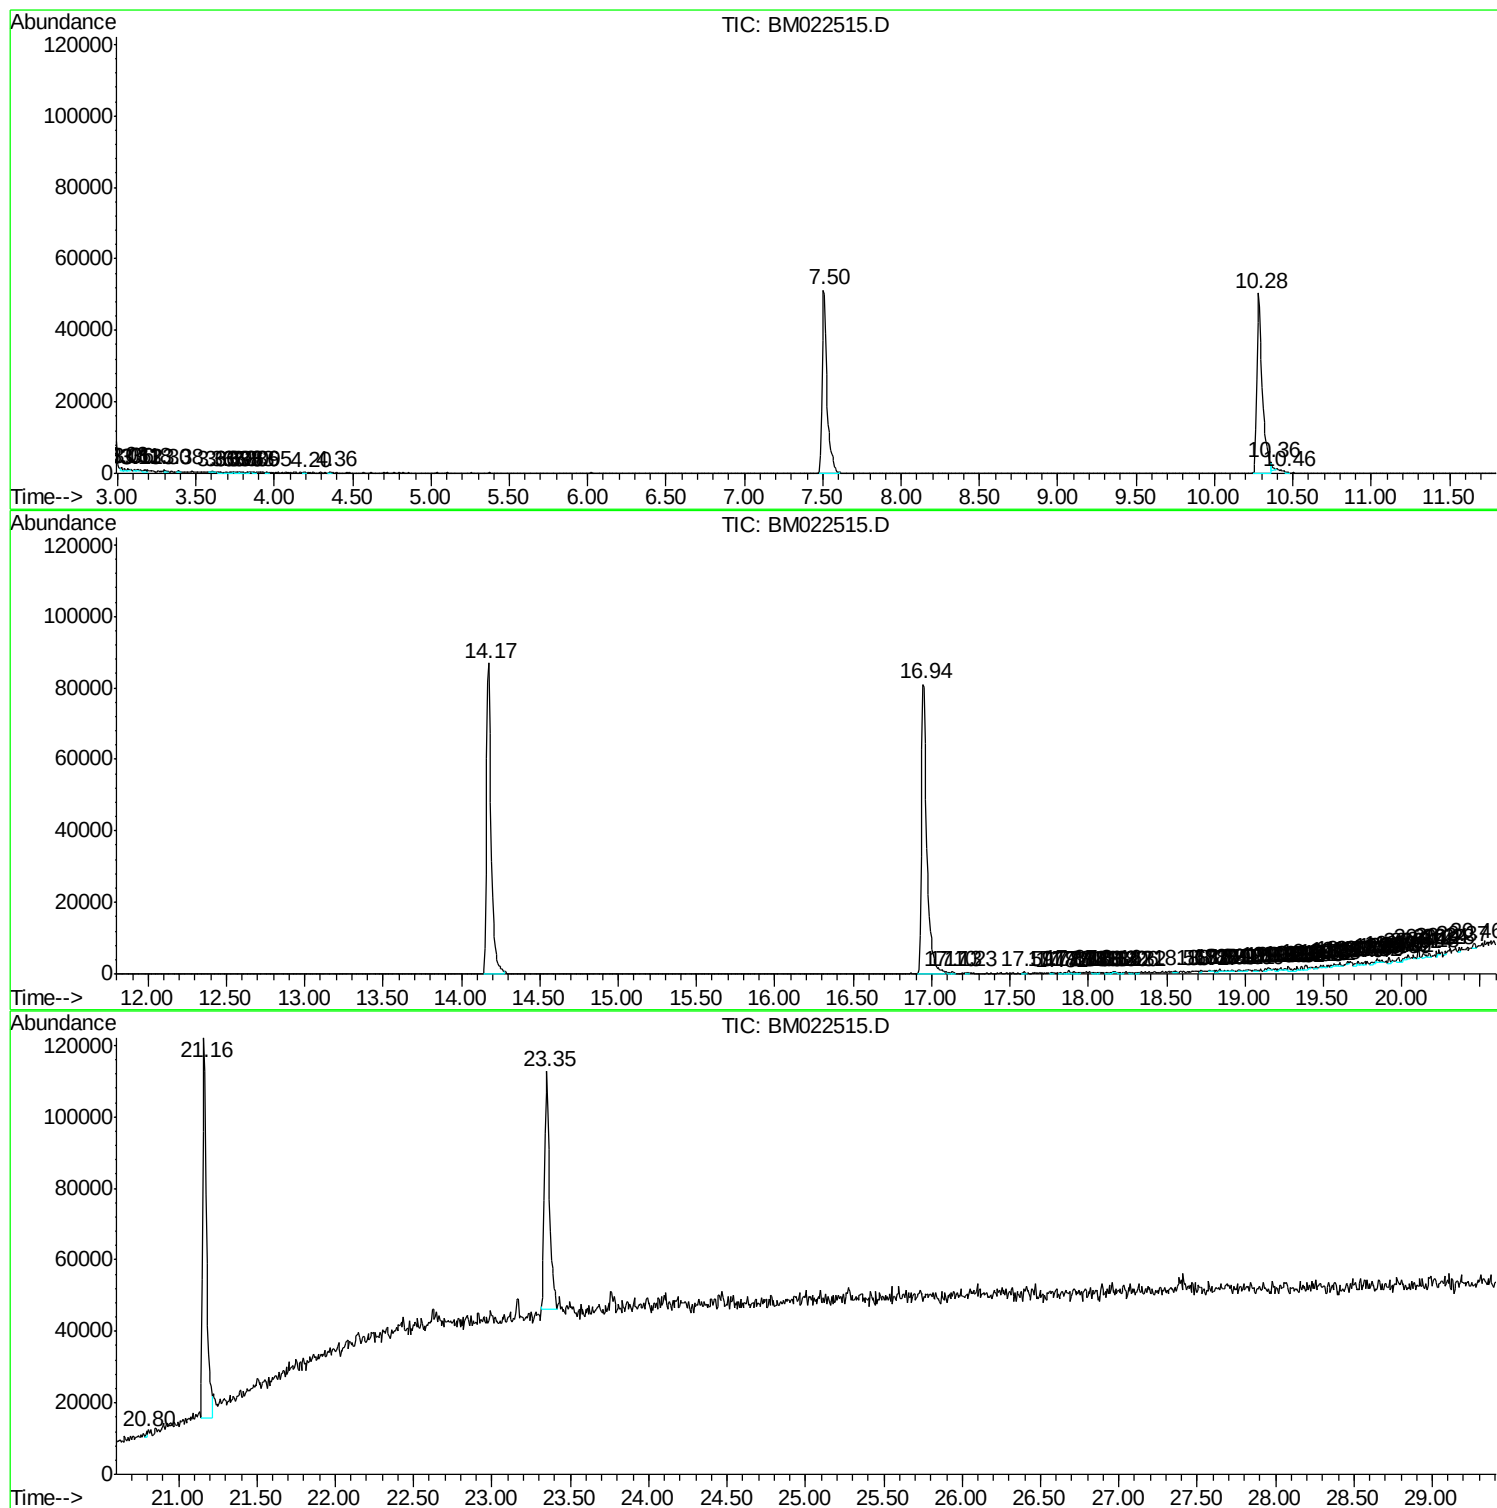

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090419\
Data_File : BM022515.D
Acq_On : 03-Sep-2019 23:133
Operator : HP/JUU
Sample : PB122681BLL
Misc : GCMS_CONFIRMATIONN
ALS_Vial : 23 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
SBLK81

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
