

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090419\
 Data File : BM022521.D
 Acq On : 04 Sep 2019 02:53
 Operator : HP/JU
 Sample : K4606-06
 Misc : GCMS CONFIRMATION
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AR8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	8	9	10	rVV	468	294	0.12%	0.022%
2	3.070	13	14	15	rVV	623	253	0.10%	0.019%
3	3.105	18	20	21	rBV	629	458	0.19%	0.034%
4	3.128	23	24	25	rVB	726	256	0.10%	0.019%
5	3.275	47	49	50	rBV	391	361	0.15%	0.026%
6	3.311	52	55	58	rBB2	1380	1246	0.50%	0.091%
7	3.769	132	133	137	rBB	724	782	0.32%	0.057%
8	7.505	763	768	783	rBV	69932	139688	56.45%	10.240%
9	7.616	785	787	788	rBB	361	249	0.10%	0.018%
10	10.275	1233	1239	1255	rBV	74276	171094	69.15%	12.543%
11	10.410	1260	1262	1267	rVB	409	656	0.27%	0.048%
12	11.816	1498	1501	1508	rBB	1938	3480	1.41%	0.255%
13	14.169	1895	1901	1919	rBB2	129057	234312	94.69%	17.177%
14	16.939	2367	2372	2394	rBV2	127512	242765	98.11%	17.797%
15	17.080	2394	2396	2397	rVB	469	319	0.13%	0.023%
16	17.233	2420	2422	2423	rBB	433	276	0.11%	0.020%
17	17.298	2431	2433	2435	rBB	373	360	0.15%	0.026%
18	17.380	2445	2447	2449	rBB	358	249	0.10%	0.018%
19	17.404	2450	2451	2453	rBB	457	276	0.11%	0.020%
20	17.533	2470	2473	2474	rBB	465	472	0.19%	0.035%
21	17.545	2474	2475	2477	rBV	498	445	0.18%	0.033%
22	17.574	2477	2480	2481	rVB	500	478	0.19%	0.035%
23	17.610	2485	2486	2487	rBV	428	261	0.11%	0.019%
24	17.669	2494	2496	2498	rVB	479	465	0.19%	0.034%
25	17.692	2498	2500	2501	rBV	355	363	0.15%	0.027%
26	17.704	2501	2502	2504	rVB	535	349	0.14%	0.026%
27	17.727	2504	2506	2508	rBB	471	467	0.19%	0.034%
28	17.745	2508	2509	2511	rBB	482	328	0.13%	0.024%
29	17.763	2511	2512	2513	rBV	426	297	0.12%	0.022%
30	17.816	2520	2521	2523	rVB	451	304	0.12%	0.022%
31	17.839	2523	2525	2526	rBV	884	610	0.25%	0.045%
32	17.851	2526	2527	2530	rVB	400	401	0.16%	0.029%
33	17.939	2540	2542	2544	rVB	735	605	0.24%	0.044%
34	17.957	2544	2545	2548	rBV	634	634	0.26%	0.046%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090419\
 Data File : BM022521.D
 Acq On : 04 Sep 2019 02:53
 Operator : HP/JU
 Sample : K4606-06
 Misc : GCMS CONFIRMATION
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AR8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	18.010	2548	2554	2558	rVB2	1366	2268	0.92%	0.166%
36	18.039	2558	2559	2562	rBV	503	648	0.26%	0.048%
37	18.310	2604	2605	2609	rBV	205	259	0.10%	0.019%
38	18.345	2609	2611	2613	rVV	407	330	0.13%	0.024%
39	18.363	2613	2614	2615	rVB	784	277	0.11%	0.020%
40	18.480	2631	2634	2635	rBV	286	266	0.11%	0.020%
41	18.533	2642	2643	2646	rBV	508	390	0.16%	0.029%
42	18.580	2649	2651	2653	rVB	469	297	0.12%	0.022%
43	18.621	2656	2658	2660	rBV	838	549	0.22%	0.040%
44	18.680	2665	2668	2672	rBV	585	900	0.36%	0.066%
45	18.727	2672	2676	2679	rBV	534	661	0.27%	0.048%
46	18.751	2679	2680	2682	rBV	519	360	0.15%	0.026%
47	18.780	2684	2685	2687	rVB	927	626	0.25%	0.046%
48	18.821	2689	2692	2694	rBV	789	957	0.39%	0.070%
49	18.851	2694	2697	2700	rBV4	2103	2392	0.97%	0.175%
50	18.880	2700	2702	2703	rVB	808	461	0.19%	0.034%
51	18.921	2703	2709	2711	rBV	817	1573	0.64%	0.115%
52	18.939	2711	2712	2713	rBV	708	281	0.11%	0.021%
53	18.980	2716	2719	2721	rVB	736	739	0.30%	0.054%
54	19.004	2721	2723	2724	rBV	516	313	0.13%	0.023%
55	19.039	2725	2729	2730	rBV	847	740	0.30%	0.054%
56	19.074	2733	2735	2736	rBV	461	289	0.12%	0.021%
57	19.104	2738	2740	2741	rBV	386	345	0.14%	0.025%
58	19.145	2741	2747	2751	rBV2	6097	7112	2.87%	0.521%
59	19.180	2751	2753	2756	rBV	388	262	0.11%	0.019%
60	19.204	2756	2757	2760	rVB	1769	1271	0.51%	0.093%
61	19.239	2760	2763	2765	rVB2	1109	997	0.40%	0.073%
62	19.257	2765	2766	2767	rBV	787	513	0.21%	0.038%
63	19.274	2767	2769	2770	rBV	751	456	0.18%	0.033%
64	19.292	2770	2772	2775	rVB2	975	978	0.40%	0.072%
65	19.327	2775	2778	2780	rBV2	1215	1309	0.53%	0.096%
66	19.351	2780	2782	2785	rVB2	1443	1378	0.56%	0.101%
67	19.380	2785	2787	2790	rBV	1201	1731	0.70%	0.127%
68	19.404	2790	2791	2792	rBV	1296	668	0.27%	0.049%
69	19.433	2795	2796	2797	rBV	1305	774	0.31%	0.057%
70	19.457	2798	2800	2803	rVB2	557	367	0.15%	0.027%
71	19.486	2803	2805	2808	rVB3	2524	1518	0.61%	0.111%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090419\
 Data File : BM022521.D
 Acq On : 04 Sep 2019 02:53
 Operator : HP/JU
 Sample : K4606-06
 Misc : GCMS CONFIRMATION
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AR8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

72	19.515	2808	2810	2811	rBV2	651	569	0.23%	0.042%
73	19.598	2820	2824	2827	rBV3	4657	5808	2.35%	0.426%
74	19.663	2833	2835	2839	rVB3	1238	1035	0.42%	0.076%
75	19.704	2839	2842	2844	rBV2	1063	1402	0.57%	0.103%
76	19.727	2844	2846	2847	rBV	2076	1029	0.42%	0.075%
77	19.745	2847	2849	2850	rVV	529	350	0.14%	0.026%
78	19.763	2850	2852	2853	rVV2	820	436	0.18%	0.032%
79	19.851	2864	2867	2869	rVB3	2681	2286	0.92%	0.168%
80	19.874	2869	2871	2874	rBV3	594	502	0.20%	0.037%
81	19.915	2875	2878	2883	rVB4	4690	6019	2.43%	0.441%
82	20.045	2898	2900	2904	rVB4	1226	1145	0.46%	0.084%
83	20.080	2904	2906	2907	rBV	1275	642	0.26%	0.047%
84	20.098	2907	2909	2912	rBV2	1468	1757	0.71%	0.129%
85	20.133	2913	2915	2917	rVB2	3340	2316	0.94%	0.170%
86	20.433	2964	2966	2967	rBV2	1959	1300	0.53%	0.095%
87	20.451	2967	2969	2973	rVV4	2942	3915	1.58%	0.287%
88	20.533	2981	2983	2984	rBV2	2117	1675	0.68%	0.123%
89	20.862	3037	3039	3040	rBV2	3249	2772	1.12%	0.203%
90	21.157	3084	3089	3100	rBV2	143896	247439	100.00%	18.139%
91	23.339	3454	3460	3472	rBV	103247	242585	98.04%	17.784%


Sum of corrected areas: 1364090

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090419\
Data File : BM022521.D
Acq On : 04 Sep 2019 02:53
Operator : HP/JU
Sample : K4606-06
Misc : GCMS CONFIRMATION
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AR8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

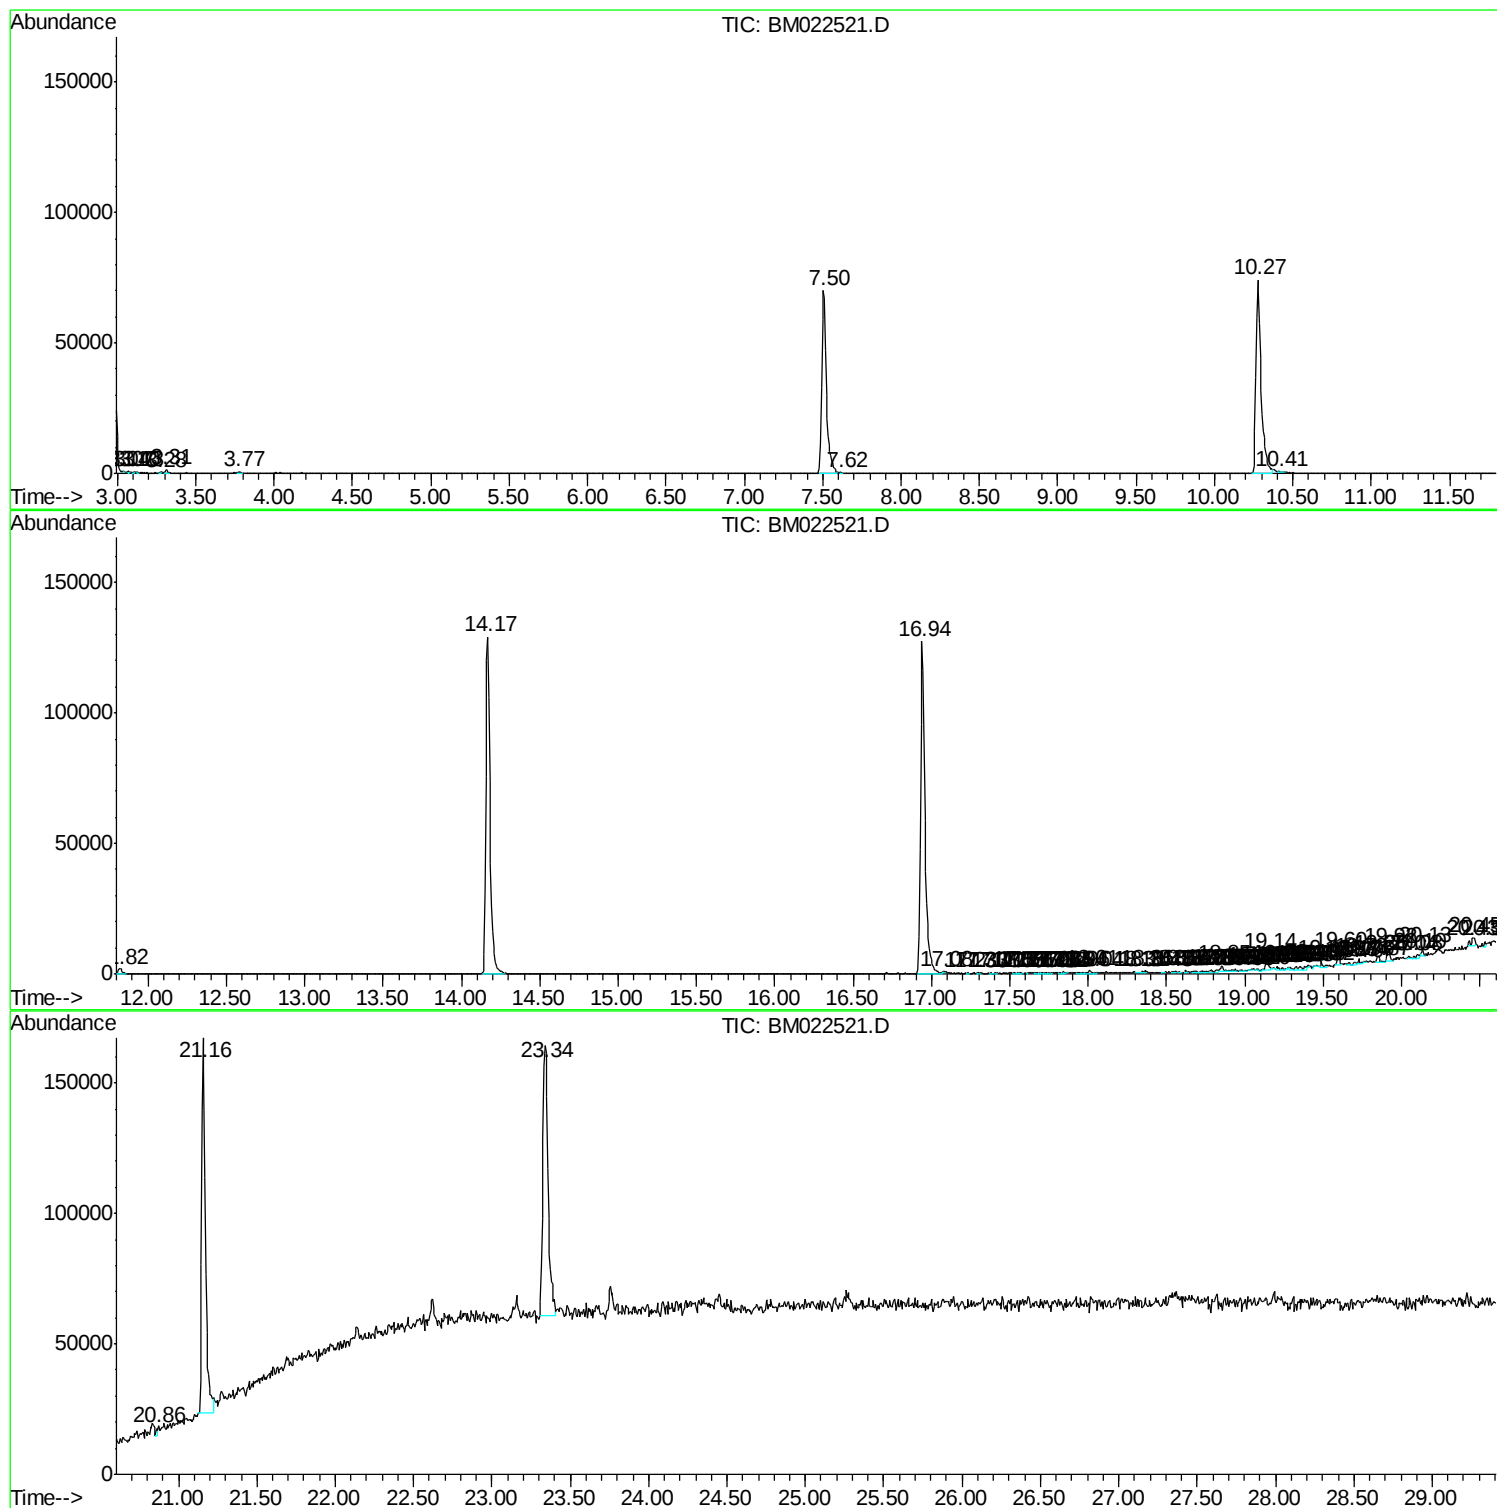

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090419\
Data File : BM022521.D
Acq On : 04 Sep 2019 02:53
Operator : HP/JU
Sample : K4606-06
Misc : GCMS CONFIRMATION
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AR8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090419\
Data File : BM022521.D
Acq On : 04 Sep 2019 02:53
Operator : HP/JU
Sample : K4606-06
Misc : GCMS CONFIRMATION
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AR8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc