

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090518\
 Data File : BM016671.D
 Acq On : 05 Sep 2018 14:53
 Operator : SJ/JU
 Sample : J4764-01RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 05 16:56:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 05 16:42:07 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.97	152	60822	20.00	ng	0.00
21) Naphthalene-d8	10.77	136	209245	20.00	ng	0.00
38) Acenaphthene-d10	14.61	164	134309	20.00	ng	0.00
63) Phenanthrene-d10	17.35	188	442174	20.00	ng	0.00
75) Chrysene-d12	21.50	240	754521	20.00	ng	0.00
86) Perylene-d12	23.77	264	995126	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	109671	35.33	ng	0.00
7) Phenol-d6	7.15	99	209945	51.12	ng	0.00
23) Nitrobenzene-d5	9.16	82	189407	41.33	ng	0.00
41) 2,4,6-Tribromophenol	16.11	330	82585	22.00	ng	0.00
44) 2-Fluorobiphenyl	13.22	172	453113	32.43	ng	0.00
78) Terphenyl-d14	19.94	244	1285795	36.07	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.07	163	122955	9.529	ng	Qvalue # 97
74) Fluoranthene	19.41	202	154172	4.601	ng	93
77) Pyrene	19.77	202	147355	3.594	ng	98
80) Benzo(a)anthracene	21.49	228	107351	2.420	ng	98
82) Chrysene	21.54	228	93234	2.203	ng	96
87) Benzo(b)fluoranthene	23.10	252	173623	3.027	ng	# 90
88) Benzo(k)fluoranthene	23.10	252	173623	2.975	ng	# 91
89) Benzo(a)pyrene	23.69	252	113579	2.035	ng	# 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090518\
Data File : BM016671.D
Acq On : 05 Sep 2018 14:53
Operator : SJ/JU
Sample : J4764-01RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 05 16:56:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 05 16:42:07 2018
Response via : Initial Calibration

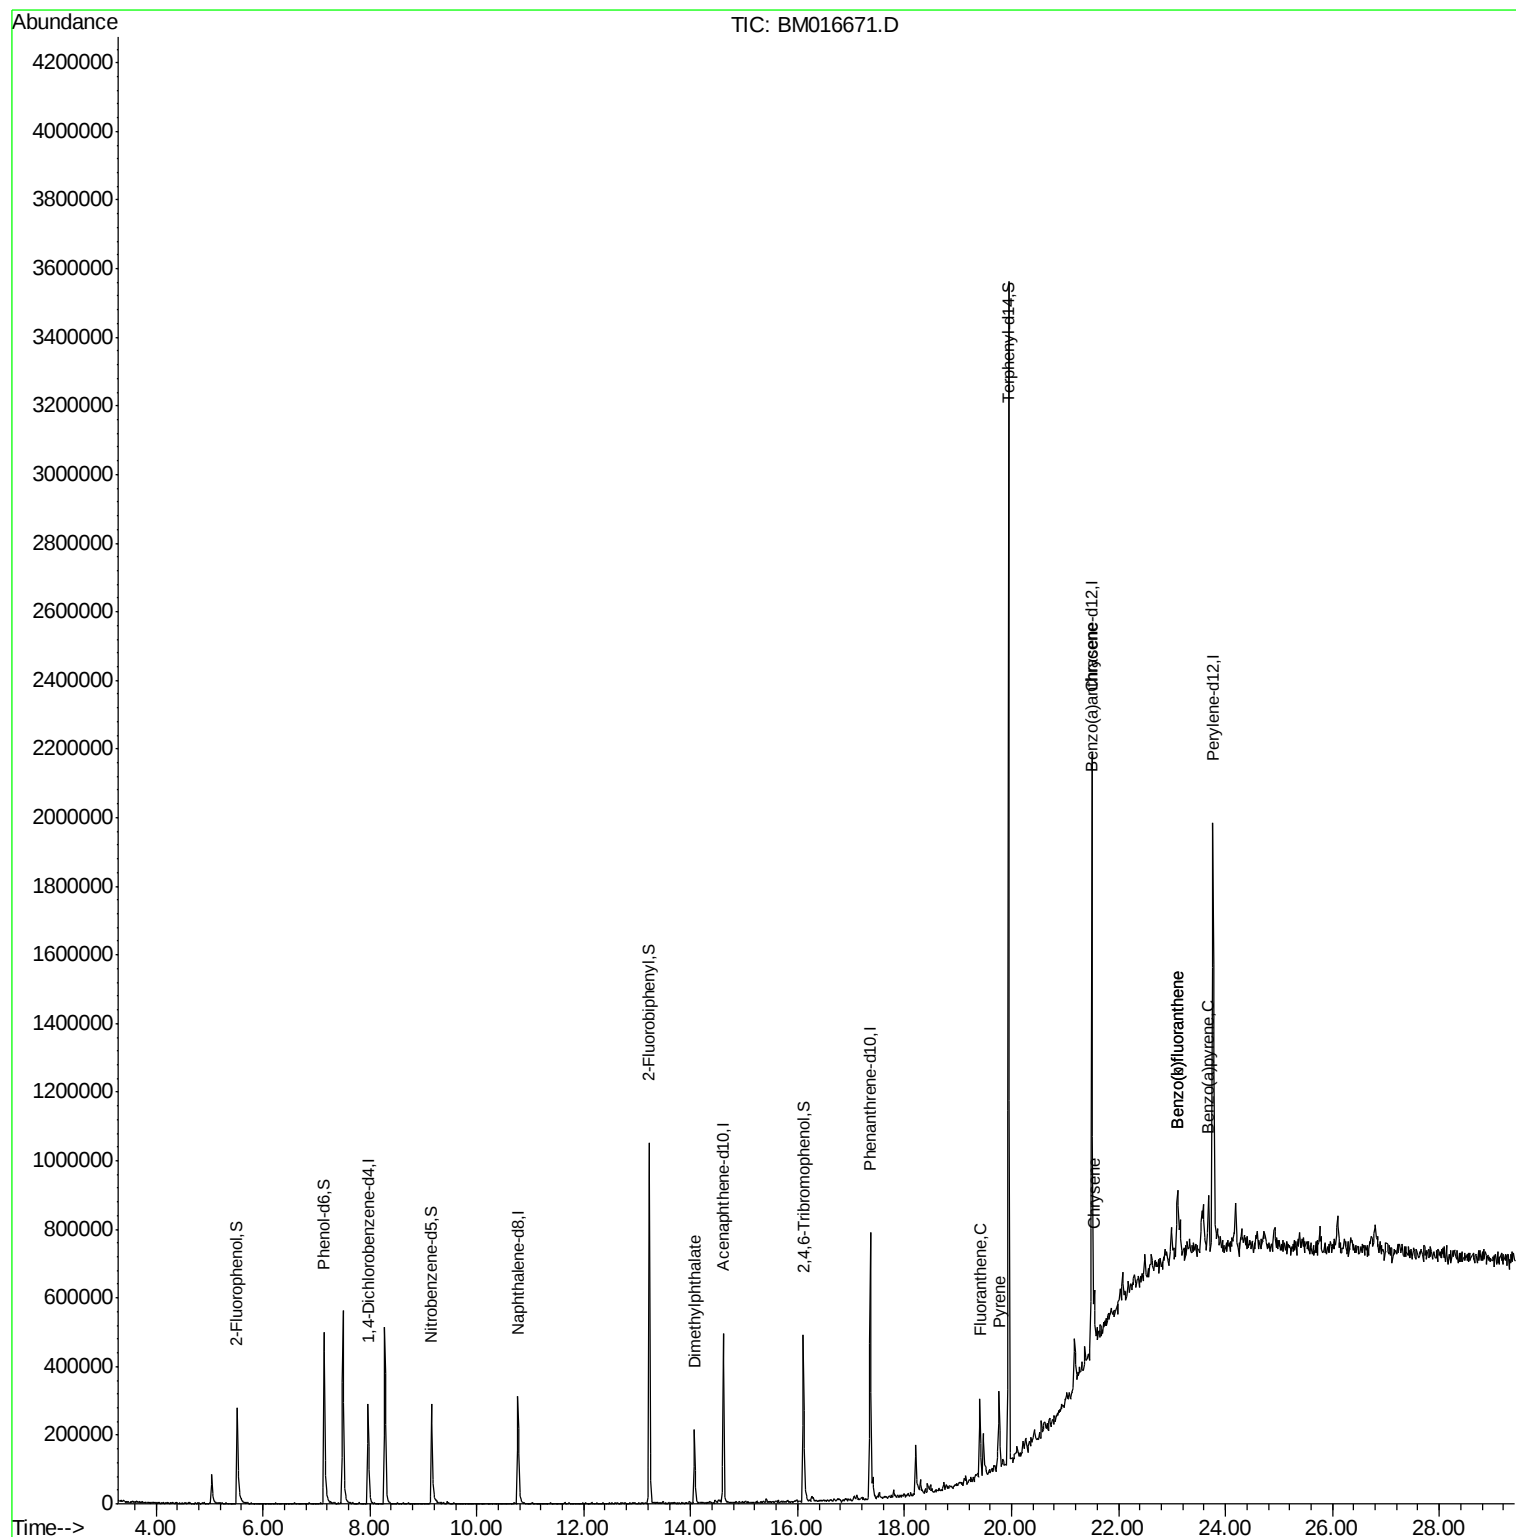

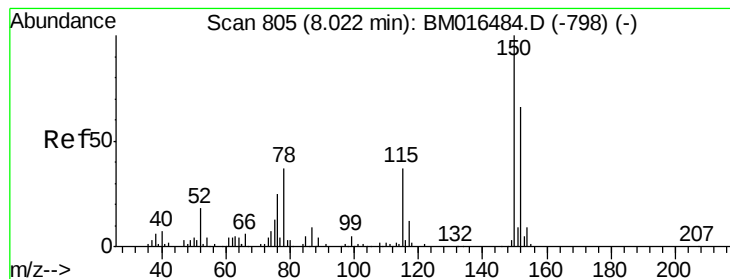


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.97 min Scan# 796
Delta R.T. 0.00 min
Lab File: BM016671.D
Acq: 05 Sep 2018 14:53

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	136.2	119.5	179.3
115	60.7	43.0	64.4



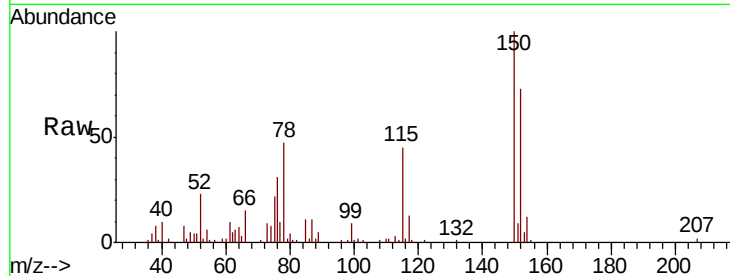


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

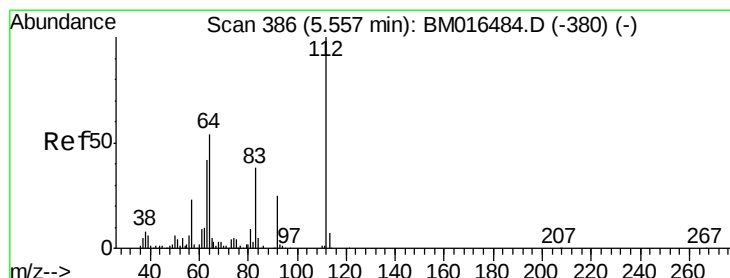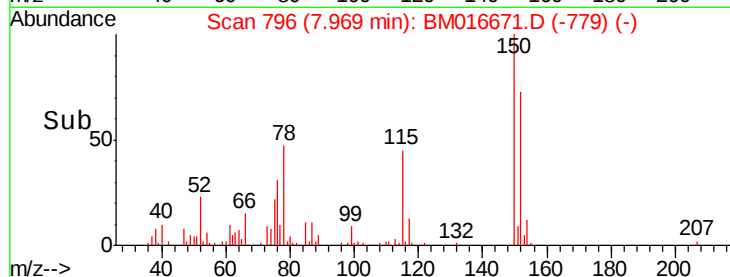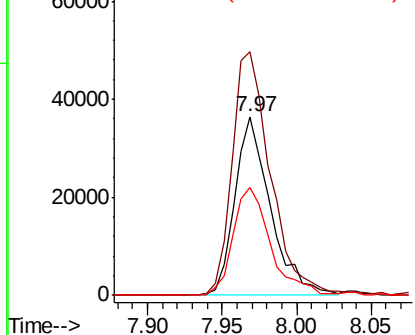

#5

2-Fluorophenol
Concen: 35.334 ng
RT: 5.52 min Scan# 379
Delta R.T. -0.00 min
Lab File: BM016671.D
Acq: 05 Sep 2018 14:53

Tgt Ion	Ratio	Lower	Upper
112	100		
64	52.4	38.6	57.8
63	49.3	19.3	28.9


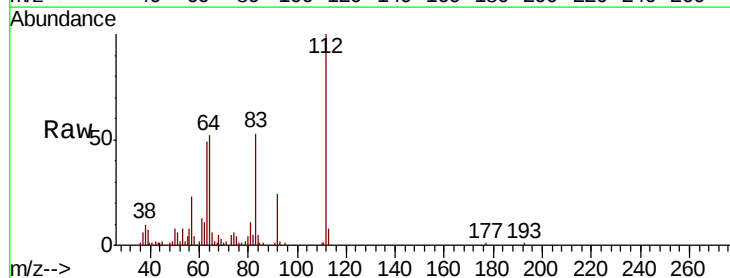



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

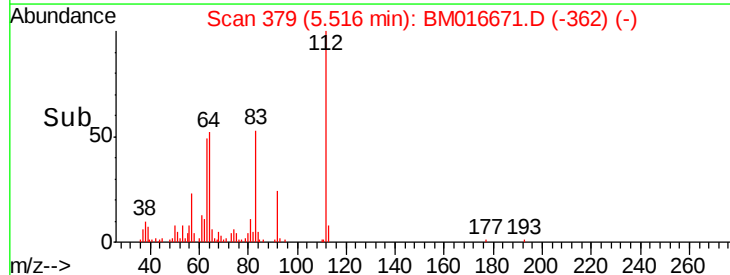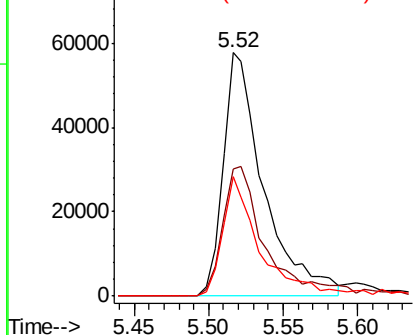



#7

Phenol-d6

Concen: 51.116 ng

RT: 7.15 min Scan# 656

Delta R.T. 0.00 min

Lab File: BM016671.D

Acq: 05 Sep 2018 14:53

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 99 Resp: 209945

Ion Ratio Lower Upper

99 100

42 26.1 11.0 16.4#

71 75.7 23.4 35.2#






Abundance

Ion 99.00 (98.70 to 99.70): BM016671.D (-639) (-)

Ion 42.00 (41.70 to 42.70): BM016671.D (-639) (-)

Ion 71.00 (70.70 to 71.70): BM016671.D (-639) (-)

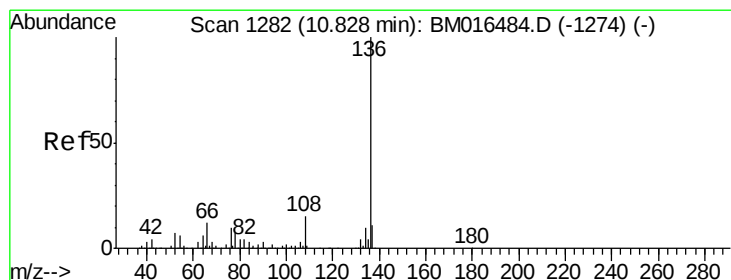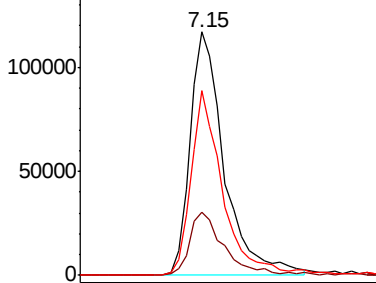

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.77 min Scan# 1272

Delta R.T. -0.00 min

Lab File: BM016671.D

Acq: 05 Sep 2018 14:53

Tgt Ion: 136 Resp: 209245


Ion Ratio Lower Upper

136 100

137 9.9 8.7 13.1

54 6.2 4.6 6.8

68 1.6 3.7 5.5#





Abundance


Ion 136.00 (135.70 to 136.70): BM016671.D (-1255) (-)

Ion 137.00 (136.70 to 137.70): BM016671.D (-1255) (-)

Ion 54.00 (53.70 to 54.70): BM016671.D (-1255) (-)

Ion 68.00 (67.70 to 68.70): BM016671.D (-1255) (-)




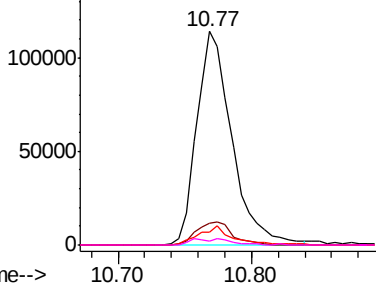




#23
 Nitrobenzene-d5
 Concen: 41.330 ng
 RT: 9.16 min Scan# 998
 Delta R.T. 0.01 min
 Lab File: BM016671.D
 Acq: 05 Sep 2018 14:53




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion	82	Resp	189407
Ion Ratio	100	Lower	Upper
128	30.2	32.8	49.2#
54	34.8	40.6	60.8#

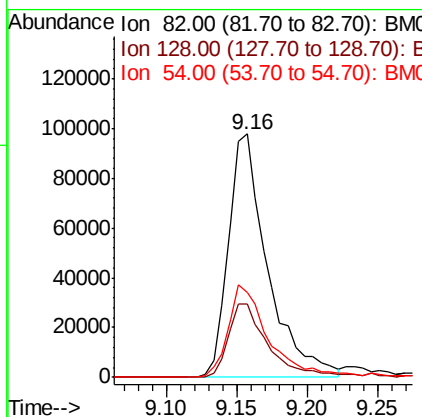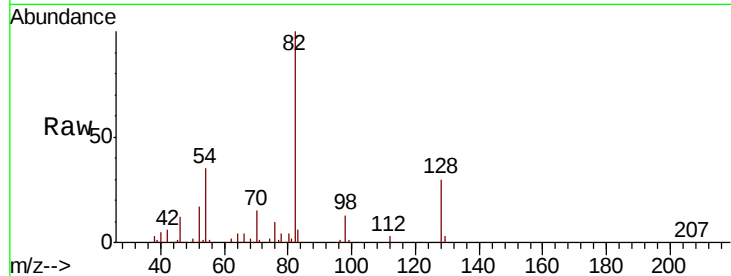

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.61 min Scan# 1925
 Delta R.T. 0.00 min
 Lab File: BM016671.D
 Acq: 05 Sep 2018 14:53

Tgt Ion	164	Resp	134309
Ion Ratio	100	Lower	Upper
162	107.4	82.4	123.6
160	48.9	35.8	53.6

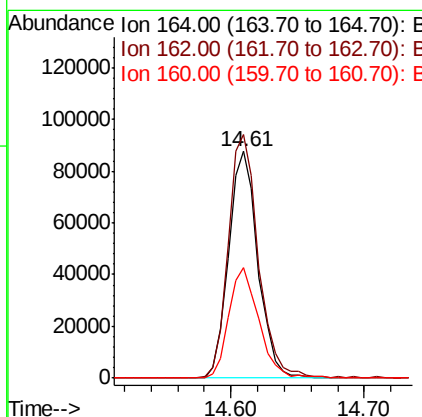




#41
 2,4,6-Tribromophenol
 Concen: 21.996 ng
 RT: 16.11 min Scan# 2180
 Delta R.T. 0.01 min
 Lab File: BM016671.D
 Acq: 05 Sep 2018 14:53

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.4	0.0	0.0#
141	44.0	0.0	0.0#






Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

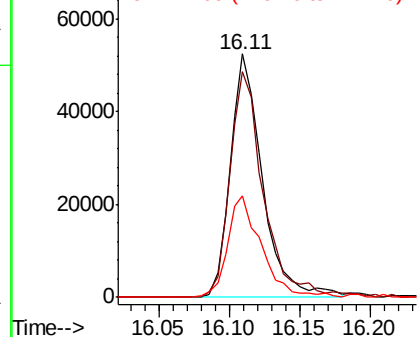

#44
 2-Fluorobiphenyl
 Concen: 32.428 ng
 RT: 13.22 min Scan# 1689
 Delta R.T. 0.00 min
 Lab File: BM016671.D
 Acq: 05 Sep 2018 14:53

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	28.5	42.7
170	23.2	18.8	28.2






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

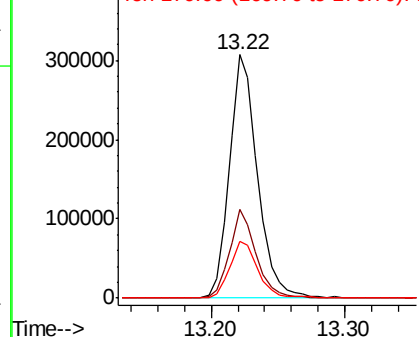

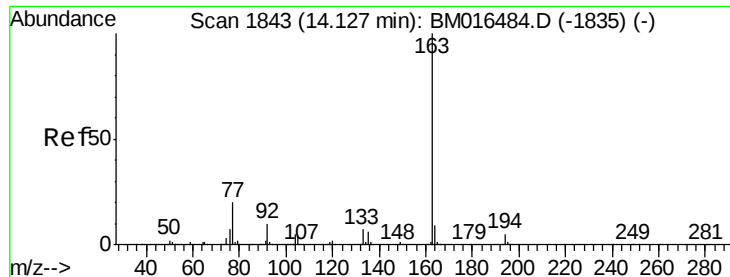

#49

Dimethylphthalate

Concen: 9.529 ng

RT: 14.07 min Scan# 1834

Delta R.T. -0.00 min

Lab File: BM016671.D

Acq: 05 Sep 2018 14:53

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 122955

Ion Ratio Lower Upper

163 100

194 5.0 2.7 4.1#




164 11.1 8.2 12.2

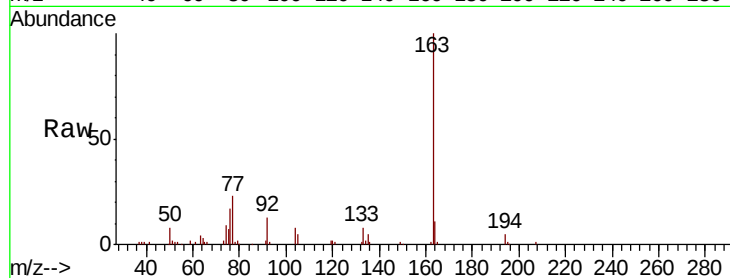

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

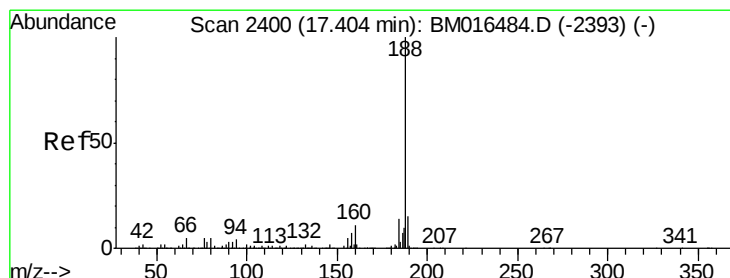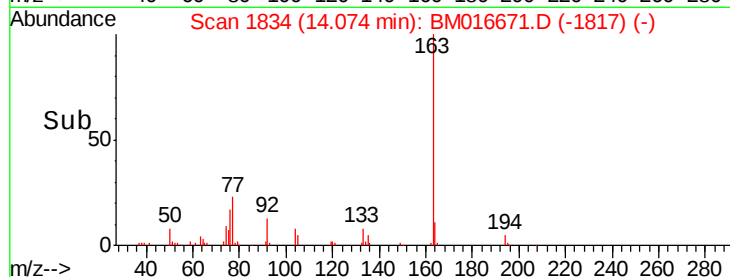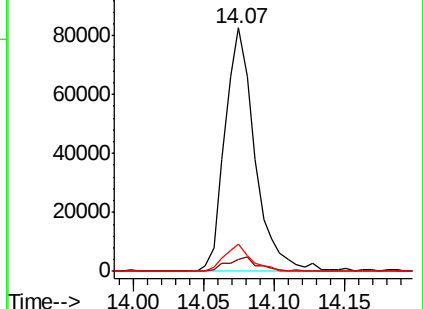

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.35 min Scan# 2391

Delta R.T. -0.01 min

Lab File: BM016671.D

Acq: 05 Sep 2018 14:53


Tgt Ion:188 Resp: 442174

Ion Ratio Lower Upper

188 100

94 2.8 8.7 13.1#



80 3.3 9.3 13.9#

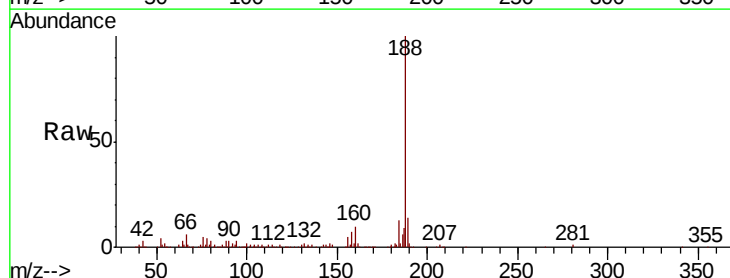


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

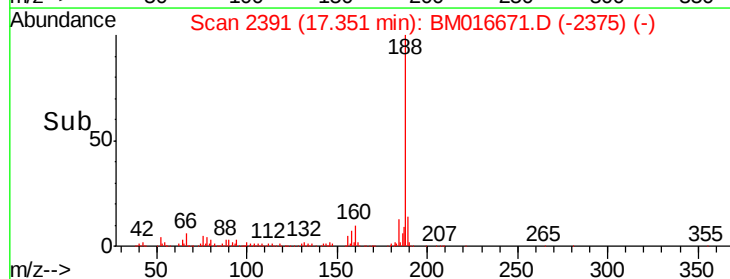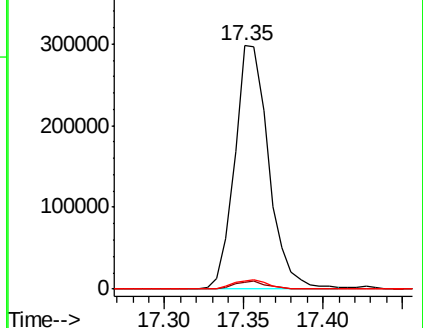







#74
 Fluoranthene
 Concen: 4.601 ng
 RT: 19.41 min Scan# 2741
 Delta R.T. 0.01 min
 Lab File: BM016671.D
 Acq: 05 Sep 2018 14:53

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:	202	Resp:	154172
Ion Ratio	Lower	Upper	
202	100		
101	2.1	0.0	28.7
203	17.4	0.0	37.2

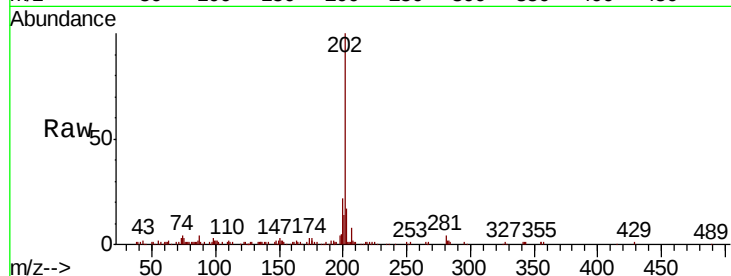


Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 203.00 (202.70 to 203.70): E


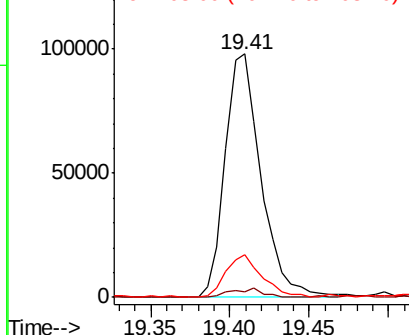



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.50 min Scan# 3097
 Delta R.T. 0.00 min
 Lab File: BM016671.D
 Acq: 05 Sep 2018 14:53

Tgt Ion:	240	Resp:	754521
Ion Ratio	Lower	Upper	
240	100		
120	2.6	8.2	12.2#
236	26.0	20.0	30.0



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E




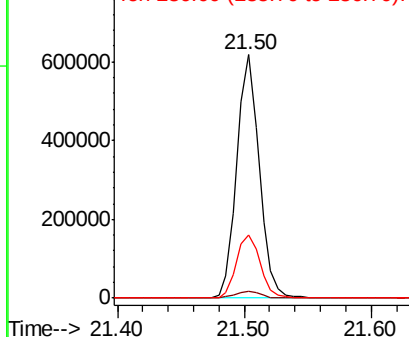


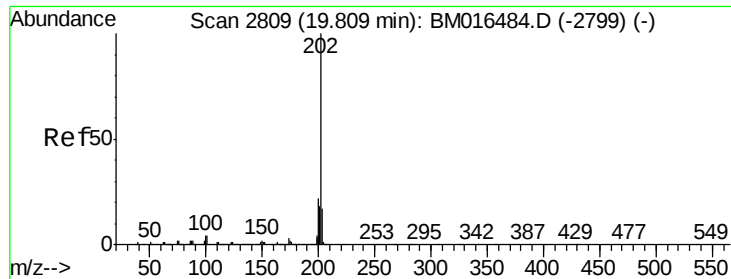

#77
Pvrene
Concen: 3.594 ng
RT: 19.77 min Scan# 2802
Delta R.T. 0.01 min
Lab File: BM016671.D
Acq: 05 Sep 2018 14:53




Instrument :
BNA_M
ClientSampled :


Tot Ion	Ratio	Lower	Upper
202	100		
200	20.6	16.9	25.3
203	16.7	14.1	21.1

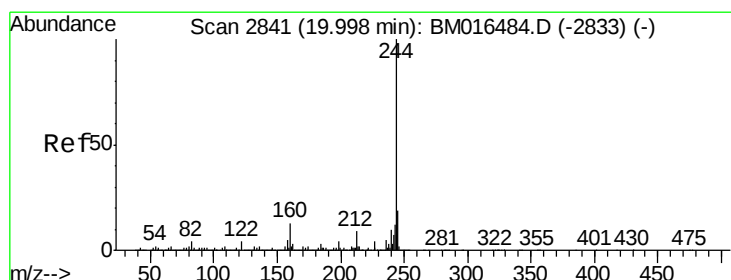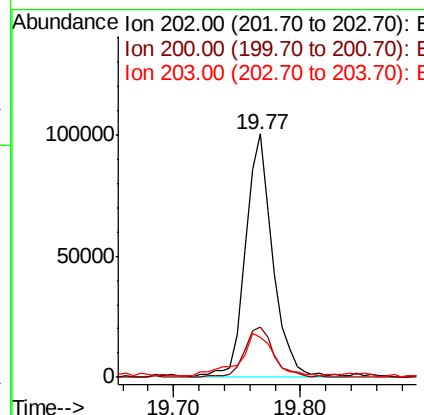

#78
Terphenyl-d14
Concen: 36.069 ng
RT: 19.94 min Scan# 2832
Delta R.T. 0.00 min
Lab File: BM016671.D
Acq: 05 Sep 2018 14:53

Tgt Ion	Ratio	Lower	Upper
244	100		
212	10.3	4.9	7.3#
122	4.0	6.2	9.4#

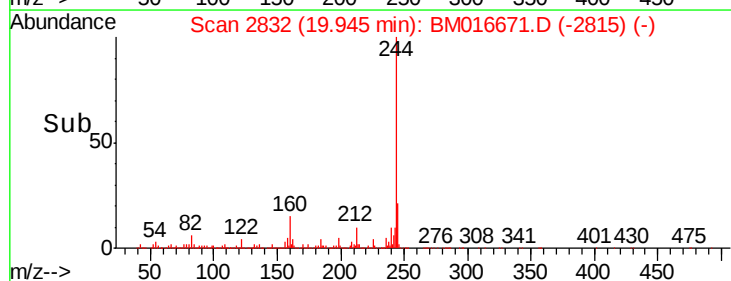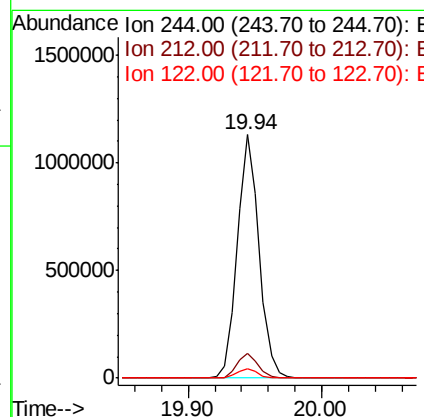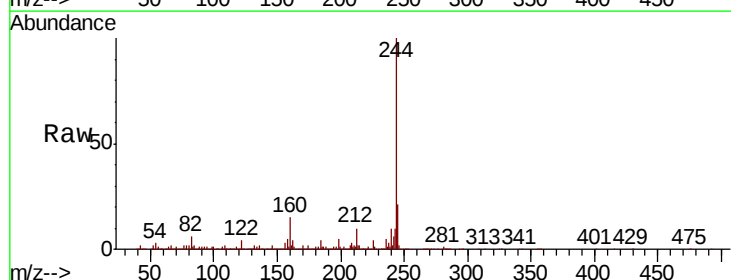

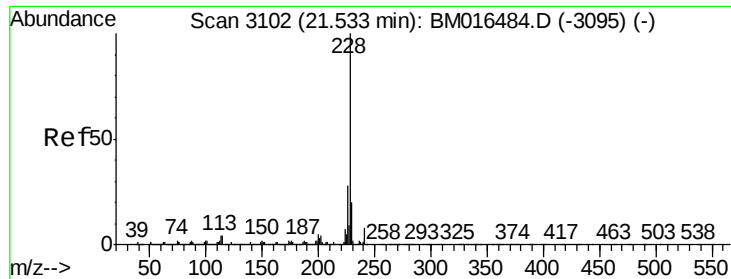

#80

Benzo(a)anthracene

Concen: 2.420 ng

RT: 21.49 min Scan# 3095

Delta R.T. 0.01 min

Lab File: BM016671.D

Acq: 05 Sep 2018 14:53

Instrument :

BNA_M

ClientSampleId :


Tot Ion:228 Resp: 107351

Ion Ratio Lower Upper

228 100

226 26.4 21.7 32.5

229 21.9 16.0 24.0



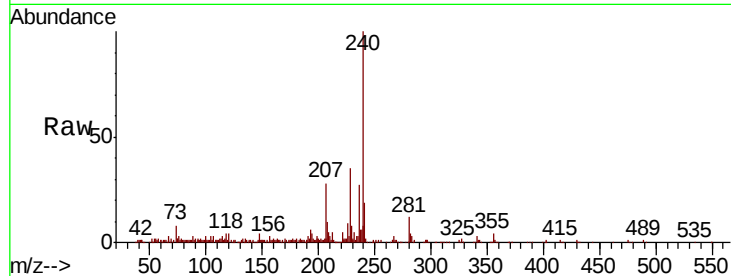


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

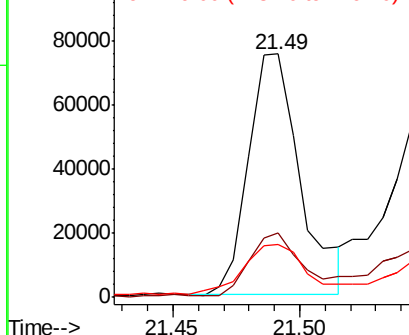

#82

Chrysene

Concen: 2.203 ng

RT: 21.54 min Scan# 3104

Delta R.T. 0.01 min

Lab File: BM016671.D

Acq: 05 Sep 2018 14:53


Tgt Ion:228 Resp: 93234

Ion Ratio Lower Upper

228 100

226 27.2 24.1 36.1

229 20.3 15.5 23.3






Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



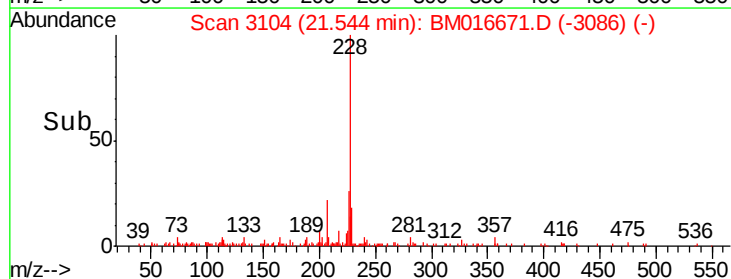
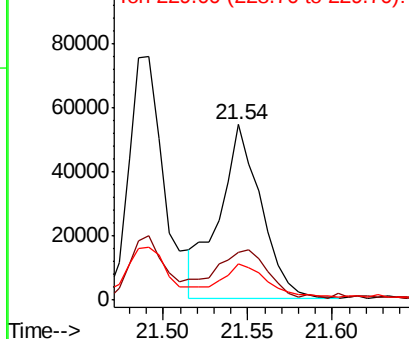




#86
Pervlene-d12
Concen: 20.000 ng
RT: 23.77 min Scan# 3482
Delta R.T. 0.00 min
Lab File: BM016671.D
Acq: 05 Sep 2018 14:53




Instrument :
BNA_M
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
264	100		
260	24.4	18.6	27.8
265	22.7	17.3	25.9

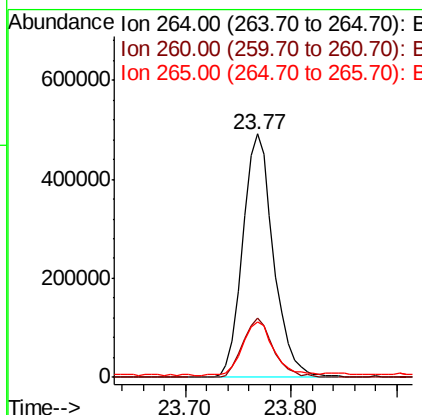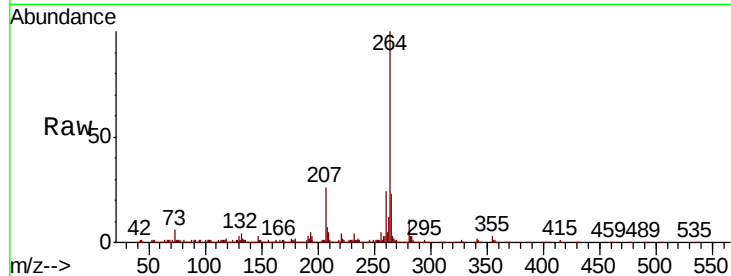

#87
Benzo(b)fluoranthene
Concen: 3.027 ng
RT: 23.10 min Scan# 3369
Delta R.T. 0.02 min
Lab File: BM016671.D
Acq: 05 Sep 2018 14:53

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.3	18.0	27.0
125	4.2	9.9	14.9

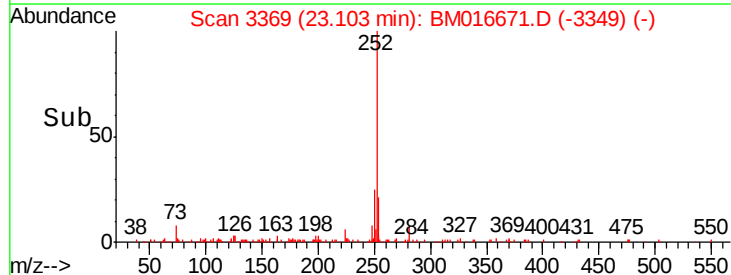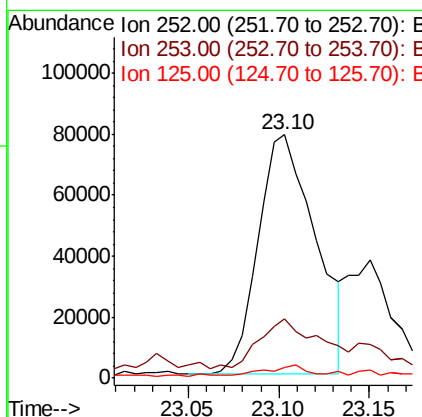



#88

Benzo(k)fluoranthene

Concen: 2.975 ng

RT: 23.10 min Scan# 3369

Delta R.T. -0.03 min

Lab File: BM016671.D





Acq: 05 Sep 2018 14:53

Instrument :

BNA_M

ClientSampleId :

Tot Ion:	252	Resp:	173623
Ion	Ratio	Lower	Upper
252	100		
253	24.3	17.2	25.8
125	4.2	8.1	12.1#

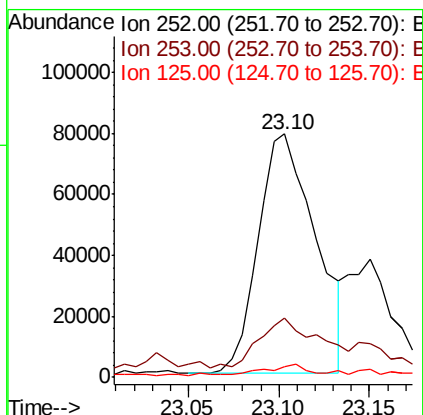

#89

Benzo(a)pyrene

Concen: 2.035 ng

RT: 23.69 min Scan# 3468

Delta R.T. 0.01 min

Lab File: BM016671.D

Acq: 05 Sep 2018 14:53

Tgt Ion:	252	Resp:	113579
Ion	Ratio	Lower	Upper
252	100		
253	30.6	17.6	26.4#
125	3.6	7.4	11.2#

