

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090518\
 Data File : BM016677.D
 Acq On : 05 Sep 2018 18:30
 Operator : SJ/JU
 Sample : J4741-21
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 06 04:01:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 27 13:01:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.97	152	67086	20.00	ng	-0.04
21) Naphthalene-d8	10.77	136	216416	20.00	ng	-0.04
38) Acenaphthene-d10	14.60	164	141218	20.00	ng	-0.04
63) Phenanthrene-d10	17.35	188	426626	20.00	ng	-0.04
75) Chrysene-d12	21.50	240	597537	20.00	ng	-0.03
86) Perylene-d12	23.76	264	736937	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	173142	50.57	ng	-0.03
7) Phenol-d6	7.15	99	137169	30.28	ng	-0.03
23) Nitrobenzene-d5	9.15	82	460171	97.09	ng	-0.04
41) 2,4,6-Tribromophenol	16.10	330	530138	134.29	ng	-0.04
44) 2-Fluorobiphenyl	13.22	172	1370709	93.30	ng	-0.04
78) Terphenyl-d14	19.94	244	3110768	110.19	ng	-0.04
Target Compounds						
15) Benzyl Alcohol	8.27	79	10953	2.604	ng	# 1
31) Naphthalene	10.83	128	53525	5.191	ng	# 94
49) Dimethylphthalate	14.07	163	141676	10.442	ng	# 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090518\
Data File : BM016677.D
Acq On : 05 Sep 2018 18:30
Operator : SJ/JU
Sample : J4741-21
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 06 04:01:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 27 13:01:22 2018
Response via : Initial Calibration

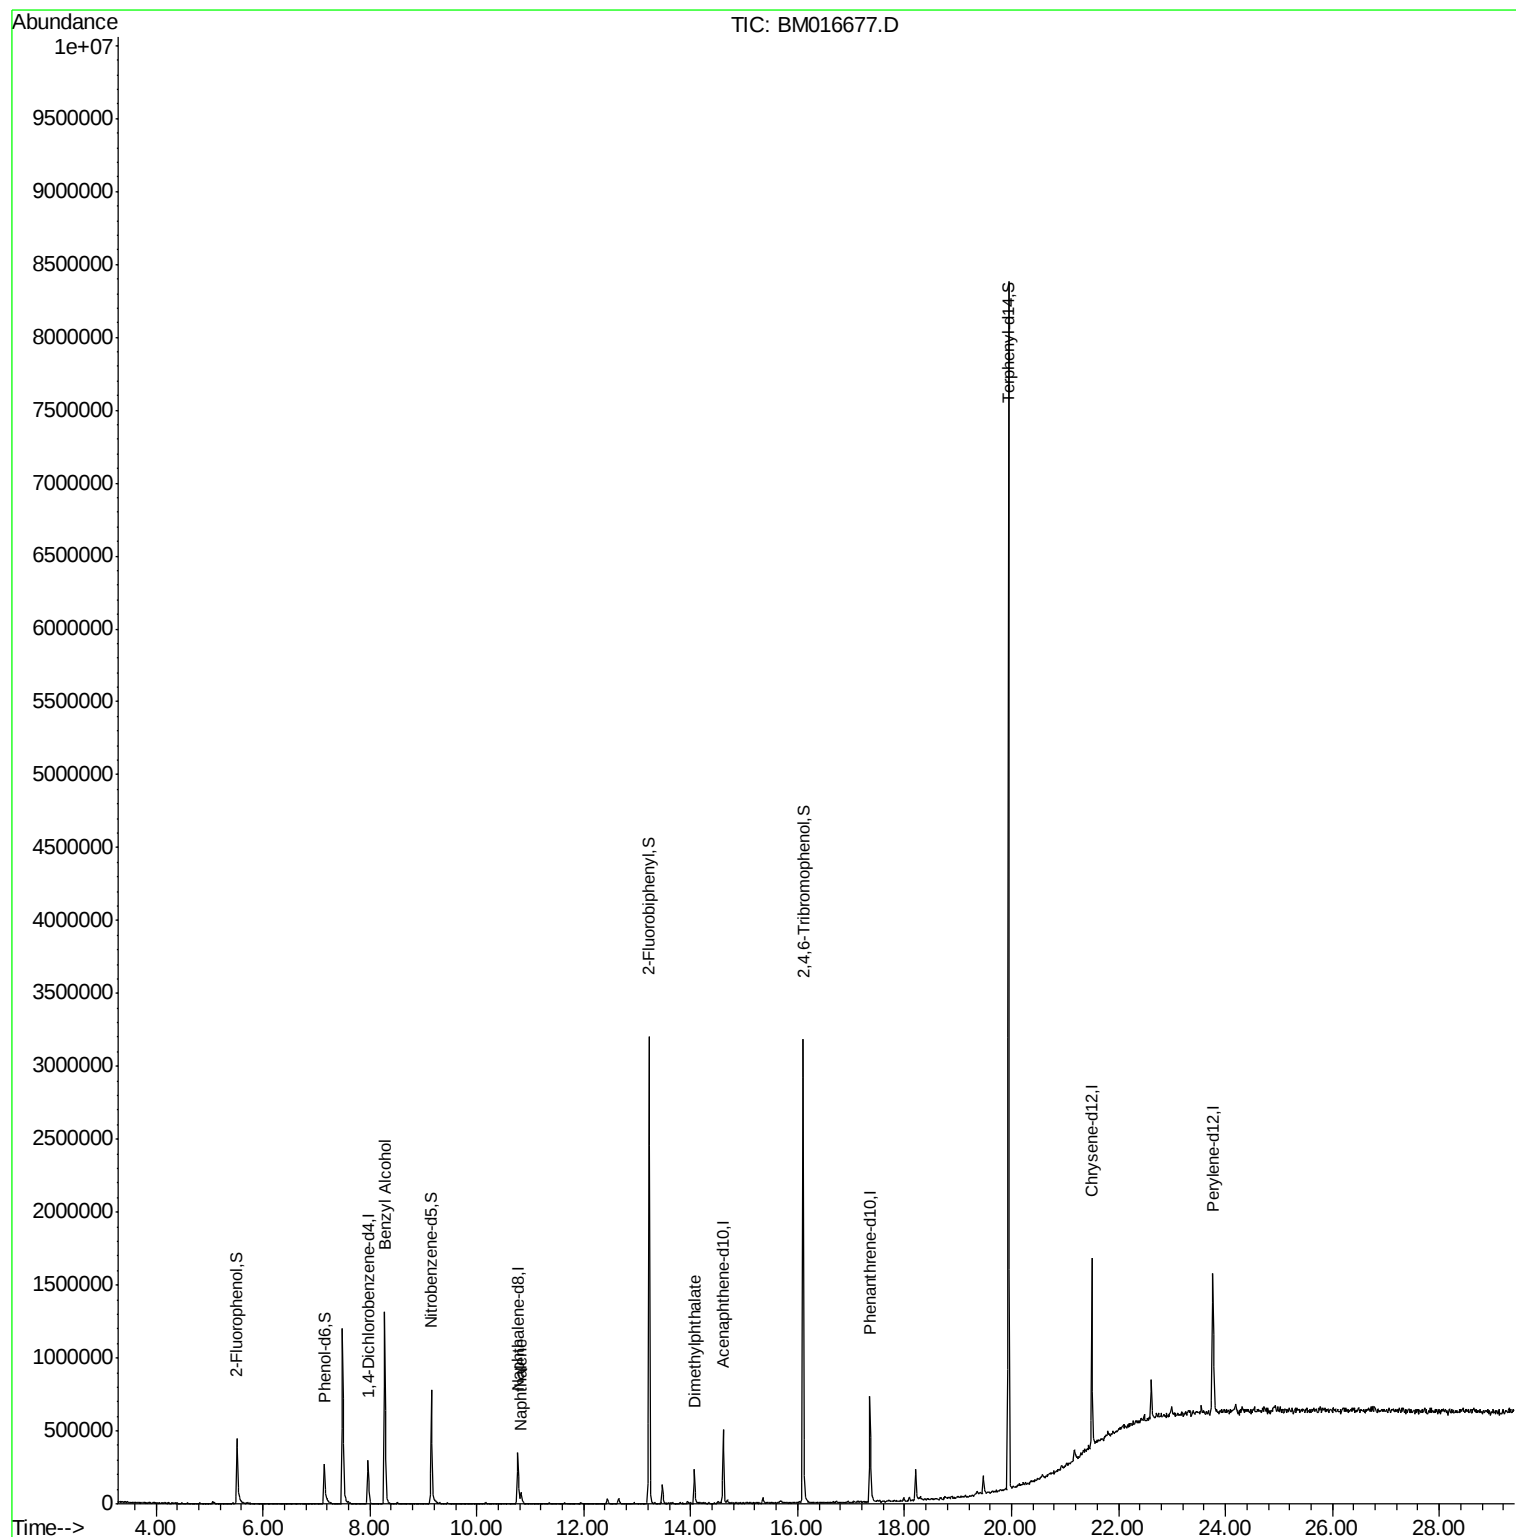




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.97 min Scan# 796
Delta R.T. -0.04 min
Lab File: BM016677.D
Acq: 05 Sep 2018 18:30

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	148.2	119.5	179.3
115	58.1	43.0	64.4

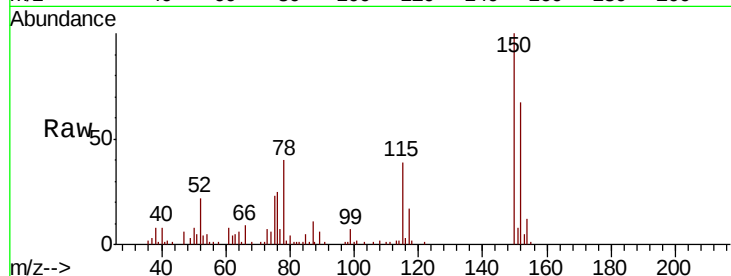


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

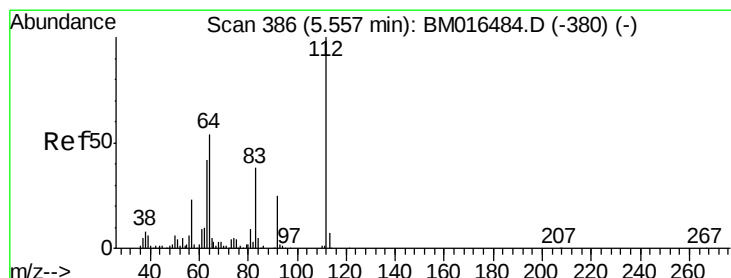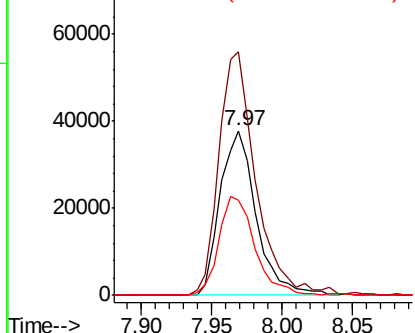



#5


2-Fluorophenol
Concen: 50.575 ng
RT: 5.52 min Scan# 379
Delta R.T. -0.03 min
Lab File: BM016677.D
Acq: 05 Sep 2018 18:30

Tgt Ion	Ratio	Lower	Upper
112	100		
64	56.9	38.6	57.8
63	44.5	19.3	28.9

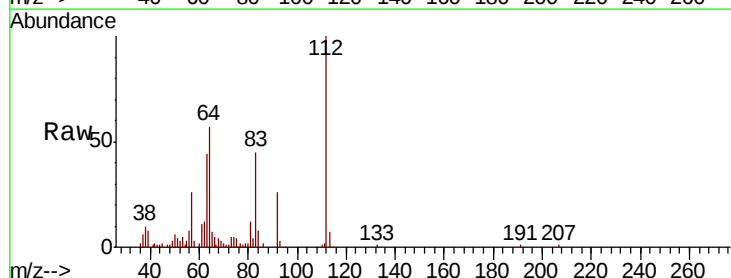

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

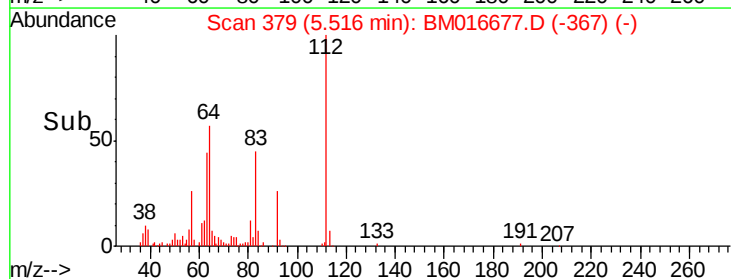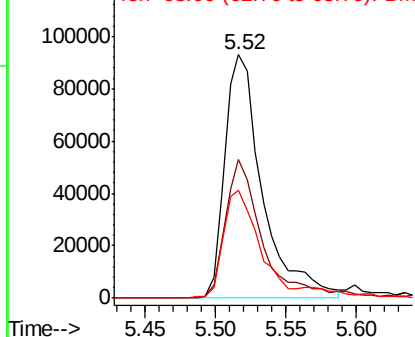

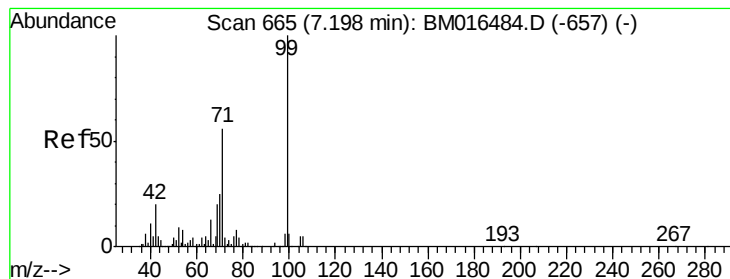

#7

Phenol-d6

Concen: 30.279 ng

RT: 7.15 min Scan# 657

Delta R.T. -0.03 min

Lab File: BM016677.D

Acq: 05 Sep 2018 18:30

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 99 Resp: 137169

Ion Ratio Lower Upper

99 100

42 18.4 11.0 16.4#




71 57.4 23.4 35.2#

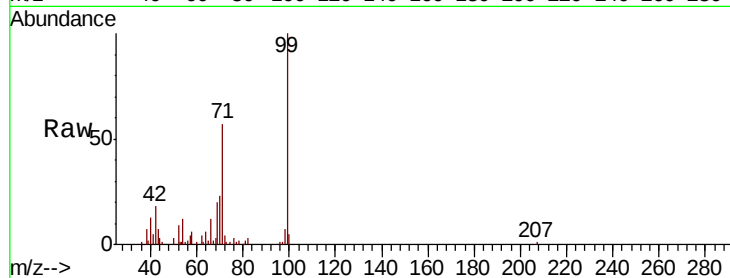

Abundance Ion 99.00 (98.70 to 99.70): BM016484.D (-657) (-)

Ion 42.00 (41.70 to 42.70): BM016484.D (-657) (-)

Ion 71.00 (70.70 to 71.70): BM016484.D (-657) (-)

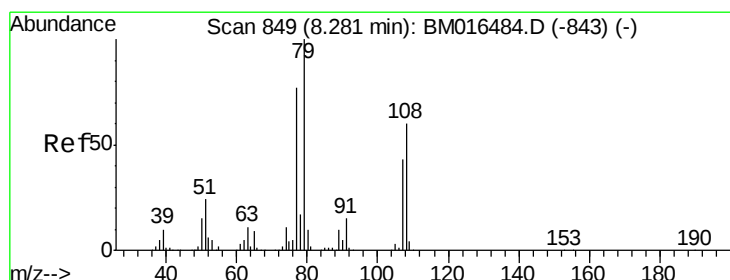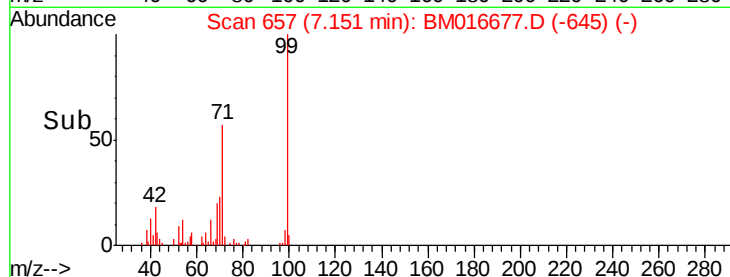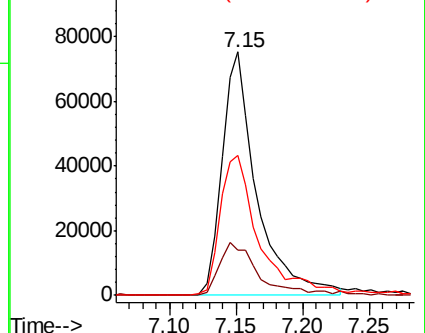

#15

Benzyl Alcohol

Concen: 2.604 ng

RT: 8.27 min Scan# 848

Delta R.T. 0.01 min

Lab File: BM016677.D

Acq: 05 Sep 2018 18:30


Tgt Ion: 79 Resp: 10953

Ion Ratio Lower Upper

79 100

108 133.3 65.0 97.4#



77 235.2 53.0 79.6#

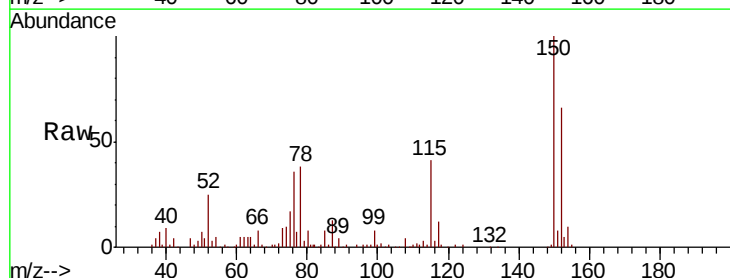


Abundance Ion 79.00 (78.70 to 79.70): BM016484.D (-843) (-)

Ion 108.00 (107.70 to 108.70): BM016484.D (-843) (-)

Ion 77.00 (76.70 to 77.70): BM016484.D (-843) (-)

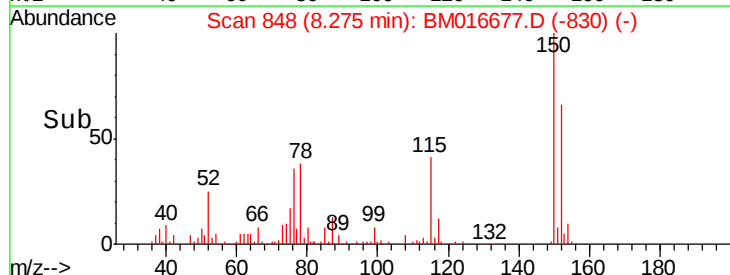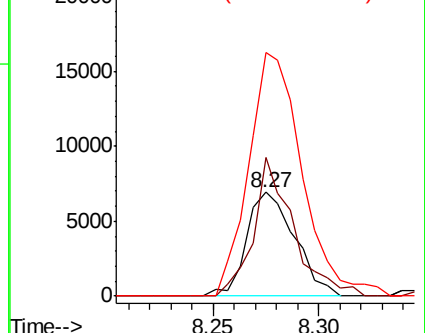


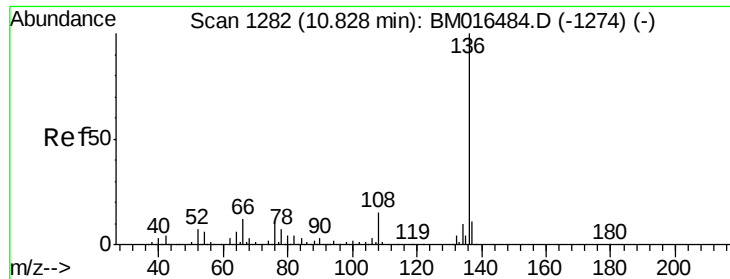




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.77 min Scan# 1272
Delta R.T. -0.04 min
Lab File: BM016677.D
Acq: 05 Sep 2018 18:30

Instrument :
BNA_M
ClientSampleId :

Tot Ion:	136	Resp:	216416
Ion	Ratio	Lower	Upper
136	100		
137	11.3	8.7	13.1
54	7.3	4.6	6.8#
68	2.2	3.7	5.5#

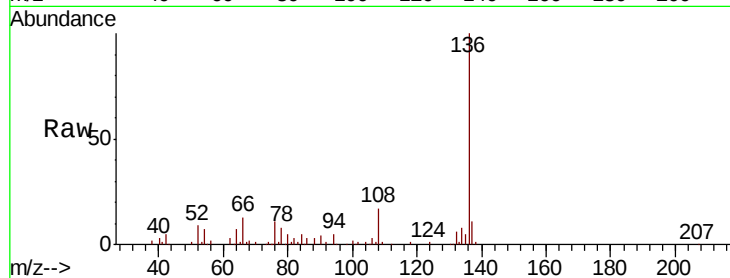


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

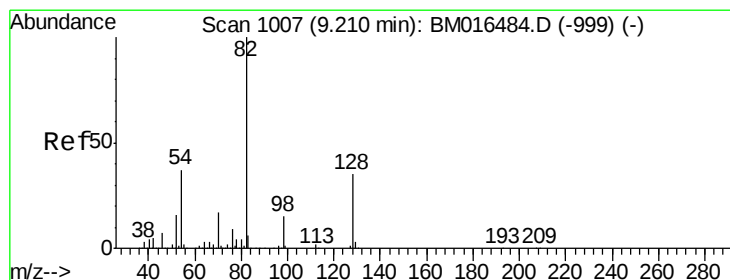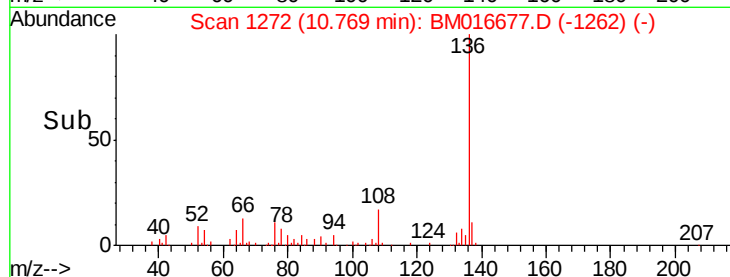
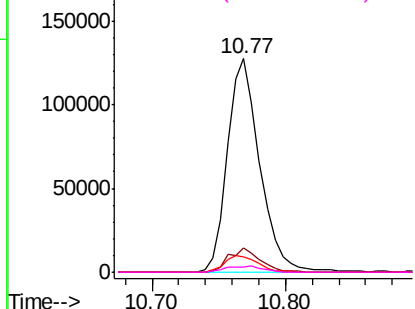



#23
Nitrobenzene-d5
Concen: 97.086 ng
RT: 9.15 min Scan# 997
Delta R.T. -0.04 min
Lab File: BM016677.D
Acq: 05 Sep 2018 18:30

Tgt Ion:	82	Resp:	460171
Ion	Ratio	Lower	Upper
82	100		
128	34.3	32.8	49.2
54	39.0	40.6	60.8#

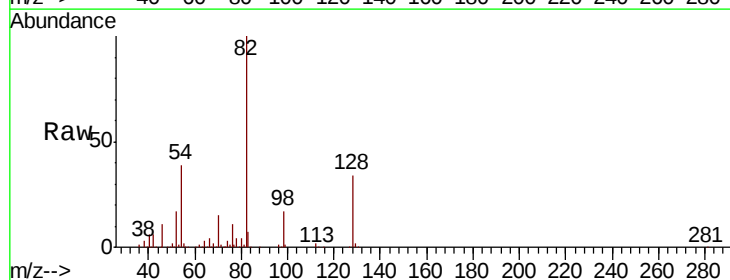

Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM



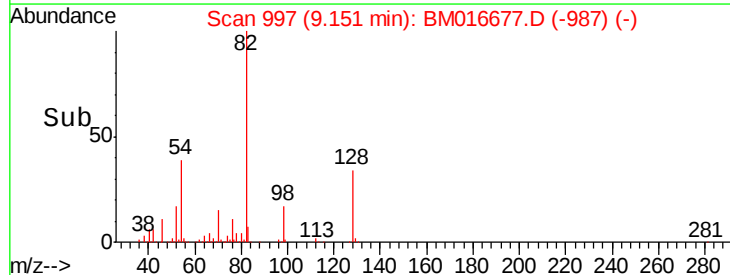
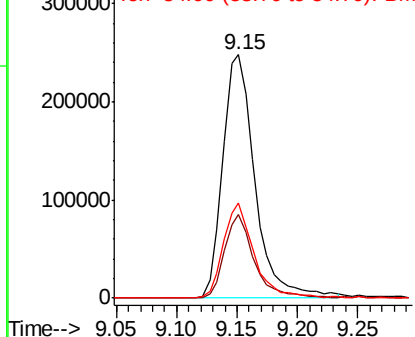


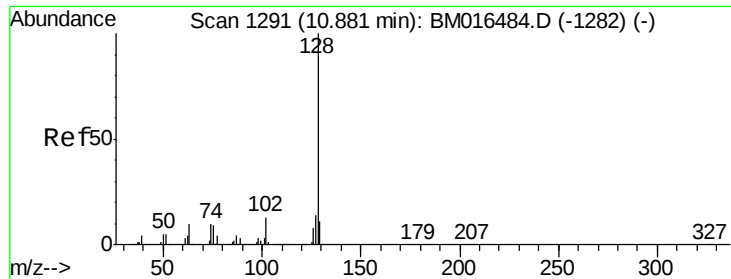

#31
Naphthalene
Concen: 5.191 ng
RT: 10.83 min Scan# 1282
Delta R.T. -0.04 min
Lab File: BM016677.D
Acq: 05 Sep 2018 18:30




Instrument :
BNA_M
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
128	100		
129	8.3	8.9	13.3#
127	11.4	10.4	15.6

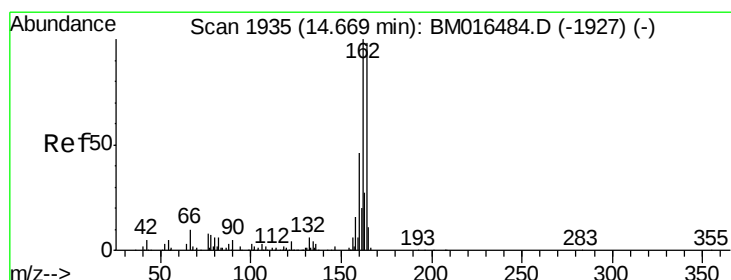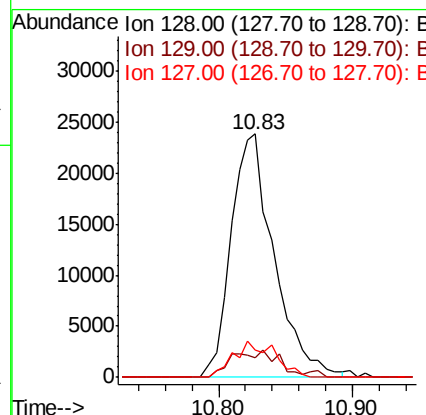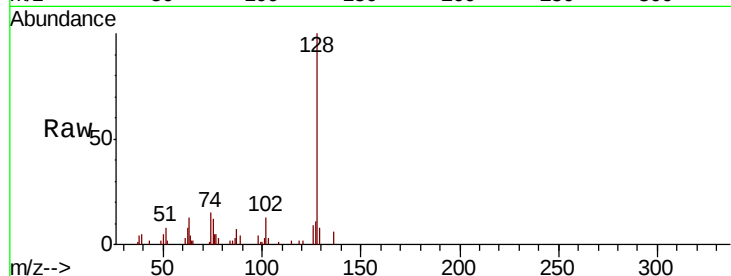

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.60 min Scan# 1924
Delta R.T. -0.04 min
Lab File: BM016677.D
Acq: 05 Sep 2018 18:30

Tgt Ion	Ratio	Lower	Upper
164	100		
162	106.0	82.4	123.6
160	51.7	35.8	53.6



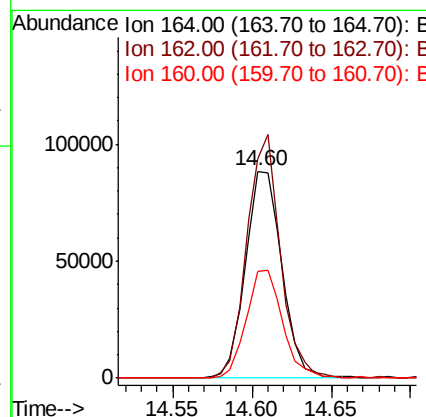
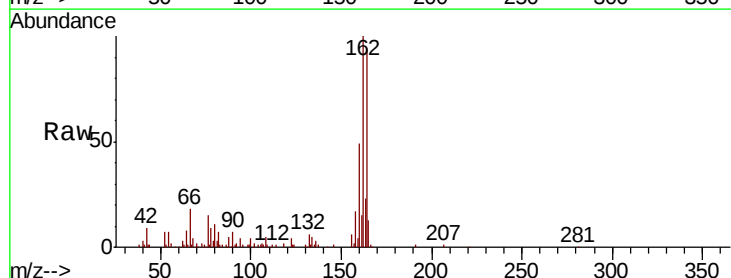




#41
 2,4,6-Tribromophenol
 Concen: 134.292 ng
 RT: 16.10 min Scan# 2179
 Delta R.T. -0.04 min
 Lab File: BM016677.D
 Acq: 05 Sep 2018 18:30




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
330	100		
332	94.6	0.0	0.0#
141	34.9	0.0	0.0#

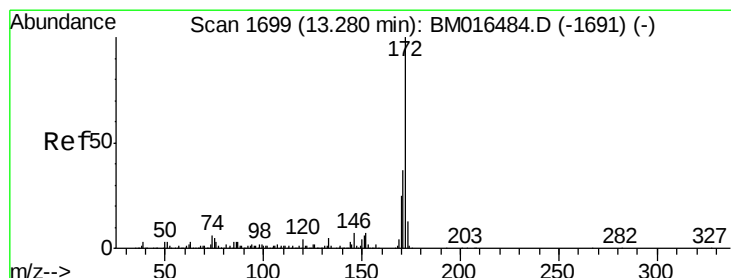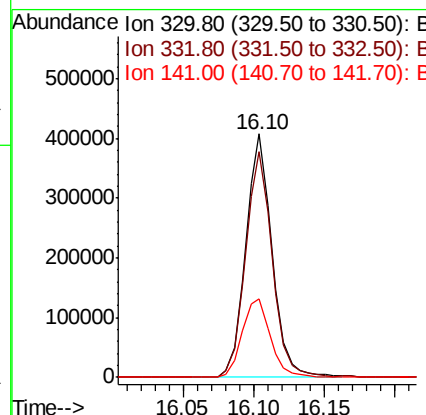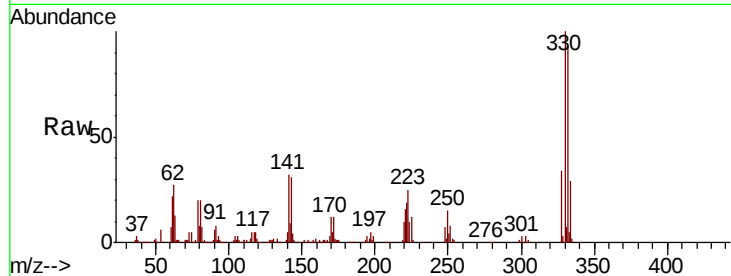

#44
 2-Fluorobiphenyl
 Concen: 93.300 ng
 RT: 13.22 min Scan# 1689
 Delta R.T. -0.04 min
 Lab File: BM016677.D
 Acq: 05 Sep 2018 18:30

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	28.5	42.7
170	24.0	18.8	28.2

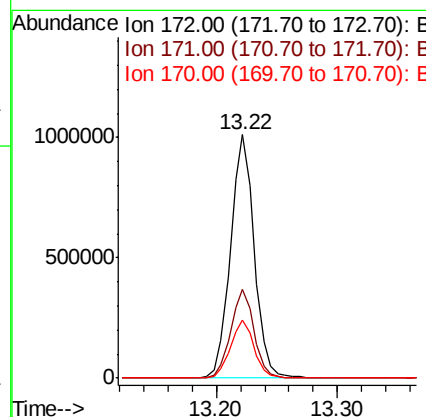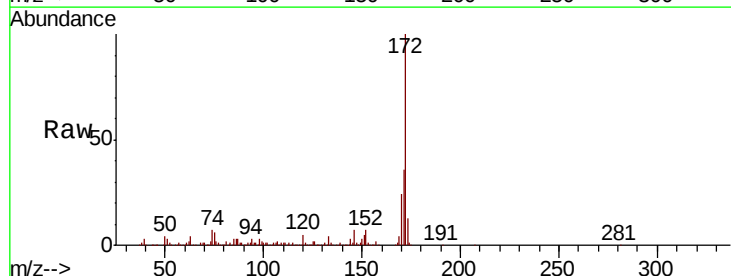

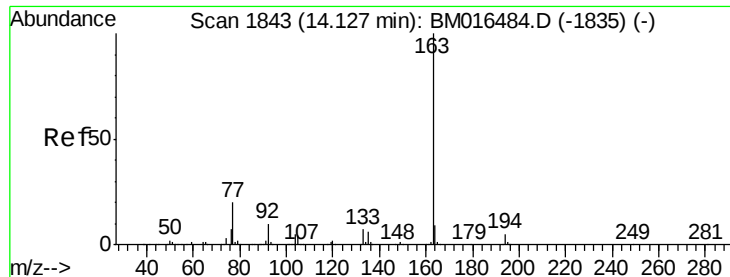

#49

Dimethylphthalate

Concen: 10.442 ng

RT: 14.07 min Scan# 1834

Delta R.T. -0.04 min

Lab File: BM016677.D

Acq: 05 Sep 2018 18:30

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 141676

Ion Ratio Lower Upper




163 100

194 6.3 2.7 4.1#

164 7.7 8.2 12.2#

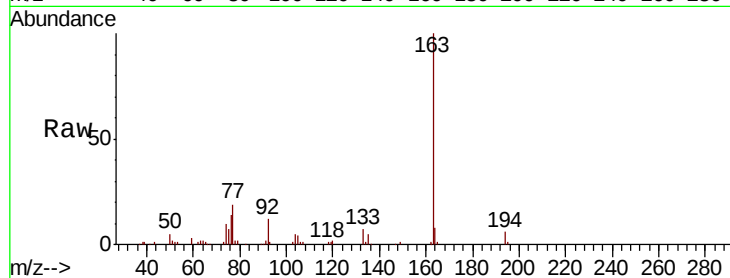

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

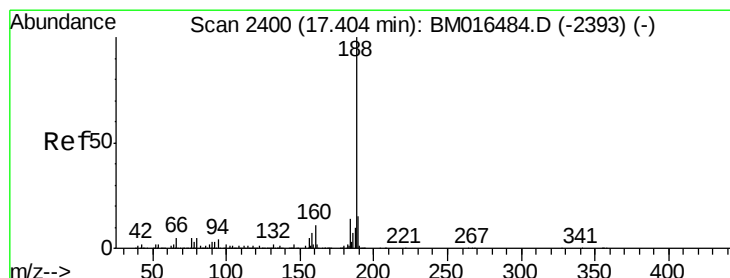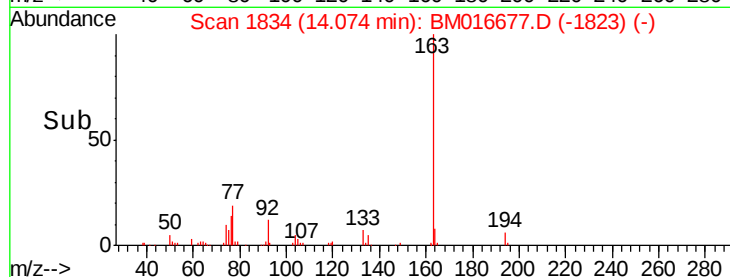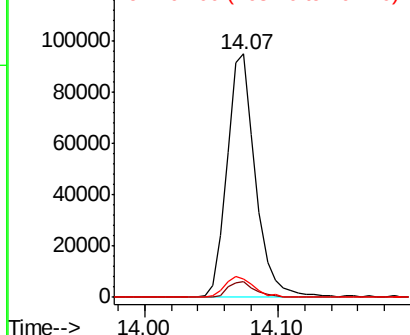

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.35 min Scan# 2391

Delta R.T. -0.04 min

Lab File: BM016677.D

Acq: 05 Sep 2018 18:30


Tgt Ion:188 Resp: 426626

Ion Ratio Lower Upper



188 100


94 4.0 8.7 13.1#

80 3.4 9.3 13.9#

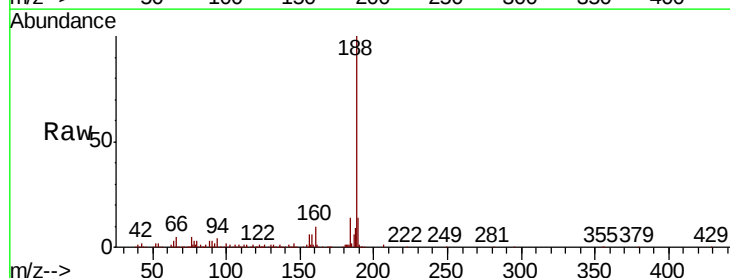

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0

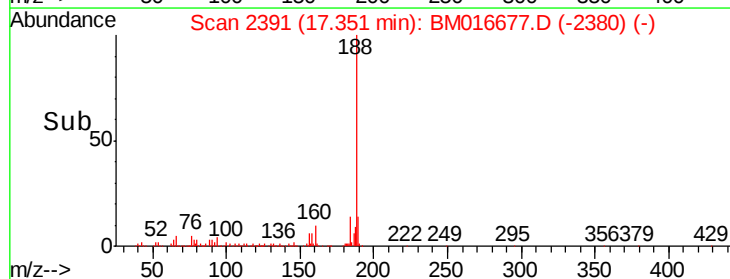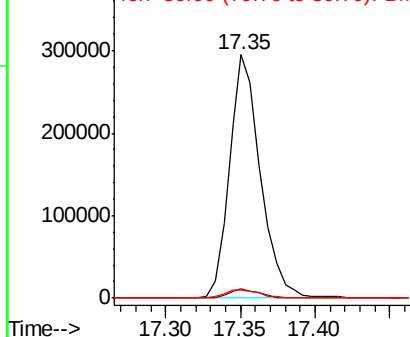



#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.50 min Scan# 3097

Delta R.T. -0.03 min

Lab File: BM016677.D

Acq: 05 Sep 2018 18:30

Instrument :

BNA_M

ClientSampleId :


Tot Ion:240 Resp: 597537

Ion Ratio Lower Upper

240 100

120 2.9 8.2 12.2#




236 25.4 20.0 30.0

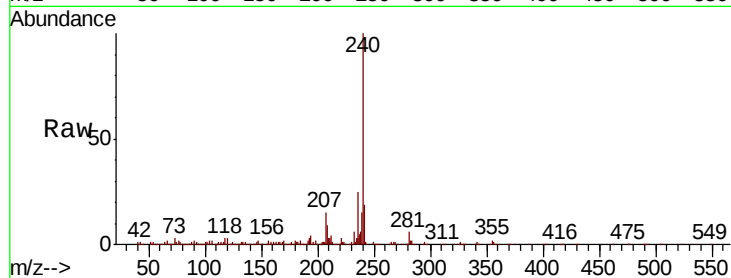

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

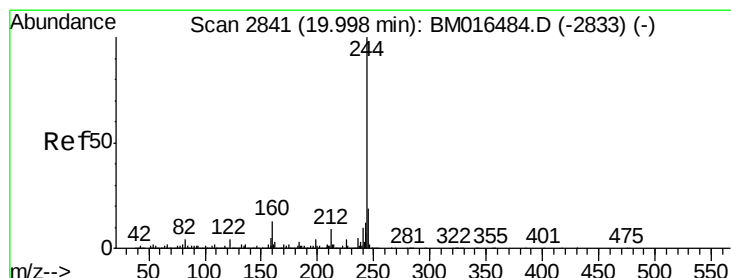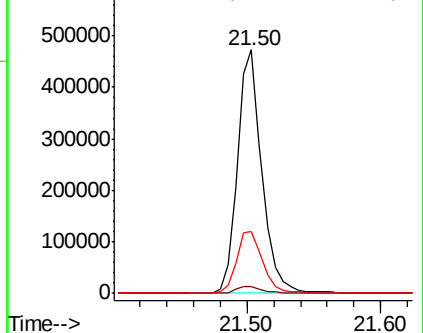

#78

Terphenyl-d14

Concen: 110.188 ng

RT: 19.94 min Scan# 2832

Delta R.T. -0.04 min

Lab File: BM016677.D

Acq: 05 Sep 2018 18:30


Tgt Ion:244 Resp: 3110768

Ion Ratio Lower Upper

244 100

212 9.4 4.9 7.3#



122 3.3 6.2 9.4#

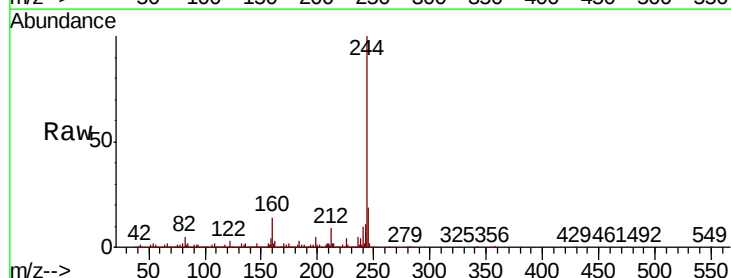


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

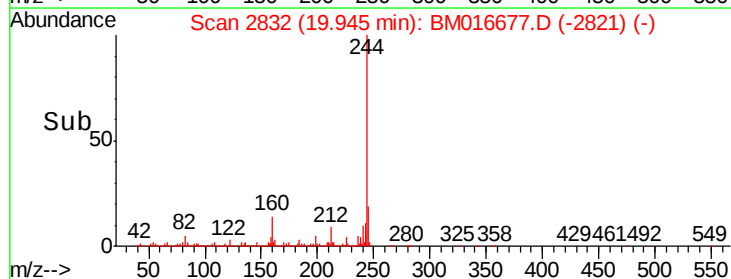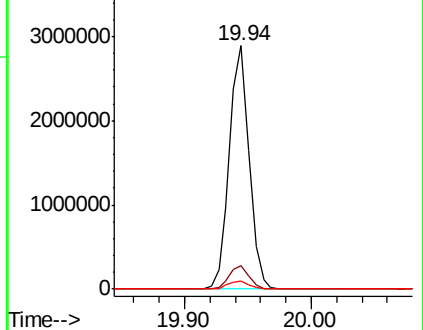



#86
Pervlene-d12
Concen: 20.000 ng
RT: 23.76 min Scan# 3481
Delta R.T. -0.05 min
Lab File: BM016677.D
Acq: 05 Sep 2018 18:30

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.4	18.6	27.8
265	21.7	17.3	25.9

