

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090518\
Data File : BM016681.D
Acq On : 05 Sep 2018 20:55
Operator : SJ/JU
Sample : PB112623BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112623BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	373	378	393	rBV	1476074	2266621	28.20%	6.541%
2	7.146	650	656	667	rBV	1454818	2279416	28.36%	6.578%
3	7.493	709	715	727	rBV	1805677	2883069	35.87%	8.320%
4	7.963	788	795	810	rBB2	301326	547668	6.81%	1.580%
5	8.275	842	848	862	rBV	1563066	2602450	32.38%	7.510%
6	9.151	990	997	1010	rBV	865503	1533472	19.08%	4.425%
7	10.769	1265	1272	1286	rBV	308868	581544	7.24%	1.678%
8	13.222	1682	1689	1699	rBV	3680360	5005673	62.28%	14.446%
9	14.604	1919	1924	1937	rVB2	488849	765878	9.53%	2.210%
10	16.098	2172	2178	2196	rBV	3326849	4792566	59.63%	13.831%
11	17.351	2385	2391	2401	rBV	628040	949888	11.82%	2.741%
12	19.945	2827	2832	2839	rBV	7388810	8037194	100.00%	23.194%
13	21.503	3092	3097	3104	rBV	826069	1176721	14.64%	3.396%
14	23.768	3476	3482	3491	rBV	632069	1229516	15.30%	3.548%


Sum of corrected areas: 34651676

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090518\
Data File : BM016681.D
Acq On : 05 Sep 2018 20:55
Operator : SJ/JU
Sample : PB112623BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112623BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

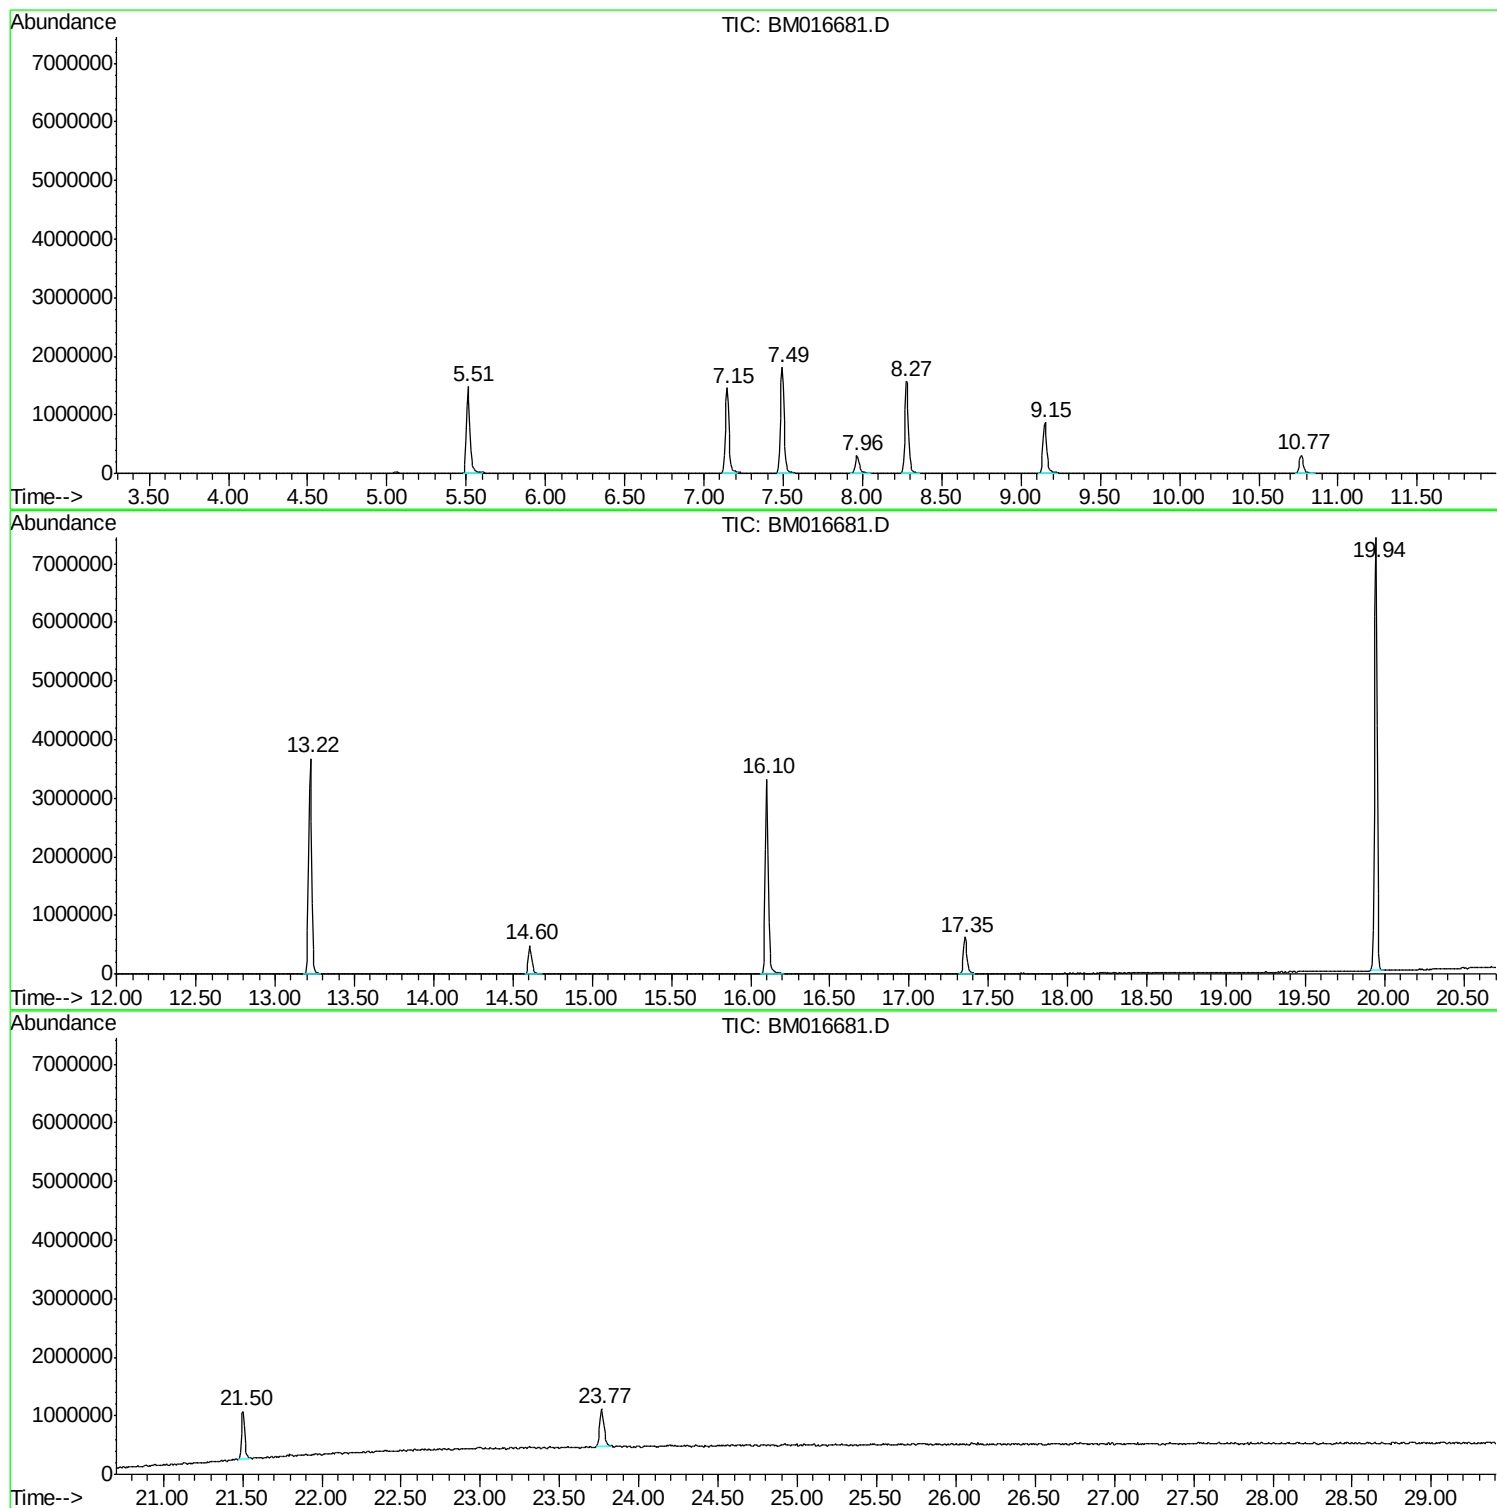

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090518\
Data File : BM016681.D
Acq On : 05 Sep 2018 20:55
Operator : SJ/JU
Sample : PB112623BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112623BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.49 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.49	105.29 ng	2883070	1,4-Dichlorobenzene-d4	7.96

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Indene, 3a,4,7,7a-tetrahydro-	120	C9H12	003048-65-5	16
2		1-Penten-3-yne	66	C5H6	000646-05-9	16
3		Tricyclo[4.2.1.0<2,5>]non-3-ene	120	C9H12	007078-40-2	16
4		1,4,4a,8a-Tetrahydro-1,4-methano...	174	C11H10O2	001200-89-1	16
5		5-Aminoindole	132	C8H8N2	005192-03-0	16

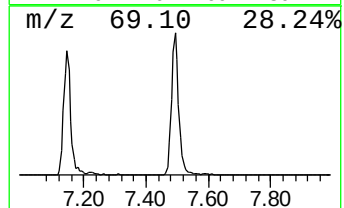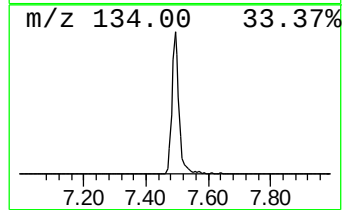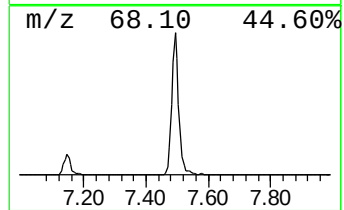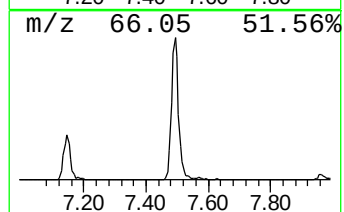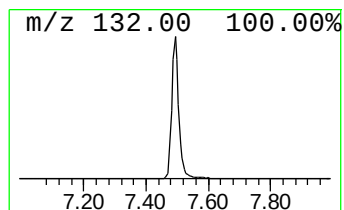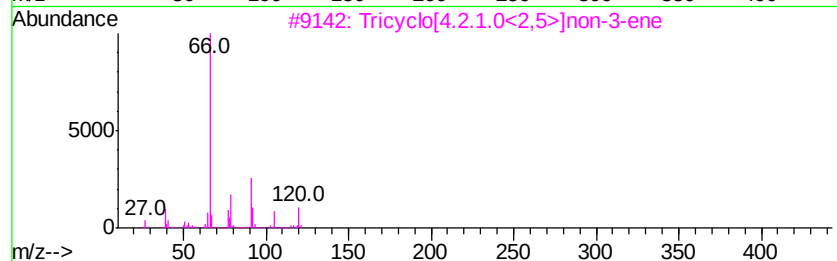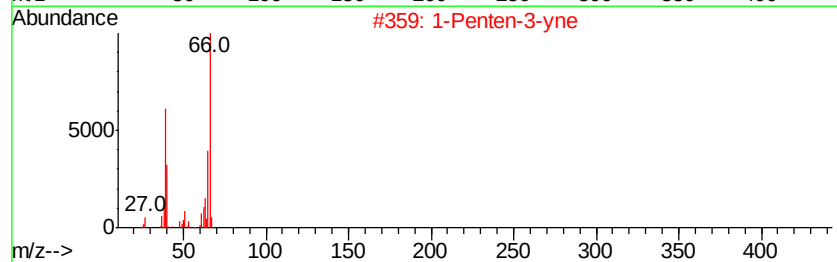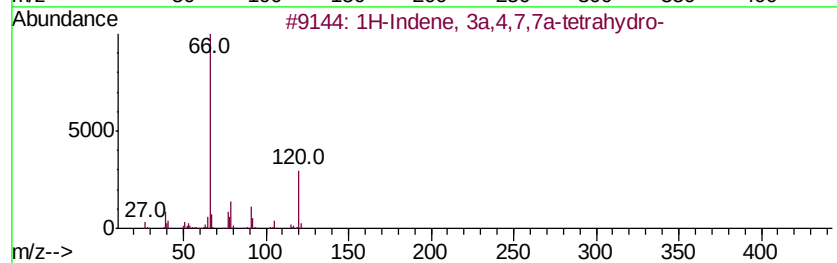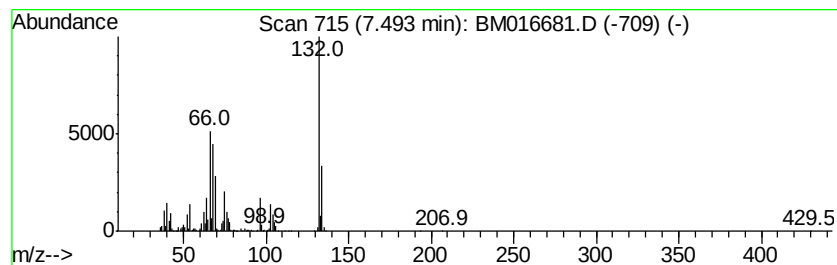

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090518\
Data File : BM016681.D
Acq On : 05 Sep 2018 20:55
Operator : SJ/JU
Sample : PB112623BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112623BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.49	7.49	105.3	ng	2883070	1	7.96	547668	20.0