
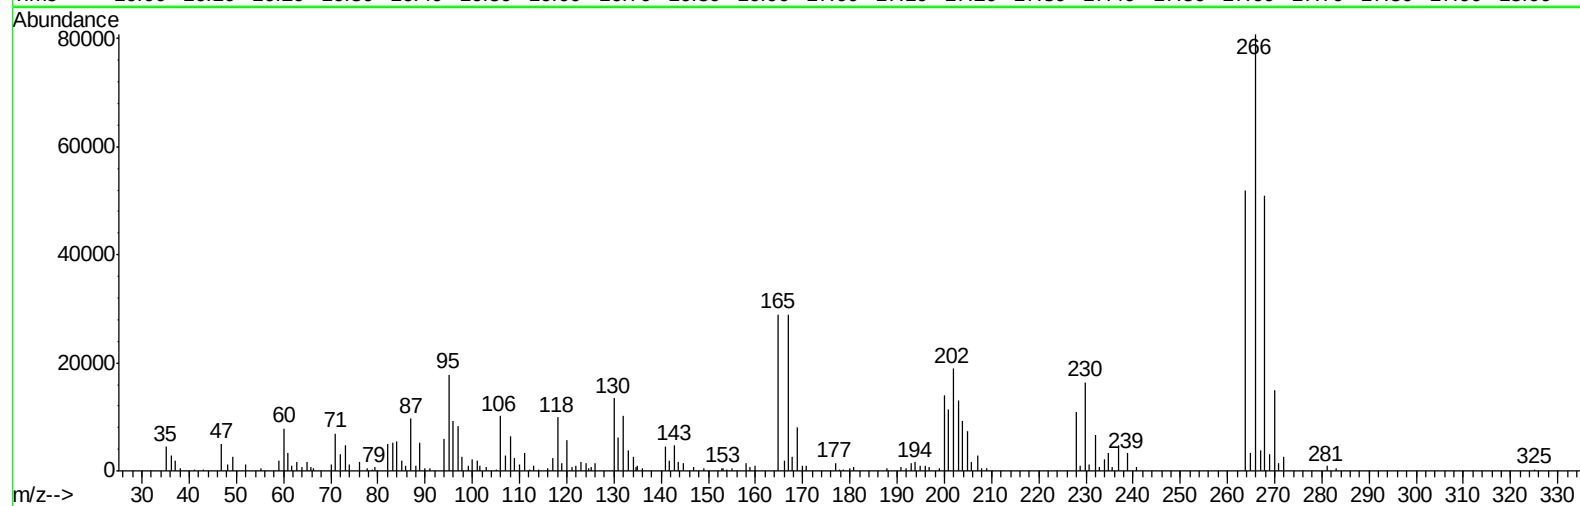


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090618\
Data File : BM016685.D
Acq On : 06 Sep 2018 15:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 08:45:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 27 13:01:22 2018
Response via : Initial Calibration

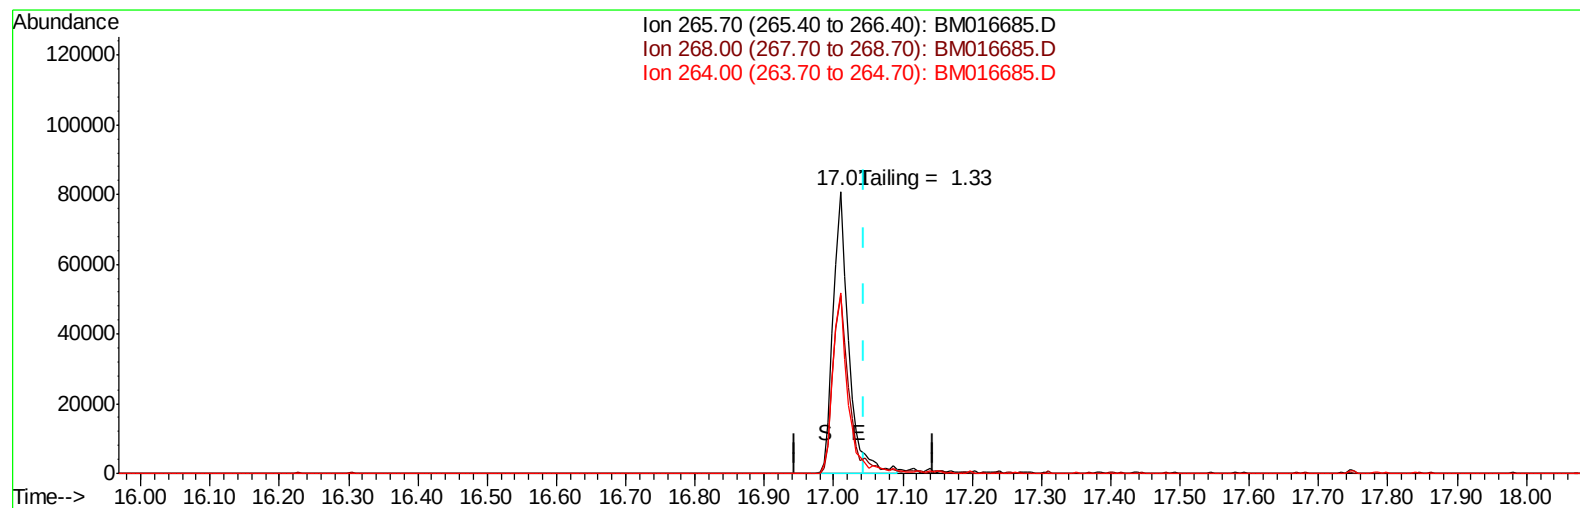

TIC: BM016685.D

(69) Pentachlorophenol (C)



17.009min (-0.035) 0.00ng

response 124961

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.11
264.00	61.20	64.28
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090618\
 Data File : BM016685.D
 Acq On : 06 Sep 2018 15:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 07 08:45:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 27 13:01:22 2018
 Response via : Initial Calibration

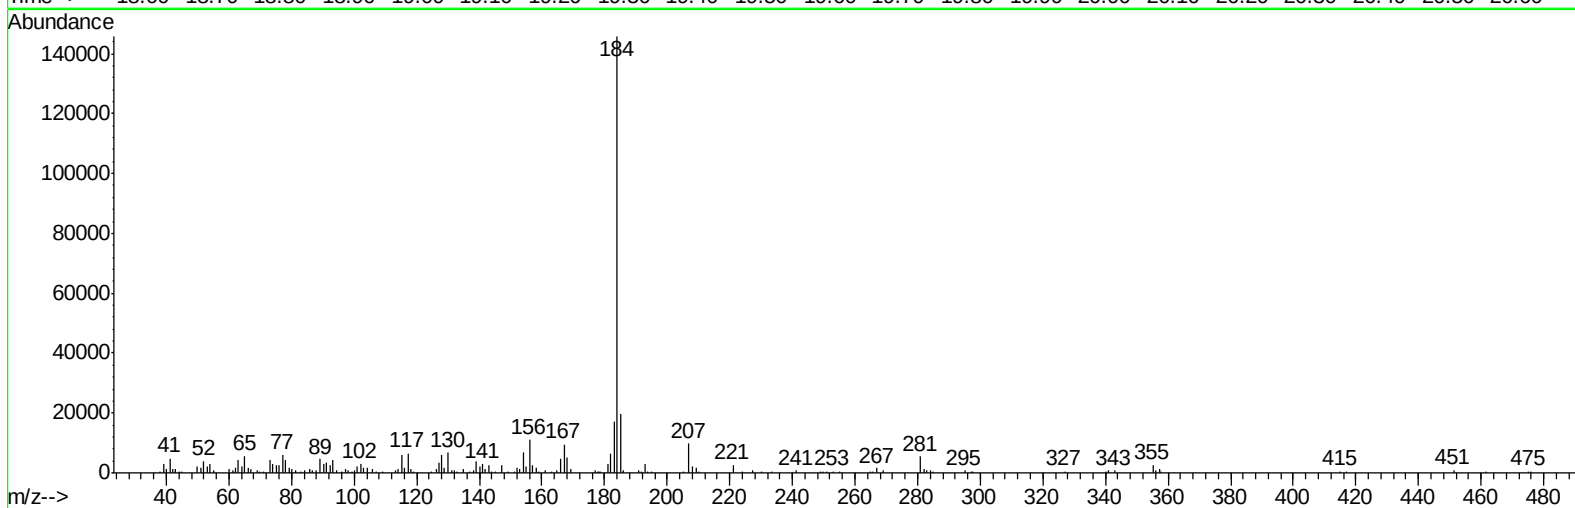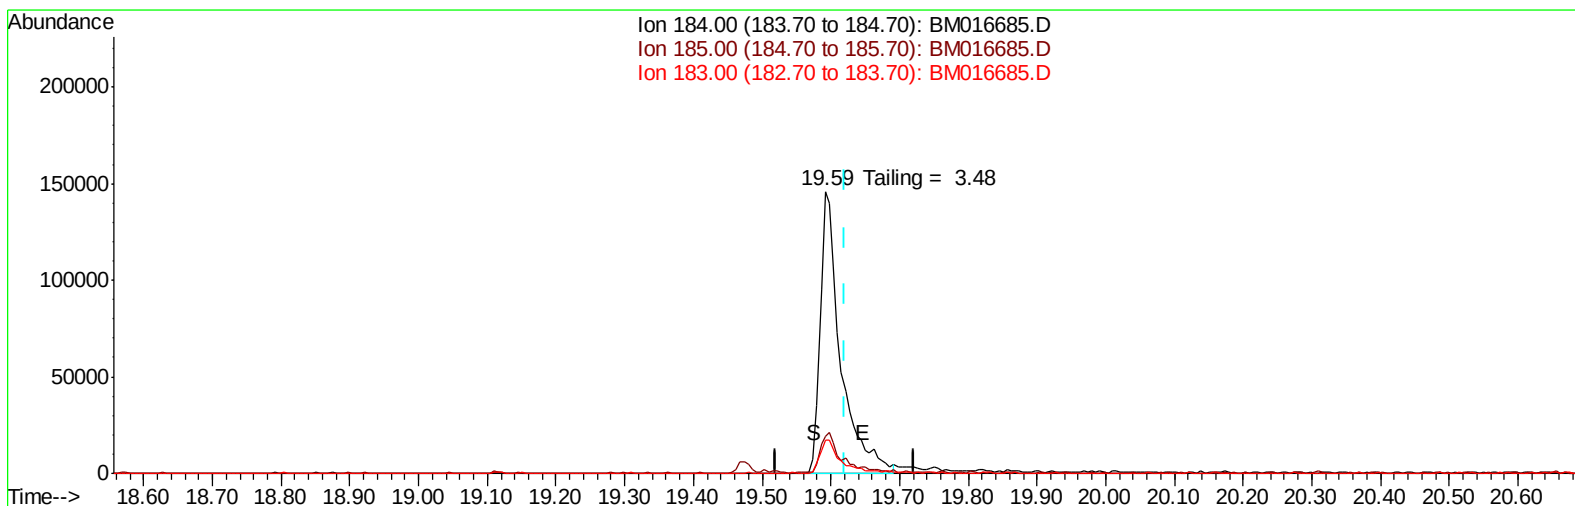

TIC: BM016685.D

(76) Benzidine

19.592min (-0.030) 22262.17ng

response 300544

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.39
183.00	11.10	11.68
0.00	0.00	0.00