

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090618\
 Data File : BM016694.D
 Acq On : 06 Sep 2018 20:48
 Operator : SJ/JU
 Sample : J4798-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 090418-SIDI-E-U-S

Quant Time: Sep 07 07:00:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 27 13:01:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.96	152	53735	20.00	ng	-0.04
21) Naphthalene-d8	10.76	136	163102	20.00	ng	-0.05
38) Acenaphthene-d10	14.60	164	112280	20.00	ng	-0.04
63) Phenanthrene-d10	17.34	188	371397	20.00	ng	-0.04
75) Chrysene-d12	21.50	240	532376	20.00	ng	-0.04
86) Perylene-d12	23.76	264	592189	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	112694	41.10	ng	-0.03
7) Phenol-d6	7.15	99	76108	20.97	ng	-0.04
23) Nitrobenzene-d5	9.15	82	528429	147.93	ng	-0.05
41) 2,4,6-Tribromophenol	16.10	330	379088	120.78	ng	-0.04
44) 2-Fluorobiphenyl	13.22	172	1550603	132.75	ng	-0.05
78) Terphenyl-d14	19.94	244	4049936	161.01	ng	-0.04
Target Compounds						
49) Dimethylphthalate	14.07	163	103994	9.641	ng	Qvalue # 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090618\
Data File : BM016694.D
Acq On : 06 Sep 2018 20:48
Operator : SJ/JU
Sample : J4798-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
090418-SIDI-E-U-S

Quant Time: Sep 07 07:00:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 27 13:01:22 2018
Response via : Initial Calibration

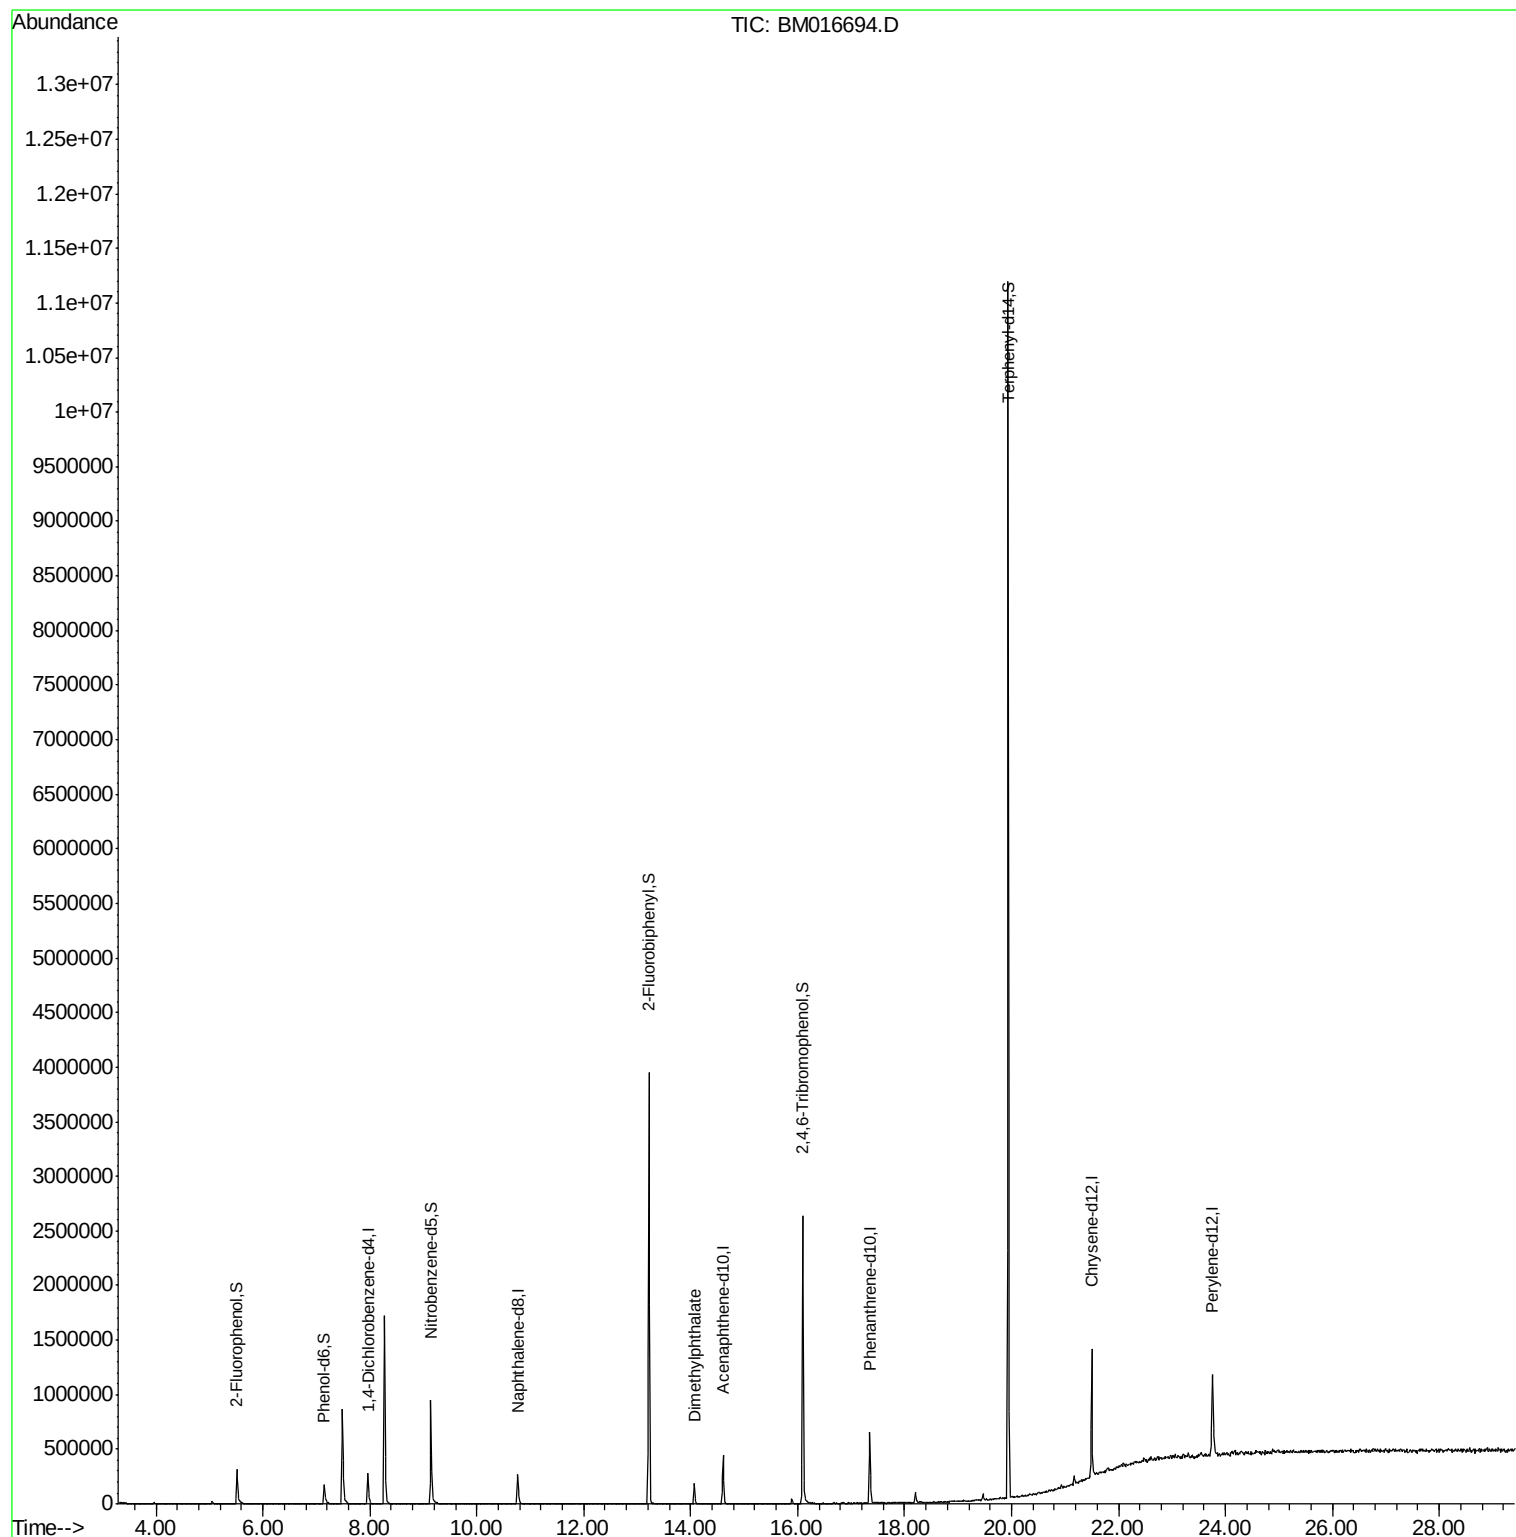

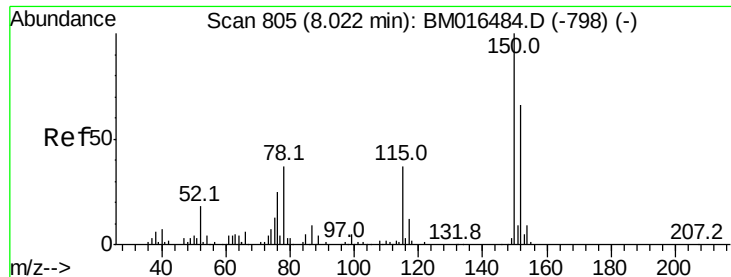


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.96 min Scan# 795
Delta R.T. -0.04 min
Lab File: BM016694.D
Acq: 06 Sep 2018 20:48

Instrument :
BNA_M
ClientSampleId :
090418-SIDI-E-U-S

Tot Ion:152 Resp: 53735
Ion Ratio Lower Upper
152 100
150 151.2 119.5 179.3
115 91.8 43.0 64.4#

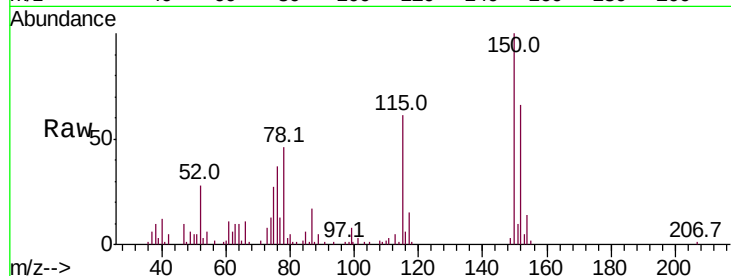


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

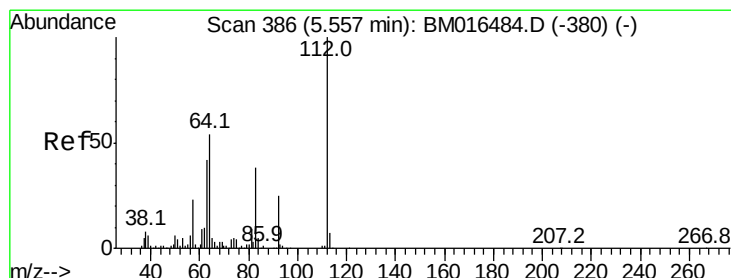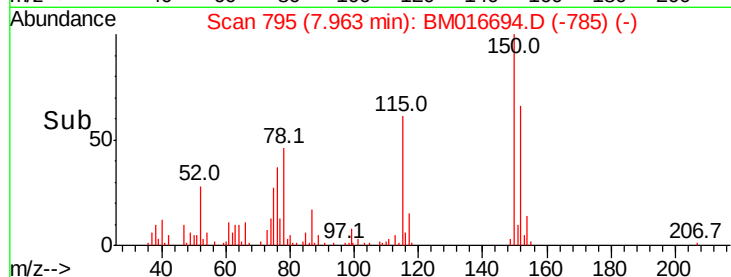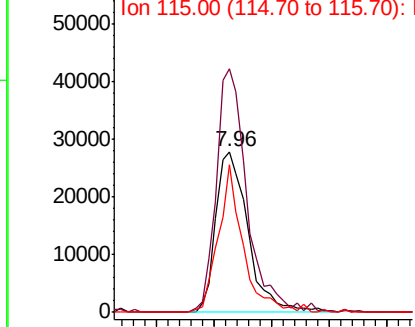



#5


2-Fluorophenol
Concen: 41.097 ng
RT: 5.52 min Scan# 379
Delta R.T. -0.03 min
Lab File: BM016694.D
Acq: 06 Sep 2018 20:48

Tgt Ion:112 Resp: 112694
Ion Ratio Lower Upper
112 100
64 56.7 38.6 57.8
63 46.6 19.3 28.9#

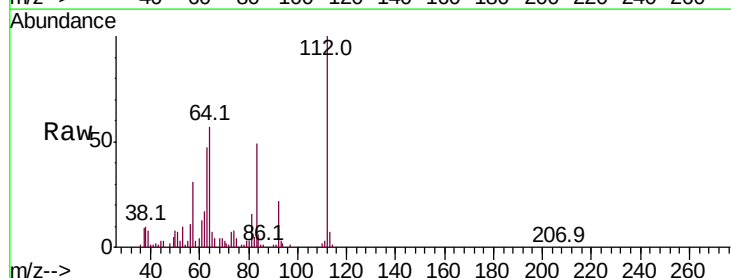

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

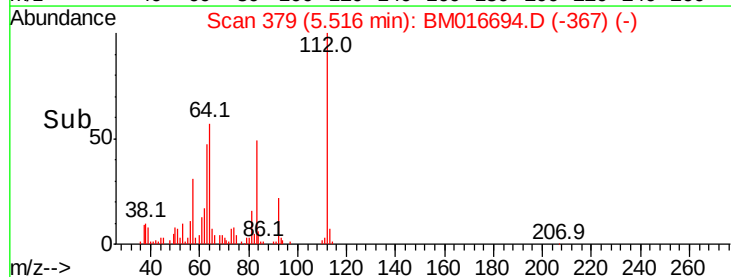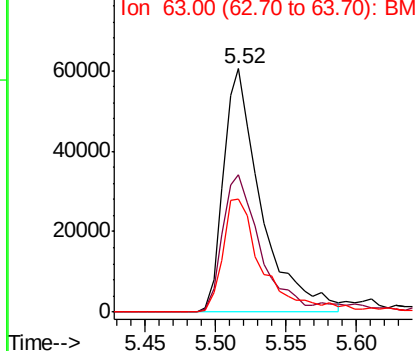

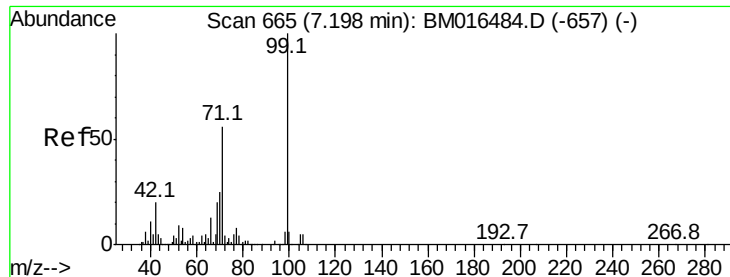

#7

Phenol-d6

Concen: 20.974 ng

RT: 7.15 min Scan# 656

Delta R.T. -0.04 min

Lab File: BM016694.D

Acq: 06 Sep 2018 20:48

Instrument :

BNA_M

ClientSampleId :

090418-SIDI-E-U-S


Tot Ion: 99 Resp: 76108

Ion Ratio Lower Upper

99 100

42 32.4 11.0 16.4#

71 69.7 23.4 35.2#



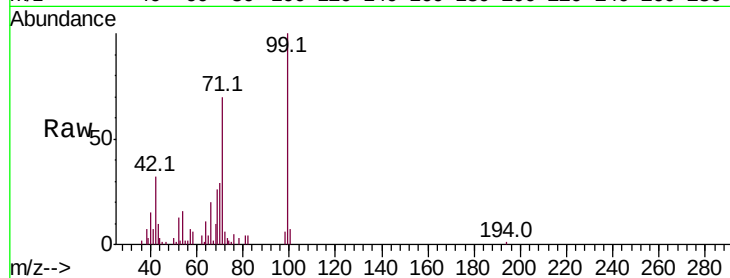


Abundance

Ion 99.00 (98.70 to 99.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 71.00 (70.70 to 71.70): BM0

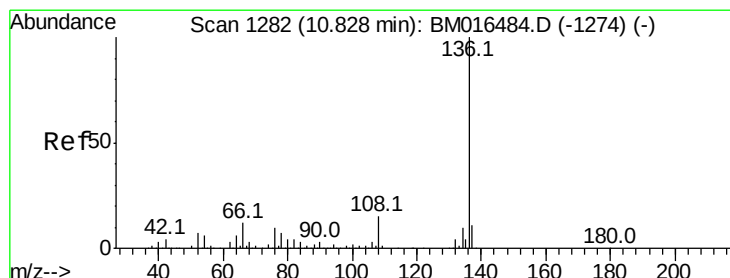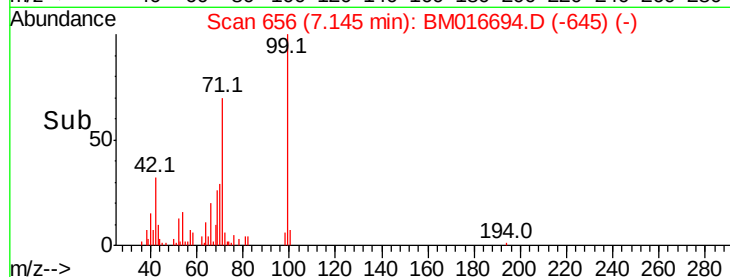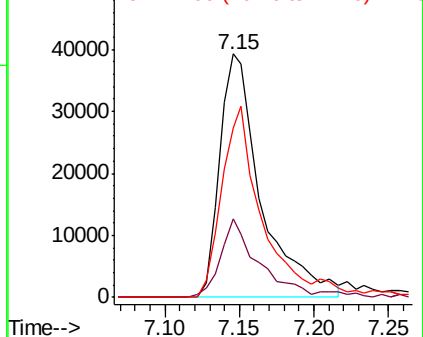

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.76 min Scan# 1271

Delta R.T. -0.05 min

Lab File: BM016694.D

Acq: 06 Sep 2018 20:48

Tgt Ion: 136 Resp: 163102


Ion Ratio Lower Upper

136 100

137 11.7 8.7 13.1

54 10.7 4.6 6.8#

68 4.0 3.7 5.5

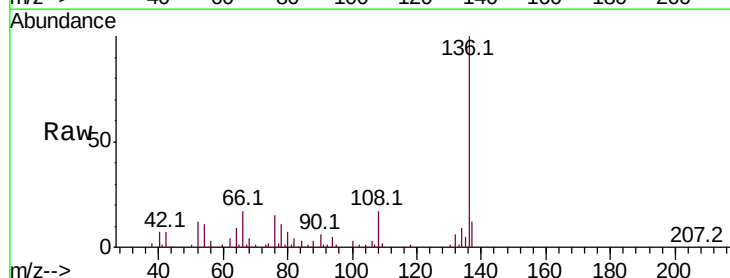



Abundance


Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BM0

Ion 68.00 (67.70 to 68.70): BM0



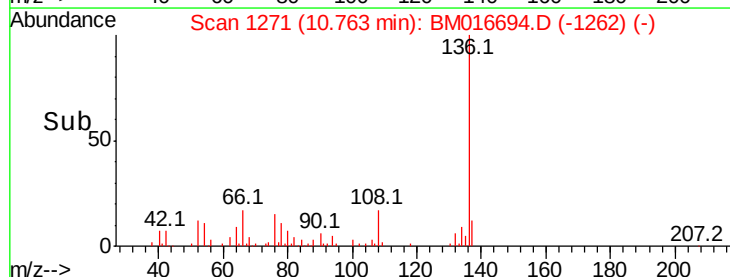
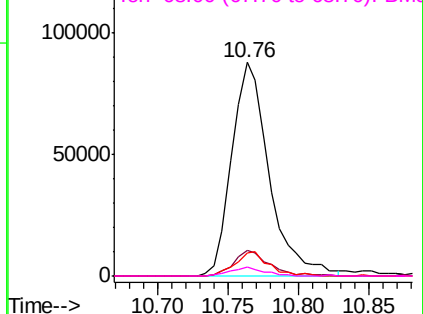


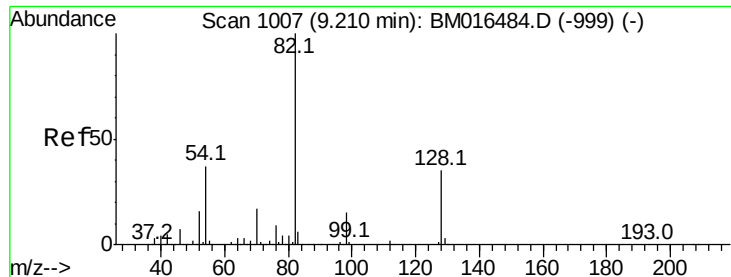

#23
 Nitrobenzene-d5
 Concen: 147.929 ng
 RT: 9.15 min Scan# 996
 Delta R.T. -0.05 min
 Lab File: BM016694.D
 Acq: 06 Sep 2018 20:48




Instrument :
 BNA_M
 ClientSampleId :
 090418-SIDI-E-U-S


Tot Ion	Ratio	Lower	Upper
82	100		
128	29.8	32.8	49.2#
54	41.3	40.6	60.8

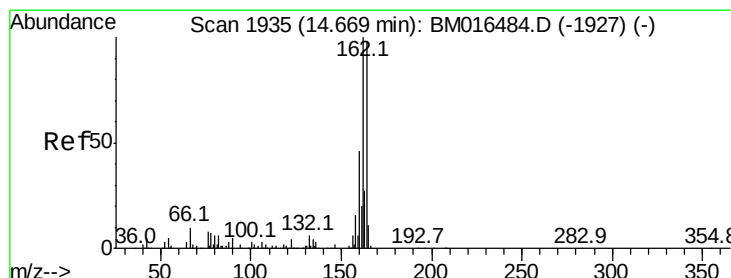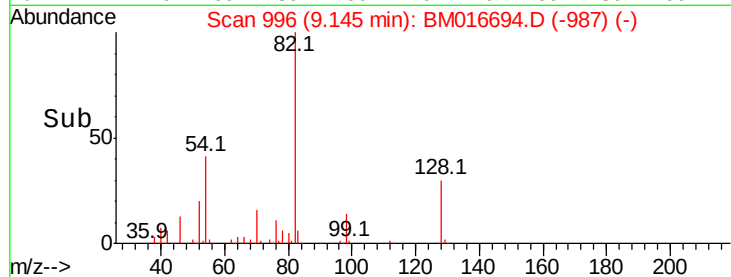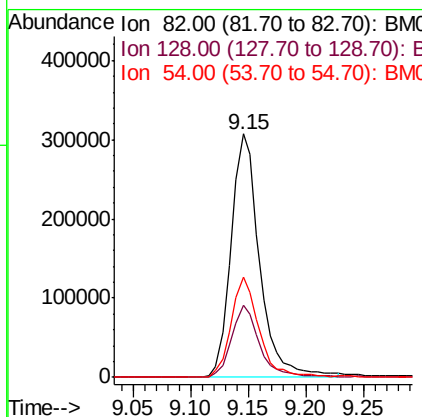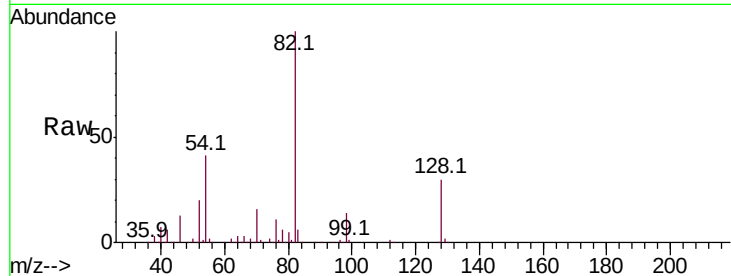

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.60 min Scan# 1924
 Delta R.T. -0.04 min
 Lab File: BM016694.D
 Acq: 06 Sep 2018 20:48

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.0	82.4	123.6
160	49.4	35.8	53.6

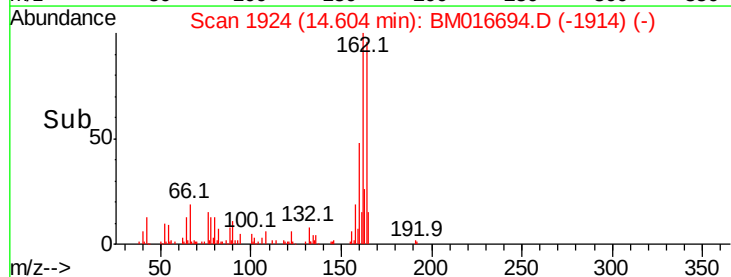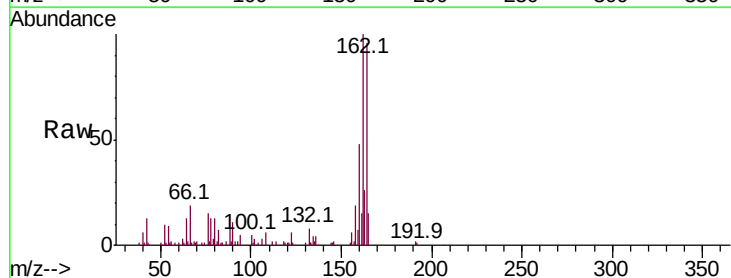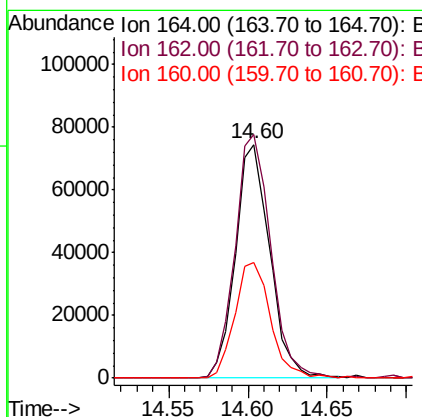


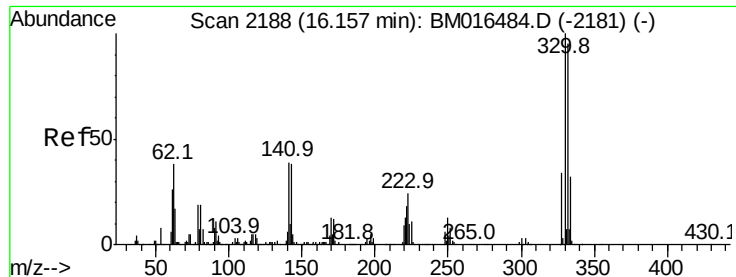




#41
2,4,6-Tribromophenol
Concen: 120.779 ng
RT: 16.10 min Scan# 2178
Delta R.T. -0.04 min
Lab File: BM016694.D
Acq: 06 Sep 2018 20:48

Instrument :
BNA_M
ClientSampleId :
090418-SIDI-E-U-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.3	0.0	0.0#
141	43.5	0.0	0.0#

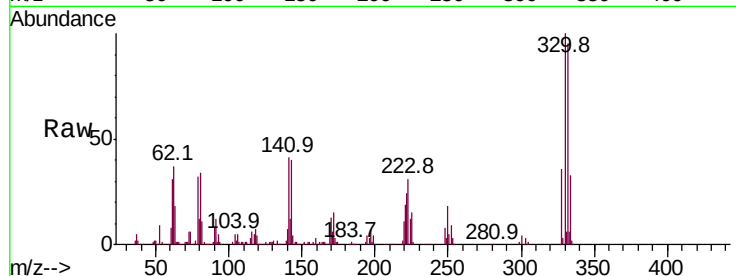


Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

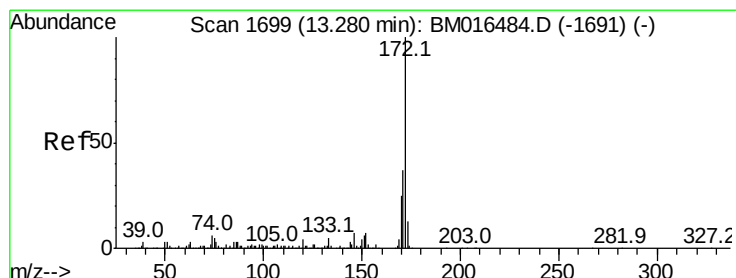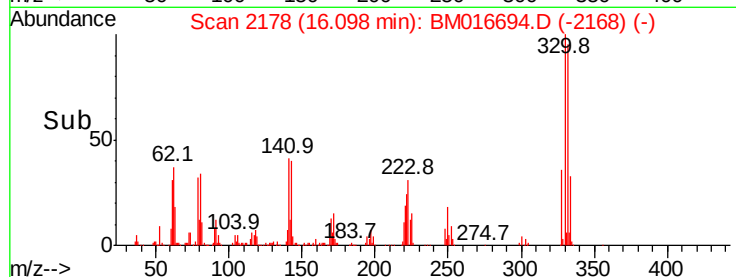
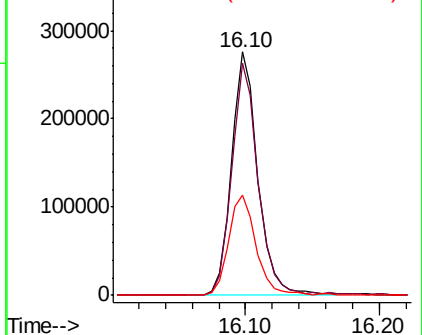



#44
2-Fluorobiphenyl
Concen: 132.746 ng
RT: 13.22 min Scan# 1688
Delta R.T. -0.05 min
Lab File: BM016694.D
Acq: 06 Sep 2018 20:48

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.0	28.5	42.7
170	23.3	18.8	28.2

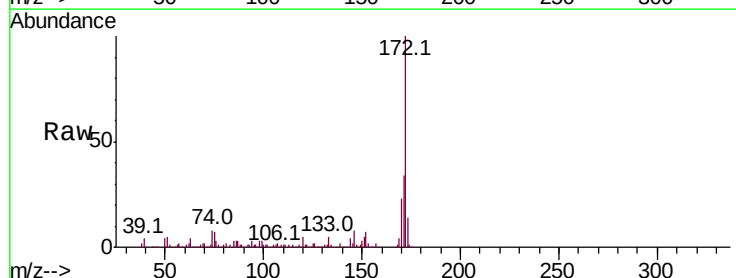

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E



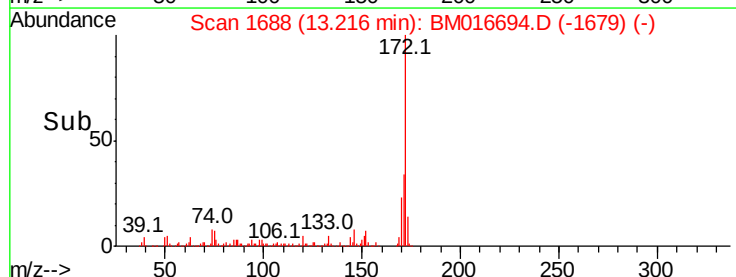
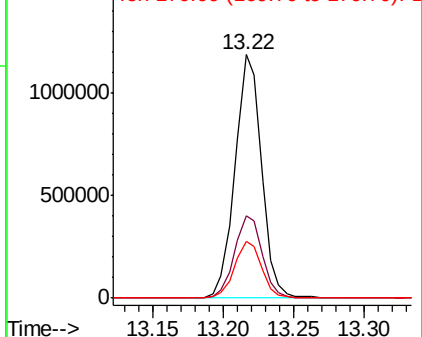


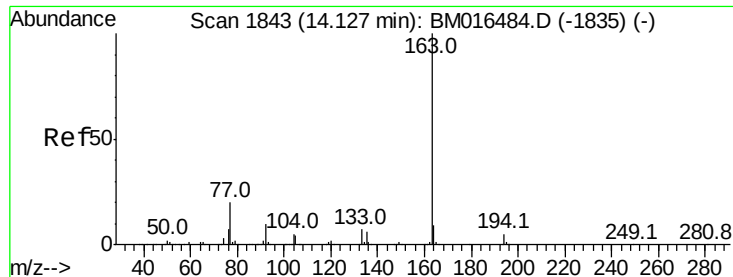

#49
Dimethylphthalate
Concen: 9.641 ng
RT: 14.07 min Scan# 1833
Delta R.T. -0.04 min
Lab File: BM016694.D
Acq: 06 Sep 2018 20:48




Instrument :
BNA_M
ClientSampleId :
090418-SIDI-E-U-S


Tot Ion	Ratio	Lower	Upper
163	100		
194	5.7	2.7	4.1#
164	9.5	8.2	12.2

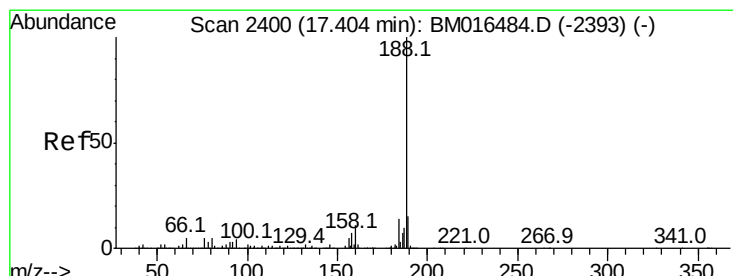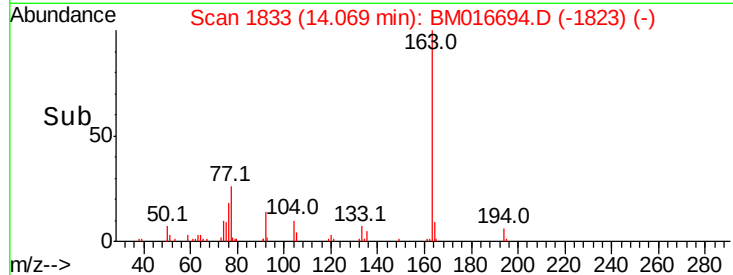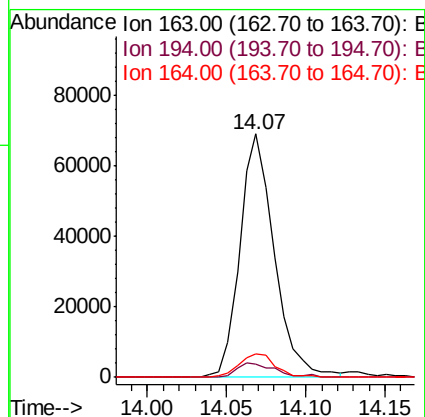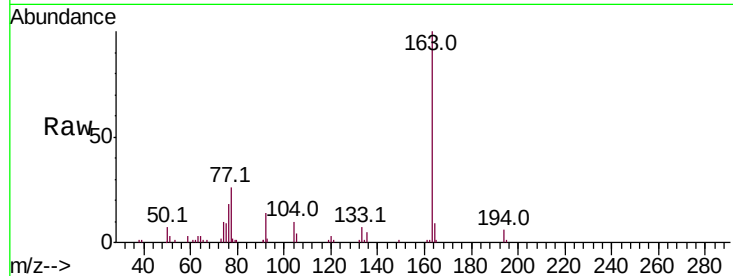

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.34 min Scan# 2390
Delta R.T. -0.04 min
Lab File: BM016694.D
Acq: 06 Sep 2018 20:48

Tgt Ion	Ratio	Lower	Upper
188	100		
94	3.0	8.7	13.1#
80	4.7	9.3	13.9#

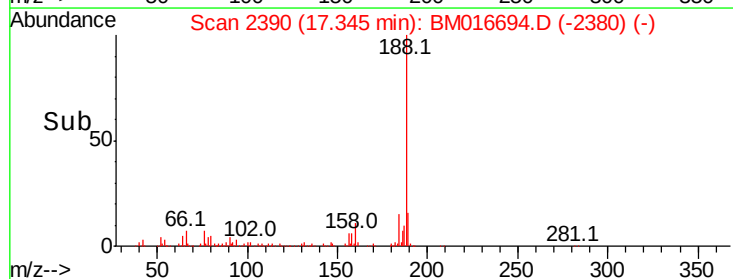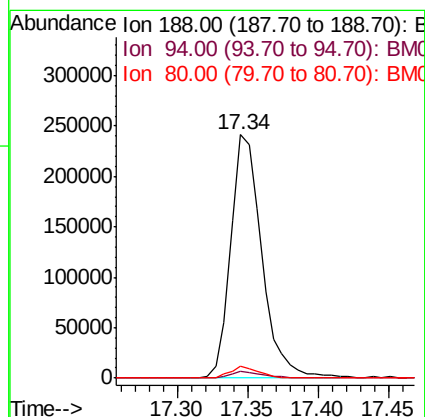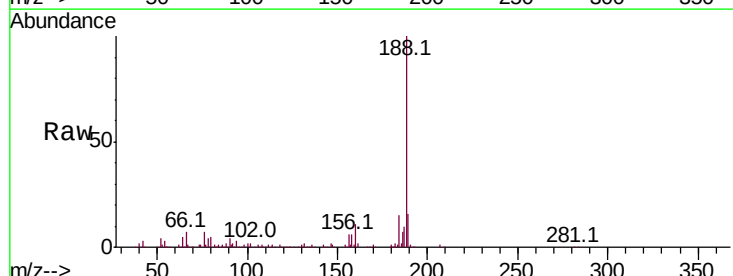

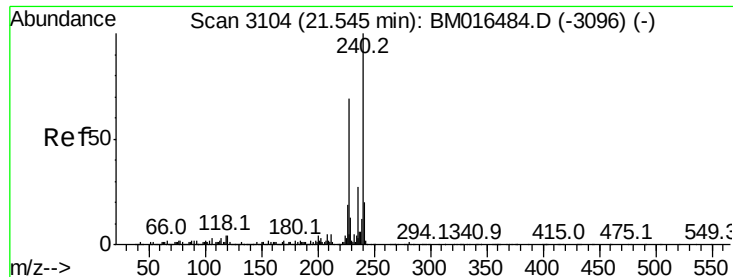

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.50 min Scan# 3096

Delta R.T. -0.04 min

Lab File: BM016694.D

Acq: 06 Sep 2018 20:48

Instrument :


BNA_M

ClientSampleId :

090418-SIDI-E-U-S

Tot Ion:240 Resp: 532376




Ion	Ratio	Lower	Upper
240	100		
120	2.5	8.2	12.2#
236	27.2	20.0	30.0

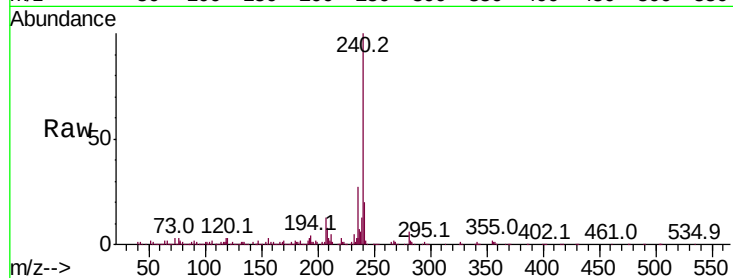

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

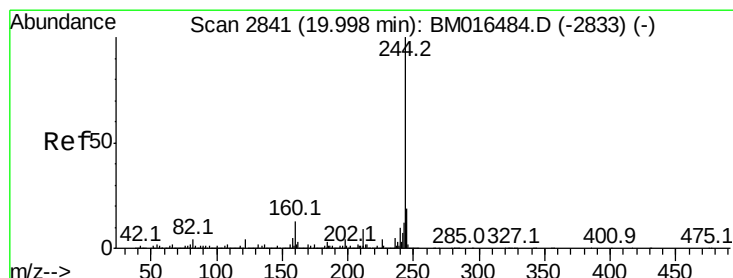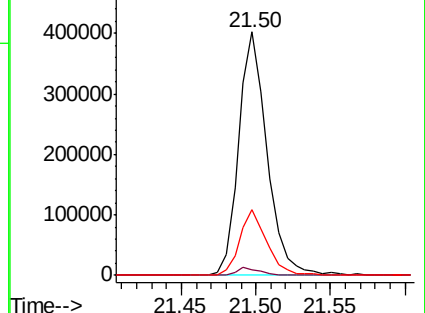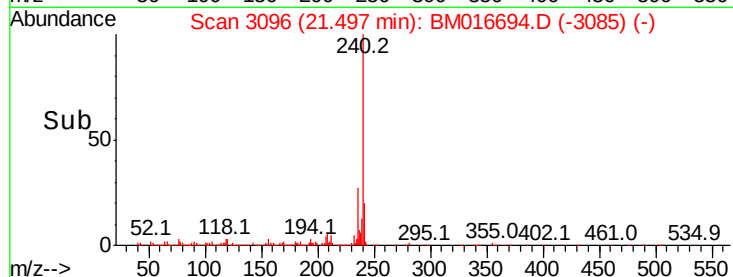

#78

Terphenyl-d14

Concen: 161.014 ng

RT: 19.94 min Scan# 2831


Delta R.T. -0.04 min

Lab File: BM016694.D

Acq: 06 Sep 2018 20:48

Tgt Ion:244 Resp: 4049936



Ion	Ratio	Lower	Upper
244	100		
212	9.9	4.9	7.3#
122	3.3	6.2	9.4#

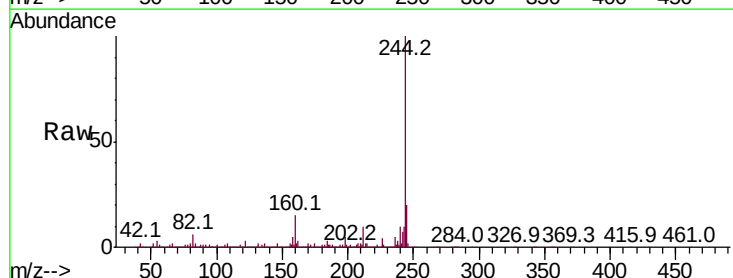


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

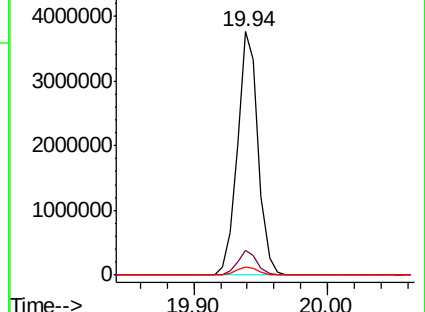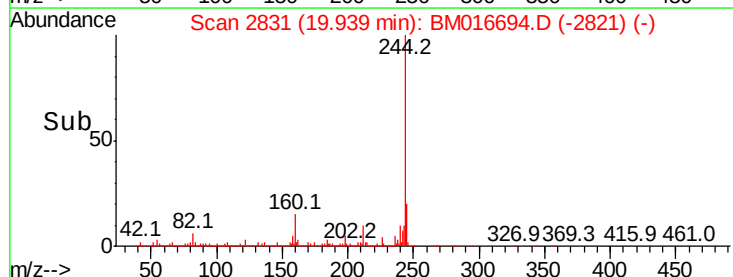


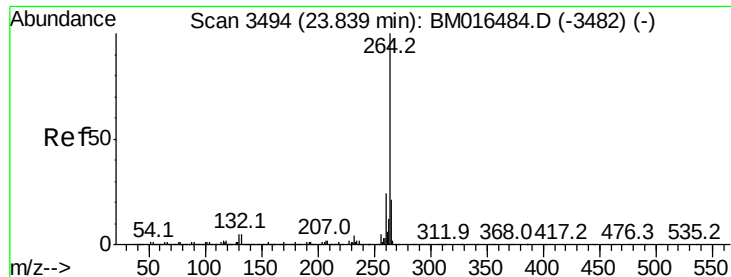

#86
Pervlene-d12
Concen: 20.000 ng
RT: 23.76 min Scan# 3480
Delta R.T. -0.06 min
Lab File: BM016694.D
Acq: 06 Sep 2018 20:48

Instrument :
BNA_M
ClientSampleId :
090418-SIDI-E-U-S

Tot Ion:	264	Resp:	592189
Ion	Ratio	Lower	Upper
264	100		
260	24.6	18.6	27.8
265	23.2	17.3	25.9

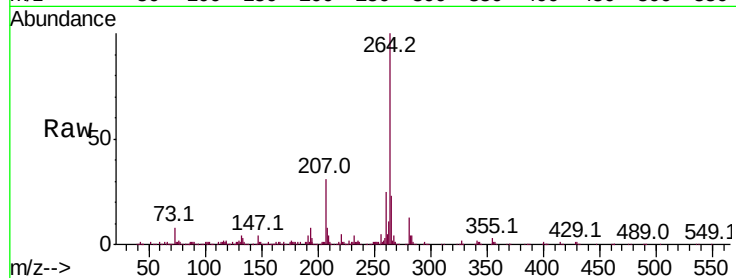

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

