

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090618\
 Data File : BM016688.D
 Acq On : 06 Sep 2018 17:11
 Operator : SJ/JU
 Sample : PB112623BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB112623BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	373	378	394	rBV	1211367	1935739	14.32%	4.924%
2	7.146	650	656	675	rBV	1213304	1942004	14.37%	4.940%
3	7.493	709	715	732	rBV	1522468	2477896	18.33%	6.303%
4	7.963	789	795	807	rBV2	264720	464654	3.44%	1.182%
5	8.275	841	848	865	rBV	1347838	2224672	16.46%	5.659%
6	9.145	990	996	1015	rBV	715121	1306644	9.67%	3.324%
7	10.763	1265	1271	1285	rBV2	265432	497429	3.68%	1.265%
8	13.216	1682	1688	1700	rBV	3005794	4201974	31.09%	10.688%
9	14.604	1918	1924	1936	rVB2	430353	683687	5.06%	1.739%
10	16.098	2172	2178	2192	rBV	4025764	5262013	38.93%	13.385%
11	17.351	2385	2391	2402	rBV	702485	1072265	7.93%	2.727%
12	19.945	2826	2832	2842	rBV	11520149	13516430	100.00%	34.381%
13	21.498	3091	3096	3105	rBV	1441785	1937883	14.34%	4.929%
14	23.762	3475	3481	3492	rBV	870125	1790902	13.25%	4.555%


Sum of corrected areas: 39314192

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090618\
Data File : BM016688.D
Acq On : 06 Sep 2018 17:11
Operator : SJ/JU
Sample : PB112623BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112623BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

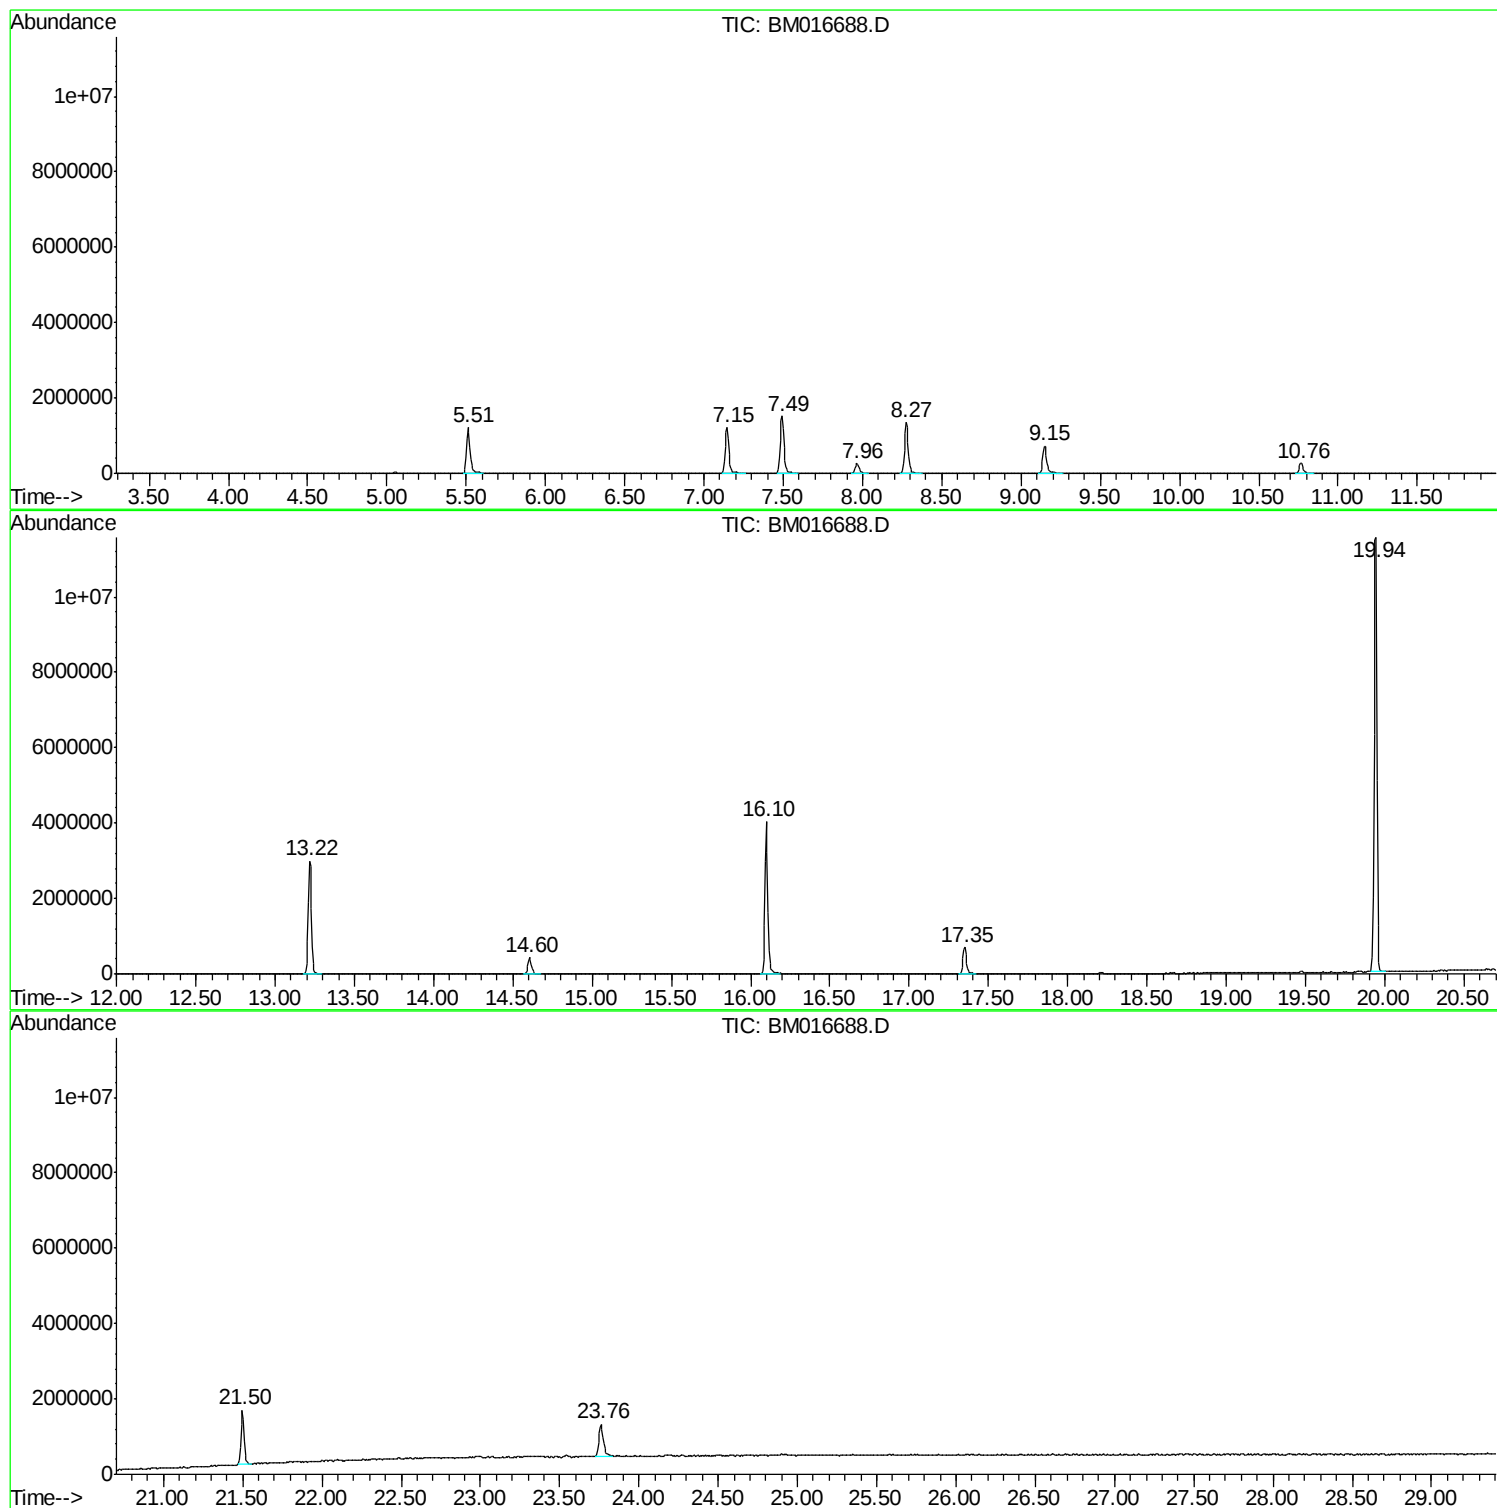

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090618\
Data File : BM016688.D
Acq On : 06 Sep 2018 17:11
Operator : SJ/JU
Sample : PB112623BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112623BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.49 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.49	106.66 ng	2477900	1,4-Dichlorobenzene-d4	7.96

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Penten-1-yne, (E)-	66	C5H6	002004-69-5	16
2		1,3-Cyclopentadiene	66	C5H6	000542-92-7	16
3		1,4,4a,8a-Tetrahydro-1,4-methano...	174	C11H10O2	001200-89-1	16
4		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	14
5		1-Penten-3-yne	66	C5H6	000646-05-9	12

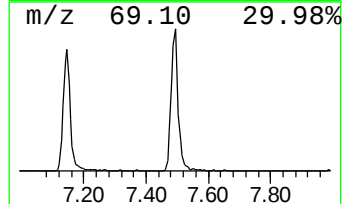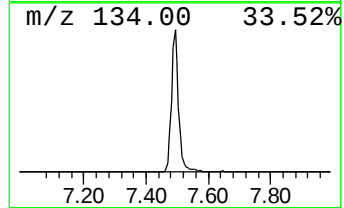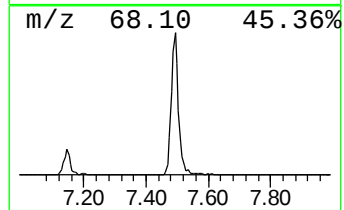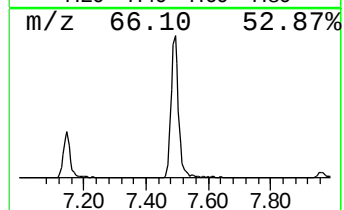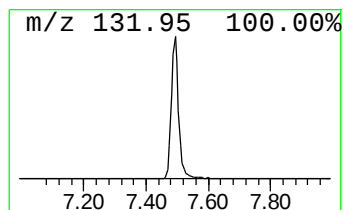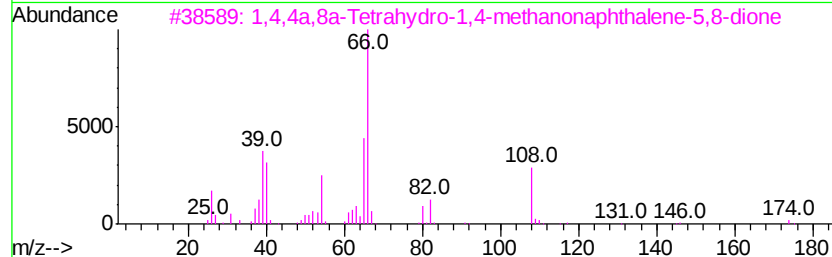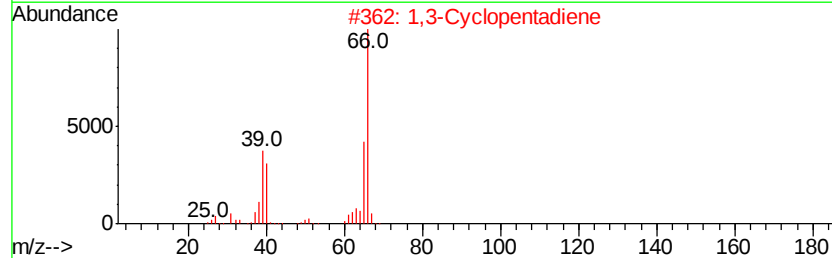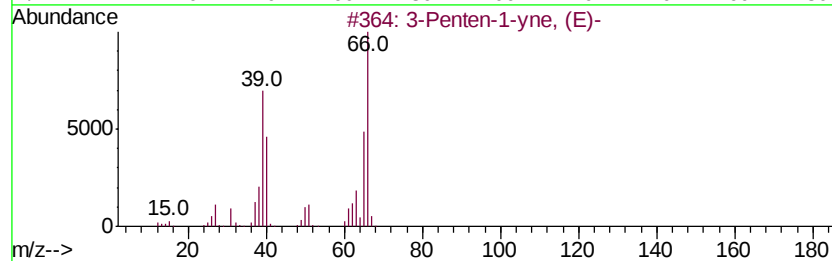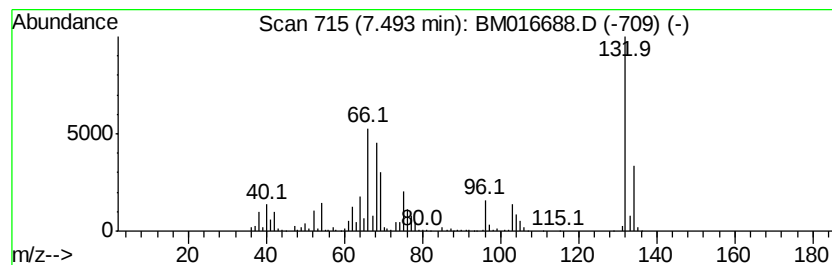

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090618\
Data File : BM016688.D
Acq On : 06 Sep 2018 17:11
Operator : SJ/JU
Sample : PB112623BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112623BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.49	7.49	106.7	ng	2477900	1	7.96	464654	20.0