

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090618\
 Data File : BM016693.D
 Acq On : 06 Sep 2018 20:12
 Operator : SJ/JU
 Sample : J4798-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 090418-SIDI-E-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	374	379	396	rBV	360113	679880	4.38%	1.722%
2	7.145	651	656	667	rBV	206397	403474	2.60%	1.022%
3	7.492	709	715	729	rBV	914419	1616258	10.41%	4.094%
4	7.963	789	795	807	rBV	283592	505588	3.26%	1.281%
5	8.275	841	848	859	rBV	1717698	2733263	17.61%	6.924%
6	9.145	990	996	1014	rBV	954246	1673923	10.78%	4.240%
7	10.763	1265	1271	1285	rBV	293516	531479	3.42%	1.346%
8	13.216	1682	1688	1699	rBV	4010613	5506680	35.47%	13.949%
9	14.068	1827	1833	1846	rBV	196283	308242	1.99%	0.781%
10	14.604	1916	1924	1937	rBV2	479225	778905	5.02%	1.973%
11	16.098	2171	2178	2194	rBV	3094016	4314451	27.79%	10.929%
12	17.351	2385	2391	2402	rBV	754101	1181268	7.61%	2.992%
13	19.939	2826	2831	2840	rBV	13740761	15525031	100.00%	39.326%
14	21.497	3091	3096	3104	rBV	1465475	1961280	12.63%	4.968%
15	23.756	3475	3480	3494	rVB	858711	1758015	11.32%	4.453%


Sum of corrected areas: 39477737

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090618\
Data File : BM016693.D
Acq On : 06 Sep 2018 20:12
Operator : SJ/JU
Sample : J4798-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
090418-SIDI-E-U-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

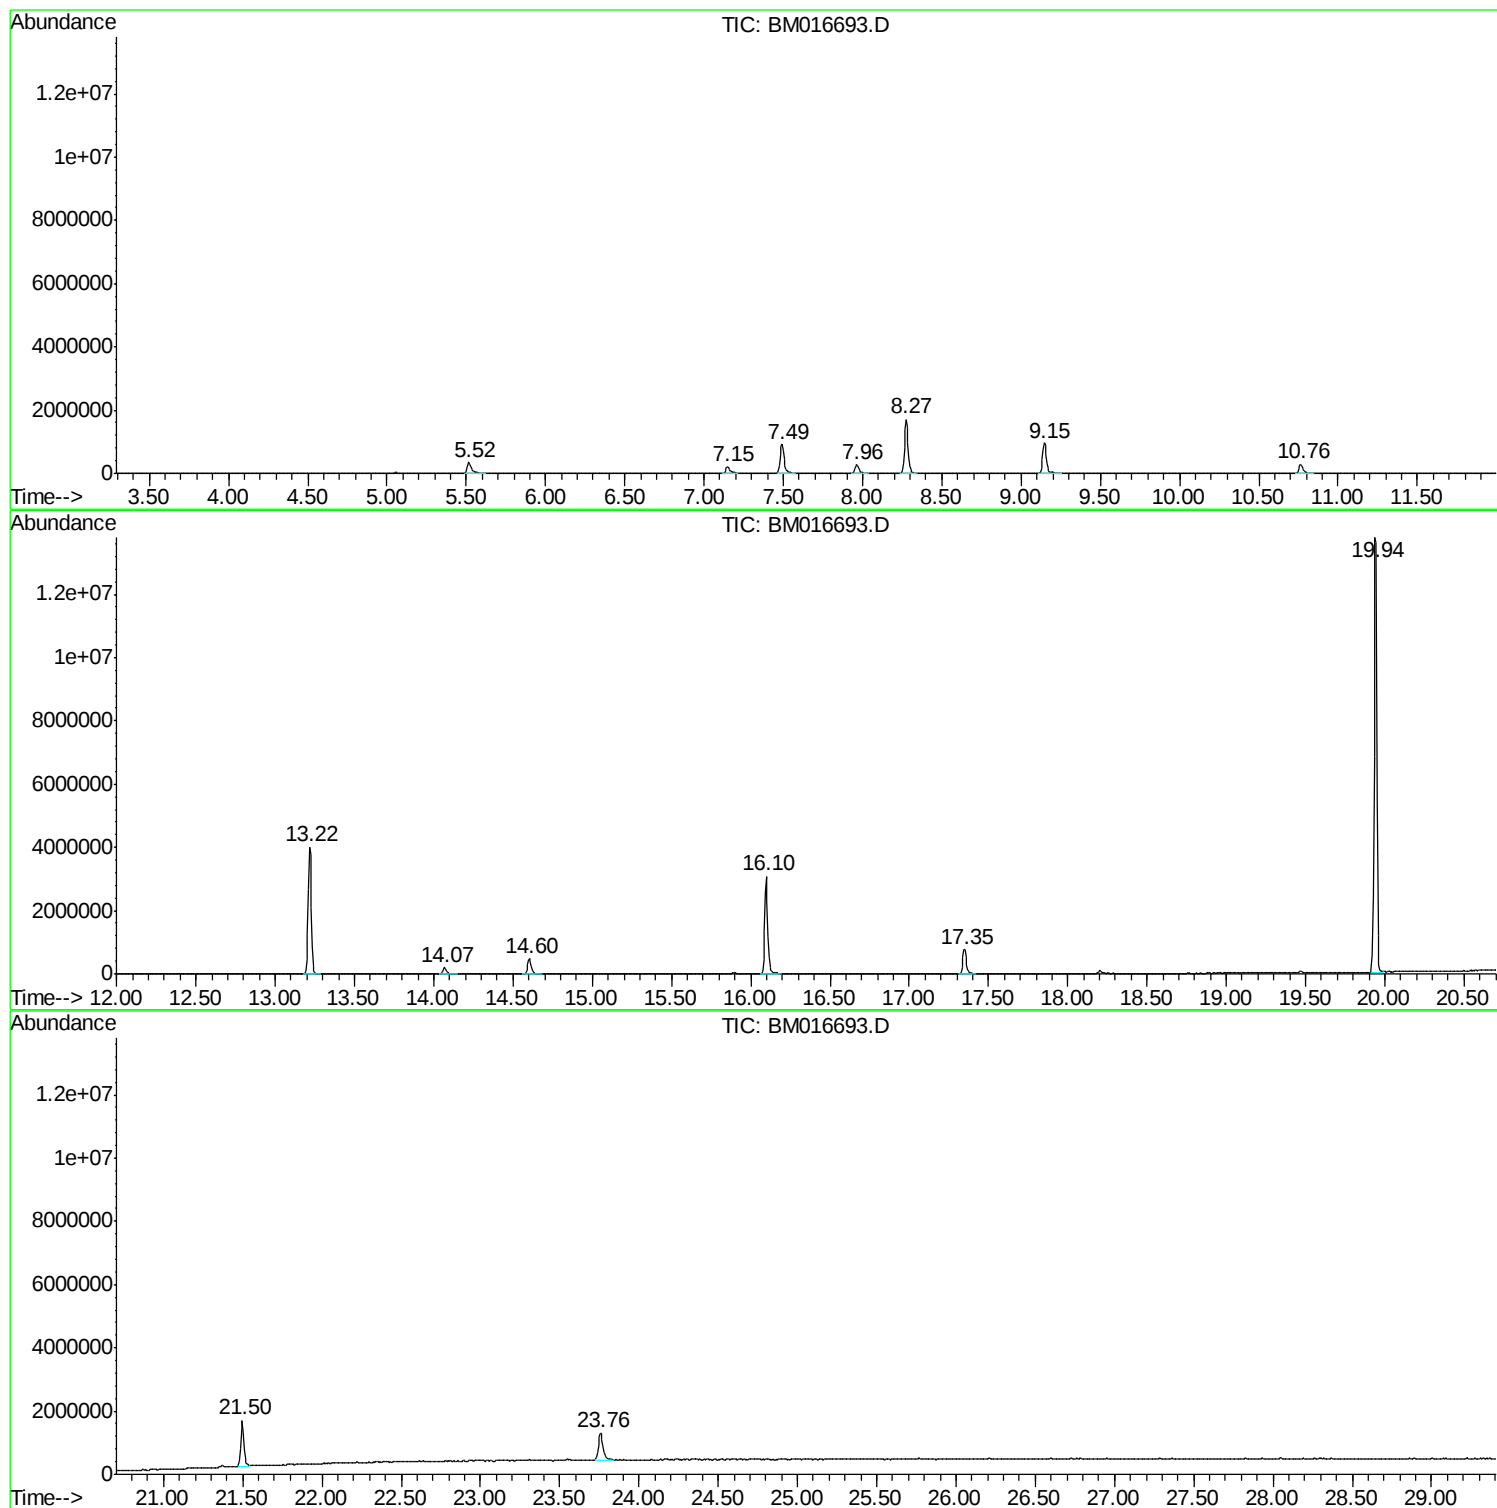

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090618\
Data File : BM016693.D
Acq On : 06 Sep 2018 20:12
Operator : SJ/JU
Sample : J4798-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
090418-SIDI-E-U-M










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.49 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.49	63.94 ng	1616260	1,4-Dichlorobenzene-d4	7.96

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4,7-Methano-1H-indene, 3a,4,7,7a...	132	C10H12	000077-73-6	38
2		1H-Indene, 3a,4,7,7a-tetrahydro-	120	C9H12	003048-65-5	27
3		3-Hexenedinitrile	106	C6H6N2	001119-85-3	16
4		1,3-Cyclopentadiene	66	C5H6	000542-92-7	16
5		1-Penten-3-yne	66	C5H6	000646-05-9	16

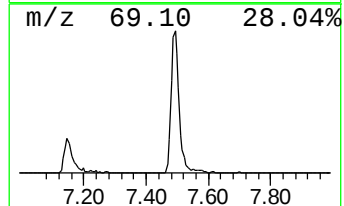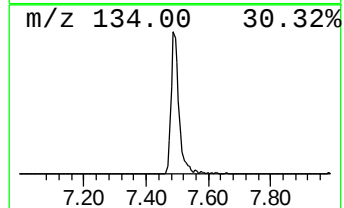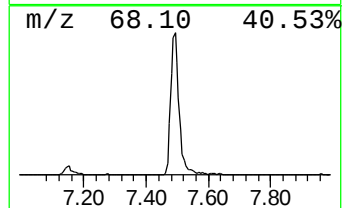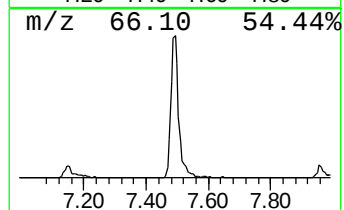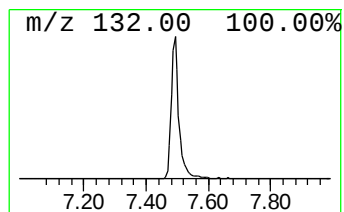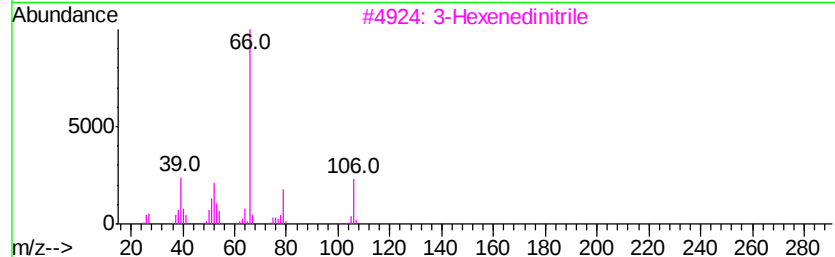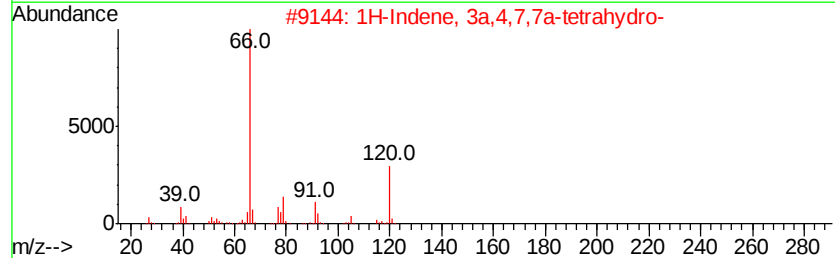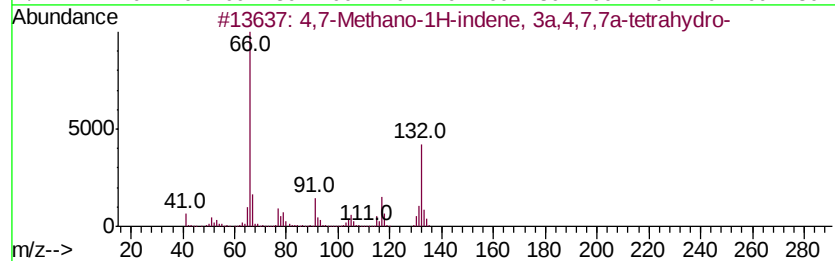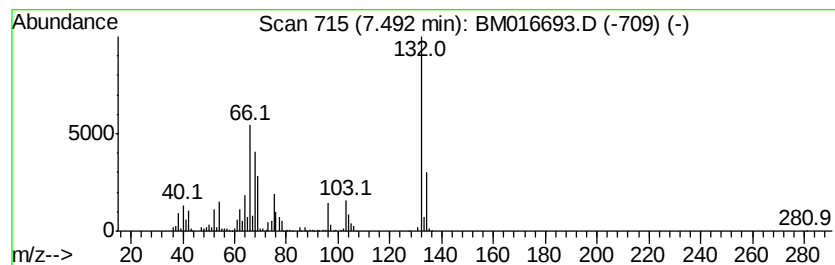

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM090618\
Data File : BM016693.D
Acq On : 06 Sep 2018 20:12
Operator : SJ/JU
Sample : J4798-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
090418-SIDI-E-U-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.49	7.49	63.9	ng	1616260	1	7.96	505588	20.0