


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090618\
 Data File : BM016685.D
 Acq On : 06 Sep 2018 15:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 27 13:01:22 2018

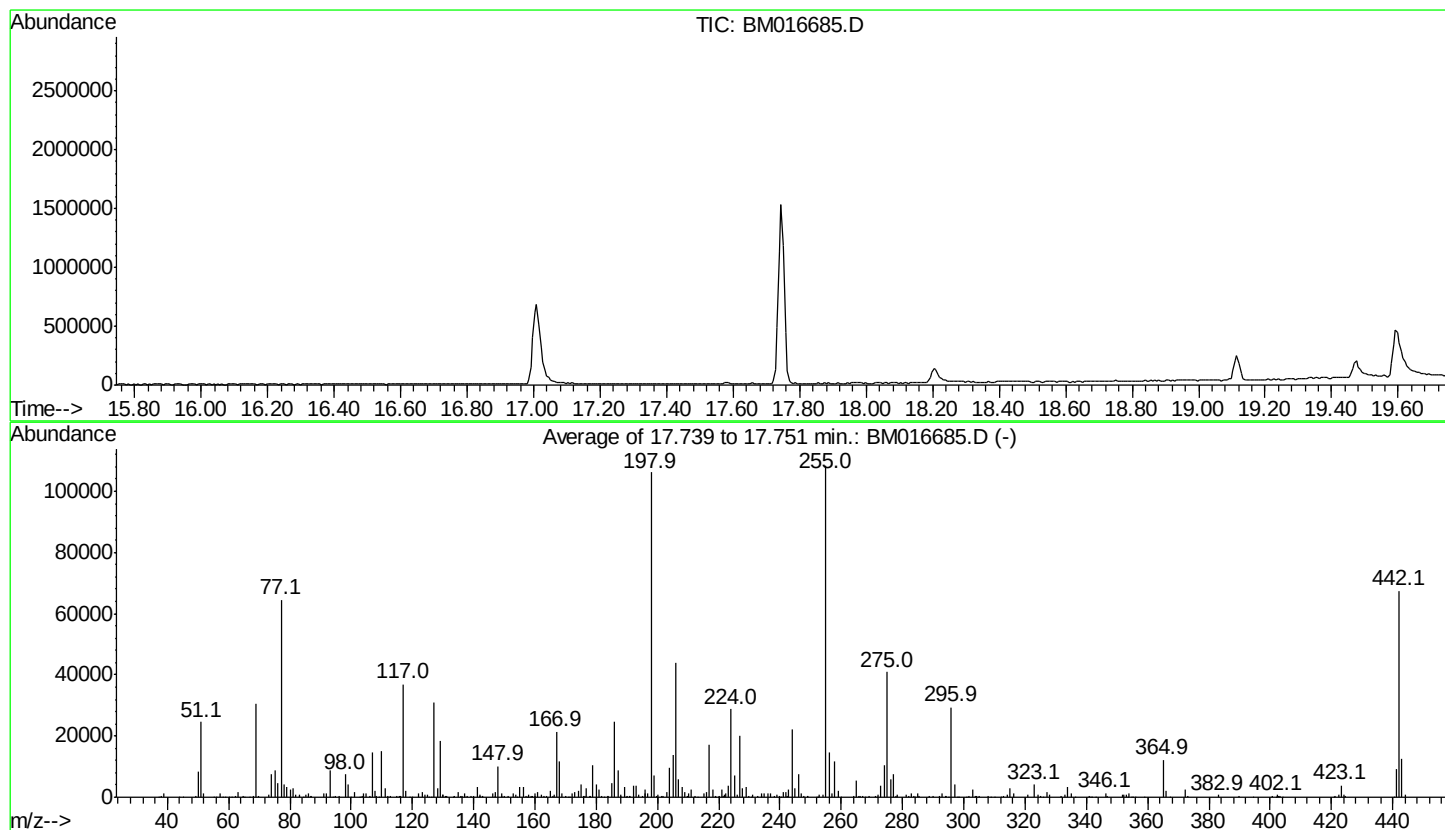

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.1	24570	PASS
68	69	0.00	2	1.8	555	PASS
69	198	0.00	100	28.6	30466	PASS
70	69	0.00	2	1.5	447	PASS
127	198	10	80	29.0	30842	PASS
197	198	0.00	2	1.2	1311	PASS
198	198	100	100	100.0	106386	PASS
199	198	5	9	6.9	7289	PASS
275	198	10	60	38.4	40829	PASS
365	198	1	100	11.6	12352	PASS
441	198	0.01	100	8.6	9163	PASS
442	198	50	100	63.5	67557	PASS
443	442	15	24	18.8	12706	PASS