

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090619\
 Data File : BM022559.D
 Acq On : 06 Sep 2019 19:22
 Operator : HP/JU
 Sample : MDL-W-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 06 23:21:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 05 19:43:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	209478	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	942167	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.49	164	611609	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.23	188	1308878	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	1385324	20.00	ng/ul	-0.01
86) Perylene-d12	23.70	264	1644717	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	32160	6.40	ng/uL	0.00
5) Phenol-d5	7.01	99	607360	31.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.19	67	377794	34.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.39	132	485646	31.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	491578	31.29	ng/ul	-0.01
19) Nitrobenzene-d5	9.01	128	231722	34.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	209144	33.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	461366	28.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.78	131	713483	33.94	ng/ul	0.00
44) Dimethylphthalate-d6	13.90	166	1632215	32.93	ng/ul	-0.01
47) Acenaphthylene-d8	14.18	160	1995393	33.62	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.66	143	278759	32.93	ng/ul	0.00
58) Fluorene-d10	15.48	176	1362493	32.83	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.59	200	166222	27.94	ng/ul	-0.01
71) Anthracene-d10	17.33	188	2178115	32.48	ng/ul	0.00
79) Pyrene-d10	19.62	212	2413658	31.40	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.56	264	2791926	31.58	ng/ul	0.00

Target Compounds

				Ovalue	
2) 1,4-Dioxane	3.34	88	8056	1.593	ng/uL# 91
4) Benzaldehyde	6.99	77	29023	2.876	ng/ul 94
6) Phenol	7.04	94	64580	3.198	ng/ul 97
8) Bis(2-Chloroethyl)ether	7.28	93	51755	3.375	ng/ul 98
10) 2-Chlorophenol	7.42	128	51348	3.201	ng/ul 93
11) 2-Methylphenol	8.29	108	46666	2.961	ng/ul 96
12) 2,2'-oxybis(1-Chloropropan	8.39	45	80938	3.589	ng/ul 98
14) Acetophenone	8.67	105	84385	3.442	ng/ul 96
15) N-Nitroso-di-n-propylamine	8.66	70	42976	3.246	ng/ul 96
16) 4-Methylphenol	8.62	108	53147	3.124	ng/ul 96
17) Hexachloroethane	8.95	117	21030	3.309	ng/ul 95
20) Nitrobenzene	9.05	77	62720	3.688	ng/ul 95
21) Isophorone	9.58	82	118356	3.106	ng/ul 100
23) 2-Nitrophenol	9.76	139	24935	3.352	ng/ul 95
24) 2,4-Dimethylphenol	9.82	107	58312	3.126	ng/ul 98
25) Bis(2-Chloroethoxy)methane	10.06	93	71870	3.216	ng/ul 98
27) 2,4-Dichlorophenol	10.29	162	47687	3.035	ng/ul 91
28) Naphthalene	10.70	128	173827	3.328	ng/ul 99
30) 4-Chloroaniline	10.80	127	69663	3.226	ng/ul 96
31) Hexachlorobutadiene	11.00	225	29718	3.070	ng/ul 99
32) Caprolactam	11.59	113	15134	2.588	ng/ul 86
33) 4-Chloro-3-methylphenol	11.92	107	50122	2.891	ng/ul 98
34) 2-Methylnaphthalene	12.32	142	126681	3.219	ng/ul 95

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090619\
 Data File : BM022559.D
 Acq On : 06 Sep 2019 19:22
 Operator : HP/JU
 Sample : MDL-W-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 06 23:21:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 05 19:43:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.53	142	122326	3.253	ng/ul	100
37) 1,2,4,5-Tetrachlorobenzene	12.68	216	59488	3.014	ng/ul	98
38) Hexachlorocyclopentadiene	12.67	237	29999	2.466	ng/ul	98
39) 2,4,6-Trichlorophenol	12.92	196	32181	2.605	ng/ul	98
40) 2,4,5-Trichlorophenol	12.99	196	36575	2.730	ng/ul	98
41) 1,1'-Biphenyl	13.33	154	165580	3.251	ng/ul	99
42) 2-Chloronaphthalene	13.36	162	125684	3.260	ng/ul	100
43) 2-Nitroaniline	13.56	65	27466	3.051	ng/ul	97
45) Dimethylphthalate	13.95	163	169747	3.374	ng/ul	100
46) 2,6-Dinitrotoluene	14.05	165	22615	2.761	ng/ul	91
48) Acenaphthylene	14.21	152	204903	3.329	ng/ul	99
49) 3-Nitroaniline	14.38	138	23252	2.618	ng/ul	96
50) Acenaphthene	14.55	153	140234	3.288	ng/ul	98
51) 2,4-Dinitrophenol	14.58	184	10931	2.909	ng/ul	89
53) 4-Nitrophenol	14.67	109	24336	3.578	ng/ul#	81
54) Dibenzofuran	14.89	168	201249	3.400	ng/ul	98
55) 2,4-Dinitrotoluene	14.84	165	36367	3.031	ng/ul#	97
56) 2,3,4,6-Tetrachlorophenol	15.11	232	29317	2.635	ng/ul#	95
57) Diethylphthalate	15.31	149	170007	3.266	ng/ul	100
59) Fluorene	15.53	166	166954	3.428	ng/ul	100
60) 4-Chlorophenyl-phenylether	15.53	204	80442	3.338	ng/ul	98
61) 4-Nitroaniline	15.53	138	26515	2.620	ng/ul	90
64) 4,6-Dinitro-2-methylphenol	15.60	198	19461	2.827	ng/ul#	62
65) N-Nitrosodiphenylamine	15.74	169	142924	3.200	ng/ul	99
66) 4-Bromophenyl-phenylether	16.42	248	48471	2.964	ng/ul	95
67) Hexachlorobenzene	16.54	284	56898	3.157	ng/ul	98
68) Atrazine	16.69	200	44039	2.565	ng/ul	99
69) Pentachlorophenol	16.87	266	21243	2.136	ng/ul	97
70) Phenanthrene	17.27	178	269299	3.360	ng/ul	99
72) Anthracene	17.36	178	274983	3.340	ng/ul	99
73) 1,2,3,4-Tetrachlorobenzene	13.29	216	60145	2.952	ng/uL	98
74) Pentachlorobenzene	14.81	250	63165	3.075	ng/uL	98
75) Carbazole	17.62	167	243708	3.294	ng/ul	99
76) Di-n-butylphthalate	18.20	149	255424	2.726	ng/ul	99
77) Fluoranthene	19.28	202	298782	3.285	ng/ul	97
80) Pvrene	19.64	202	330401	3.296	ng/ul	99
81) Butylbenzylphthalate	20.55	149	98170	2.322	ng/ul	97
82) 3,3'-Dichlorobenzidine	21.32	252	74307	2.109	ng/ul	95
83) Benzo(a)anthracene	21.39	228	335171	3.261	ng/ul	99
84) Bis(2-ethylhexyl)phthalate	21.33	149	154947	2.416	ng/ul#	96
85) Chrysene	21.44	228	317682	3.359	ng/ul	98
87) Di-n-octyl phthalate	22.23	149	243244	2.066	ng/ul	100
88) Benzo(b)fluoranthene	23.00	252	332676	3.075	ng/ul	99
89) Benzo(k)fluoranthene	23.05	252	335600	3.192	ng/ul	99
91) Benzo(a)pyrene	23.60	252	342933	3.322	ng/ul	98
92) Indeno(1,2,3-cd)pyrene	26.03	276	387793	3.251	ng/ul	98
93) Dibenzo(a,h)anthracene	26.04	278	327897	3.304	ng/ul	98
94) Benzo(a,h,i)perylene	26.73	276	318669	3.253	ng/ul	98


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090619\
Data File : BM022559.D
Acq On : 06 Sep 2019 19:22
Operator : HP/JU
Sample : MDL-W-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 06 23:21:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 05 19:43:58 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						

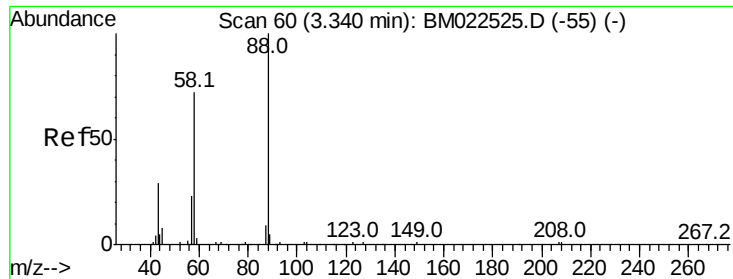

#2

1,4-Dioxane

Concen: 1.593 ng/uL

RT: 3.34 min Scan# 60

Delta R.T. 0.00 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :





Tot Ion: 88 Resp: 8056

Ion Ratio Lower Upper

88 100

43 58.4 37.9 56.9#

58 78.0 59.4 89.0

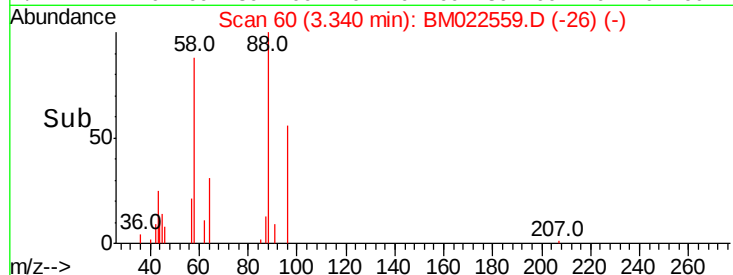

#4

Benzaldehyde

Concen: 2.876 ng/uL

RT: 6.99 min Scan# 681

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22




Tgt Ion: 77 Resp: 29023


Ion Ratio Lower Upper

77 100

105 93.1 79.0 118.6

106 87.0 75.1 112.7





#6

Phenol

Concen: 3.198 ng/ul

RT: 7.04 min Scan# 689

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampled :


Tot Ion: 94 Resp: 64580

Ion Ratio Lower Upper

94 100

65 30.7 22.8 34.2




66 37.2 29.1 43.7



Abundance Ion 94.00 (93.70 to 94.70): BMC

Ion 65.00 (64.70 to 65.70): BMC

Ion 66.00 (65.70 to 66.70): BMC

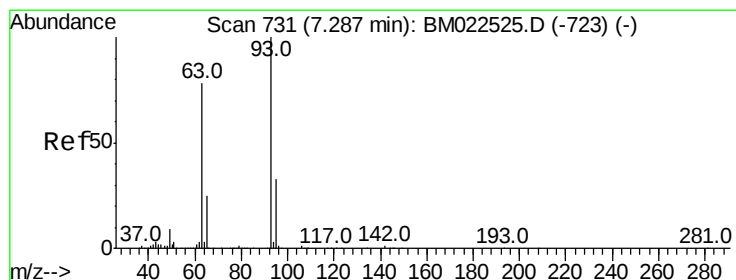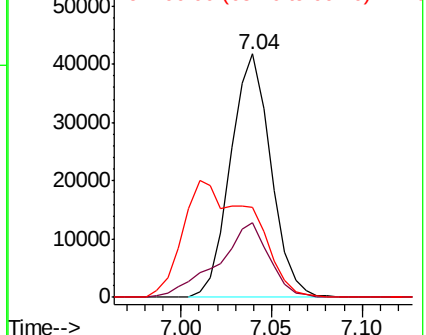

#8

Bis(2-Chloroethyl)ether

Concen: 3.375 ng/ul

RT: 7.28 min Scan# 730

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion: 93 Resp: 51755

Ion Ratio Lower Upper

93 100

63 80.3 62.2 93.2



95 32.8 26.6 39.8




Abundance Ion 93.00 (92.70 to 93.70): BMC

Ion 63.00 (62.70 to 63.70): BMC

Ion 95.00 (94.70 to 95.70): BMC

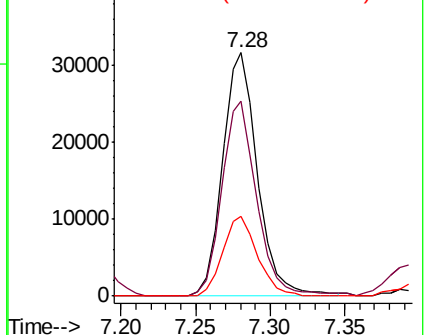

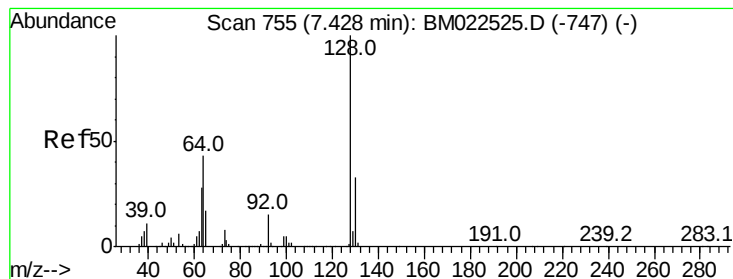

#10

2-Chlorophenol

Concen: 3.201 ng/ul

RT: 7.42 min Scan# 754

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:128 Resp: 51348

Ion Ratio Lower Upper

128 100

64 51.6 36.0 54.0




130 33.9 26.1 39.1



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 64.00 (63.70 to 64.70): BM

Ion 130.00 (129.70 to 130.70): E

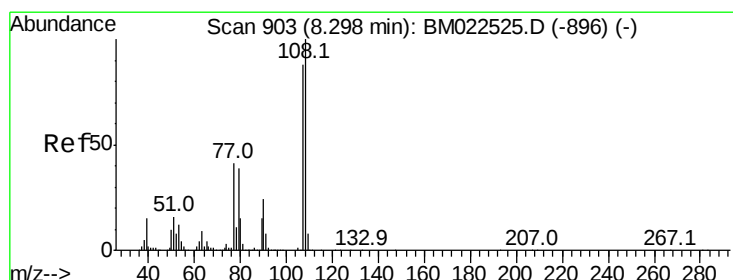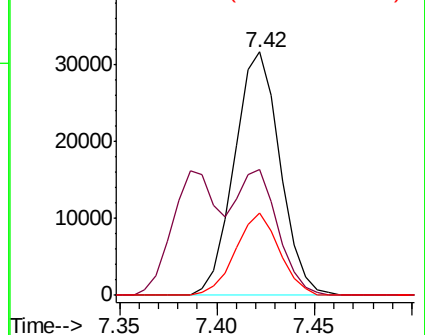

#11

2-Methylphenol

Concen: 2.961 ng/ul

RT: 8.29 min Scan# 902

Delta R.T. -0.01 min

Lab File: BM022559.D


Acq: 06 Sep 2019 19:22

Tgt Ion:108 Resp: 46666

Ion Ratio Lower Upper



108 100


107 91.9 70.7 106.1



Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E




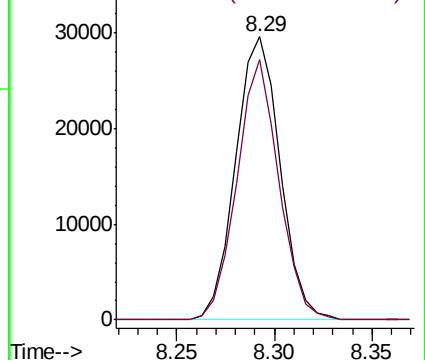


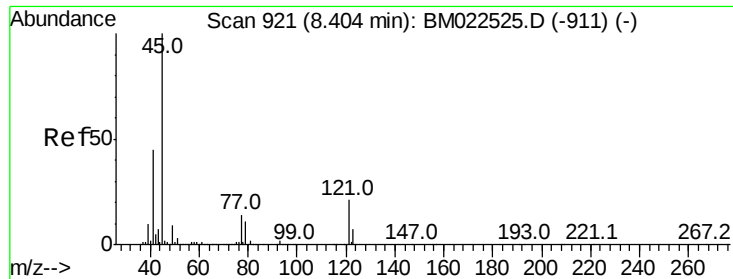

#12
2,2'-oxvbis(1-Chloropropane)
Concen: 3.589 ng/ul
RT: 8.39 min Scan# 918
Delta R.T. -0.02 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22




Instrument :
BNA_M
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
45	100		
77	14.3	11.6	17.4
79	9.5	9.0	13.6

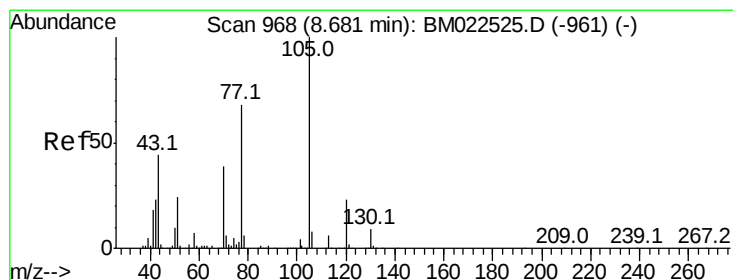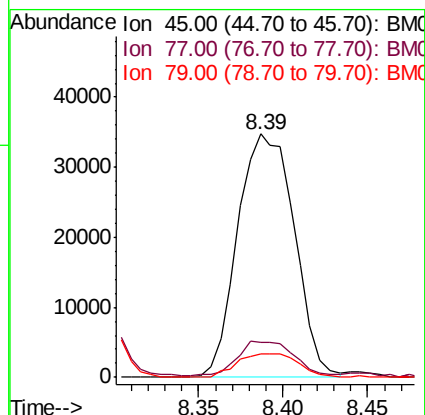

#14
Acetophenone
Concen: 3.442 ng/ul
RT: 8.67 min Scan# 967
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Tgt Ion	Ratio	Lower	Upper
105	100		
77	80.4	62.1	93.1
51	29.6	21.8	32.6

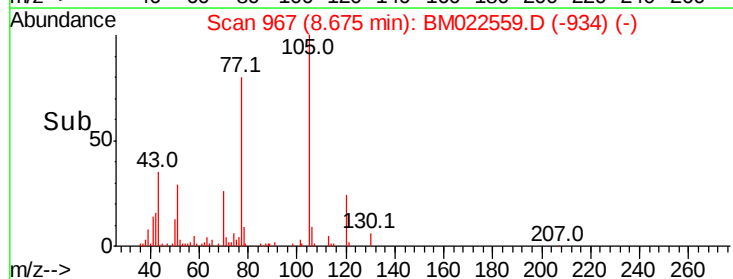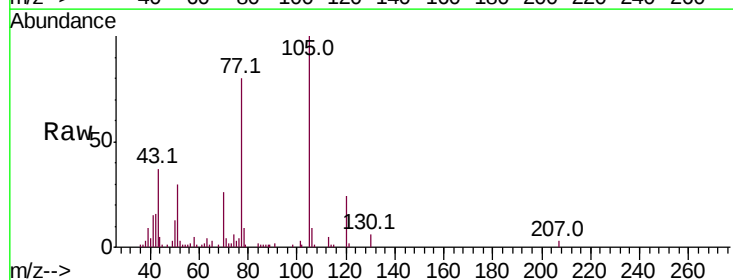



#15

N-Nitroso-di-n-propylamine

Concen: 3.246 ng/ul

RT: 8.66 min Scan# 965

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :

Tot Ion: 70 Resp: 42976


Ion	Ratio	Lower	Upper
70	100		
42	63.5	48.3	72.5
101	9.4	8.2	12.2
130	20.7	18.1	27.1

70 100

42 63.5 48.3 72.5

101 9.4 8.2 12.2

130 20.7 18.1 27.1



Abundance

Ion 70.00 (69.70 to 70.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

Time-->

8.66

40000



30000

20000

10000

0

8.60 8.65 8.70



#16

4-Methylphenol

Concen: 3.124 ng/ul

RT: 8.62 min Scan# 957

Delta R.T. -0.01 min

Lab File: BM022559.D


Acq: 06 Sep 2019 19:22

Tgt Ion:108 Resp: 53147

Ion	Ratio	Lower	Upper
108	100		
107	113.3	87.2	130.8

108 100

107 113.3 87.2 130.8



Abundance

Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

Time-->

8.62

40000


30000


20000

10000

0

8.55 8.60 8.65





#17

Hexachloroethane

Concen: 3.309 ng/ul

RT: 8.95 min Scan# 1013

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:117 Resp: 21030

Ion Ratio Lower Upper

117 100

201 89.7 77.6 116.4




199 58.2 47.6 71.4



Abundance Ion 117.00 (116.70 to 117.70): E

Ion 201.00 (200.70 to 201.70): E

Ion 199.00 (198.70 to 199.70): E

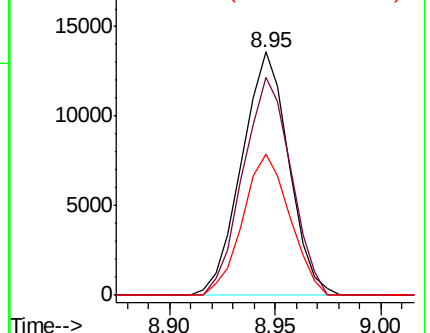

#20

Nitrobenzene

Concen: 3.688 ng/ul

RT: 9.05 min Scan# 1031

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion: 77 Resp: 62720

Ion Ratio Lower Upper

77 100

123 41.1 35.8 53.6



65 15.0 10.5 15.7




Abundance Ion 77.00 (76.70 to 77.70): BM0

Ion 123.00 (122.70 to 123.70): E

Ion 65.00 (64.70 to 65.70): BM0

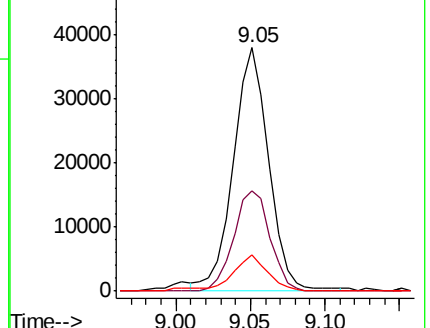



#21

Isophorone

Concen: 3.106 ng/ul

RT: 9.58 min Scan# 1121

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 82 Resp: 118356

Ion Ratio Lower Upper

82 100

95 7.1 5.6 8.4




138 18.0 14.4 21.6



Abundance Ion 82.00 (81.70 to 82.70): BM022525.D (-1115) (-)

Ion 95.00 (94.70 to 95.70): BM022559.D (-1088) (-)

Ion 138.00 (137.70 to 138.70): BM022559.D (-1088) (-)

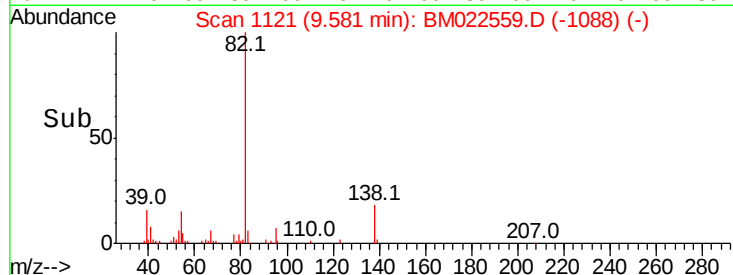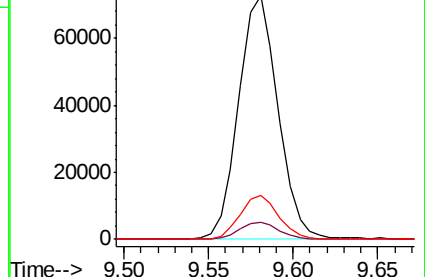

#23

2-Nitrophenol

Concen: 3.352 ng/ul

RT: 9.76 min Scan# 1152

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion: 139 Resp: 24935

Ion Ratio Lower Upper

139 100

65 51.1 39.3 58.9



109 33.7 23.5 35.3




Abundance Ion 139.00 (138.70 to 139.70): BM022525.D (-1146) (-)

Ion 65.00 (64.70 to 65.70): BM022559.D (-1119) (-)

Ion 109.00 (108.70 to 109.70): BM022559.D (-1119) (-)

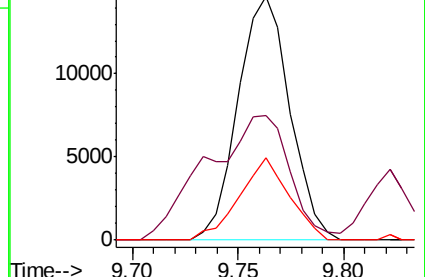



#24

2,4-Dimethylphenol

Concen: 3.126 ng/ul

RT: 9.82 min Scan# 1162

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:107 Resp: 58312

Ion Ratio Lower Upper

107 100

121 52.4 40.2 60.4




122 89.4 70.2 105.2



Abundance Ion 107.00 (106.70 to 107.70): E

Ion 121.00 (120.70 to 121.70): E

Ion 122.00 (121.70 to 122.70): E

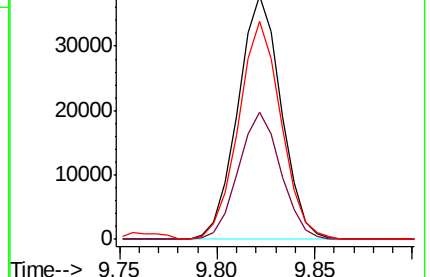

#25

Bis(2-Chloroethoxy)methane

Concen: 3.216 ng/ul

RT: 10.06 min Scan# 1203

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion: 93 Resp: 71870

Ion Ratio Lower Upper

93 100

95 33.2 26.1 39.1



123 9.7 9.2 13.8




Abundance Ion 93.00 (92.70 to 93.70): BM0

Ion 95.00 (94.70 to 95.70): BM0

Ion 123.00 (122.70 to 123.70): E




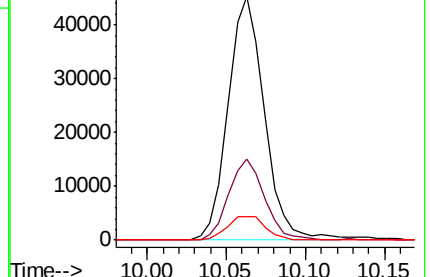


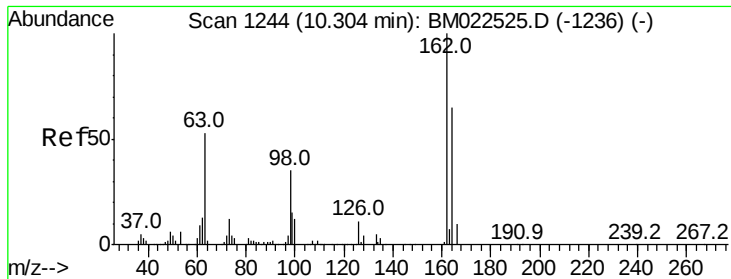

#27
 2,4-Dichlorophenol
 Concen: 3.035 ng/ul
 RT: 10.29 min Scan# 1242
 Delta R.T. -0.01 min
 Lab File: BM022559.D
 Acq: 06 Sep 2019 19:22




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
162	100		
164	75.7	52.1	78.1
98	37.3	28.9	43.3



#28
 Naphthalene
 Concen: 3.328 ng/ul
 RT: 10.70 min Scan# 1312
 Delta R.T. -0.01 min
 Lab File: BM022559.D
 Acq: 06 Sep 2019 19:22

Tgt Ion	Ratio	Lower	Upper
128	100		
129	10.8	8.9	13.3
127	13.1	10.6	16.0


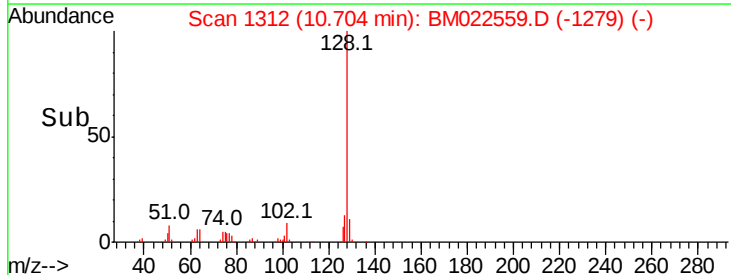






#30
4-Chloroaniline
Concen: 3.226 ng/ul
RT: 10.80 min Scan# 1329
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22




Instrument :
BNA_M
ClientSampled :


Tot Ion:127 Resp: 69663
Ion Ratio Lower Upper
127 100
129 34.2 25.4 38.2

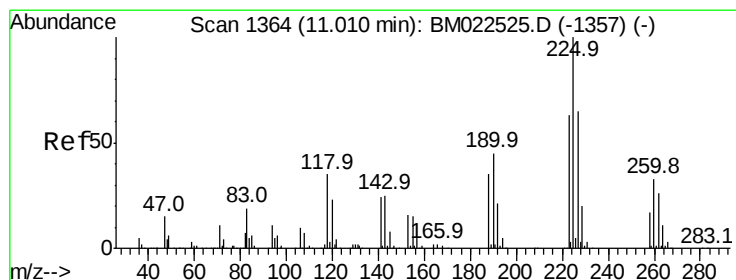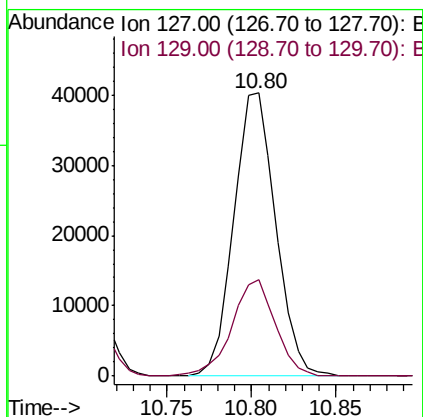

#31
Hexachlorobutadiene
Concen: 3.070 ng/ul
RT: 11.00 min Scan# 1362
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Tgt Ion:225 Resp: 29718
Ion Ratio Lower Upper
225 100
223 61.9 50.1 75.1
227 63.7 51.8 77.8

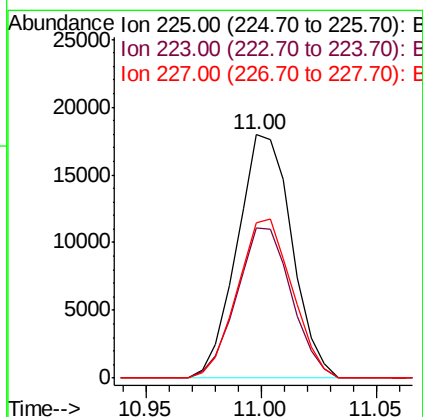



#32

Caprolactam

Concen: 2.588 ng/ul

RT: 11.59 min Scan# 1462

Delta R.T. 0.03 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:113 Resp: 15134

Ion Ratio Lower Upper

113 100

55 195.1 135.6 203.4




56 132.7 98.4 147.6



Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BM

Ion 56.00 (55.70 to 56.70): BM

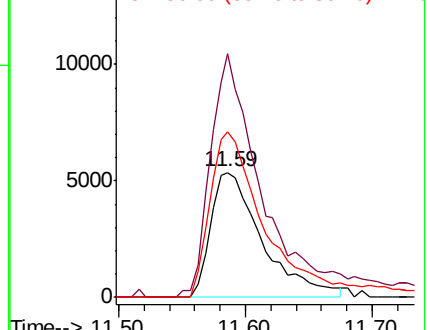

#33

4-Chloro-3-methylphenol

Concen: 2.891 ng/ul

RT: 11.92 min Scan# 1519

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion:107 Resp: 50122

Ion Ratio Lower Upper

107 100

144 27.5 22.6 34.0



142 82.1 67.0 100.4




Abundance Ion 107.00 (106.70 to 107.70): E

Ion 144.00 (143.70 to 144.70): E

Ion 142.00 (141.70 to 142.70): E




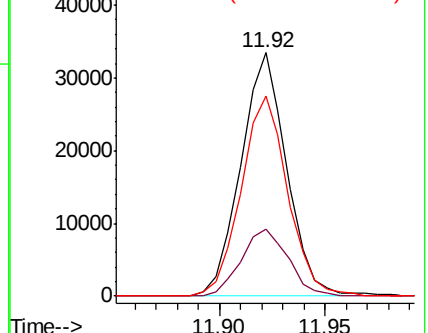




#34
2-Methylnaphthalene
Concen: 3.219 ng/ul
RT: 12.32 min Scan# 1586
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22




Instrument :
BNA_M
ClientSampleId :


Tot Ion:142 Resp: 126681
Ion Ratio Lower Upper
142 100
141 84.3 71.0 106.4

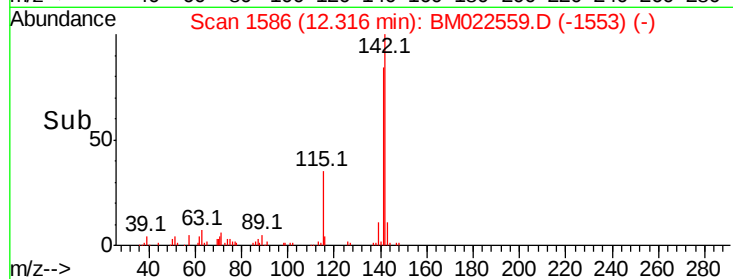

#35
1-Methylnaphthalene
Concen: 3.253 ng/ul
RT: 12.53 min Scan# 1623
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Tgt Ion:142 Resp: 122326
Ion Ratio Lower Upper
142 100
141 90.6 72.6 108.8
116 3.7 3.0 4.4









#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 3.014 ng/ul
 RT: 12.68 min Scan# 1648
 Delta R.T. -0.01 min
 Lab File: BM022559.D
 Acq: 06 Sep 2019 19:22




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion:	216	Resp:	59488
Ion	Ratio	Lower	Upper
216	100		
214	79.9	63.4	95.0
179	22.5	16.7	25.1
108	19.3	14.4	21.6

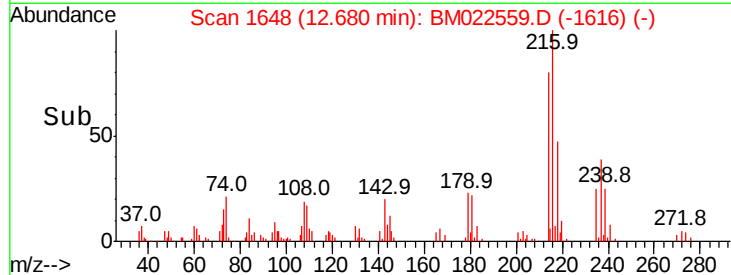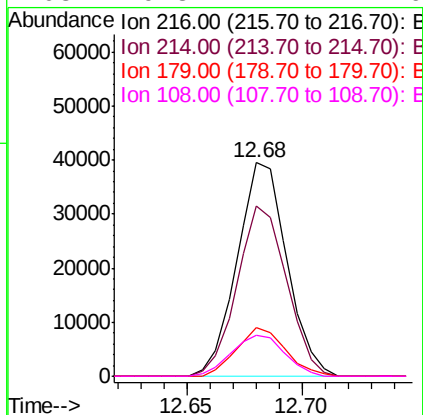

#38
 Hexachlorocyclopentadiene
 Concen: 2.466 ng/ul
 RT: 12.67 min Scan# 1647
 Delta R.T. -0.01 min
 Lab File: BM022559.D
 Acq: 06 Sep 2019 19:22

Tgt Ion:	237	Resp:	29999
Ion	Ratio	Lower	Upper
237	100		
235	60.6	50.1	75.1
272	13.5	10.2	15.4

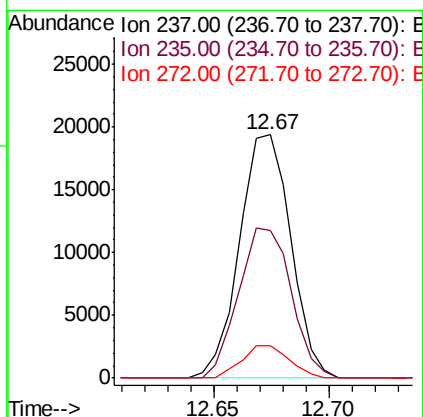



#39

2,4,6-Trichlorophenol

Concen: 2.605 ng/ul

RT: 12.92 min Scan# 1688

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :





Tot Ion:196 Resp: 32181

Ion Ratio Lower Upper

196 100

198 96.1 77.7 116.5

200 33.3 24.6 37.0



#40

2,4,5-Trichlorophenol

Concen: 2.730 ng/ul

RT: 12.99 min Scan# 1700

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22




Tgt Ion:196 Resp: 36575


Ion Ratio Lower Upper

196 100

198 97.8 77.4 116.0

200 32.0 24.0 36.0





#41

1,1'-Biphenyl

Concen: 3.251 ng/ul

RT: 13.33 min Scan# 1758

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:154 Resp: 165580

Ion Ratio Lower Upper

154 100

153 40.7 32.1 48.1




76 12.9 10.2 15.2

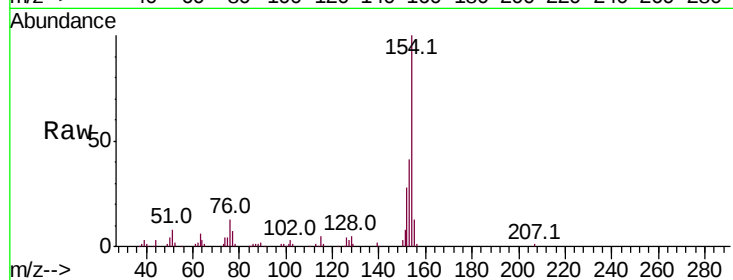

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 76.00 (75.70 to 76.70): BM

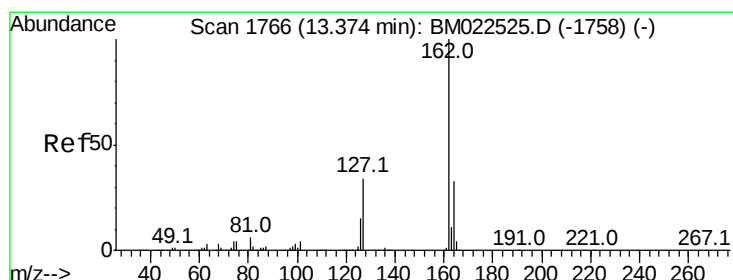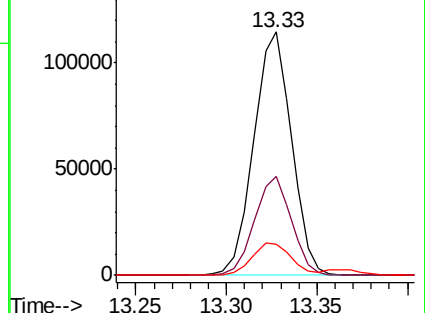

#42

2-Chloronaphthalene

Concen: 3.260 ng/ul

RT: 13.36 min Scan# 1764

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion:162 Resp: 125684

Ion Ratio Lower Upper

162 100

164 32.5 26.1 39.1



127 37.7 30.1 45.1




Abundance Ion 162.00 (161.70 to 162.70): E

Ion 164.00 (163.70 to 164.70): E

Ion 127.00 (126.70 to 127.70): E



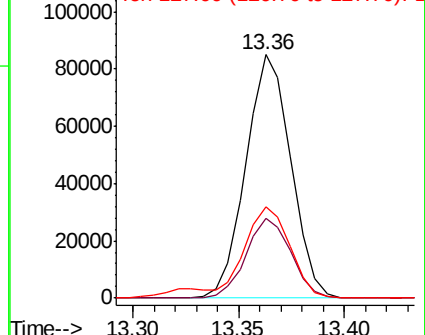



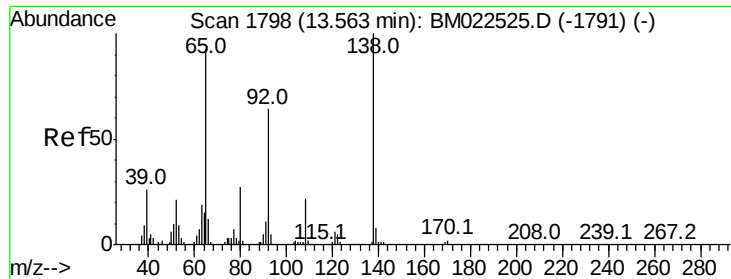

#43
2-Nitroaniline
Concen: 3.051 ng/ul
RT: 13.56 min Scan# 1797
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22




Instrument :
BNA_M
ClientSampled :


Tot Ion: 65 Resp: 27466
Ion Ratio Lower Upper
65 100
92 70.8 55.7 83.5
138 102.6 86.0 129.0

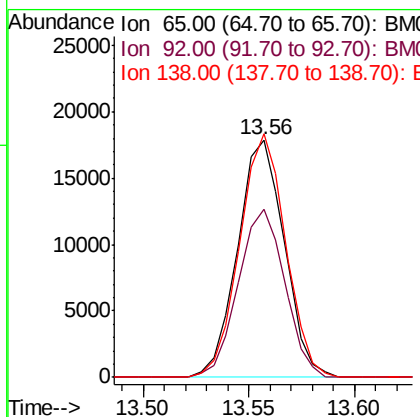

#45
Dimethylphthalate
Concen: 3.374 ng/ul
RT: 13.95 min Scan# 1863
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Tgt Ion:163 Resp: 169747
Ion Ratio Lower Upper
163 100
194 3.9 3.2 4.8
164 10.0 7.8 11.8



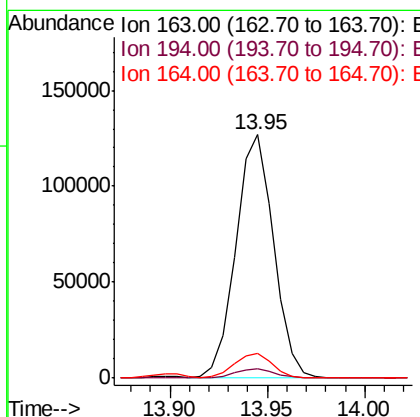





#46
 2,6-Dinitrotoluene
 Concen: 2.761 ng/ul
 RT: 14.05 min Scan# 1881
 Delta R.T. -0.01 min
 Lab File: BM022559.D
 Acq: 06 Sep 2019 19:22




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
165	100		
89	67.8	47.7	71.5
121	25.8	18.4	27.6

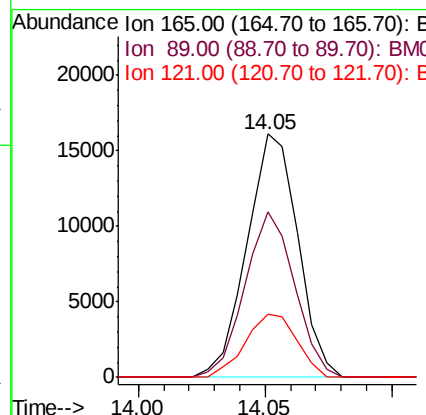

#48
 Acenaphthylene
 Concen: 3.329 ng/ul
 RT: 14.21 min Scan# 1908
 Delta R.T. -0.01 min
 Lab File: BM022559.D
 Acq: 06 Sep 2019 19:22

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.7	15.8	23.8
153	13.1	10.4	15.6

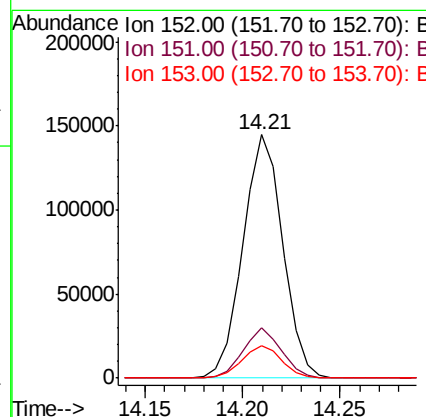



#49

3-Nitroaniline

Concen: 2.618 ng/ul

RT: 14.38 min Scan# 1937

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampled :


Tot Ion:138 Resp: 23252

Ion Ratio Lower Upper

138 100

108 19.0 13.5 20.3




92 113.1 93.7 140.5



Abundance Ion 138.00 (137.70 to 138.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 92.00 (91.70 to 92.70): BM

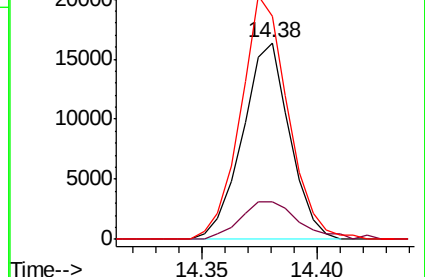

#50

Acenaphthene

Concen: 3.288 ng/ul

RT: 14.55 min Scan# 1966

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion:153 Resp: 140234

Ion Ratio Lower Upper

153 100

152 48.8 37.5 56.3



154 90.9 71.4 107.0




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

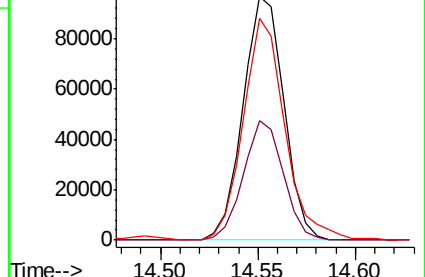



#51

2,4-Dinitrophenol

Concen: 2.909 ng/ul

RT: 14.58 min Scan# 1971

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampled :


Tot Ion:184 Resp: 10931

Ion Ratio Lower Upper

184 100

63 67.9 51.5 77.3




154 86.4 81.9 122.9



Abundance Ion 184.00 (183.70 to 184.70): E

Ion 63.00 (62.70 to 63.70): BM0

Ion 154.00 (153.70 to 154.70): E

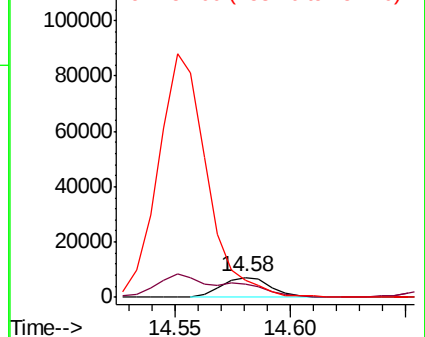

#53

4-Nitrophenol

Concen: 3.578 ng/ul

RT: 14.67 min Scan# 1987

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion:109 Resp: 24336

Ion Ratio Lower Upper

109 100

139 140.8 107.6 161.4



65 165.2 101.9 152.9#




Abundance Ion 109.00 (108.70 to 109.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 65.00 (64.70 to 65.70): BM0

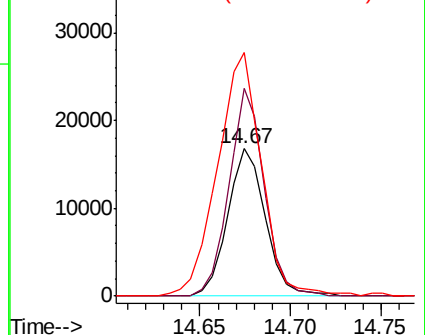

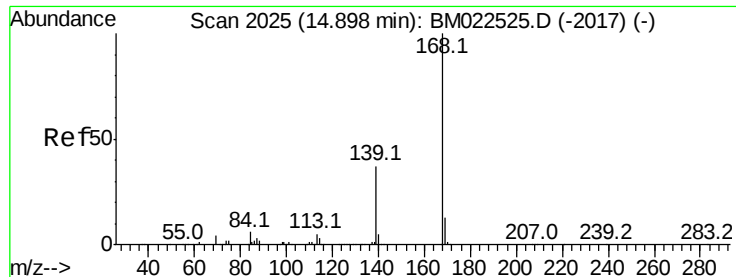

#54

Dibenzenofuran

Concen: 3.400 ng/ul

RT: 14.89 min Scan# 2023

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M


ClientSampleId :

Tot Ion:168 Resp: 201249

Ion Ratio Lower Upper

168 100

139 38.1 29.5 44.3

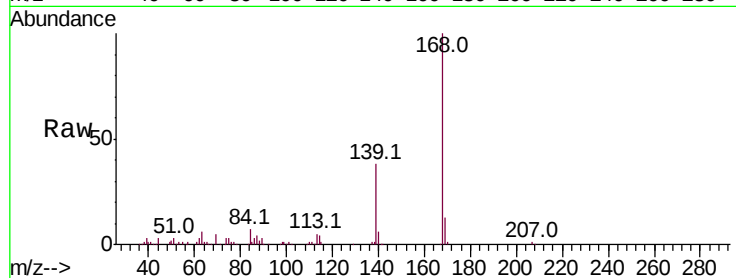

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

150000



100000

50000

0

14.85 14.90

Time-->

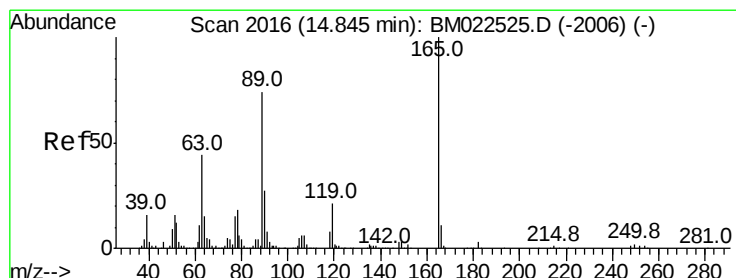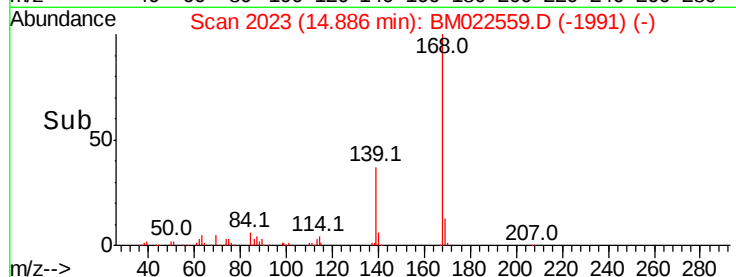

#55

2,4-Dinitrotoluene

Concen: 3.031 ng/ul

RT: 14.84 min Scan# 2015

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion:165 Resp: 36367

Ion Ratio Lower Upper

165 100

63 46.4 35.7 53.5

182 2.1 2.2 3.2#

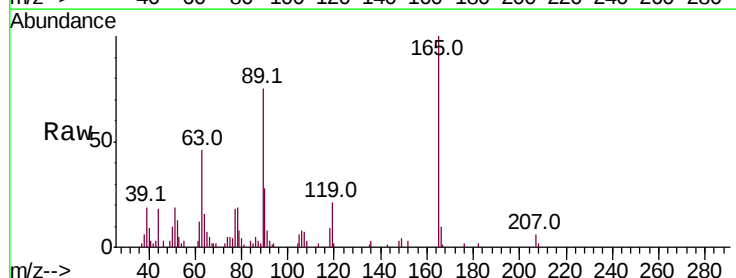

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BM0

Ion 182.00 (181.70 to 182.70): E

30000


20000


10000

0

14.80 14.85

Time-->

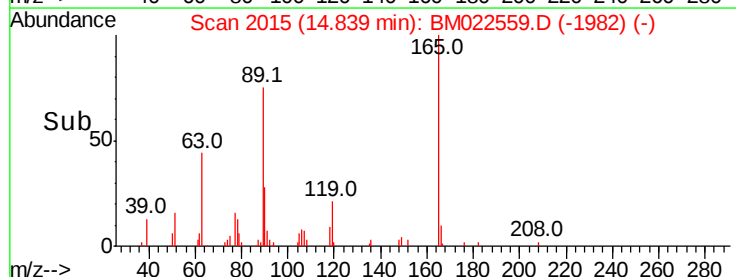


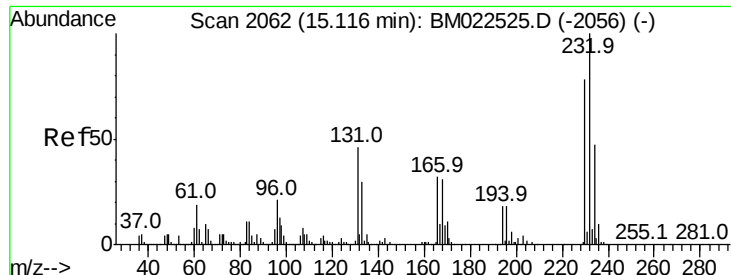




#56
 2,3,4,6-Tetrachlorophenol
 Concen: 2.635 ng/ul
 RT: 15.11 min Scan# 2061
 Delta R.T. -0.01 min
 Lab File: BM022559.D
 Acq: 06 Sep 2019 19:22

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:	232	Resp:	29317
Ion	Ratio	Lower	Upper
232	100		
131	49.6	36.9	55.3
130	3.0	2.0	3.0#
166	34.3	25.2	37.8




Abundance Ion 232.00 (231.70 to 232.70): E
 Ion 131.00 (130.70 to 131.70): E
 Ion 130.00 (129.70 to 130.70): E
 Ion 166.00 (165.70 to 166.70): E

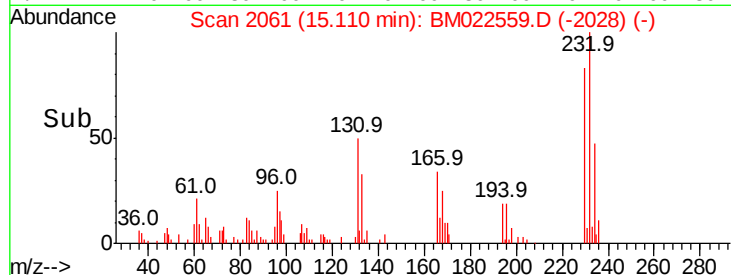
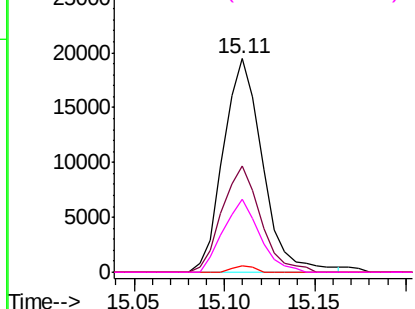



#57
 Diethylphthalate
 Concen: 3.266 ng/ul
 RT: 15.31 min Scan# 2095
 Delta R.T. -0.01 min
 Lab File: BM022559.D
 Acq: 06 Sep 2019 19:22

Tgt Ion:	149	Resp:	170007
Ion	Ratio	Lower	Upper
149	100		
177	21.4	17.3	25.9
150	12.5	10.2	15.2



Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 177.00 (176.70 to 177.70): E
 Ion 150.00 (149.70 to 150.70): E

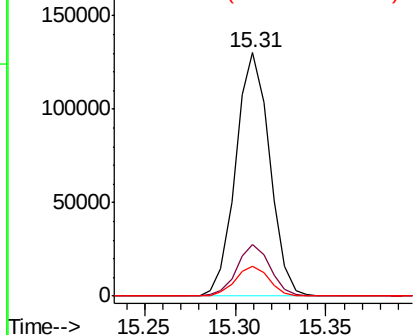

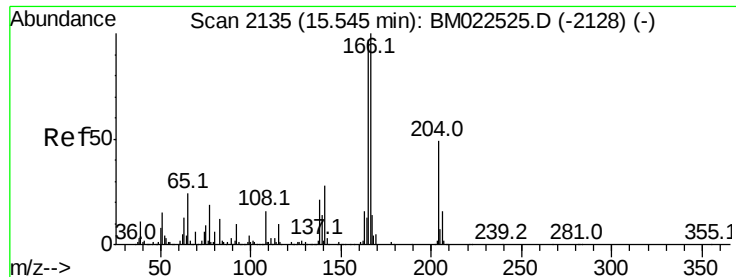

#59

Fluorene

Concen: 3.428 ng/ul

RT: 15.53 min Scan# 2133

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:166 Resp: 166954

Ion Ratio Lower Upper




166 100

165 97.0 77.8 116.8

167 13.8 10.9 16.3

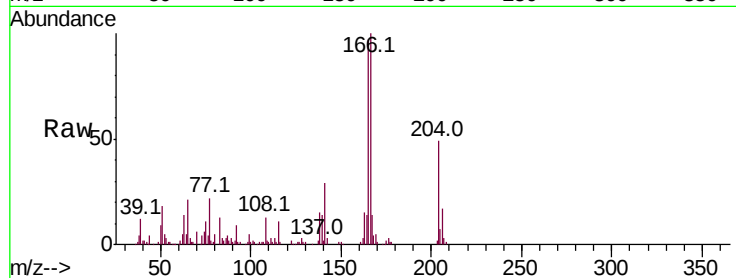

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

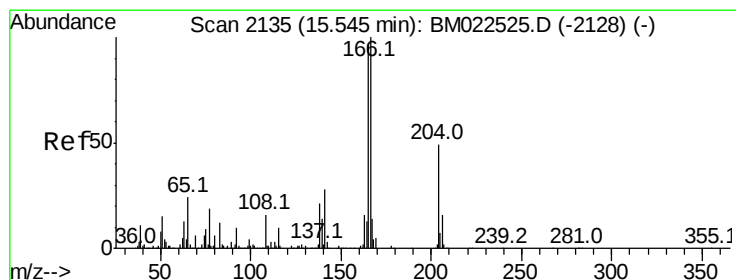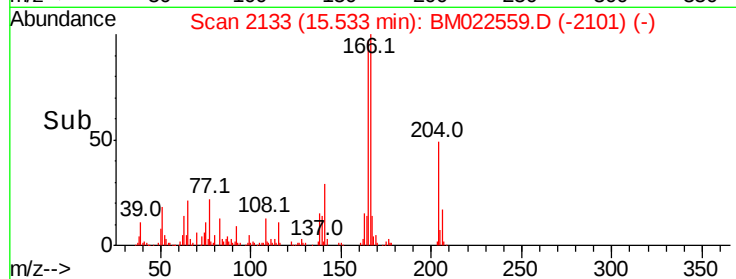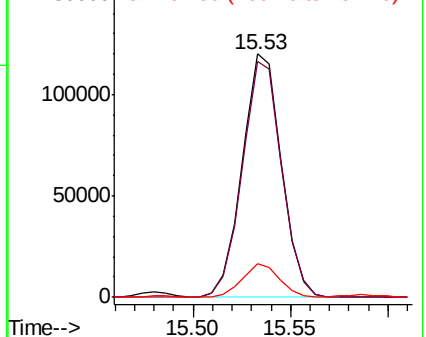

#60

4-Chlorophenyl-phenylether

Concen: 3.338 ng/ul

RT: 15.53 min Scan# 2133

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion:204 Resp: 80442

Ion Ratio Lower Upper



204 100


206 33.6 26.0 39.0

141 58.6 45.4 68.2

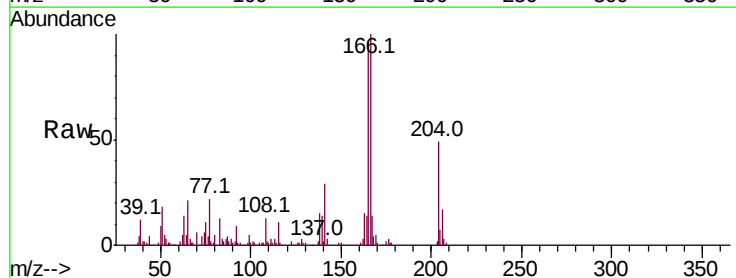

Abundance Ion 204.00 (203.70 to 204.70): E
Ion 206.00 (205.70 to 206.70): E
Ion 141.00 (140.70 to 141.70): E

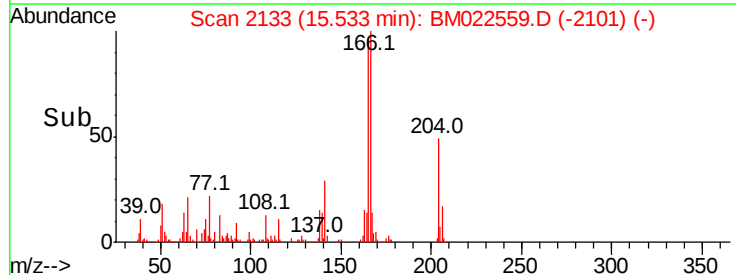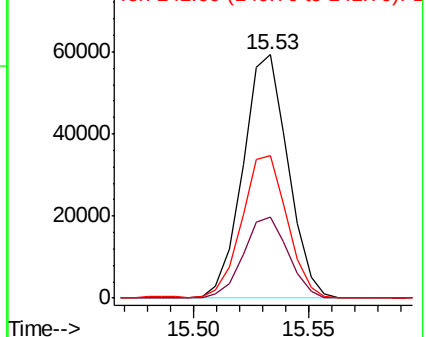

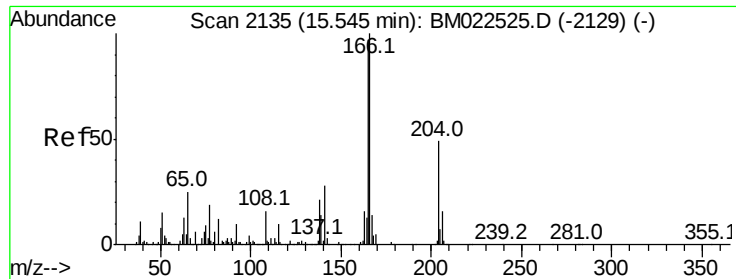

#61

4-Nitroaniline

Concen: 2.620 ng/ul

RT: 15.53 min Scan# 2133

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampled :


Tot Ion:138 Resp: 26515

Ion Ratio Lower Upper

138 100

92 57.2 40.3 60.5




108 85.8 62.2 93.2

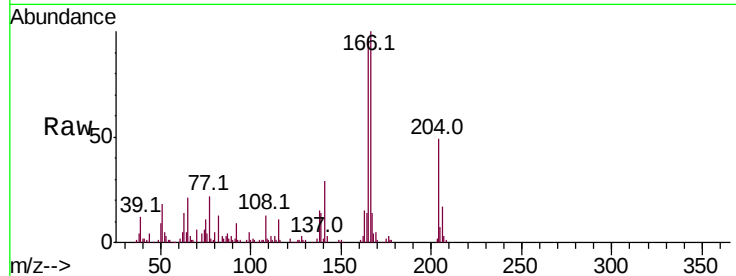

Abundance Ion 138.00 (137.70 to 138.70): E

Ion 92.00 (91.70 to 92.70): BM

Ion 108.00 (107.70 to 108.70): E

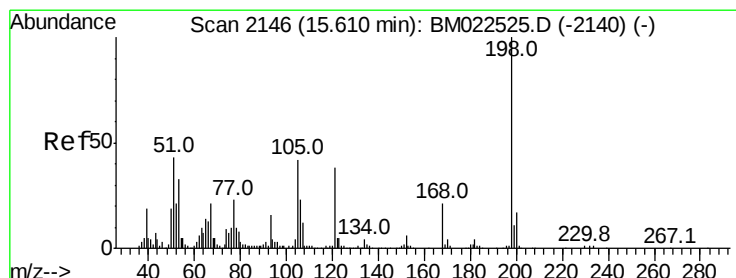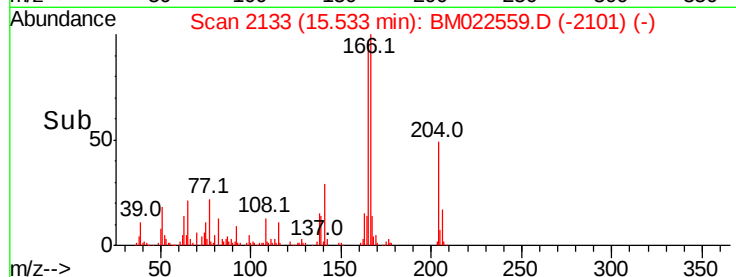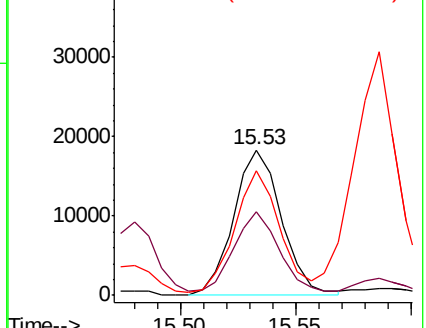

#64

4,6-Dinitro-2-methylphenol

Concen: 2.827 ng/ul

RT: 15.60 min Scan# 2144

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion:198 Resp: 19461

Ion Ratio Lower Upper

198 100

182 8.8 3.4 5.0#



77 45.6 19.7 29.5#

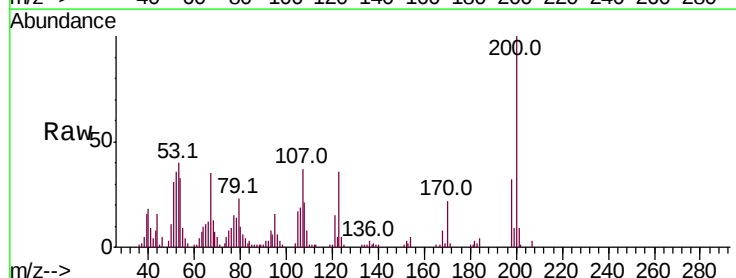


Abundance Ion 198.00 (197.70 to 198.70): E

Ion 182.00 (181.70 to 182.70): E

Ion 77.00 (76.70 to 77.70): BM



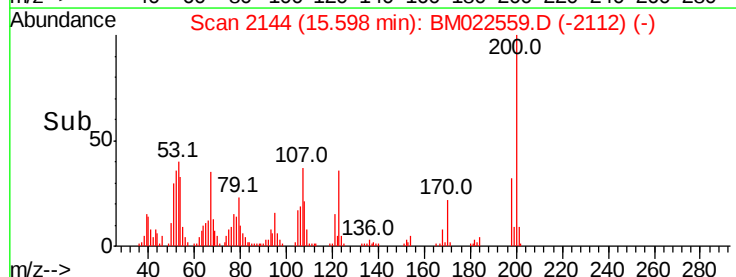
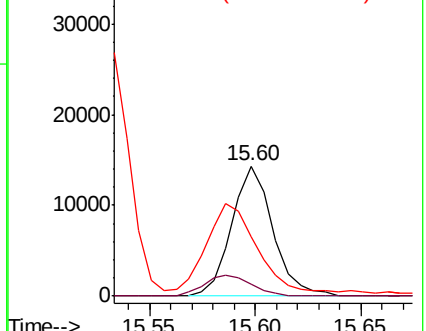




#65
N-Nitrosodiphenylamine
Concen: 3.200 ng/ul
RT: 15.74 min Scan# 2168
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22




Instrument :
BNA_M
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
169	100		
168	67.9	53.5	80.3
167	36.8	29.5	44.3

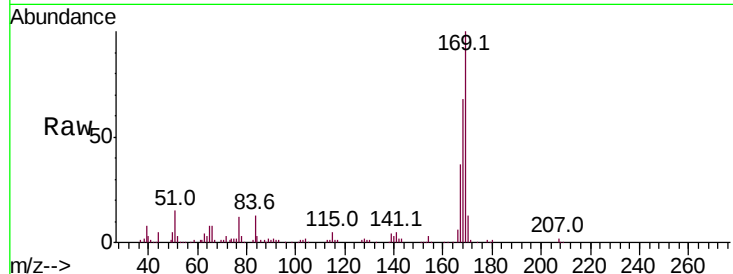

#66
4-Bromophenyl-phenylether
Concen: 2.964 ng/ul
RT: 16.42 min Scan# 2284
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Tgt Ion	Ratio	Lower	Upper
248	100		
250	100.3	76.3	114.5
141	75.1	57.0	85.4


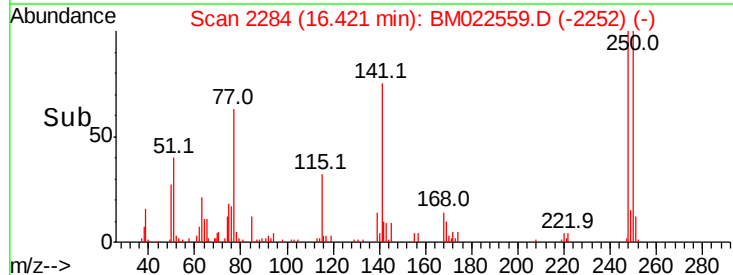




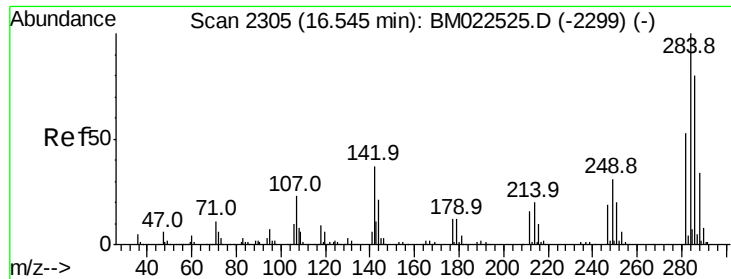

#67
Hexachlorobenzene
Concen: 3.157 ng/ul
RT: 16.54 min Scan# 2304
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22




Instrument :
BNA_M
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
284	100		
142	38.2	29.3	43.9
249	31.4	24.7	37.1

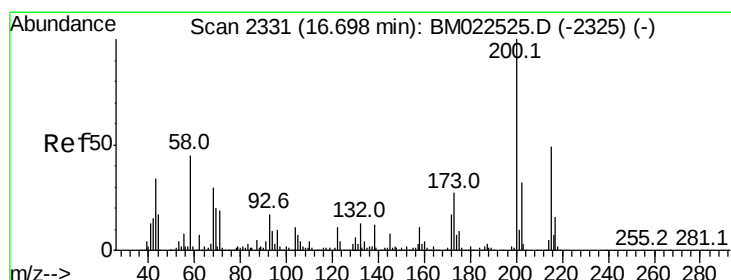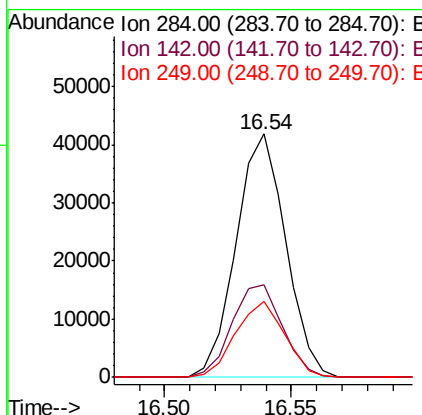

#68
Atrazine
Concen: 2.565 ng/ul
RT: 16.69 min Scan# 2329
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Tgt Ion	Ratio	Lower	Upper
200	100		
173	27.6	21.6	32.4
215	48.9	39.0	58.4

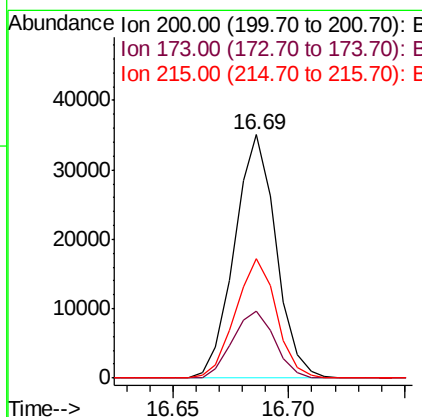


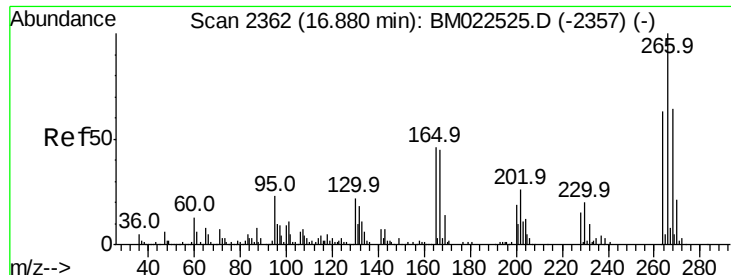




#69
 Pentachlorophenol
 Concen: 2.136 ng/ul
 RT: 16.87 min Scan# 2361
 Delta R.T. -0.01 min
 Lab File: BM022559.D
 Acq: 06 Sep 2019 19:22

Instrument :
 BNA_M
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
266	100		
264	67.3	50.8	76.2
268	64.1	50.9	76.3




Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

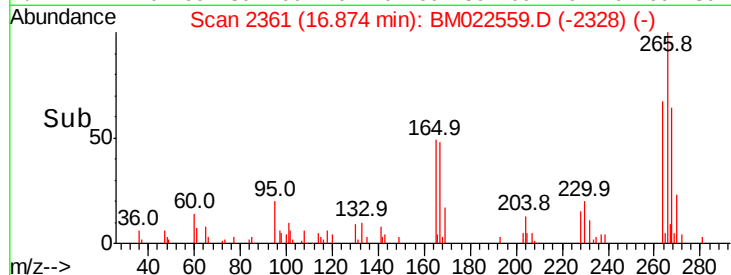
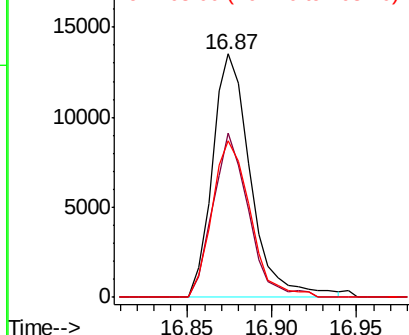



#70
 Phenanthrene
 Concen: 3.360 ng/ul
 RT: 17.27 min Scan# 2428
 Delta R.T. -0.01 min
 Lab File: BM022559.D
 Acq: 06 Sep 2019 19:22

Tgt Ion	Ratio	Lower	Upper
178	100		
179	14.6	12.0	18.0
176	18.9	15.4	23.0



Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

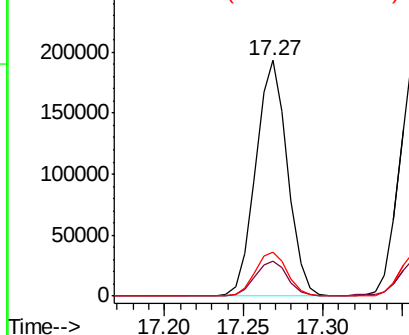



#72

Anthracene

Concen: 3.340 ng/ul

RT: 17.36 min Scan# 2443

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampled :


Tot Ion:178 Resp: 274983

Ion Ratio Lower Upper

178 100

179 15.0 12.3 18.5




176 17.7 14.7 22.1



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

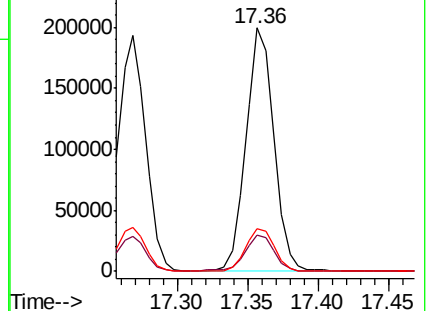

#73

1,2,3,4-Tetrachlorobenzene

Concen: 2.952 ng/uL

RT: 13.29 min Scan# 1752

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion:216 Resp: 60145

Ion Ratio Lower Upper

216 100

214 75.7 62.5 93.7



218 47.1 38.2 57.4




Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

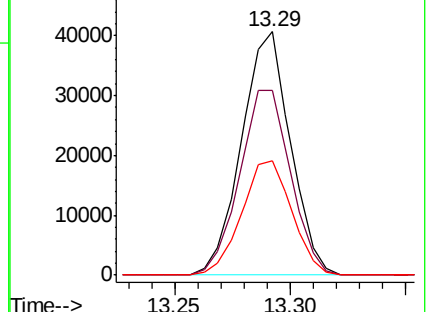

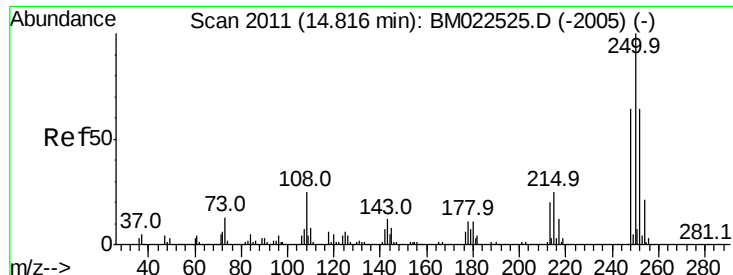

#74

Pentachlorobenzene

Concen: 3.075 ng/uL

RT: 14.81 min Scan# 2010

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:250 Resp: 63165

Ion Ratio Lower Upper

250 100

248 61.9 51.3 76.9

252 62.8 51.1 76.7






Abundance

Ion 250.00 (249.70 to 250.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 252.00 (251.70 to 252.70): E

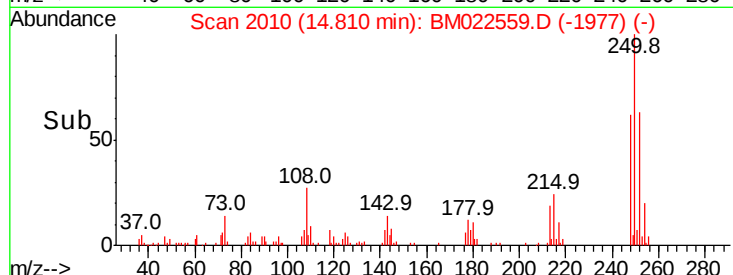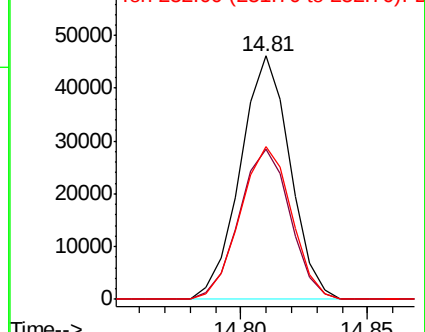

#75

Carbazole

Concen: 3.294 ng/uL

RT: 17.62 min Scan# 2488

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion:167 Resp: 243708

Ion Ratio Lower Upper

167 100

166 21.8 17.4 26.0

139 12.6 10.6 15.8






Abundance

Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E




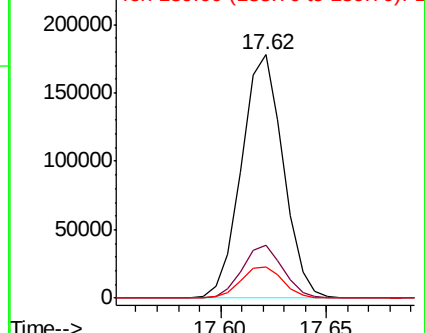




#76
Di-n-butylphthalate
Concen: 2.726 ng/ul
RT: 18.20 min Scan# 2586
Delta R.T. -0.02 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22




Instrument :
BNA_M
ClientSampleId :


Tot Ion:149 Resp: 255424
Ion Ratio Lower Upper
149 100
150 8.8 7.3 10.9
104 5.5 3.9 5.9

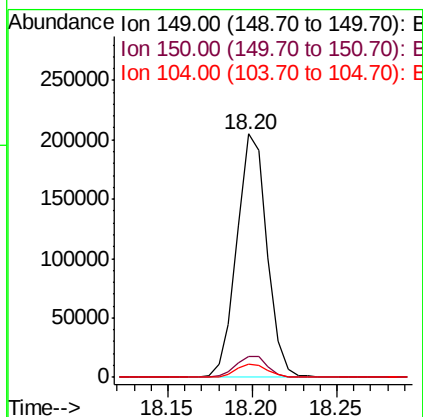

#77
Fluoranthene
Concen: 3.285 ng/ul
RT: 19.28 min Scan# 2770
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Tgt Ion:202 Resp: 298782
Ion Ratio Lower Upper
202 100
101 11.8 8.8 13.2
100 9.0 6.3 9.5

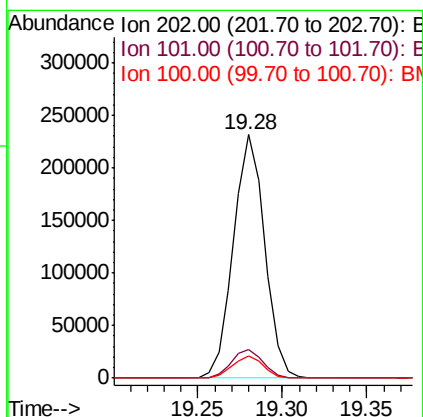

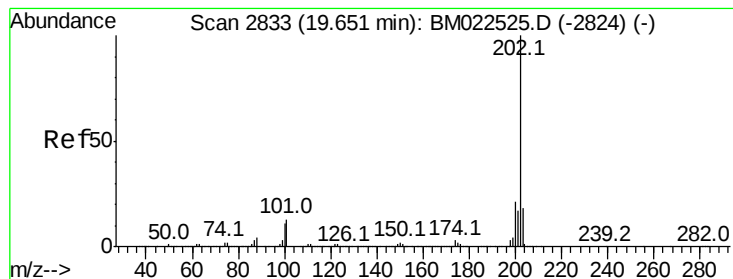

#80

Pvrene

Concen: 3.296 ng/ul

RT: 19.64 min Scan# 2832

Delta R.T. -0.01 min

Lab File: BM022559.D





Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :

Tot Ion:	202	Resp:	330401
Ion	Ratio	Lower	Upper
202	100		
101	13.8	10.6	16.0
100	11.0	8.6	13.0

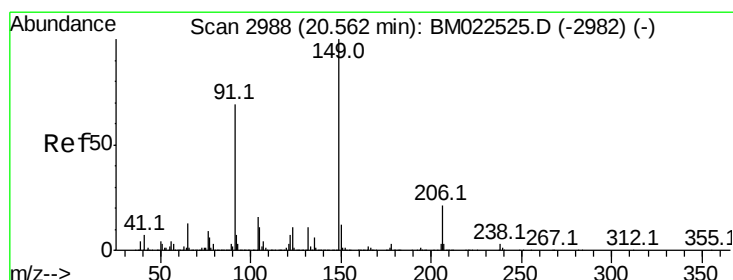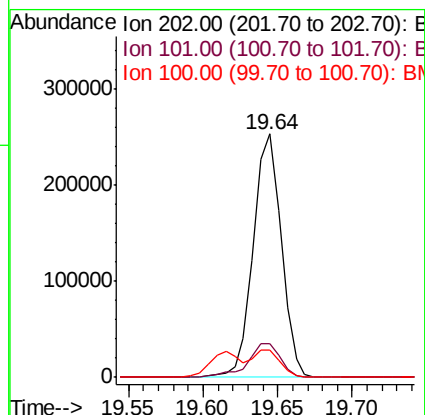

#81

Butylbenzylphthalate

Concen: 2.322 ng/ul




RT: 20.55 min Scan# 2986


Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Tgt Ion:	149	Resp:	98170
Ion	Ratio	Lower	Upper
149	100		
91	71.2	55.4	83.0
206	19.2	17.0	25.4



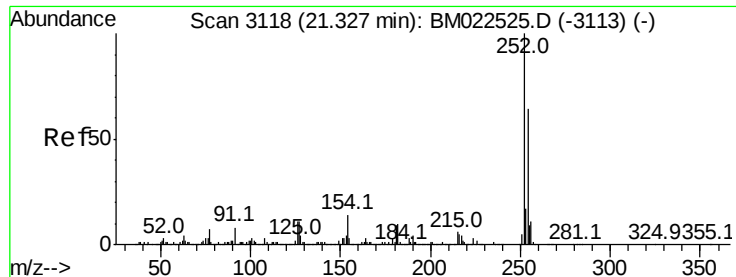


#82

3,3'-Dichlorobenzidine
Concen: 2.109 ng/ul
RT: 21.32 min Scan# 3117
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
252	100		
254	67.7	51.2	76.8
126	12.7	8.6	13.0



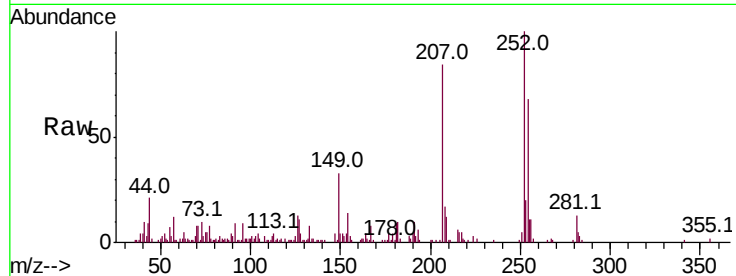


Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 254.00 (253.70 to 254.70): E


Ion 126.00 (125.70 to 126.70): E

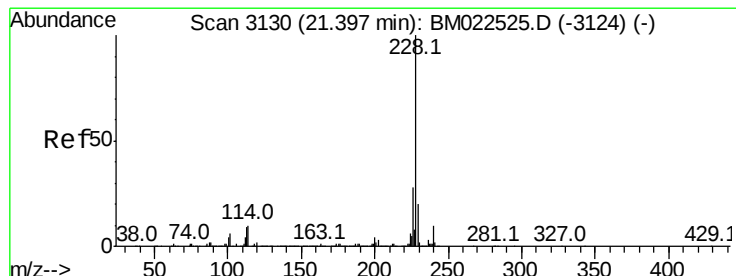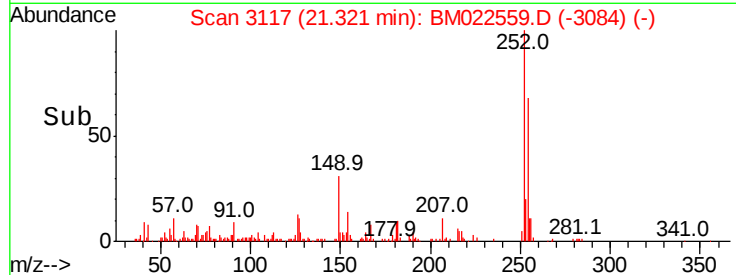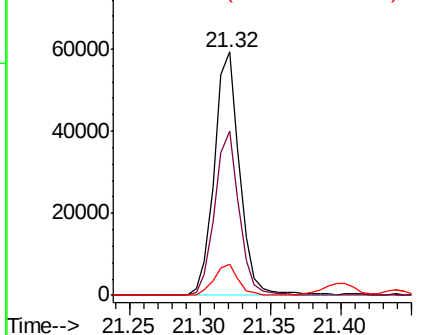

#83

Benzo(a)anthracene
Concen: 3.261 ng/ul
RT: 21.39 min Scan# 3128
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Tgt Ion	Ratio	Lower	Upper
228	100		
229	19.7	15.7	23.5
226	26.8	22.2	33.2


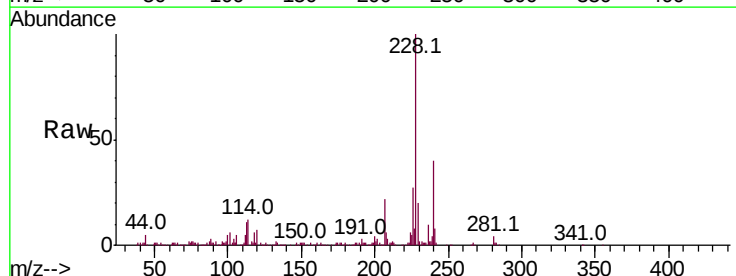



Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

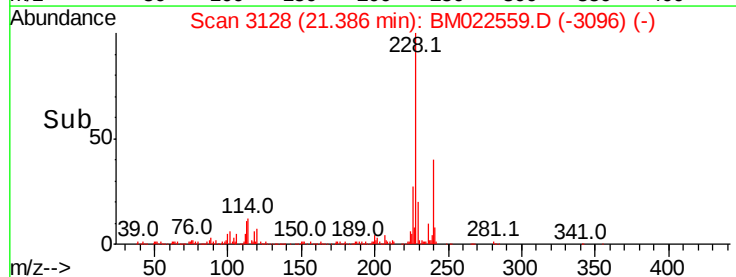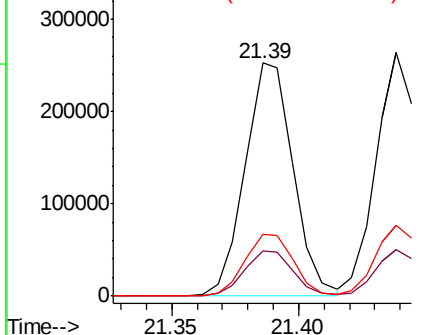







#84
Bis(2-ethylhexyl)phthalate
Concen: 2.416 ng/ul
RT: 21.33 min Scan# 3119
Delta R.T. -0.02 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Instrument :
BNA_M
ClientSampleId :

Tot Ion:149 Resp: 154947
Ion Ratio Lower Upper
149 100
167 25.2 21.7 32.5
279 3.1 3.5 5.3#




Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E


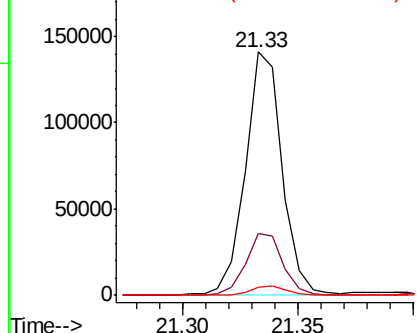



#85
Chrysene
Concen: 3.359 ng/ul
RT: 21.44 min Scan# 3137
Delta R.T. -0.01 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Tgt Ion:228 Resp: 317682
Ion Ratio Lower Upper
228 100
226 29.3 24.2 36.4
229 19.1 15.8 23.6



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

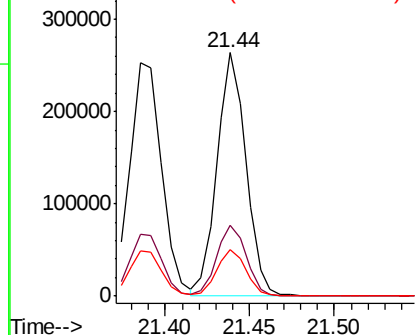







#87
 Di-n-octyl phthalate
 Concen: 2.066 ng/ul
 RT: 22.23 min Scan# 3272
 Delta R.T. -0.02 min
 Lab File: BM022559.D
 Acq: 06 Sep 2019 19:22

Instrument :
 BNA_M
 ClientSampleId :

Tgt Ion:149 Resp: 243244




Abundance Ion 149.00 (148.70 to 149.70): E

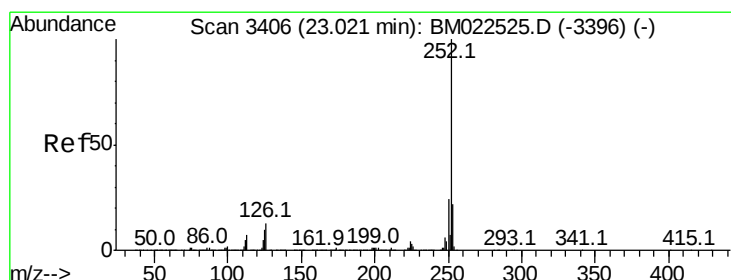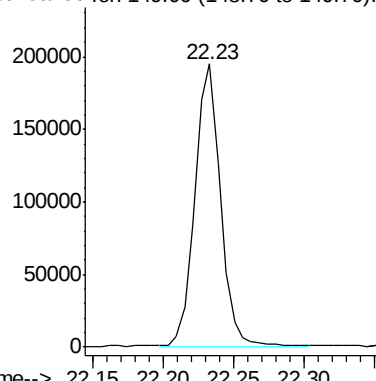

#88
 Benzo(b)fluoranthene
 Concen: 3.075 ng/ul
 RT: 23.00 min Scan# 3403
 Delta R.T. -0.02 min
 Lab File: BM022559.D
 Acq: 06 Sep 2019 19:22

Tgt Ion:252 Resp: 332676



Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.8	26.6
125	10.6	8.0	12.0




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

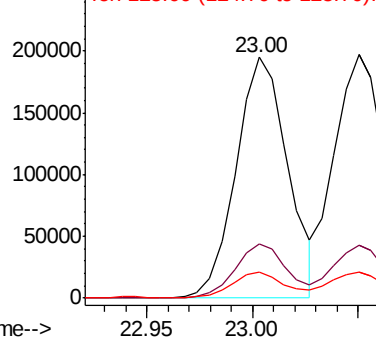



#89

Benzo(k)fluoranthene

Concen: 3.192 ng/ul

RT: 23.05 min Scan# 3411

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 335600

Ion Ratio Lower Upper

252 100

253 21.5 17.4 26.2




125 10.6 8.2 12.2



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

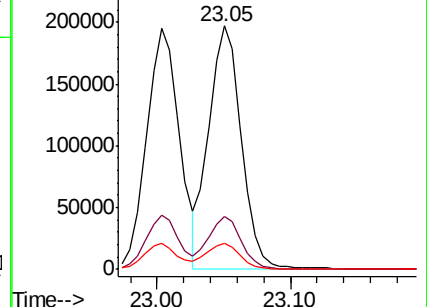

#91

Benzo(a)pyrene

Concen: 3.322 ng/ul

RT: 23.60 min Scan# 3504

Delta R.T. -0.01 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22


Tgt Ion:252 Resp: 342933

Ion Ratio Lower Upper

252 100

253 22.8 17.5 26.3



125 11.8 8.9 13.3




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

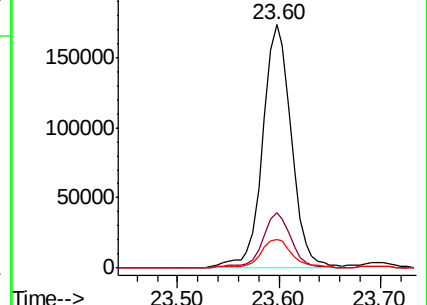




#92




Indeno(1,2,3-cd)pyrene
Concen: 3.251 ng/ul
RT: 26.03 min Scan# 3917
Delta R.T. -0.03 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Instrument :
BNA_M
ClientSampleId :

Tot Ion:276 Resp: 387793
Ion Ratio Lower Upper
276 100
138 25.0 19.2 28.8
277 25.8 19.8 29.8




Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

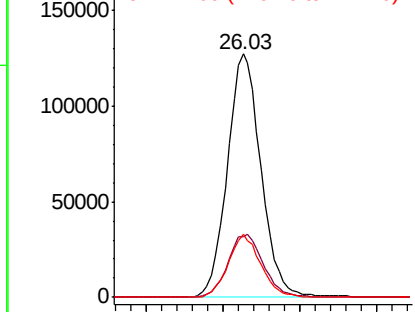



#93


Dibenzo(a,h)anthracene
Concen: 3.304 ng/ul
RT: 26.04 min Scan# 3919
Delta R.T. -0.03 min
Lab File: BM022559.D
Acq: 06 Sep 2019 19:22

Tgt Ion:278 Resp: 327897
Ion Ratio Lower Upper
278 100
139 17.7 13.3 19.9
279 23.0 19.2 28.8



Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

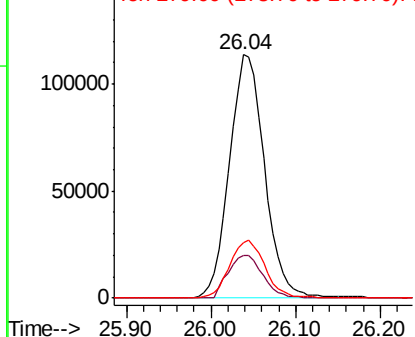



#94

Benzo(a,h,i)perylene

Concen: 3.253 ng/ul

RT: 26.73 min Scan# 4037

Delta R.T. -0.04 min

Lab File: BM022559.D

Acq: 06 Sep 2019 19:22

Instrument :

BNA_M

ClientSampleId :



Tot Ion:276 Resp: 318669

Ion Ratio Lower Upper

276 100

138 22.2 17.0 25.6

277 22.9 18.8 28.2



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

