

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041676.D
 Acq On : 07 Sep 2023 02:04
 Operator : MA/JU
 Sample : 04209-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH467

Quant Time: Sep 07 03:21:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 06 02:20:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	6656	0.400	ng/ul	0.00
4) Naphthalene-d8	10.823	136	15929	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.643	164	8040	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.396	188	15308	0.400	ng/ul	0.00
17) Chrysene-d12	21.565	240	8949	0.400	ng/ul	# 0.00
23) Perylene-d12	23.997	264	11680	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	45140	4.438	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.401	152	8225	0.401	ng/ul	0.00
18) Fluoranthene-d10	19.413	212	14113	0.325	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.785	202	3552	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.842	252	6987	0.082	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041676.D
Acq On : 07 Sep 2023 02:04
Operator : MA/JU
Sample : 04209-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH467

Quant Time: Sep 07 03:21:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 06 02:20:07 2023
Response via : Initial Calibration

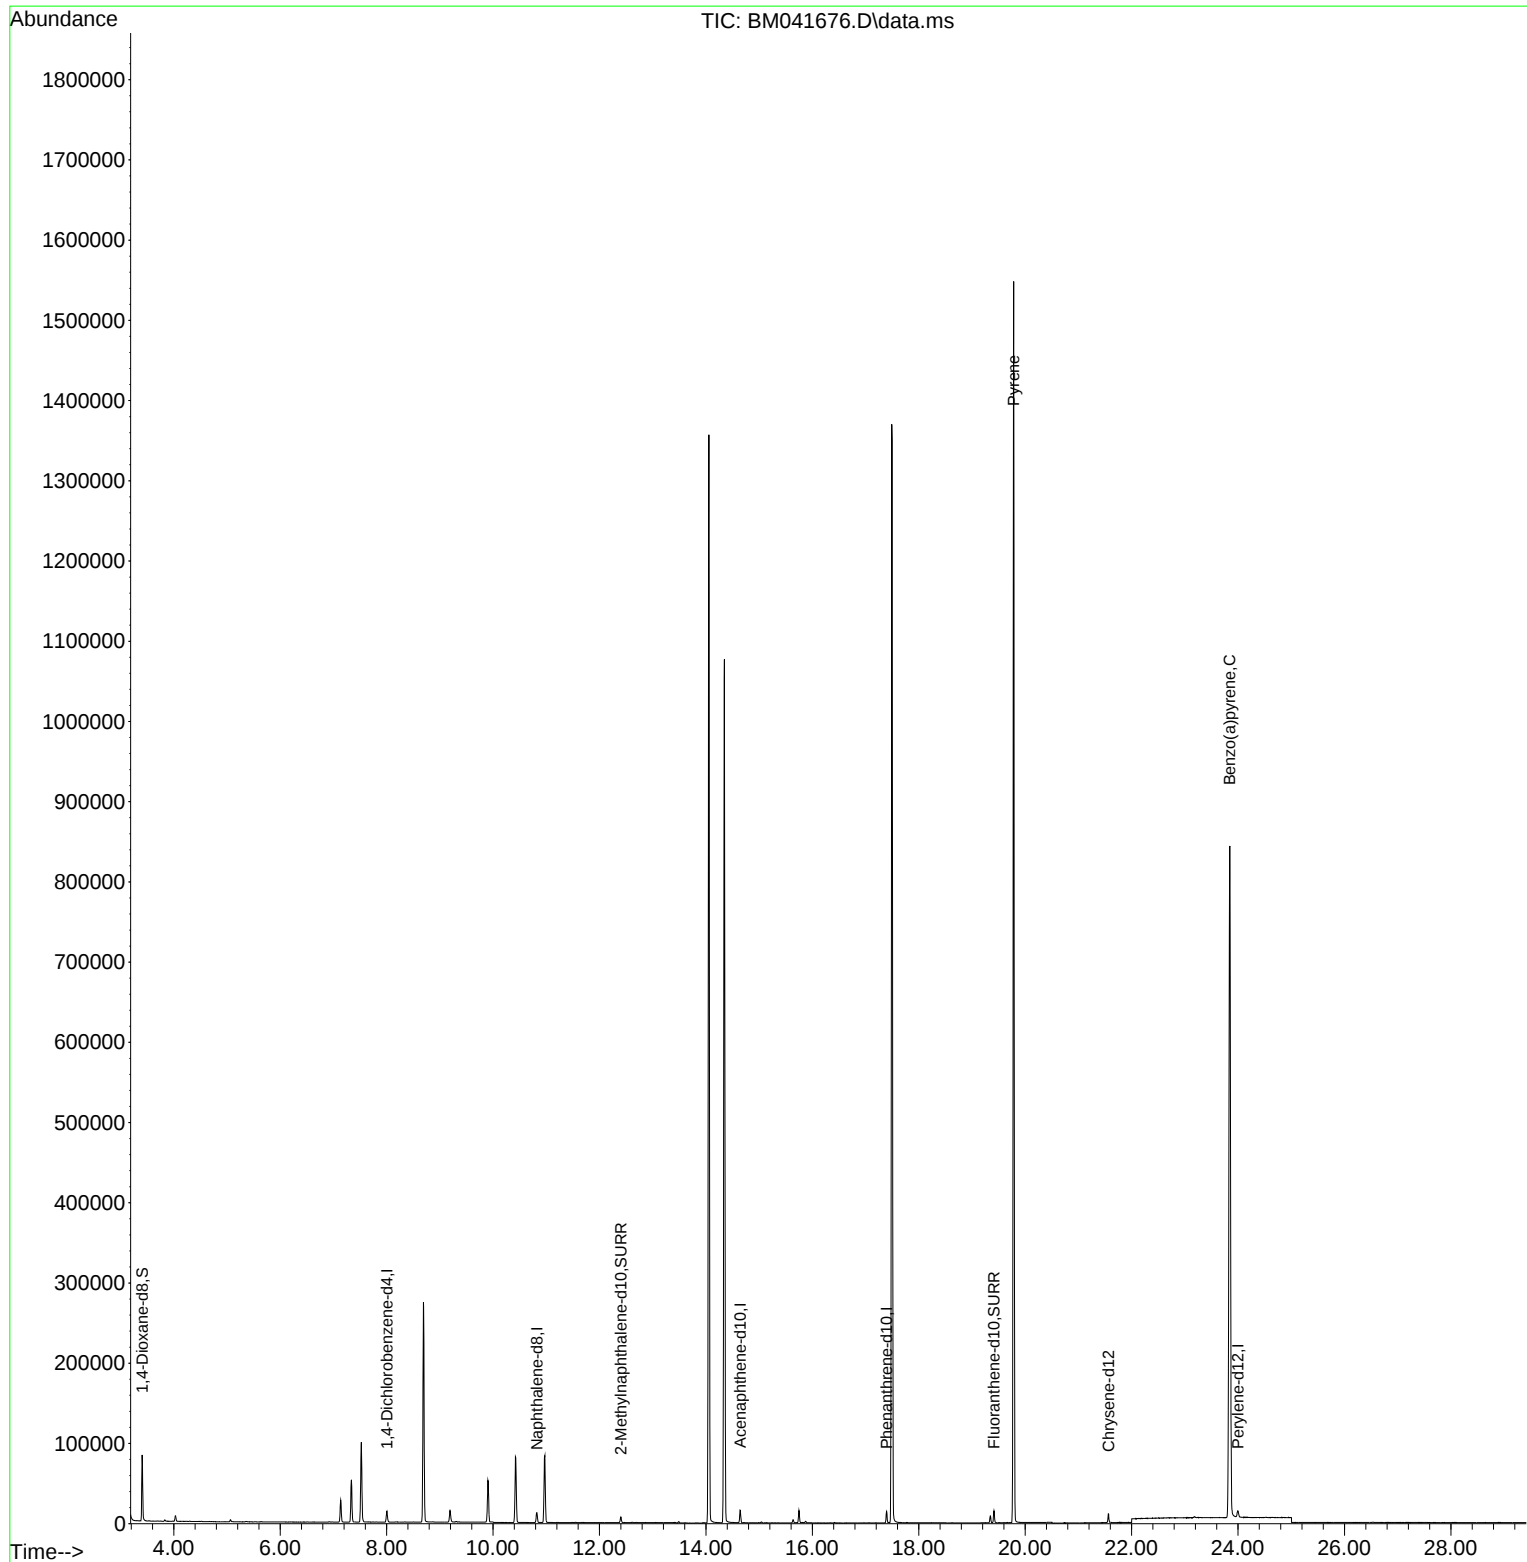

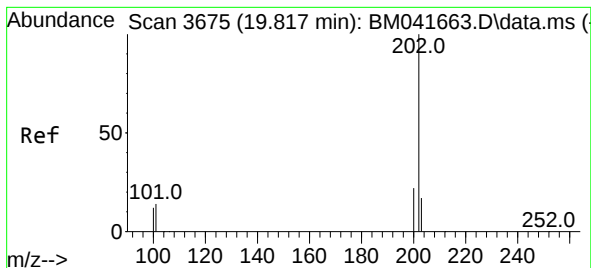

#20

Pyrene

Concen: 0.034 ng/ul

RT: 19.785 min Scan# 3668

Delta R.T. -0.032 min

Lab File: BM041676.D

Acq: 07 Sep 2023 02:04

Instrument :

BNA_M

ClientSampleId :

BH467





Tgt Ion:202 Resp: 3552

Ion Ratio Lower Upper

202 100

101 155.9 11.8 17.8#

100 1138.0 9.8 14.6#

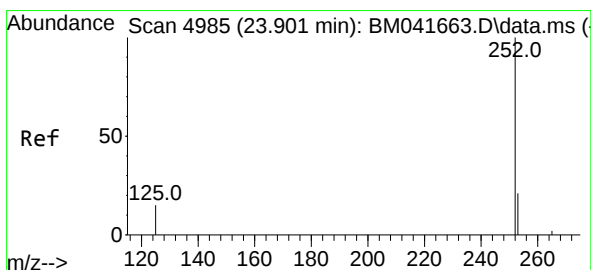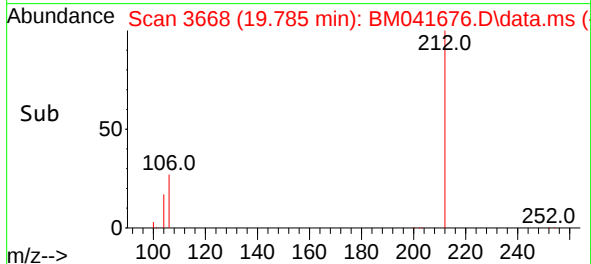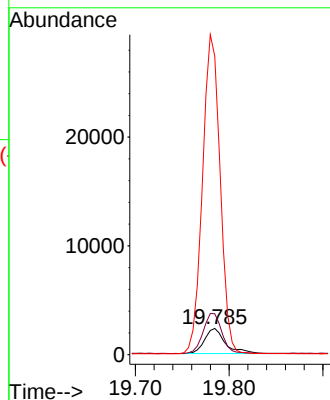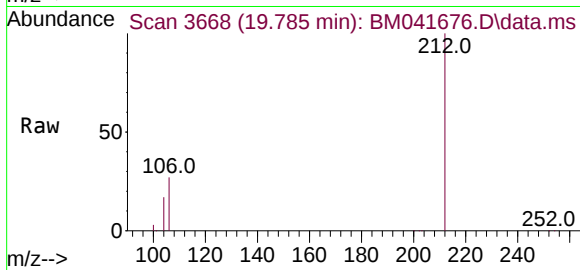

#26

Benzo(a)pyrene

Concen: 0.082 ng/ul

RT: 23.842 min Scan# 4965

Delta R.T. -0.055 min

Lab File: BM041676.D

Acq: 07 Sep 2023 02:04

Tgt Ion:252 Resp: 6987

Ion Ratio Lower Upper

252 100

253 45.4 22.4 33.6#

125 51.0 21.0 31.4#

