

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041677.D
 Acq On : 07 Sep 2023 02:41
 Operator : MA/JU
 Sample : 04209-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH468

Quant Time: Sep 07 03:22:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 06 02:20:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	7208	0.400	ng/ul	0.00
4) Naphthalene-d8	10.823	136	18491	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.643	164	9634	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.396	188	17865	0.400	ng/ul	0.00
17) Chrysene-d12	21.562	240	8841	0.400	ng/ul	# 0.00
23) Perylene-d12	23.994	264	10794	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	47277	4.292	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.401	152	9918	0.417	ng/ul	0.00
18) Fluoranthene-d10	19.413	212	15742	0.367	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.444	88	385	0.034	ng/ul#	27
20) Pyrene	19.785	202	3842	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.839	252	6798	0.087	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041677.D
Acq On : 07 Sep 2023 02:41
Operator : MA/JU
Sample : 04209-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH468

Quant Time: Sep 07 03:22:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 06 02:20:07 2023
Response via : Initial Calibration




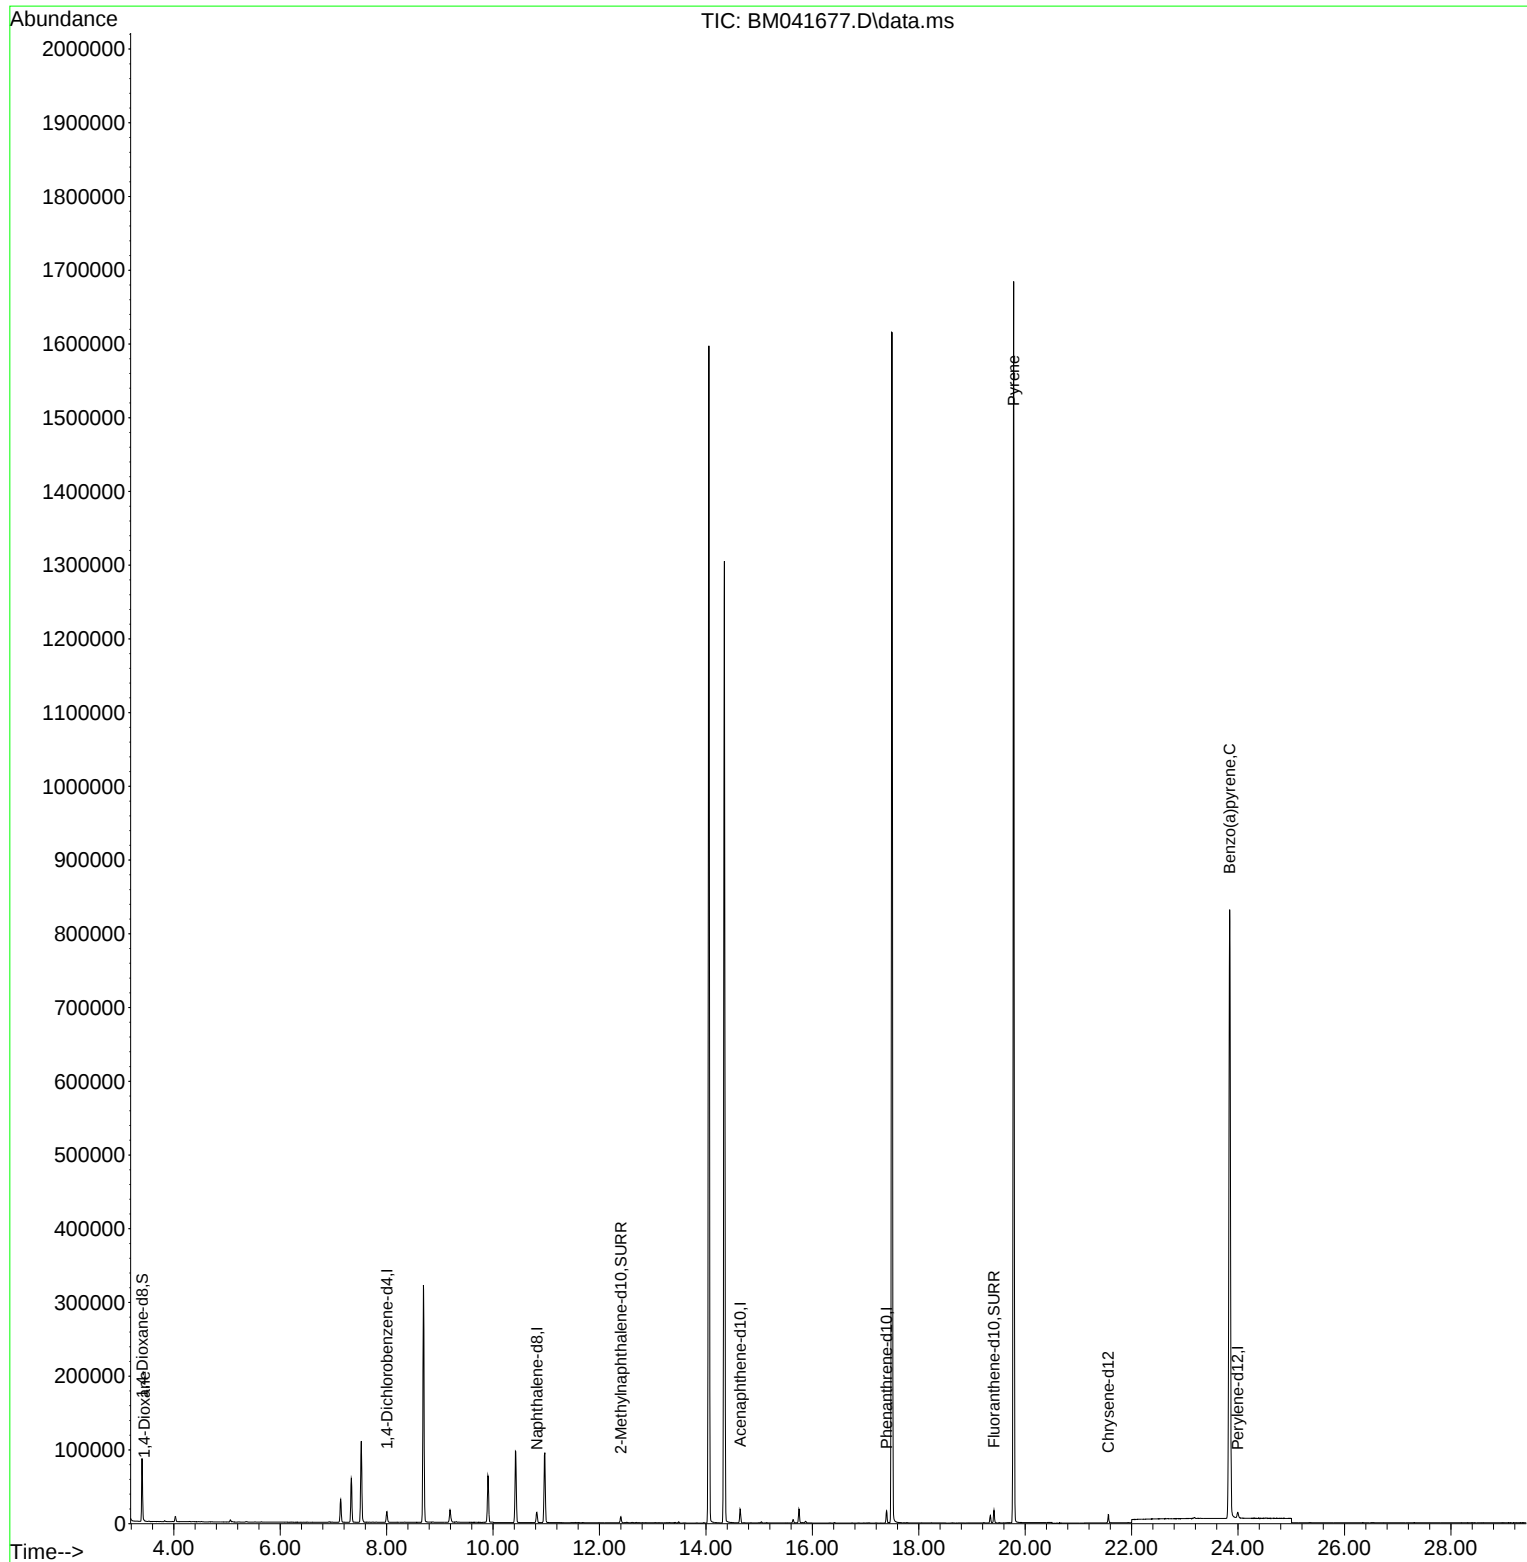


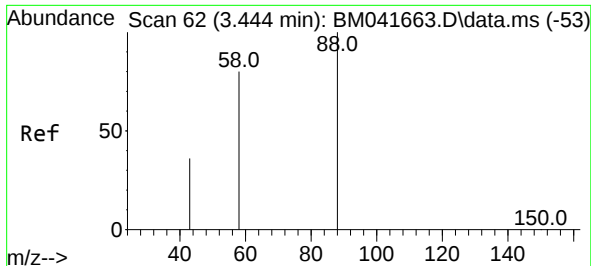

#2
1,4-Dioxane
Concen: 0.034 ng/ul
RT: 3.444 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM041677.D
Acq: 07 Sep 2023 02:41




Instrument :
BNA_M
ClientSampleId :
BH468


Tgt Ion: 88 Resp: 385
Ion Ratio Lower Upper
88 100
43 129.0 33.8 50.6#
58 41.2 54.2 81.2#

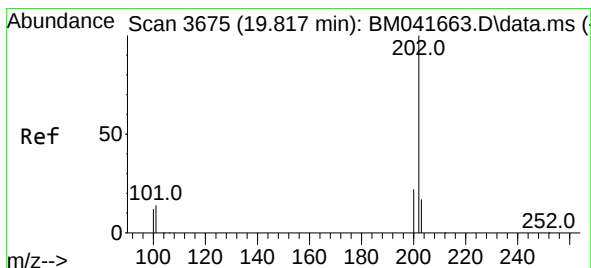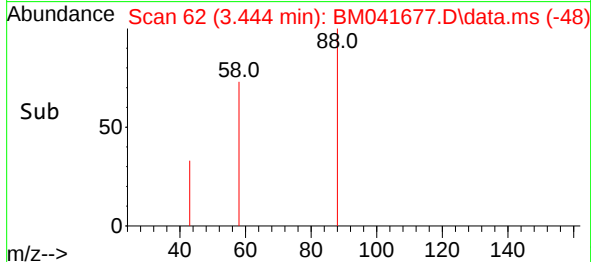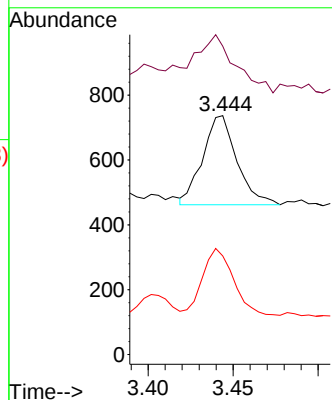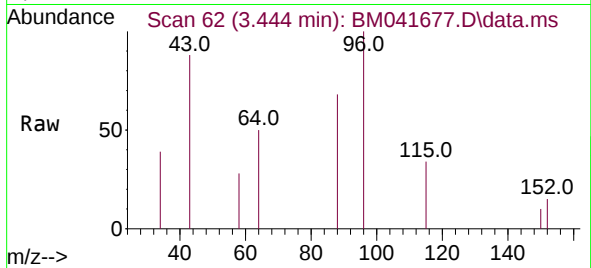

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.785 min Scan# 3668
Delta R.T. -0.032 min
Lab File: BM041677.D
Acq: 07 Sep 2023 02:41


Tgt Ion: 202 Resp: 3842
Ion Ratio Lower Upper
202 100
101 157.3 11.8 17.8#
100 1157.4 9.8 14.6#

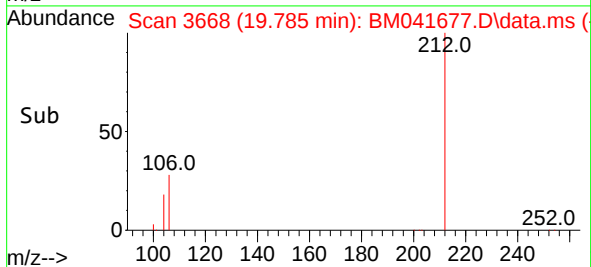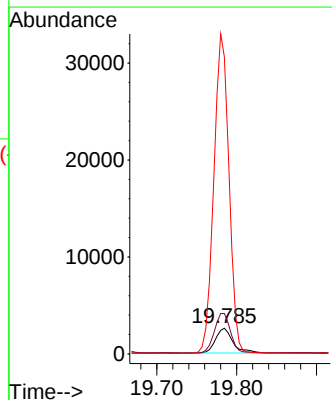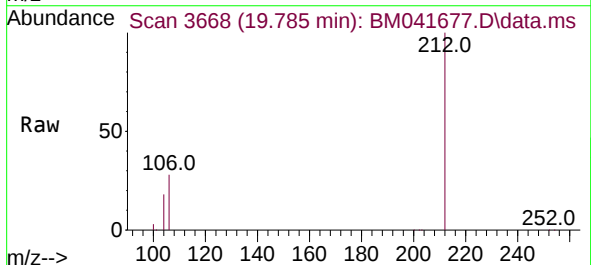

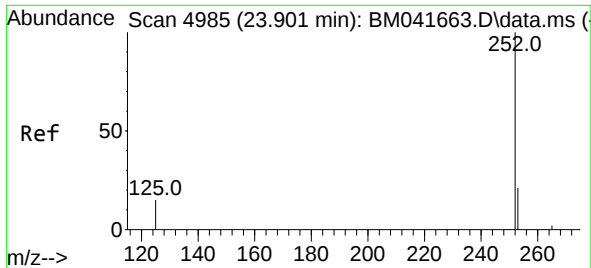

#26
 Benzo(a)pyrene
 Concen: 0.087 ng/ul
 RT: 23.839 min Scan# 49
 Delta R.T. -0.058 min
 Lab File: BM041677.D
 Acq: 07 Sep 2023 02:41

Instrument :
 BNA_M
 ClientSampleId :
 BH468

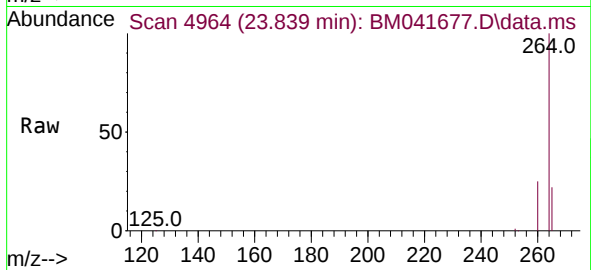

Tgt Ion:252 Resp: 6798
 Ion Ratio Lower Upper
 252 100
 253 45.4 22.4 33.6#
 125 47.9 21.0 31.4#

