

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
 Data File : BM041689.D
 Acq On : 07 Sep 2023 11:20
 Operator : MA/JU
 Sample : PB155169BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK079

Quant Time: Sep 08 02:52:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 06 02:20:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.001	152	5452	0.400	ng/ul	0.00
4) Naphthalene-d8	10.818	136	12734	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.643	164	5728	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.392	188	10441	0.400	ng/ul	0.00
17) Chrysene-d12	21.565	240	4100	0.400	ng/ul	0.00
23) Perylene-d12	23.997	264	5857	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	49994	6.000	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	5216	0.318	ng/ul	-0.01
18) Fluoranthene-d10	19.413	212	6437	0.324	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.780	202	2214	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.842	252	4386	0.103	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090623\
Data File : BM041689.D
Acq On : 07 Sep 2023 11:20
Operator : MA/JU
Sample : PB155169BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK079

Quant Time: Sep 08 02:52:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 06 02:20:07 2023
Response via : Initial Calibration

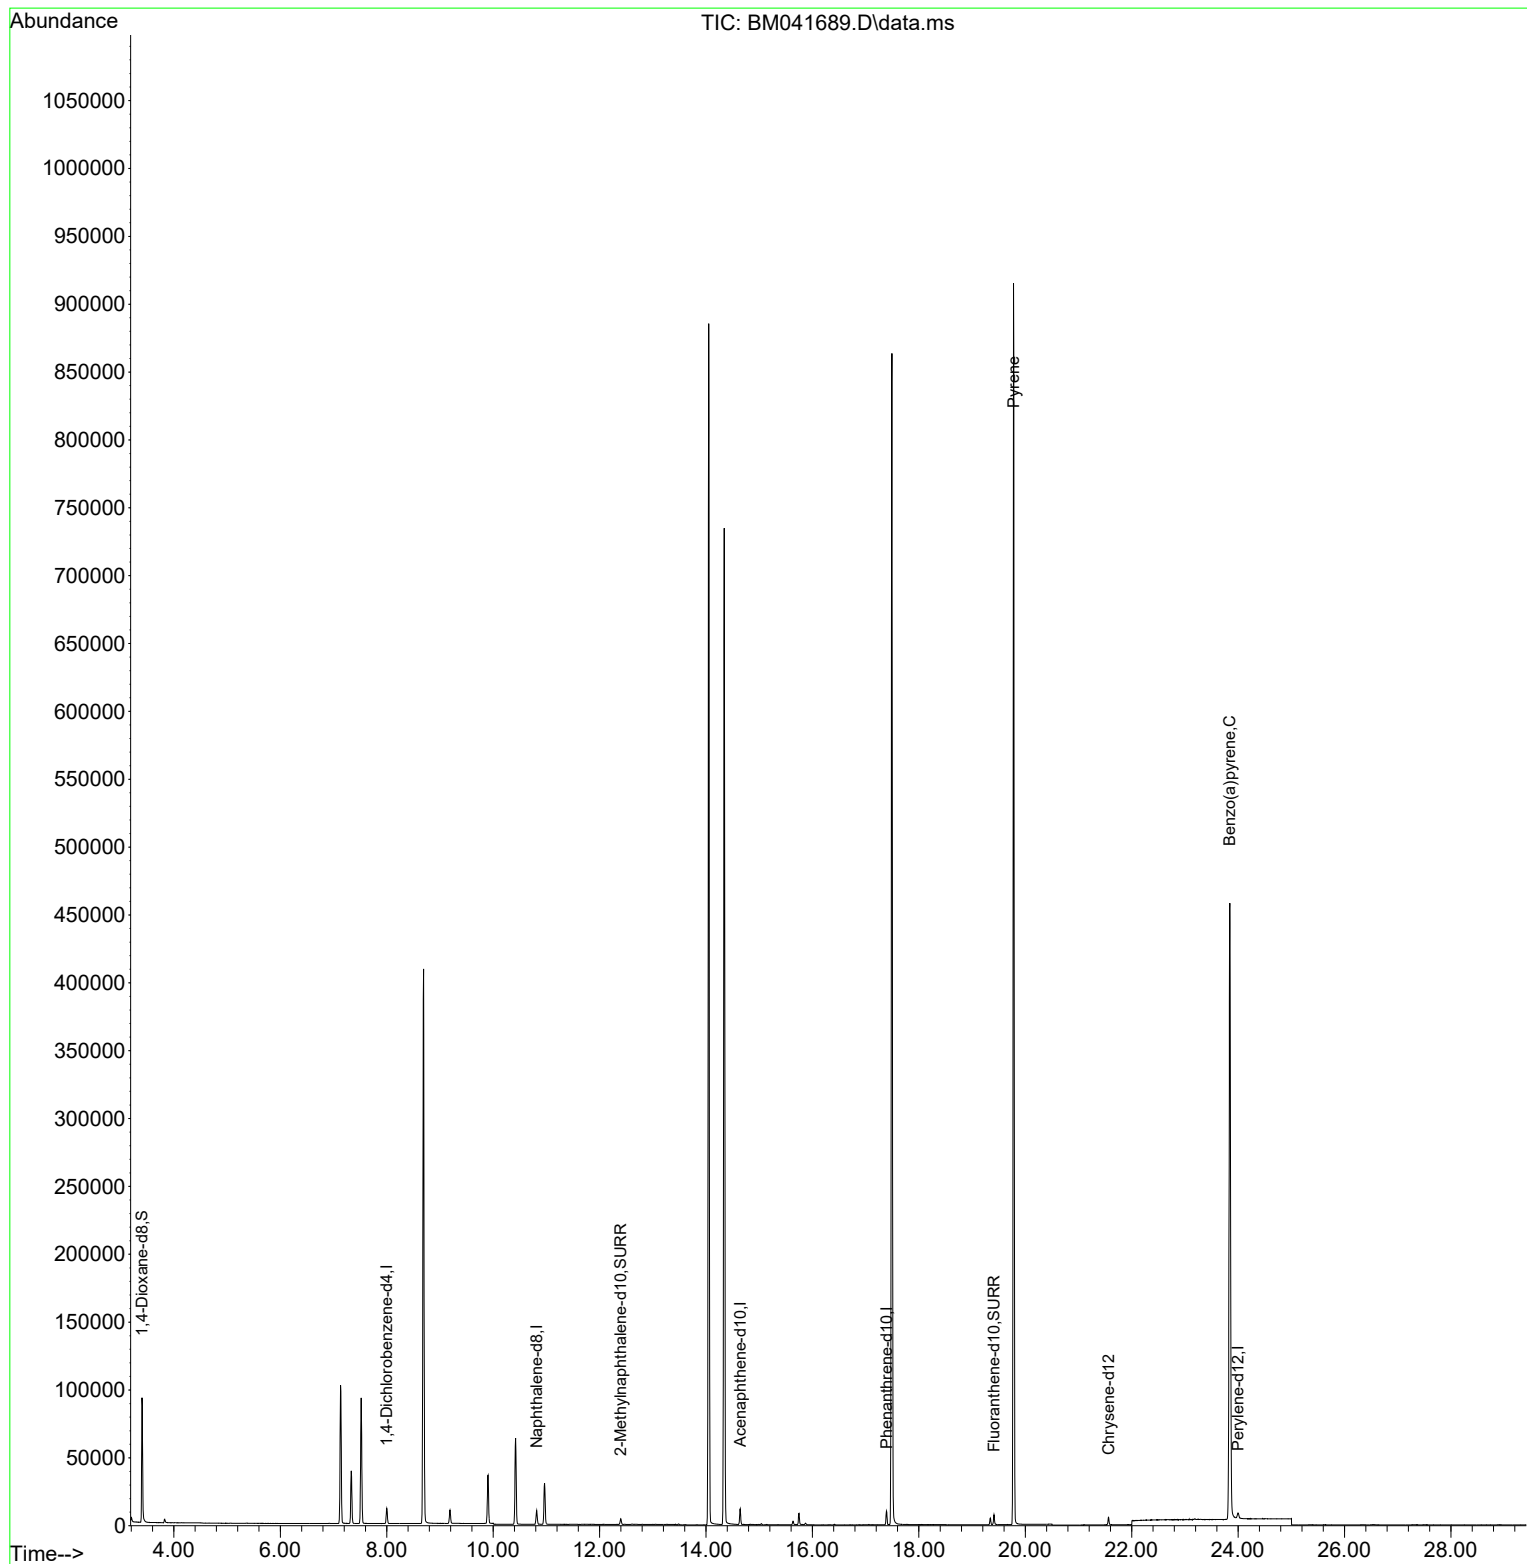

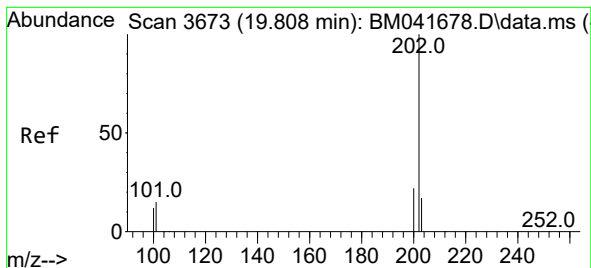

#20

Pyrene

Concen: 0.046 ng/ul

RT: 19.780 min Scan# 3

Delta R.T. -0.037 min

Lab File: BM041689.D

Acq: 07 Sep 2023 11:20

Instrument :

BNA_M

ClientSampleId :

SBLK079





Tgt Ion:202 Resp: 2214

Ion Ratio Lower Upper

202 100

101 172.0 11.8 17.8#

100 1268.2 9.8 14.6#

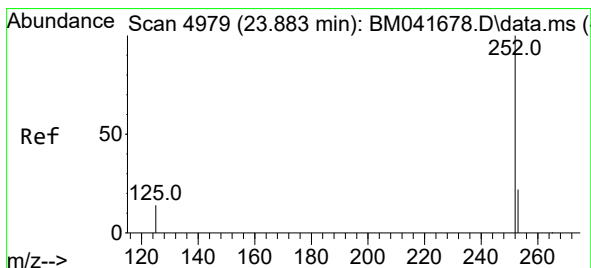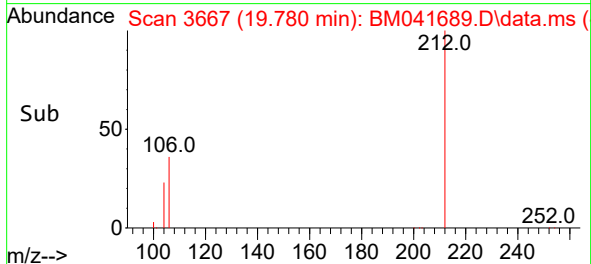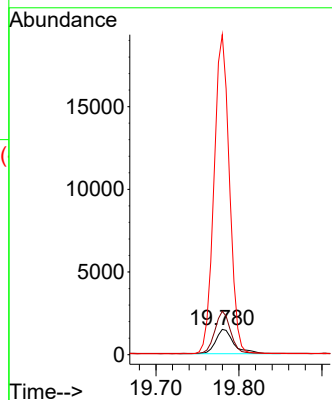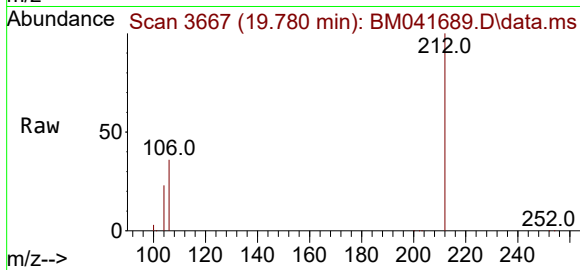

#26

Benzo(a)pyrene

Concen: 0.103 ng/ul

RT: 23.842 min Scan# 4965

Delta R.T. -0.055 min

Lab File: BM041689.D

Acq: 07 Sep 2023 11:20

Tgt Ion:252 Resp: 4386

Ion Ratio Lower Upper

252 100

253 46.4 22.4 33.6#

125 48.9 21.0 31.4#

